

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092418\  
 Data File : PS001812.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 24 Sep 2018 21:42  
 Operator : EI\SJ  
 Sample : J4777-24  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 25 06:30:31 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS091718.M  
 Quant Title : 8080.M  
 QLast Update : Tue Sep 18 03:01:16 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml     |
|-----------------------------|--------------|--------|--------|----------|----------|---------|-----------|
| -----                       |              |        |        |          |          |         |           |
| System Monitoring Compounds |              |        |        |          |          |         |           |
| 4) S                        | 2,4-DCAA     | 11.458 | 10.956 | 65117891 | 63802785 | 290.296 | 251.176   |
| Target Compounds            |              |        |        |          |          |         |           |
| 1) T                        | Dalapon      | 2.889  | 2.370  | 4824446  | 44889780 | 14.837  | 151.954 # |
| 2) T                        | 3,5-DICHL... | 0.000  | 9.112  | 0        | 290294   | N.D.    | 0.920 #   |
| 6) T                        | MCPD         | 12.145 | 0.000  | 25897431 | 0        | 40.640  | N.D. #    |
| 15) T                       | Picloram     | 0.000  | 16.890 | 0        | 10629475 | N.D.    | 6.250 #   |
| 16) T                       | DCPA         | 0.000  | 16.890 | 0        | 10629475 | N.D.    | 5.763 #   |
| -----                       |              |        |        |          |          |         |           |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092418\  
Data File : PS001812.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 Sep 2018 21:42  
Operator : EI\SJ  
Sample : J4777-24  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 25 06:30:31 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS091718.M  
Quant Title : 8080.M  
QLast Update : Tue Sep 18 03:01:16 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

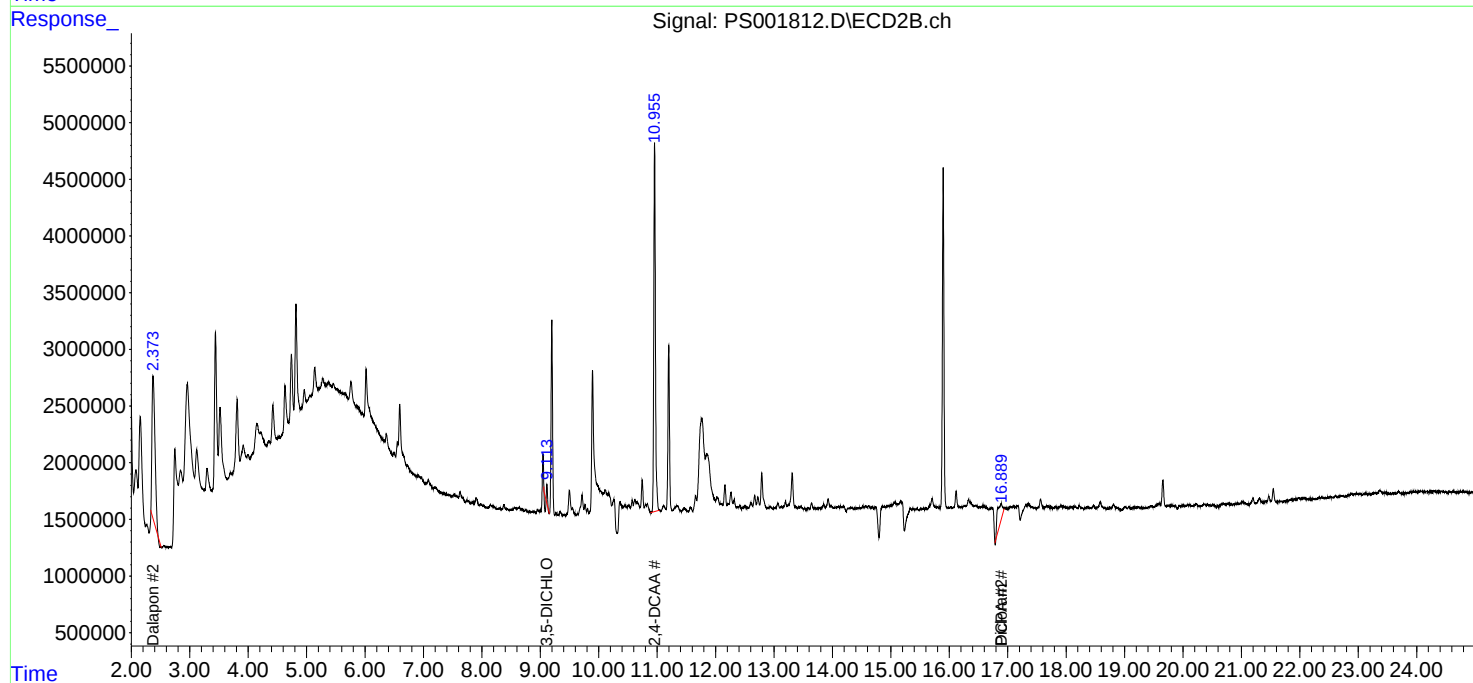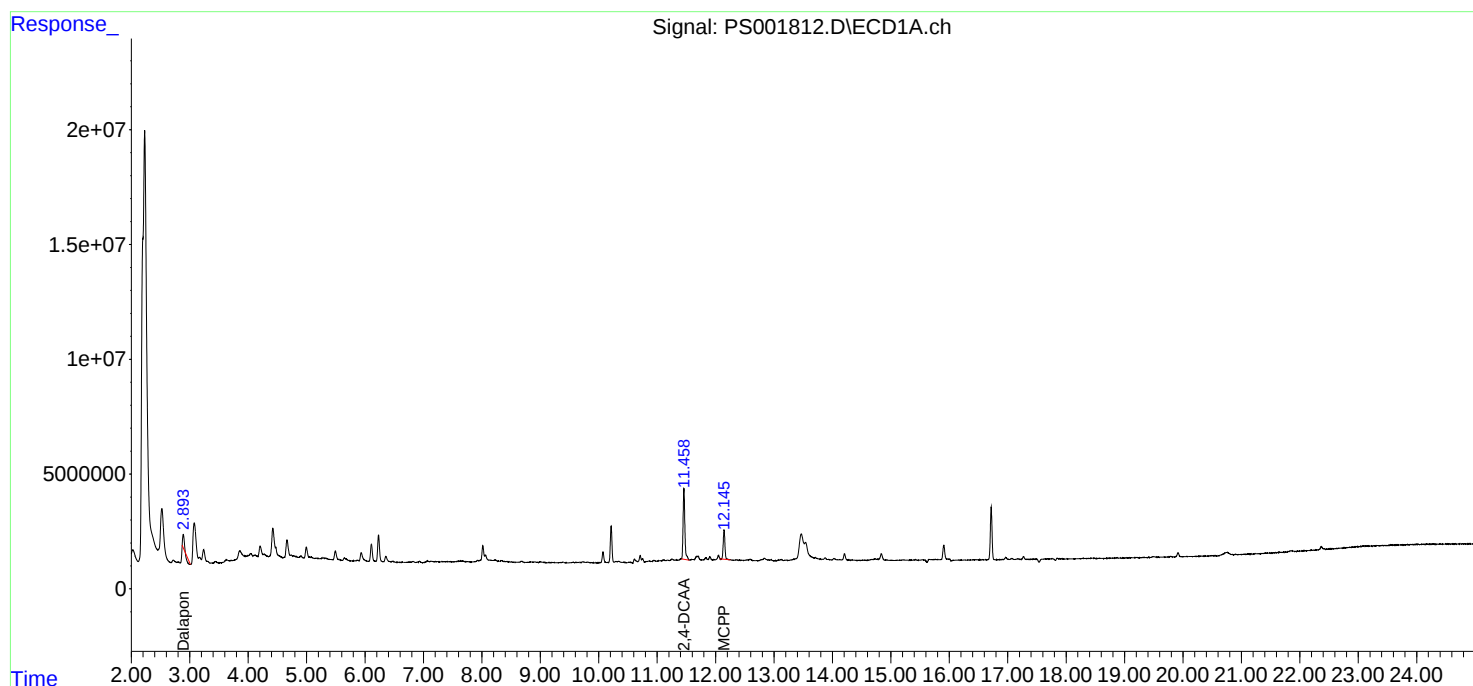


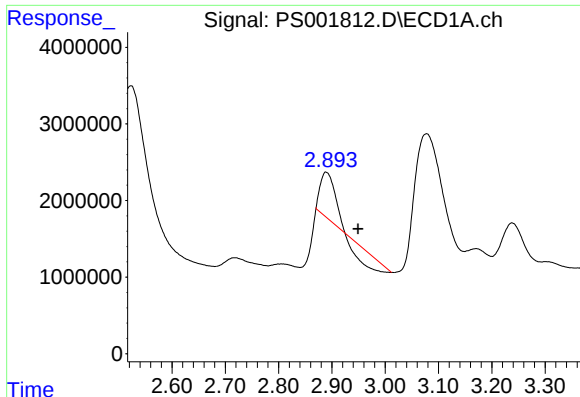

#1 Dalapon


R.T.: 2.889 min  
Delta R.T.: -0.060 min  
Response: 4824446  
Conc: 14.84 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

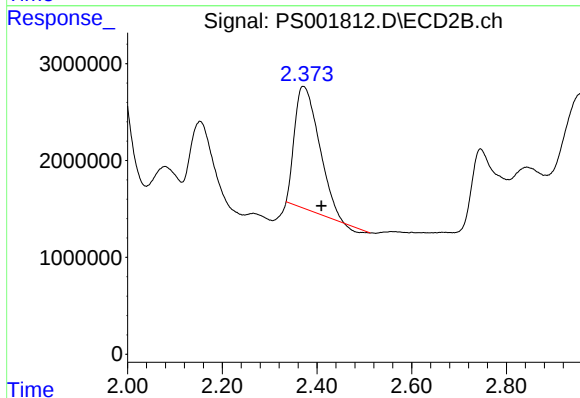


#1 Dalapon

R.T.: 2.370 min  
Delta R.T.: -0.039 min  
Response: 44889780  
Conc: 151.95 ng/ml

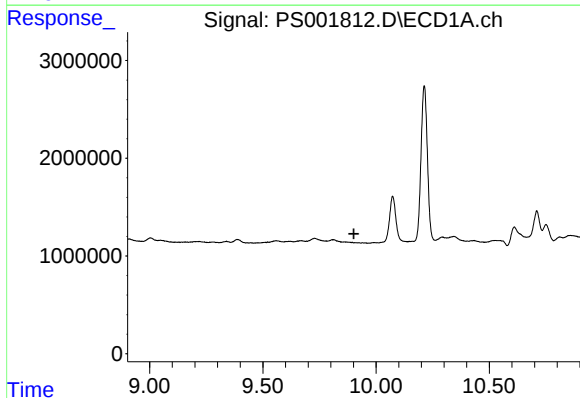


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T. : 9.902 min  
Response: 0  
Conc: N.D.

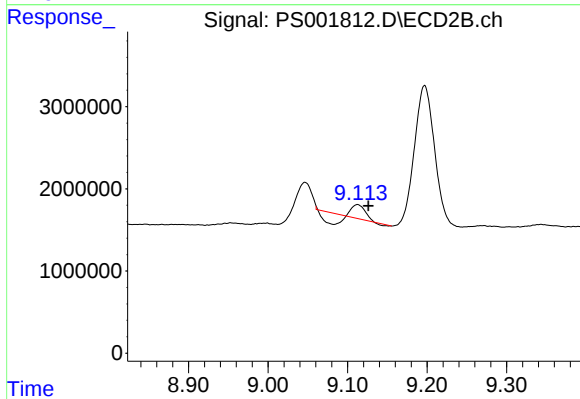

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.112 min  
Delta R.T.: -0.014 min  
Response: 290294  
Conc: 0.92 ng/ml

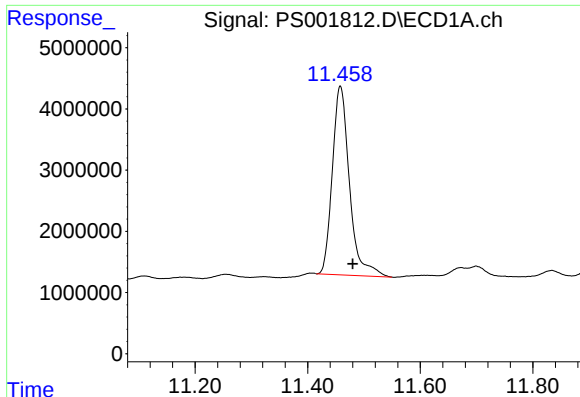

#4 2,4-DCAA


R.T.: 11.458 min  
Delta R.T.: -0.022 min  
Response: 65117891  
Conc: 290.30 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

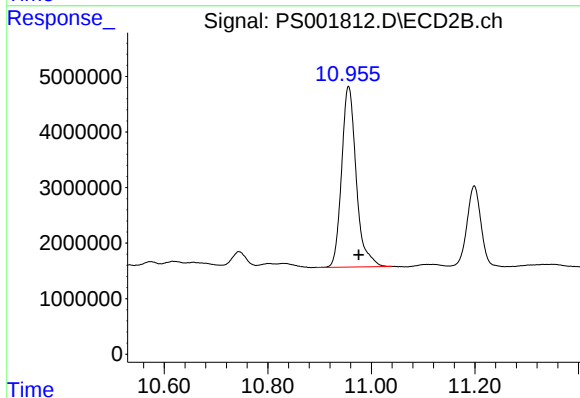


#4 2,4-DCAA

R.T.: 10.956 min  
Delta R.T.: -0.020 min  
Response: 63802785  
Conc: 251.18 ng/ml

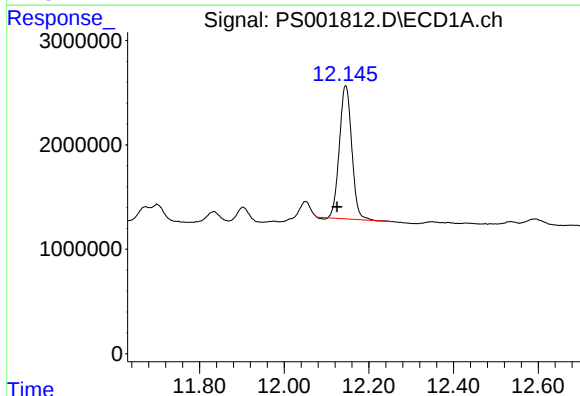


#6 MCP

R.T.: 12.145 min  
Delta R.T.: 0.020 min  
Response: 25897431  
Conc: 40.64 ug/ml

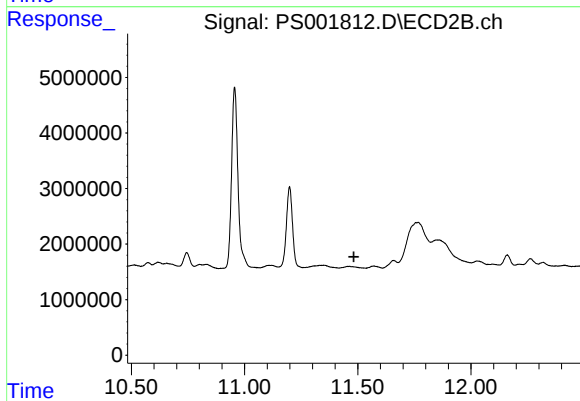

#6 MCP


R.T.: 0.000 min  
Exp R.T.: 11.483 min  
Response: 0  
Conc: N.D.

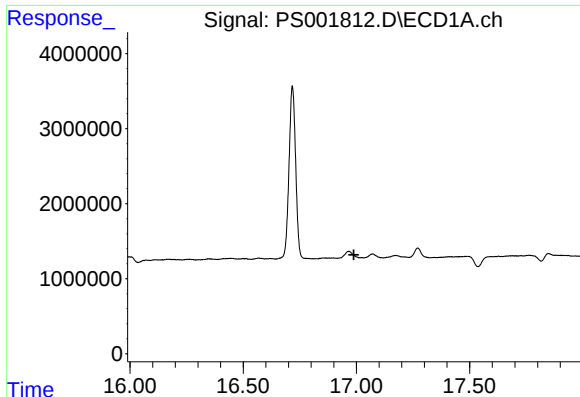

#15 Picloram


R.T.: 0.000 min  
Exp R.T. : 16.988 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

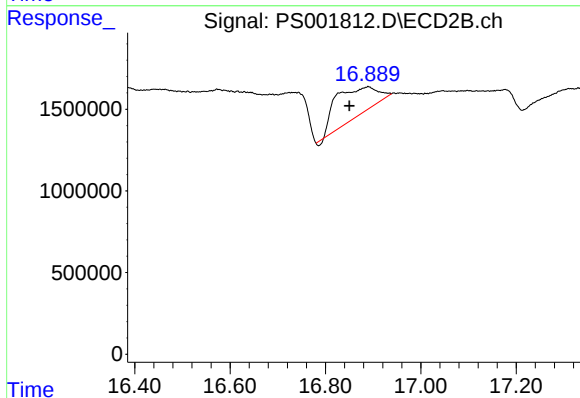


#15 Picloram

R.T.: 16.890 min  
Delta R.T.: 0.040 min  
Response: 10629475  
Conc: 6.25 ng/ml

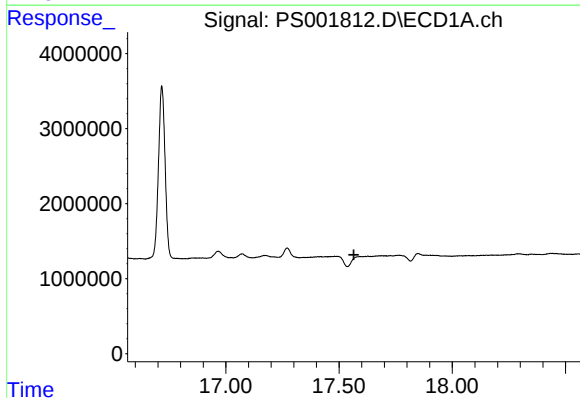

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 17.565 min  
Response: 0  
Conc: N.D.

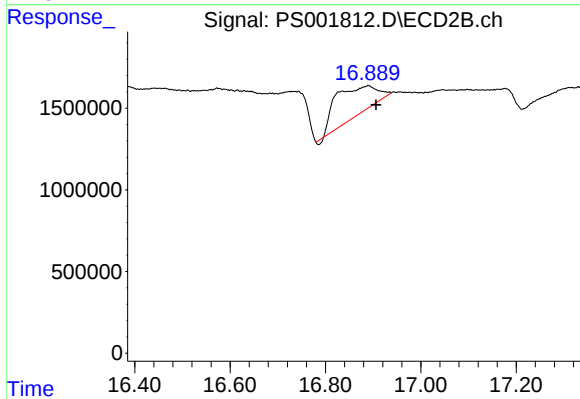

#16 DCPA

R.T.: 16.890 min  
Delta R.T.: -0.016 min  
Response: 10629475  
Conc: 5.76 ng/ml