

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
 Data File : PS001813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2018 22:13
 Operator : EI\SJ
 Sample : J4777-26
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 06:30:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.475	10.972	97254277	96418390	433.560	379.575
Target Compounds							
1) T	Dalapon	2.907	2.389	39900416	60055448	122.707	203.290 #
5) T	DICAMBA	11.849	11.216	1067785	23578477	1.232	26.437 #
6) T	MCPD	12.163	0.000	24345480	0	38.205	N.D. #
9) T	2,4-D	0.000	12.807	0	2494115	N.D.	8.017 #
15) T	Picloram	0.000	16.907	0	2767167	N.D.	1.627 #
16) T	DCPA	0.000	16.907	0	2767167	N.D.	1.500 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
Data File : PS001813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2018 22:13
Operator : EI\SJ
Sample : J4777-26
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 06:30:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

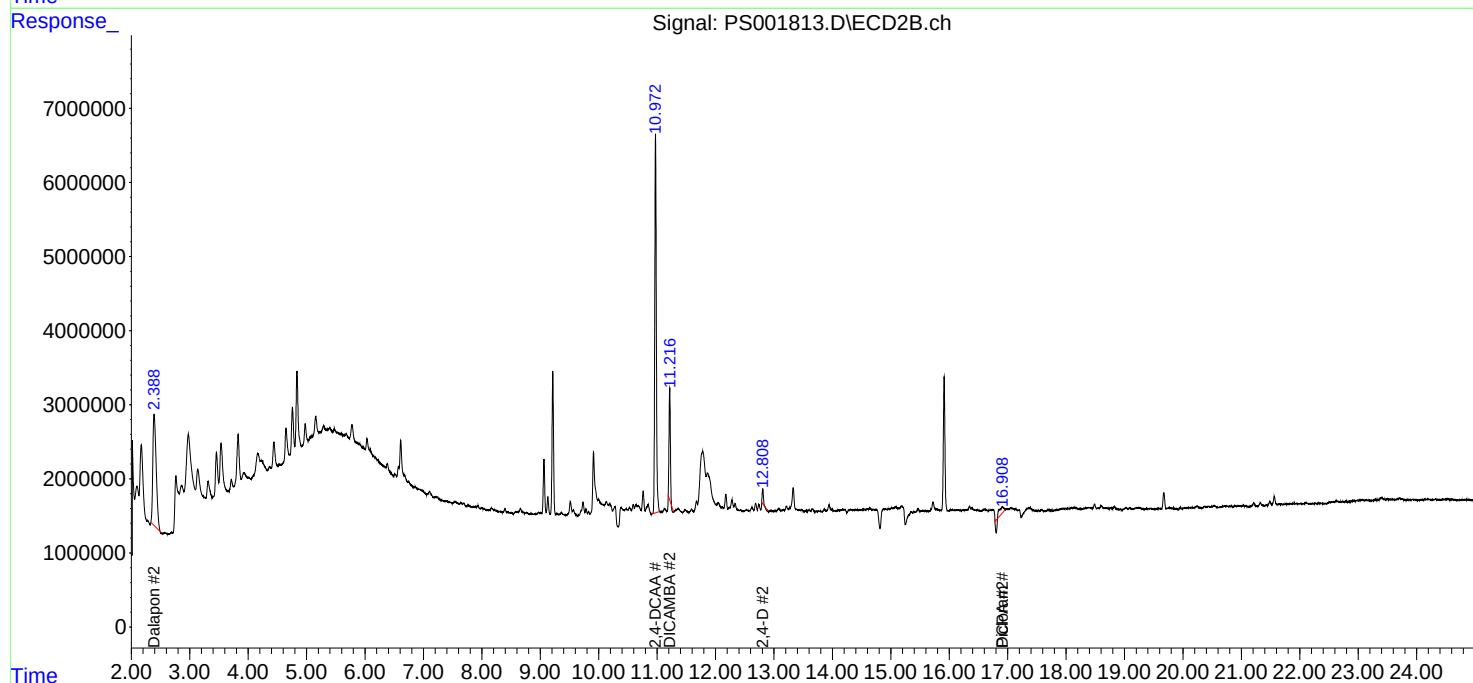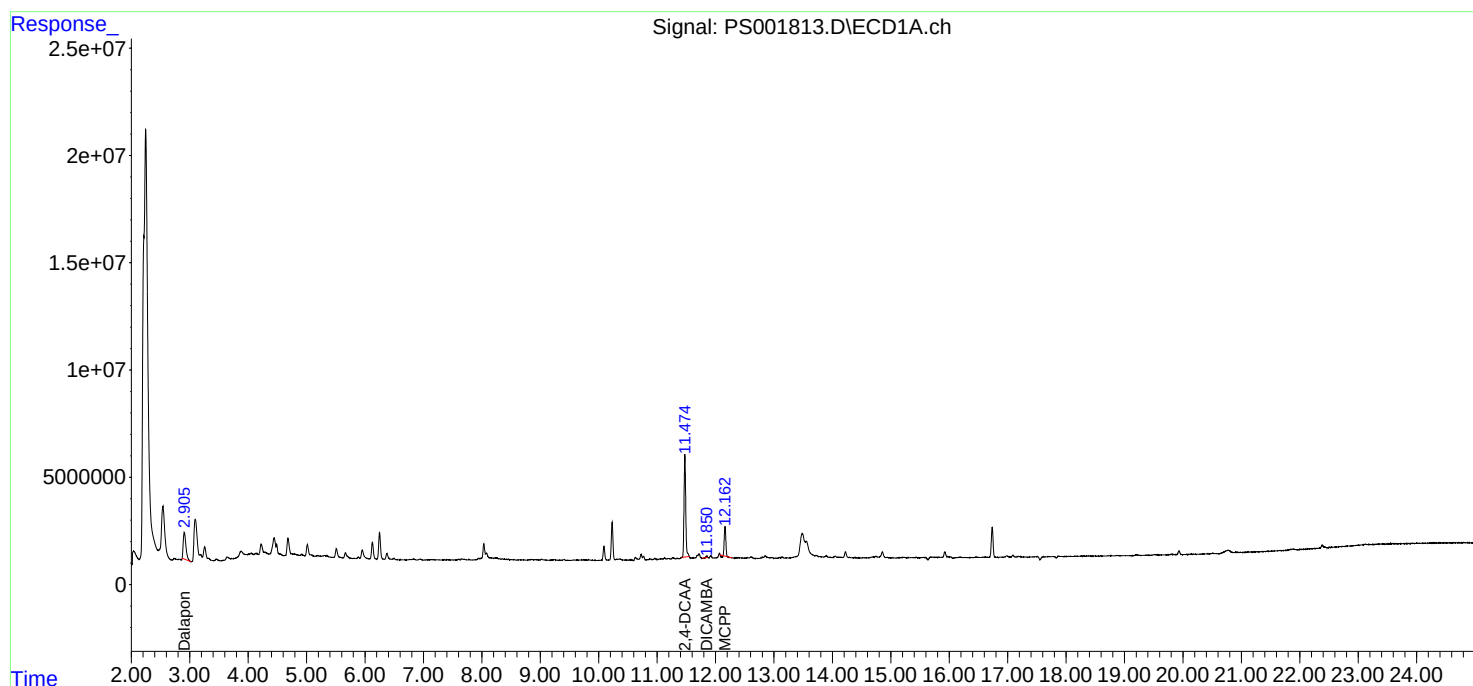


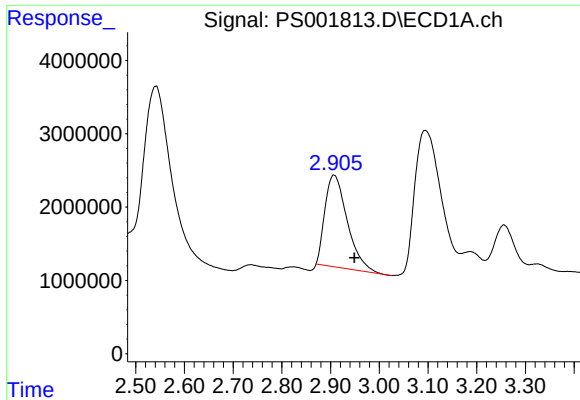

#1 Dalapon


R.T.: 2.907 min
Delta R.T.: -0.042 min
Response: 39900416
Conc: 122.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

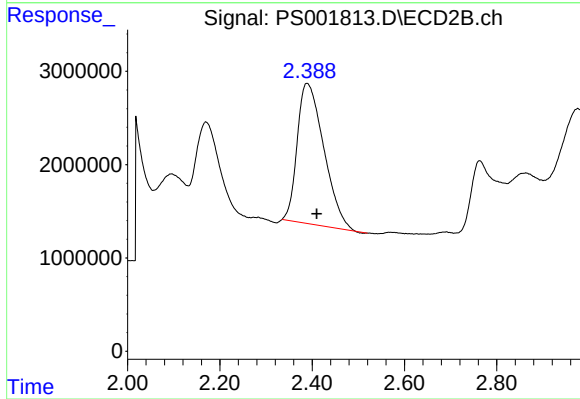


#1 Dalapon

R.T.: 2.389 min
Delta R.T.: -0.021 min
Response: 60055448
Conc: 203.29 ng/ml

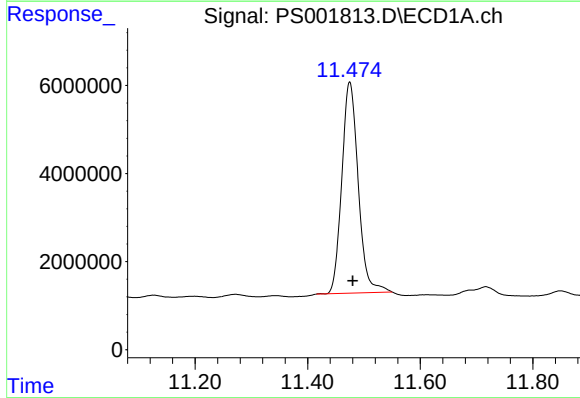


#4 2,4-DCAA

R.T.: 11.475 min
Delta R.T.: -0.005 min
Response: 97254277
Conc: 433.56 ng/ml

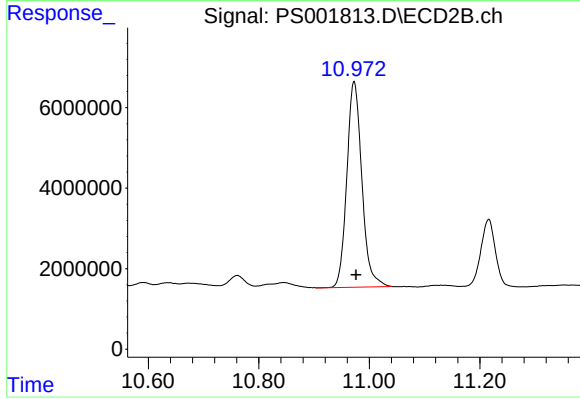

#4 2,4-DCAA


R.T.: 10.972 min
Delta R.T.: -0.004 min
Response: 96418390
Conc: 379.58 ng/ml

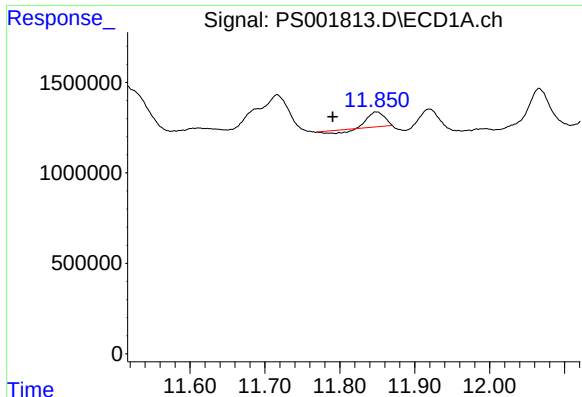

#5 DICAMBA


R.T.: 11.849 min
Delta R.T.: 0.059 min
Response: 1067785
Conc: 1.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

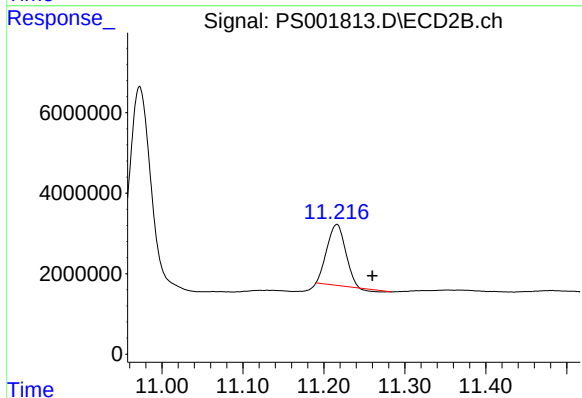


#5 DICAMBA

R.T.: 11.216 min
Delta R.T.: -0.044 min
Response: 23578477
Conc: 26.44 ng/ml

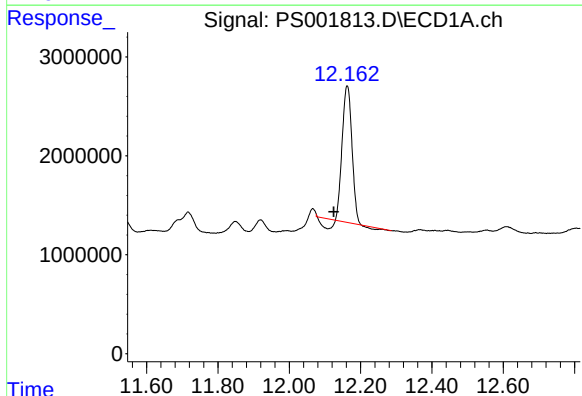


#6 MCP

R.T.: 12.163 min
Delta R.T.: 0.038 min
Response: 24345480
Conc: 38.20 ug/ml

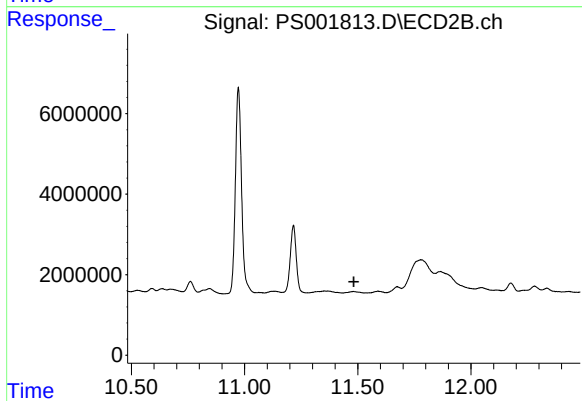

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.483 min
Response: 0
Conc: N.D.

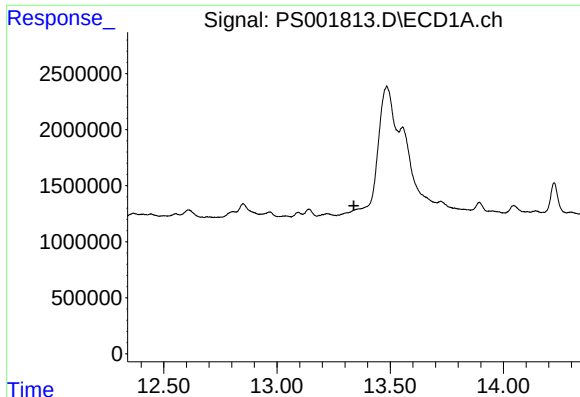

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

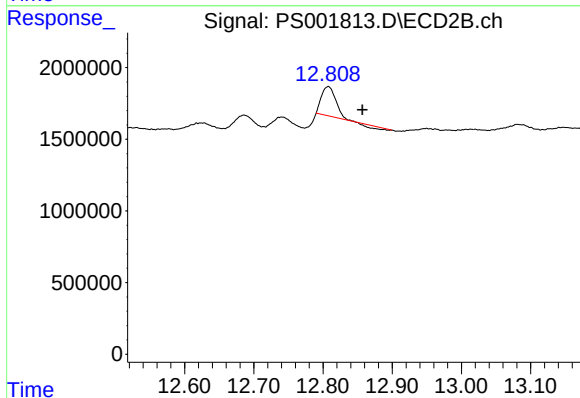


#9 2,4-D

R.T.: 12.807 min
Delta R.T.: -0.050 min
Response: 2494115
Conc: 8.02 ng/ml

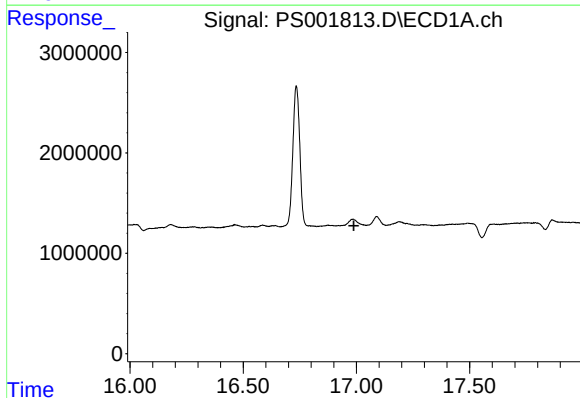


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.988 min
Response: 0
Conc: N.D.

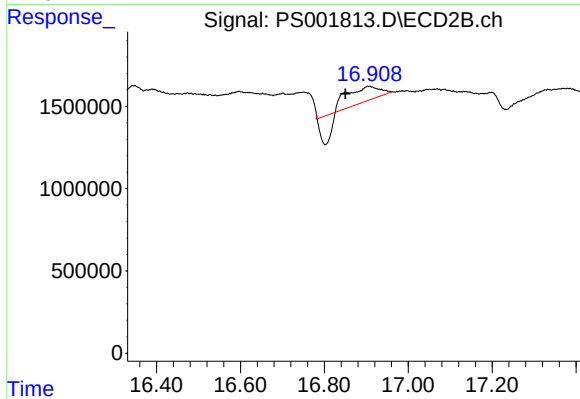

#15 Picloram


R.T.: 16.907 min
Delta R.T.: 0.056 min
Response: 2767167
Conc: 1.63 ng/ml

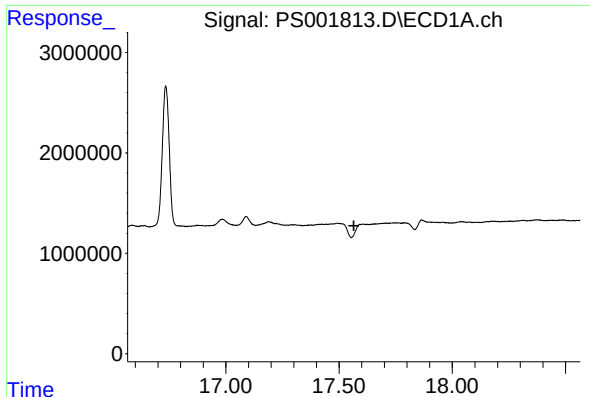

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

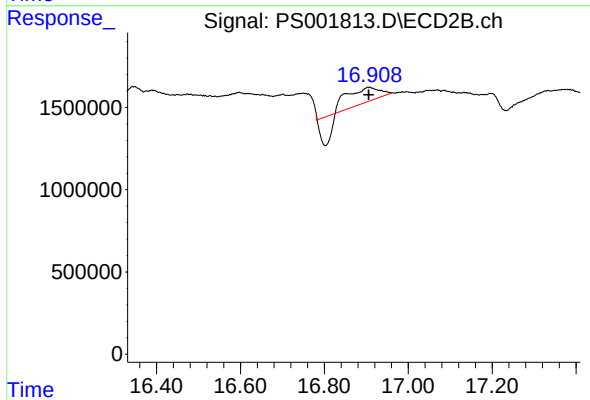

#16 DCPA

R.T.: 16.907 min
Delta R.T.: 0.000 min
Response: 2767167
Conc: 1.50 ng/ml