

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
 Data File : PS001814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2018 22:44
 Operator : EI\SJ
 Sample : J4777-28
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 06:31:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.471	10.954	109.9E6	108.1E6	489.738	425.570
Target Compounds							
1) T	Dalapon	2.904	2.369	43968858	69320850	135.219	234.654 #
2) T	3,5-DICHL...	0.000	9.112	0	108250	N.D.	0.343 #
5) T	DICAMBA	11.845	0.000	1607457	0	1.855	N.D. #
6) T	MCP	12.159	0.000	27050619	0	42.450	N.D. #
15) T	Picloram	0.000	16.887	0	11755048	N.D.	6.912 #
16) T	DCPA	0.000	16.887	0	11755048	N.D.	6.373 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
Data File : PS001814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2018 22:44
Operator : EI\SJ
Sample : J4777-28
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 06:31:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

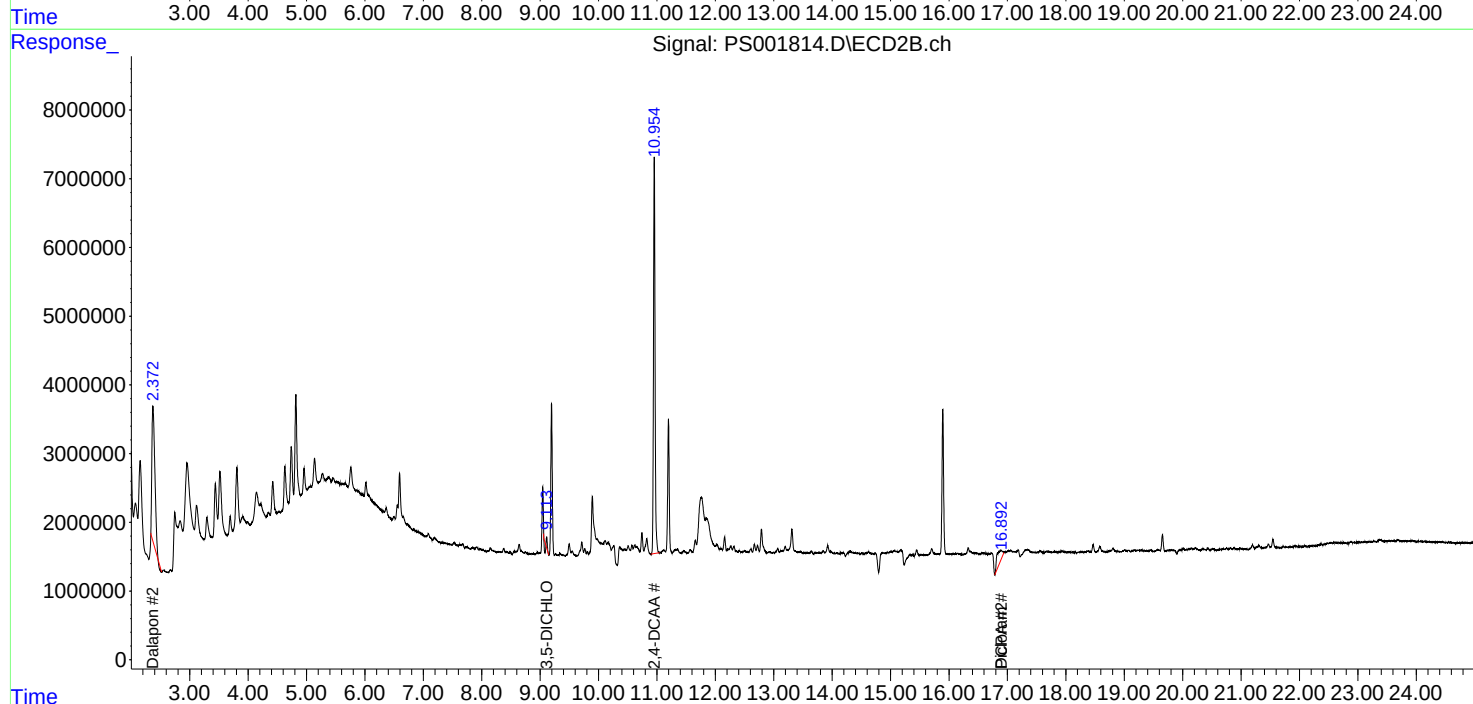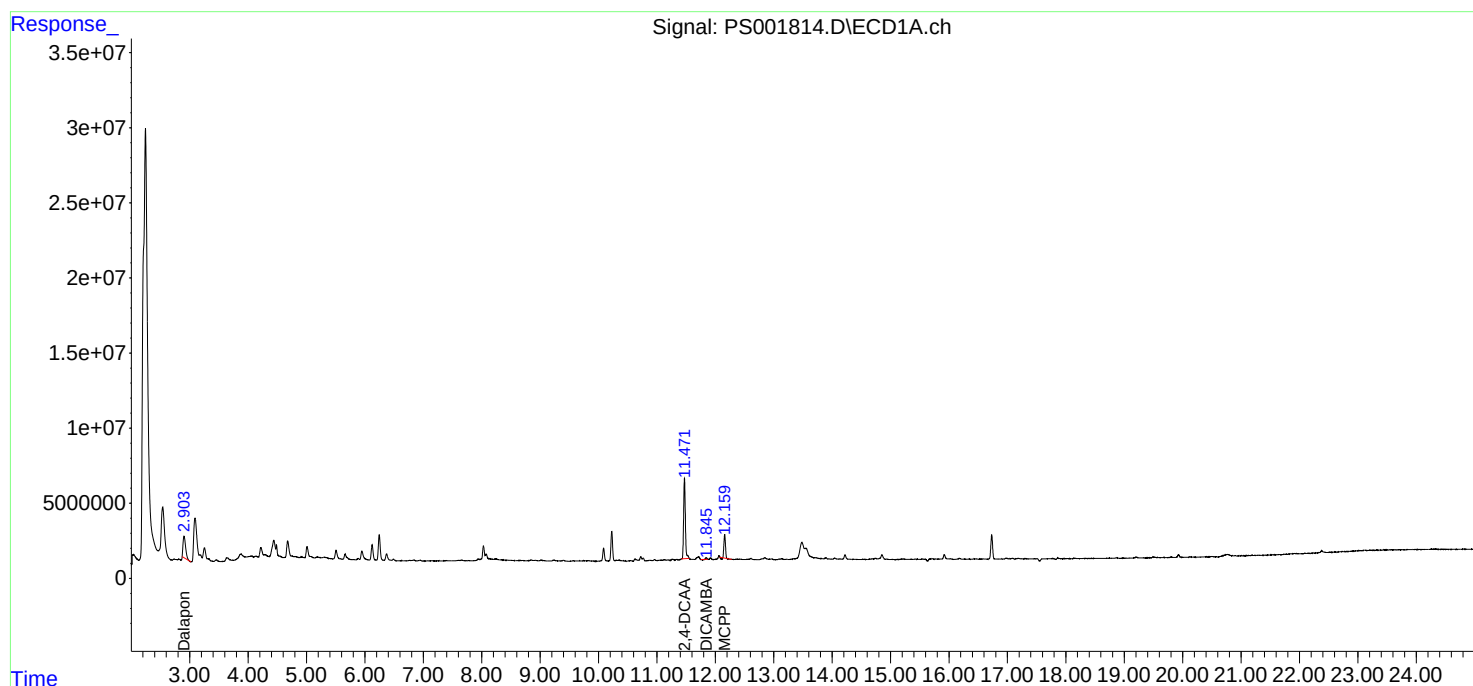


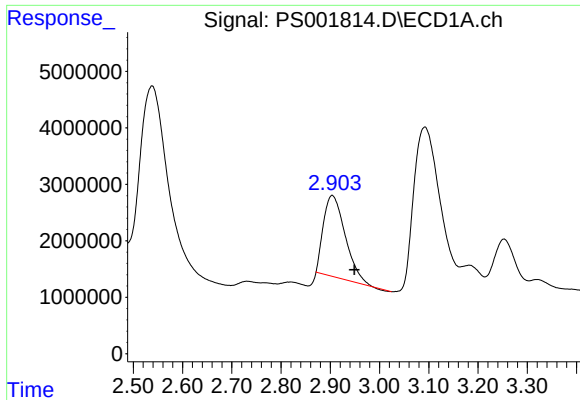

#1 Dalapon


R.T.: 2.904 min
Delta R.T.: -0.045 min
Response: 43968858
Conc: 135.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

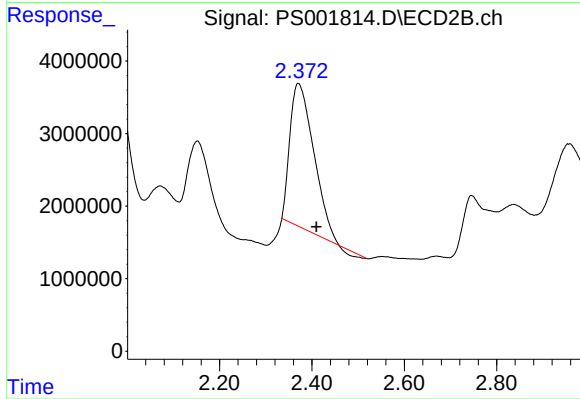


#1 Dalapon

R.T.: 2.369 min
Delta R.T.: -0.040 min
Response: 69320850
Conc: 234.65 ng/ml

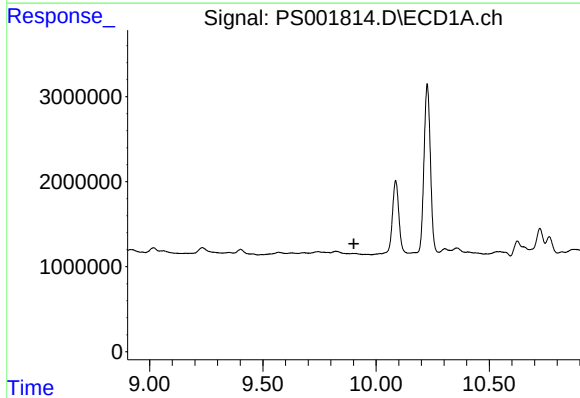


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.902 min
Response: 0
Conc: N.D.

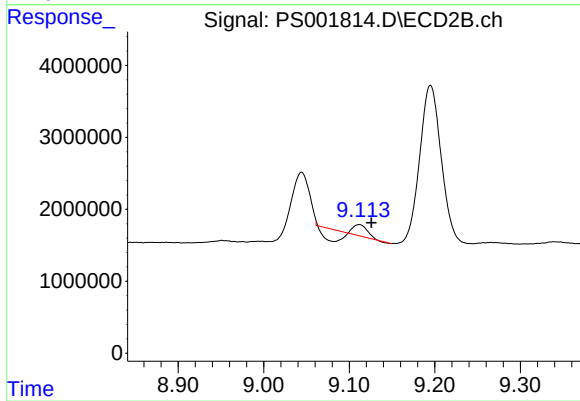

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.112 min
Delta R.T.: -0.014 min
Response: 108250
Conc: 0.34 ng/ml

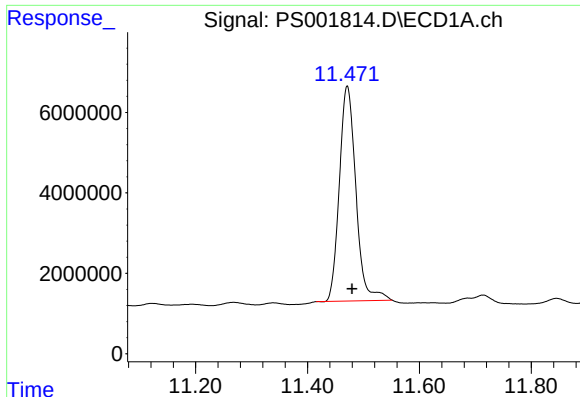

#4 2,4-DCAA


R.T.: 11.471 min
Delta R.T.: -0.009 min
Response: 109855916
Conc: 489.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

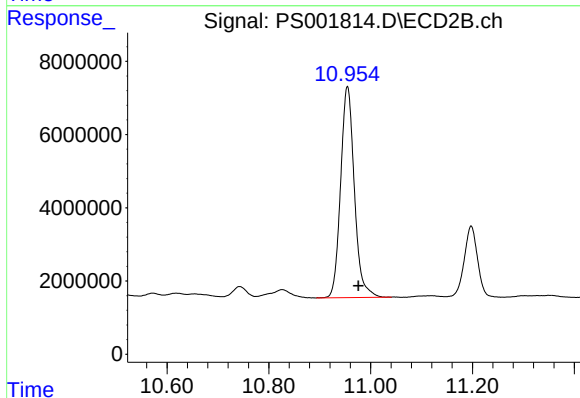


#4 2,4-DCAA

R.T.: 10.954 min
Delta R.T.: -0.022 min
Response: 108101837
Conc: 425.57 ng/ml

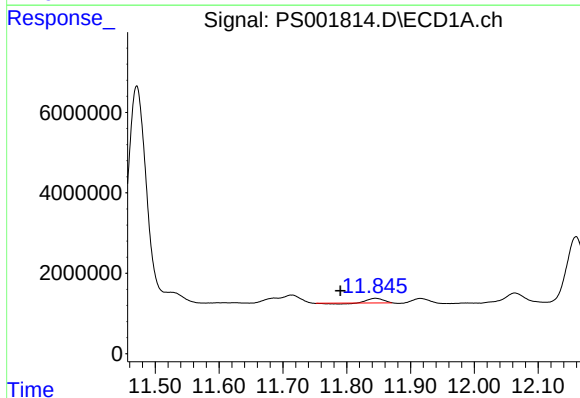


#5 DICAMBA

R.T.: 11.845 min
Delta R.T.: 0.055 min
Response: 1607457
Conc: 1.85 ng/ml

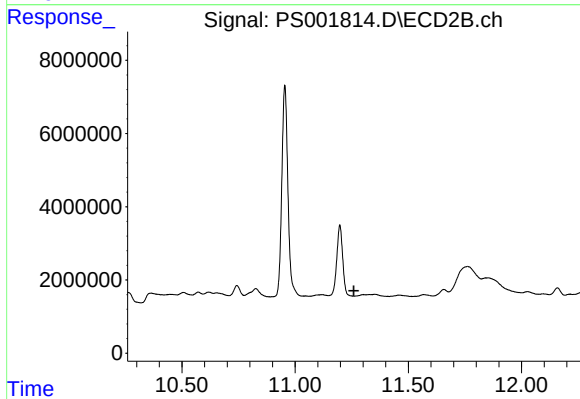

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.260 min
Response: 0
Conc: N.D.

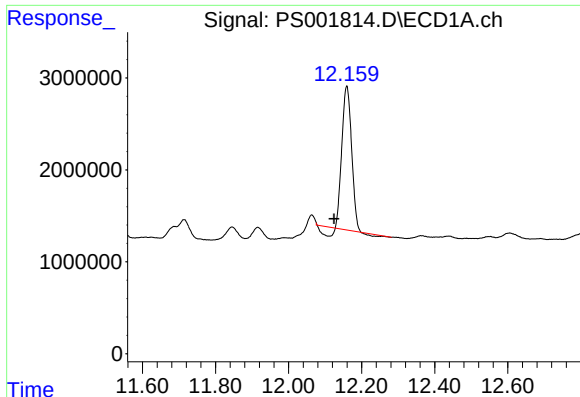

#6 MCP


R.T.: 12.159 min
Delta R.T.: 0.034 min
Response: 27050619
Conc: 42.45 ug/ml

Instrument :
ECD_S
ClientSampleId :

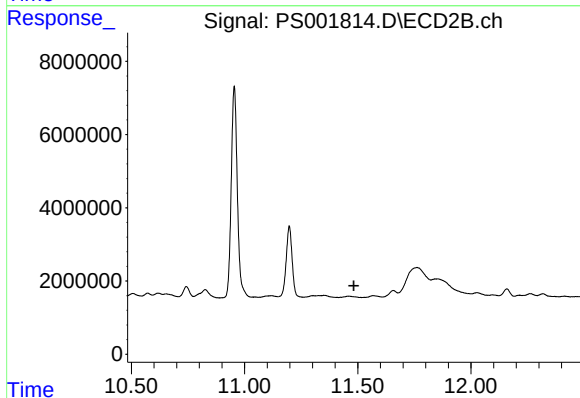


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

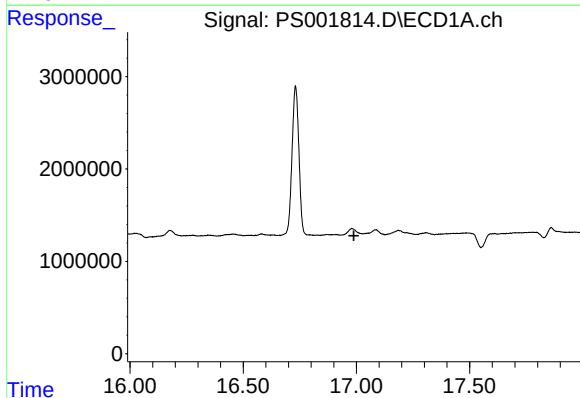


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.988 min
Response: 0
Conc: N.D.

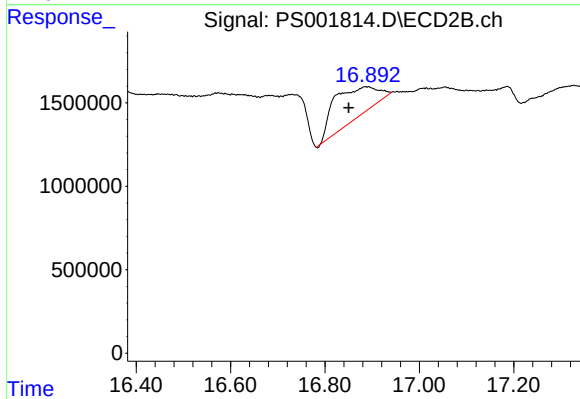

#15 Picloram

R.T.: 16.887 min
Delta R.T.: 0.037 min
Response: 11755048
Conc: 6.91 ng/ml

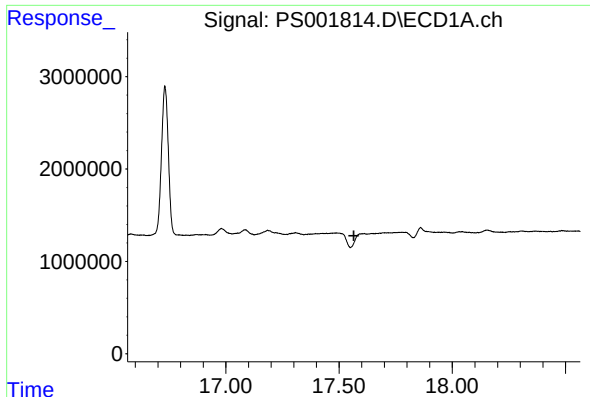

#16 DCPA

R.T.: 0.000 min

Exp R.T.: 17.565 min

Response: 0

Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

#16 DCPA

R.T.: 16.887 min

Delta R.T.: -0.019 min

Response: 11755048

Conc: 6.37 ng/ml