

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
 Data File : PS001819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2018 01:20
 Operator : EI\SJ
 Sample : J5021-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 06:32:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.490	10.988	89298229	88971712	398.092	350.259
Target Compounds							
1) T	Dalapon	2.920	2.401	27686070	24670431	85.144	83.511
2) T	3,5-DICHL...	0.000	9.078	0	5690827	N.D.	18.030 #
5) T	DICAMBA	0.000	11.230	0	27880690	N.D.	31.261 #
6) T	MCP	12.177	0.000	24372854	0	38.248	N.D. #
7) T	MCPA	0.000	11.801	0	7580634	N.D.	8.745 #
9) T	2,4-D	0.000	12.823	0	2807283	N.D.	9.024 #
10) T	Pentachlo...	13.759	0.000	11185061	0	3.639	N.D. #
15) T	Picloram	17.004	16.918	10359663	6780186	5.950	3.987 #
16) T	DCPA	0.000	16.918	0	6780186	N.D.	3.676 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
Data File : PS001819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2018 01:20
Operator : EI\SJ
Sample : J5021-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 06:32:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

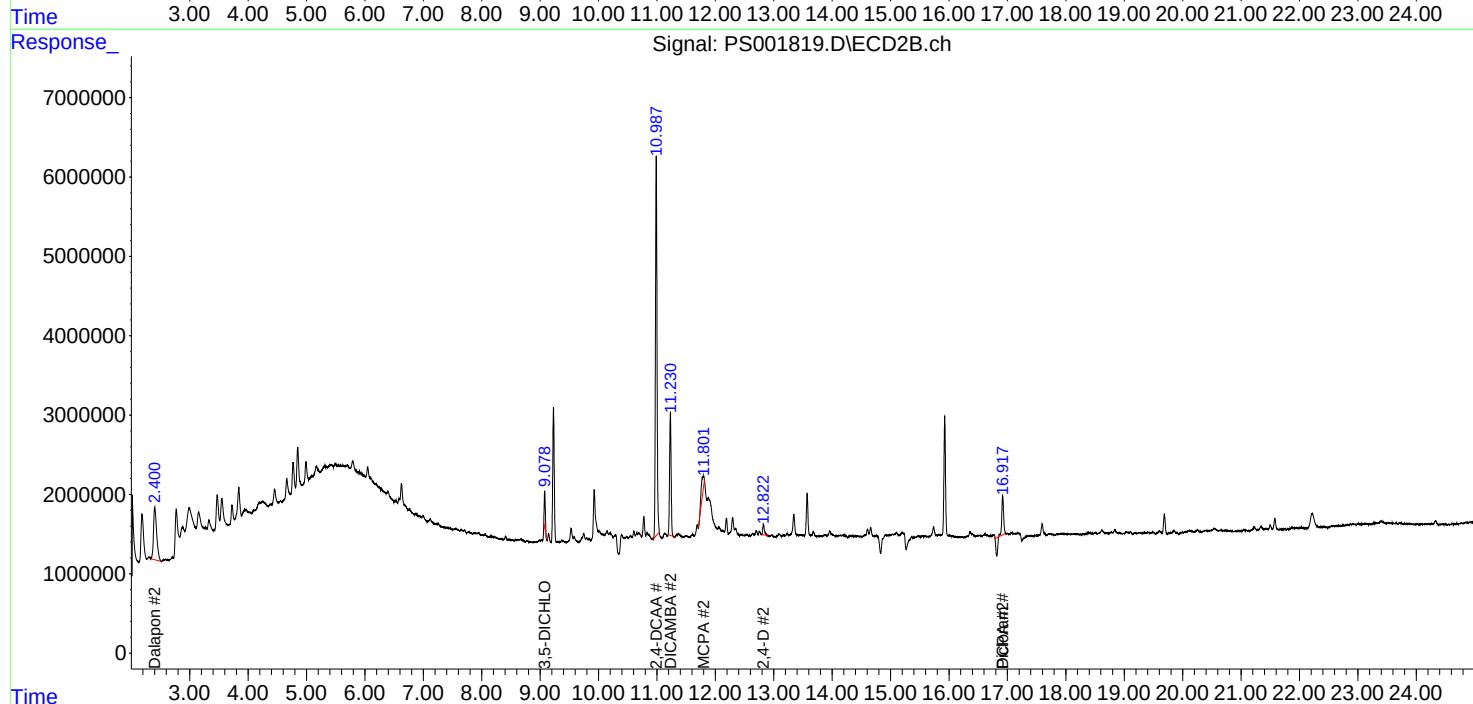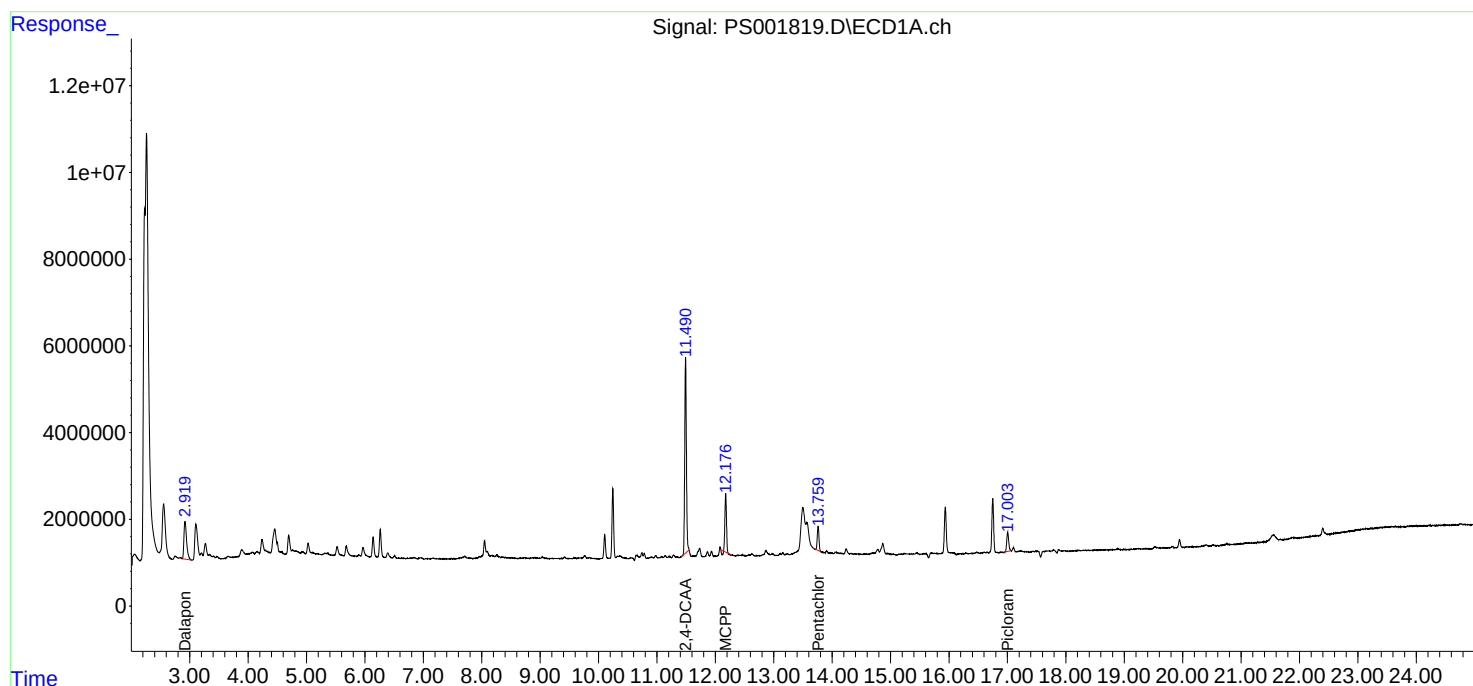


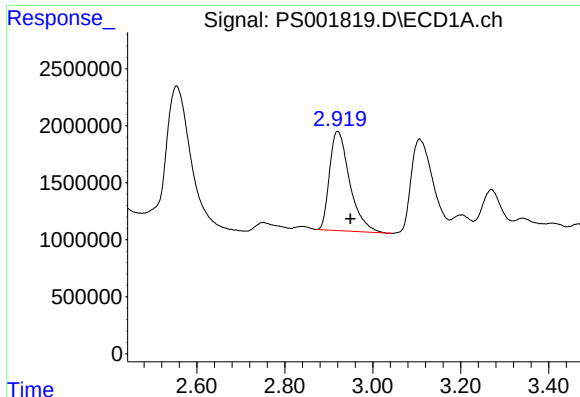

#1 Dalapon


R.T.: 2.920 min
Delta R.T.: -0.029 min
Response: 27686070
Conc: 85.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

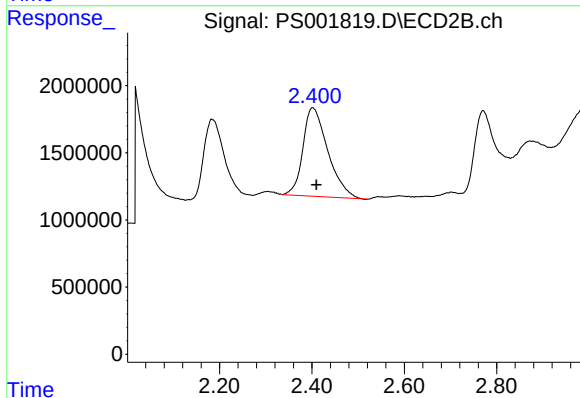


#1 Dalapon

R.T.: 2.401 min
Delta R.T.: -0.008 min
Response: 24670431
Conc: 83.51 ng/ml

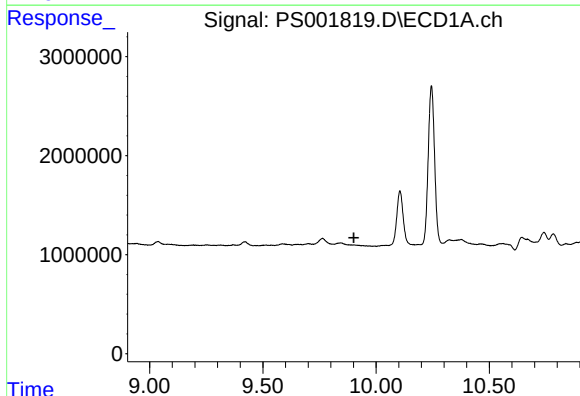


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.902 min
Response: 0
Conc: N.D.

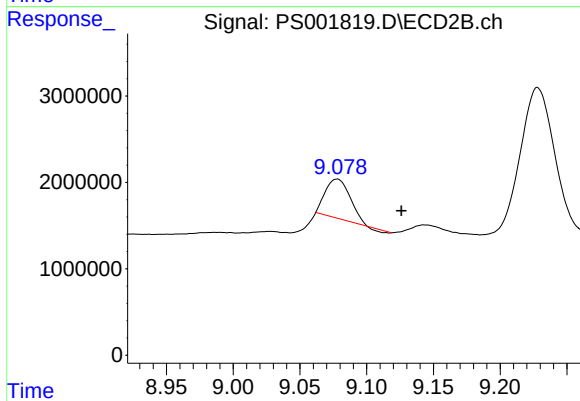

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.078 min
Delta R.T.: -0.048 min
Response: 5690827
Conc: 18.03 ng/ml

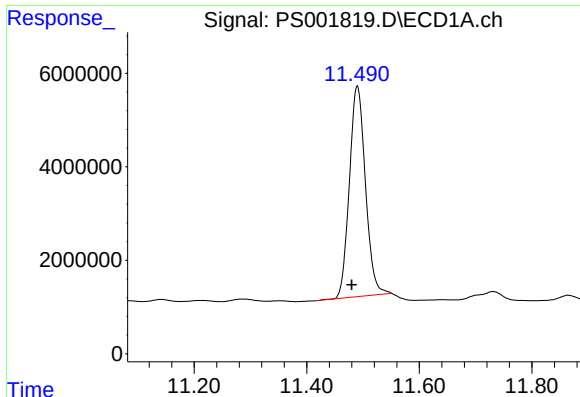

#4 2,4-DCAA


R.T.: 11.490 min
Delta R.T.: 0.010 min
Response: 89298229
Conc: 398.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

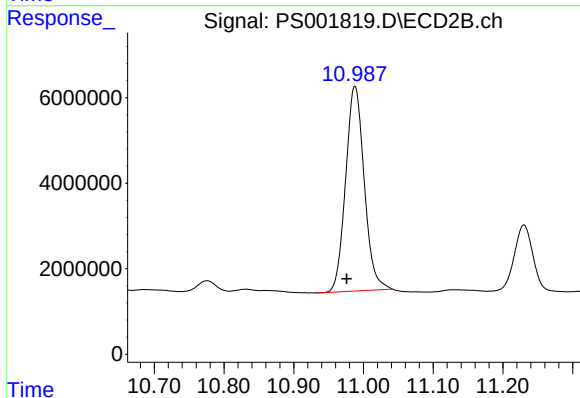


#4 2,4-DCAA

R.T.: 10.988 min
Delta R.T.: 0.012 min
Response: 88971712
Conc: 350.26 ng/ml

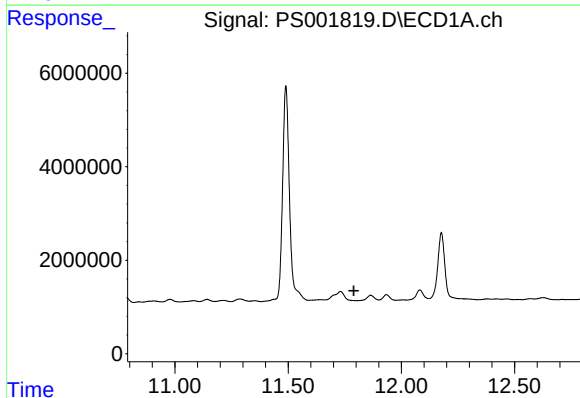


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.790 min
Response: 0
Conc: N.D.

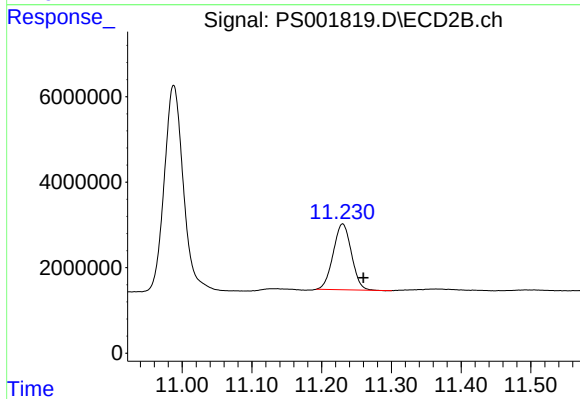

#5 DICAMBA


R.T.: 11.230 min
Delta R.T.: -0.030 min
Response: 27880690
Conc: 31.26 ng/ml

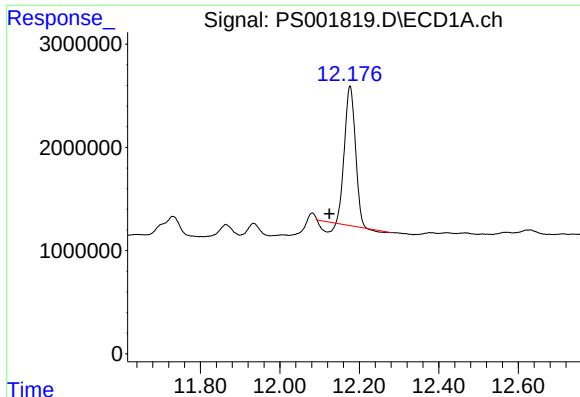

#6 MCPP


R.T.: 12.177 min
Delta R.T.: 0.052 min
Response: 24372854
Conc: 38.25 ug/ml

Instrument :
ECD_S
ClientSampleId :

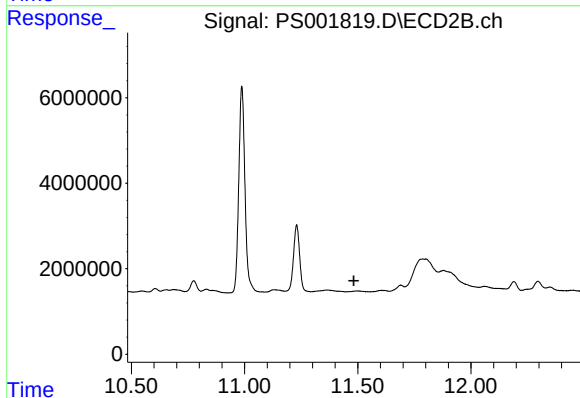


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

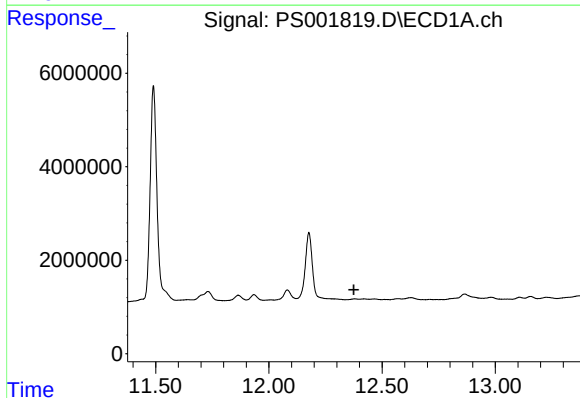


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.375 min
Response: 0
Conc: N.D.

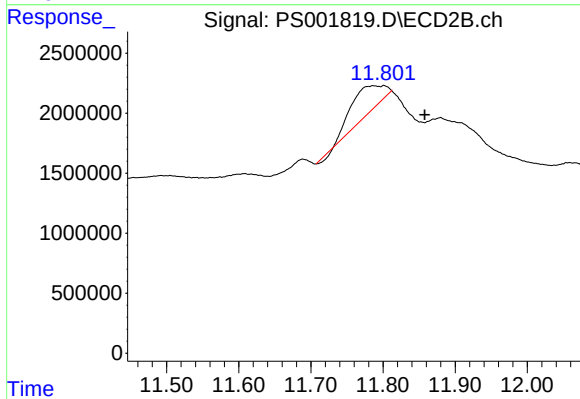

#7 MCPA


R.T.: 11.801 min
Delta R.T.: -0.057 min
Response: 7580634
Conc: 8.75 ug/ml

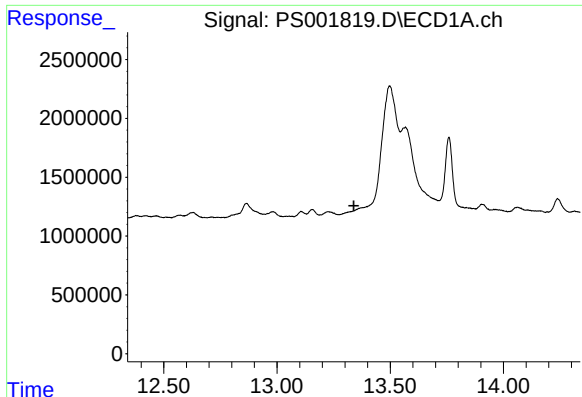

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

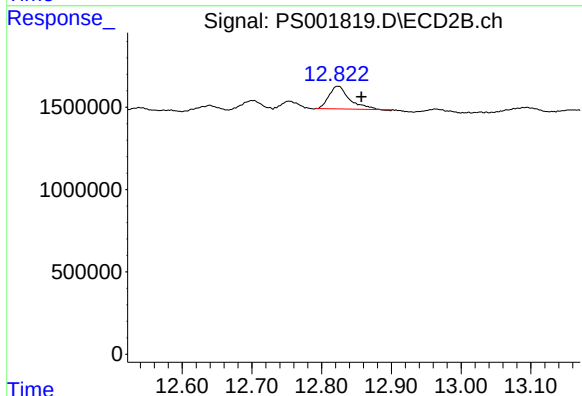


#9 2,4-D

R.T.: 12.823 min
Delta R.T.: -0.034 min
Response: 2807283
Conc: 9.02 ng/ml

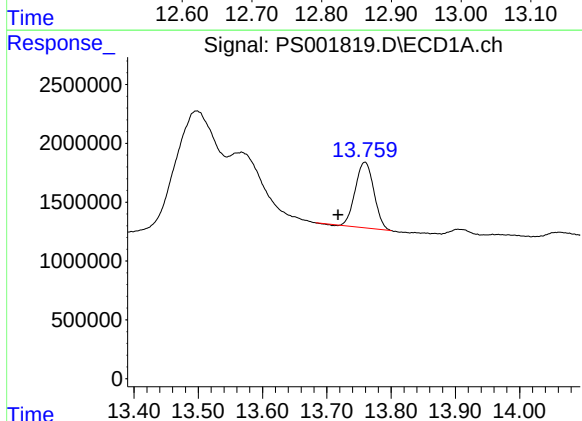


#10 Pentachlorophenol

R.T.: 13.759 min
Delta R.T.: 0.041 min
Response: 11185061
Conc: 3.64 ng/ml

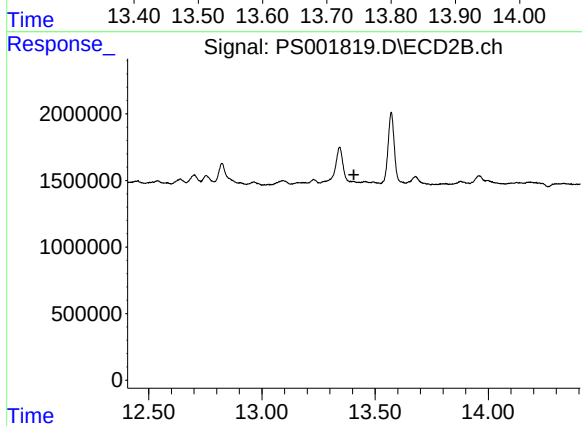

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.407 min
Response: 0
Conc: N.D.

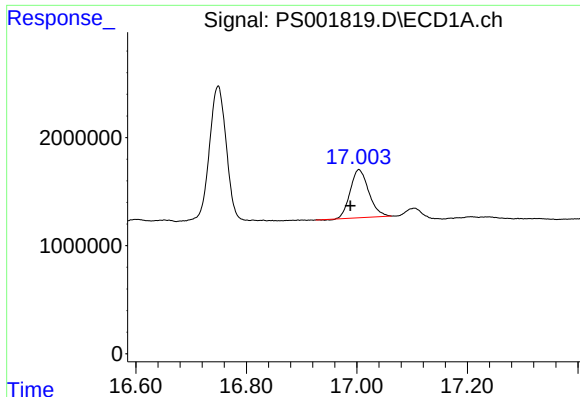

#15 Picloram


R.T.: 17.004 min
Delta R.T.: 0.015 min
Response: 10359663
Conc: 5.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

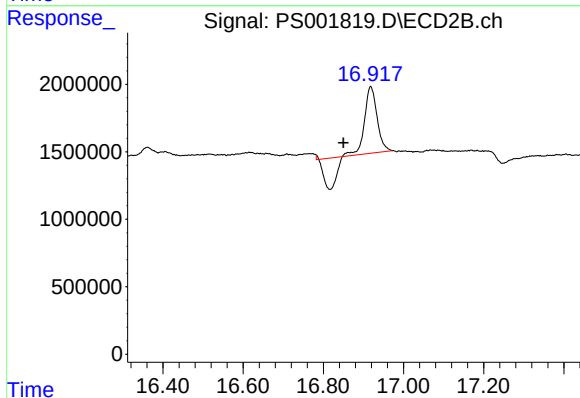


#15 Picloram

R.T.: 16.918 min
Delta R.T.: 0.068 min
Response: 6780186
Conc: 3.99 ng/ml

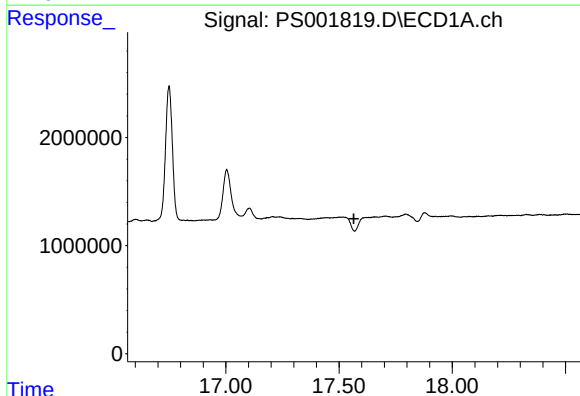

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.565 min
Response: 0
Conc: N.D.

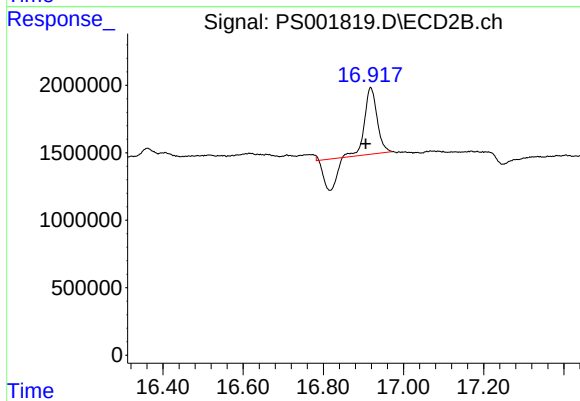

#16 DCPA

R.T.: 16.918 min
Delta R.T.: 0.012 min
Response: 6780186
Conc: 3.68 ng/ml