

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
 Data File : PS001820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2018 01:51
 Operator : EI\SJ
 Sample : J5021-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 06:32:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.471	10.968	61511799	60194298	274.220	236.970
Target Compounds							
1) T	Dalapon	2.902	2.384	26087846	38947088	80.229	131.838 #
5) T	DICAMBA	0.000	11.211	0	13521582	N.D.	15.161 #
6) T	MCPD	12.157	0.000	20782740	0	32.614	N.D. #
15) T	Picloram	16.983	16.900	3469248	4135941	1.992	2.432
16) T	DCPA	0.000	16.900	0	4135941	N.D.	2.242 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
Data File : PS001820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2018 01:51
Operator : EI\SJ
Sample : J5021-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 06:32:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

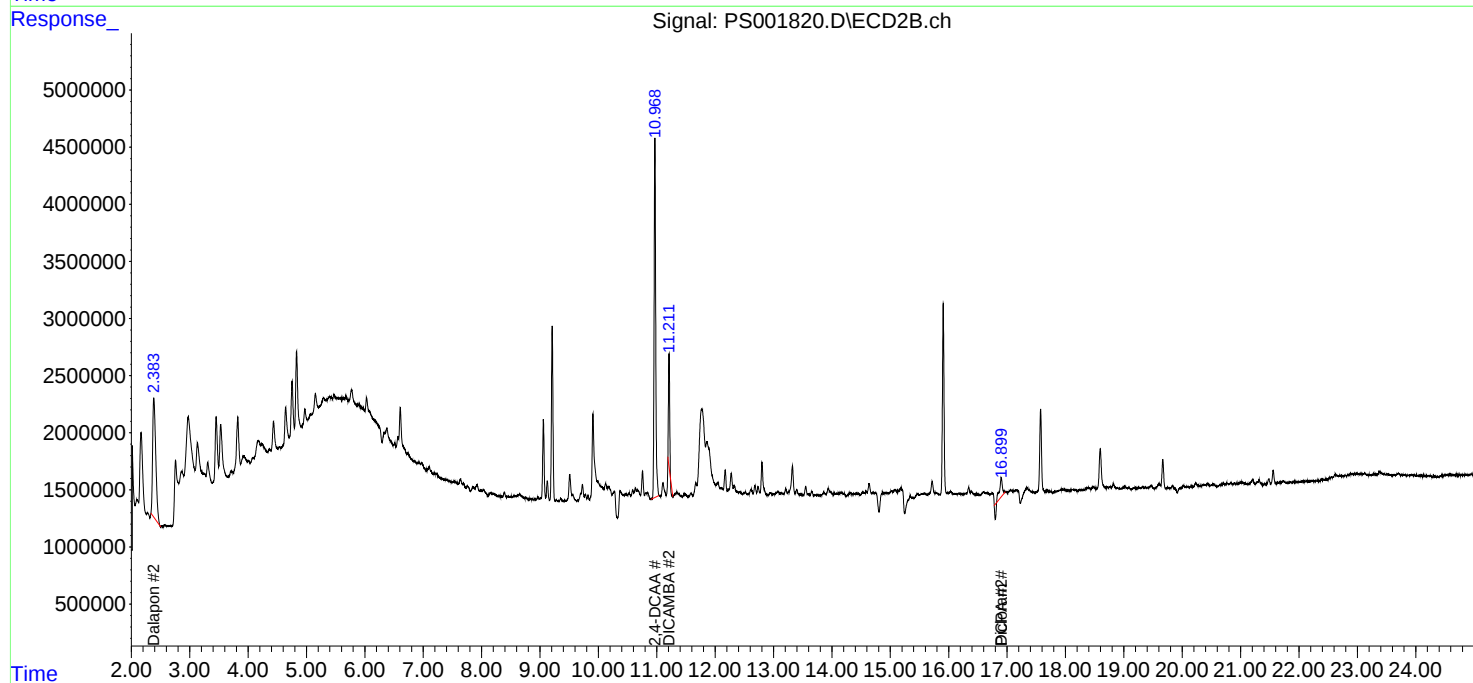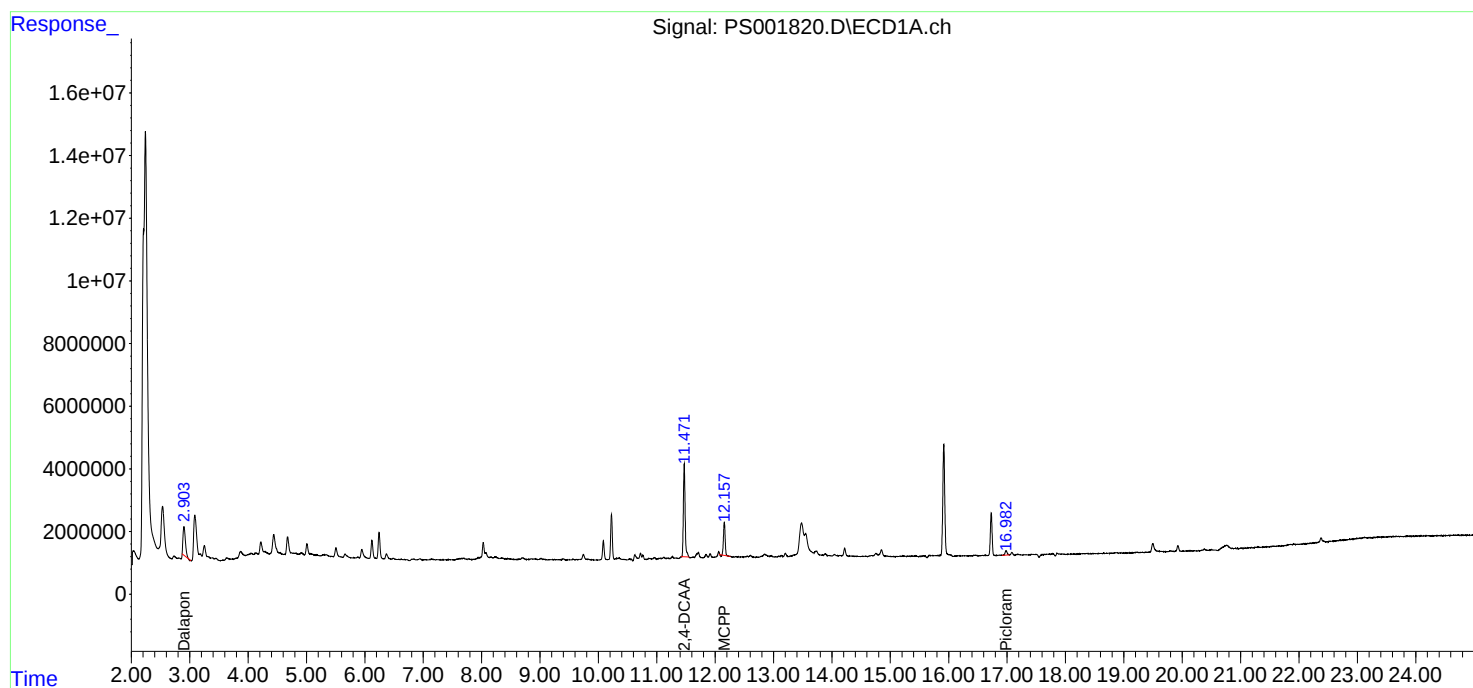


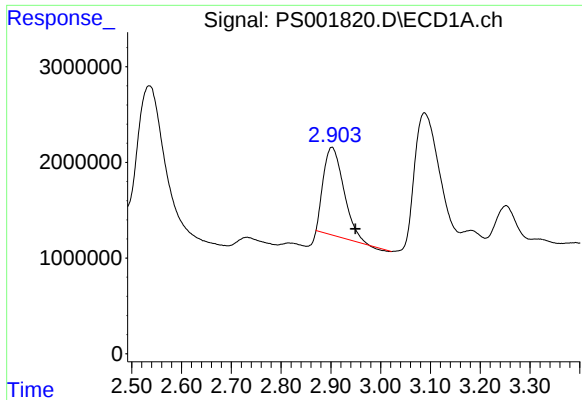

#1 Dalapon


R.T.: 2.902 min
Delta R.T.: -0.047 min
Response: 26087846
Conc: 80.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

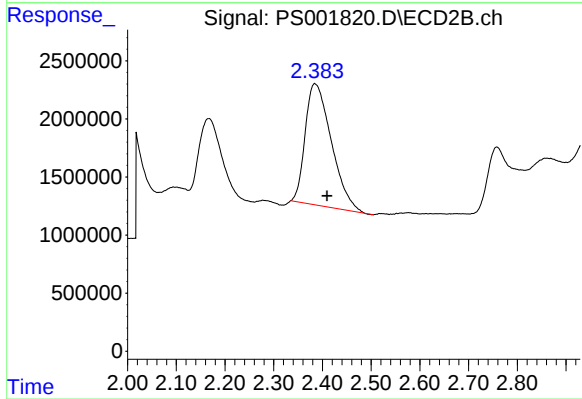


#1 Dalapon

R.T.: 2.384 min
Delta R.T.: -0.026 min
Response: 38947088
Conc: 131.84 ng/ml

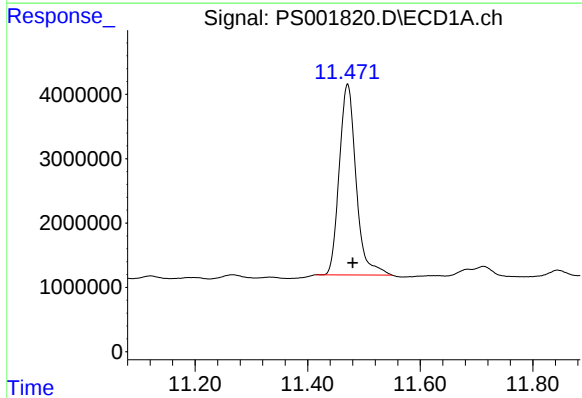


#4 2,4-DCAA

R.T.: 11.471 min
Delta R.T.: -0.009 min
Response: 61511799
Conc: 274.22 ng/ml

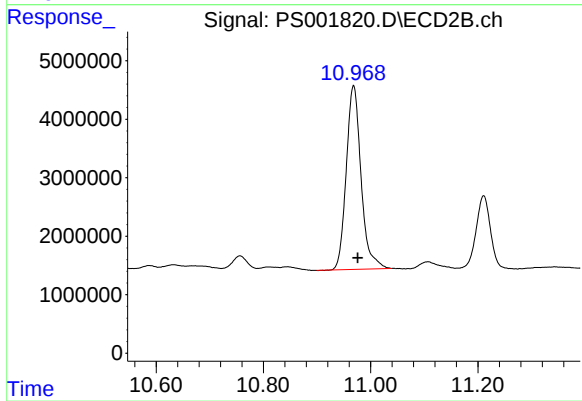

#4 2,4-DCAA


R.T.: 10.968 min
Delta R.T.: -0.008 min
Response: 60194298
Conc: 236.97 ng/ml

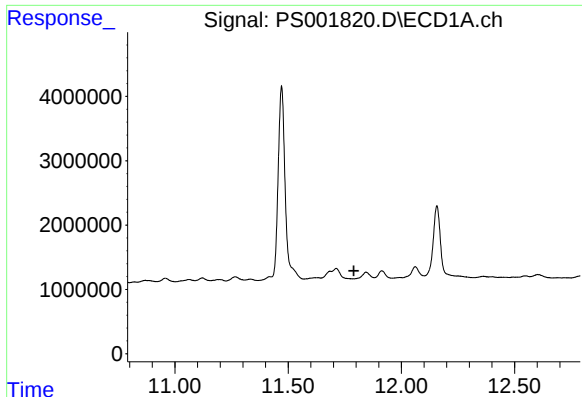

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

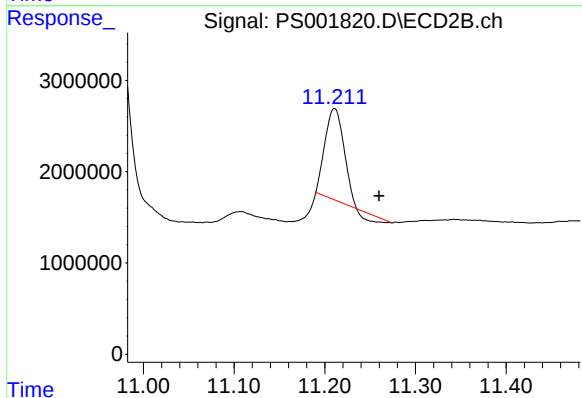


#5 DICAMBA

R.T.: 11.211 min
Delta R.T.: -0.049 min
Response: 13521582
Conc: 15.16 ng/ml

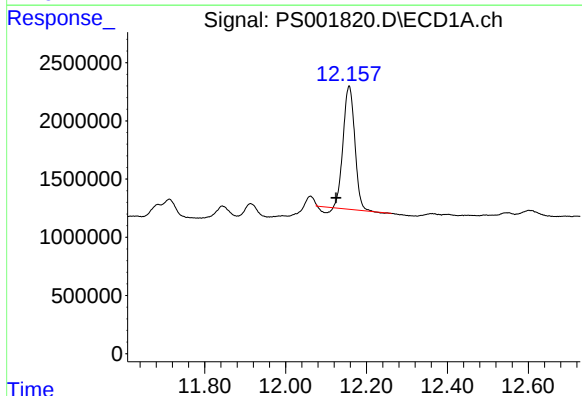


#6 MCP

R.T.: 12.157 min
Delta R.T.: 0.032 min
Response: 20782740
Conc: 32.61 ug/ml

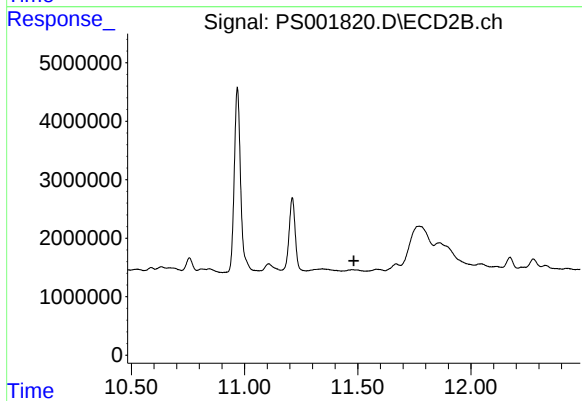

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.483 min
Response: 0
Conc: N.D.

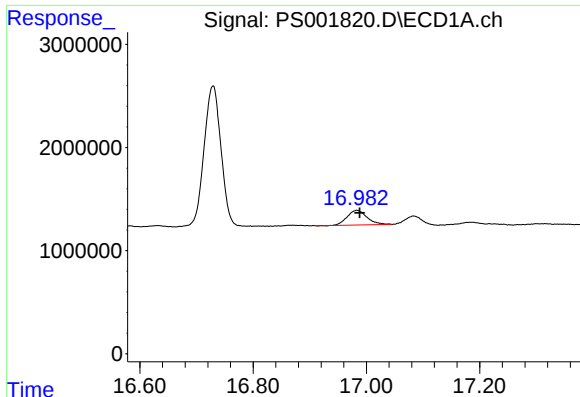

#15 Picloram


R.T.: 16.983 min
Delta R.T.: -0.005 min
Response: 3469248
Conc: 1.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

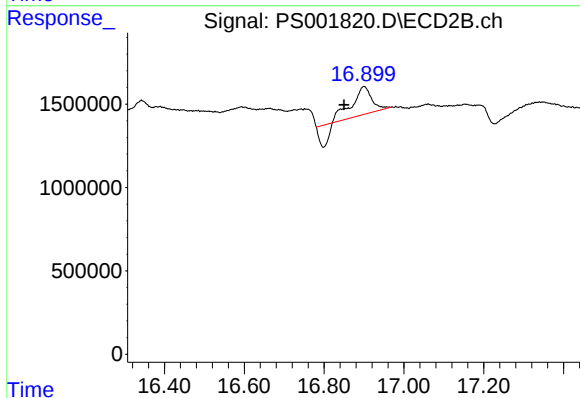


#15 Picloram

R.T.: 16.900 min
Delta R.T.: 0.050 min
Response: 4135941
Conc: 2.43 ng/ml

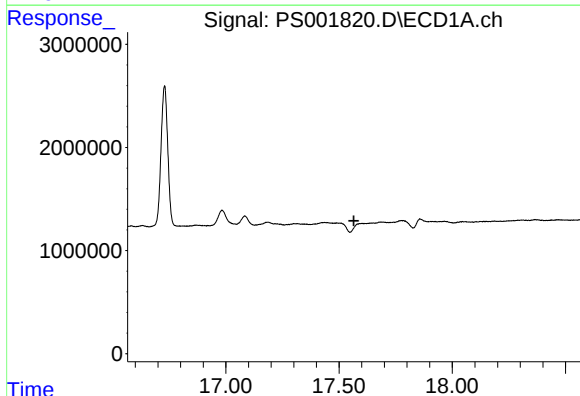

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.565 min
Response: 0
Conc: N.D.

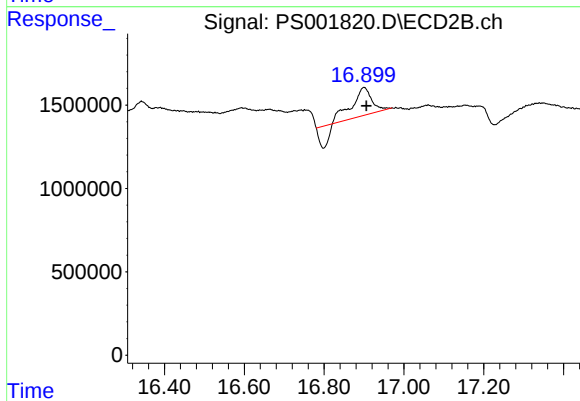

#16 DCPA

R.T.: 16.900 min
Delta R.T.: -0.006 min
Response: 4135941
Conc: 2.24 ng/ml