

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
 Data File : PS001821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2018 02:22
 Operator : EI\SJ
 Sample : J5021-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 06:33:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.479	10.977	60955934	60367830	271.742	237.653
Target Compounds							
1) T	Dalapon	2.911	2.393	29497951	29906517	90.716	101.235
5) T	DICAMBA	0.000	11.219	0	18418115	N.D.	20.651 #
6) T	MCPD	12.167	0.000	16672137	0	26.163	N.D. #
9) T	2,4-D	0.000	12.810	0	3255447	N.D.	10.464 #
15) T	Picloram	0.000	16.909	0	1129736	N.D.	0.664 #
16) T	DCPA	0.000	16.909	0	1129736	N.D.	0.613 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092418\
Data File : PS001821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2018 02:22
Operator : EI\SJ
Sample : J5021-12
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 06:33:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

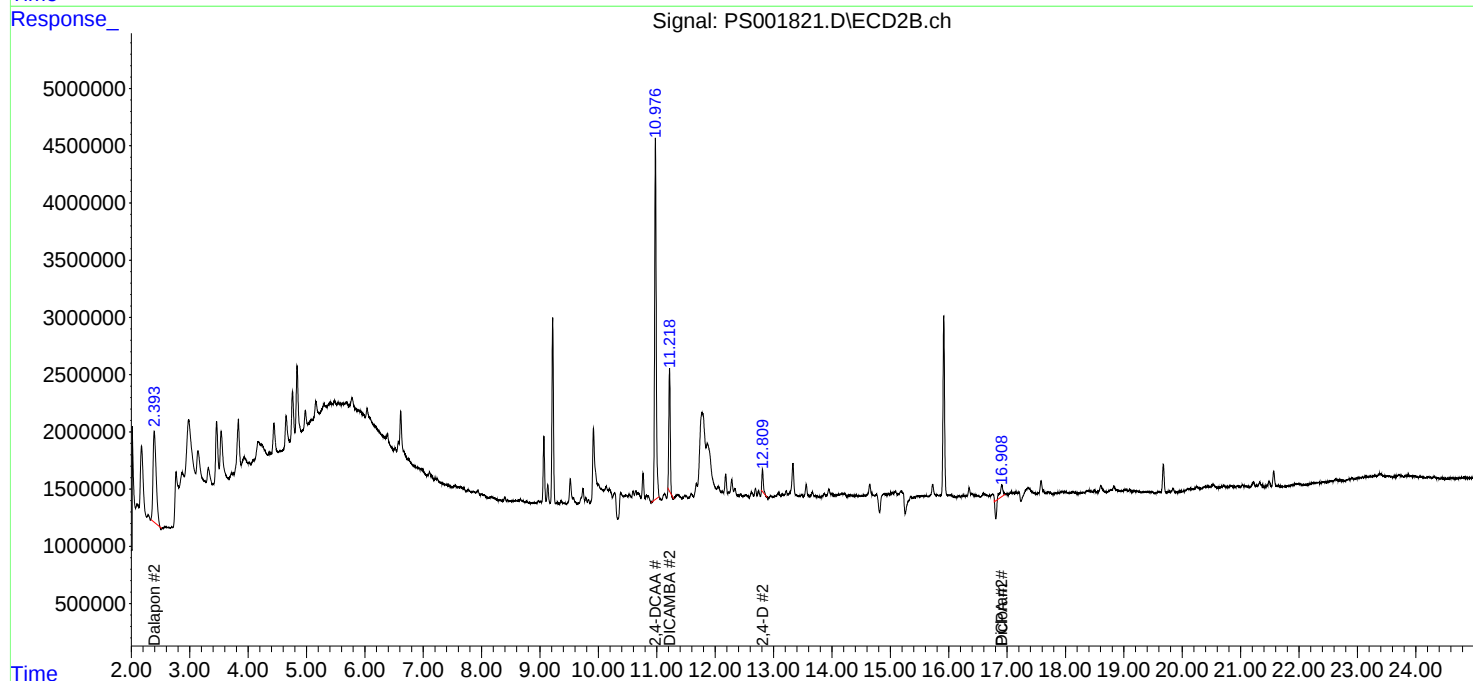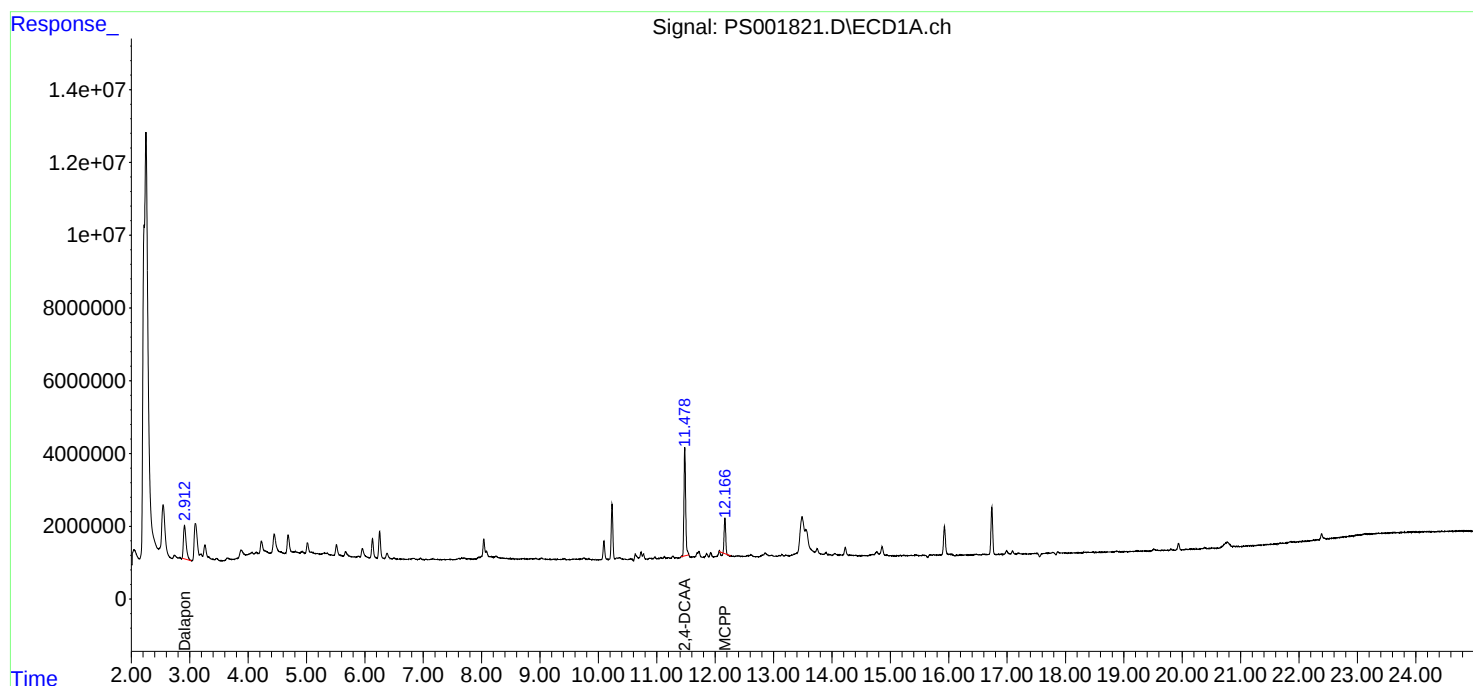


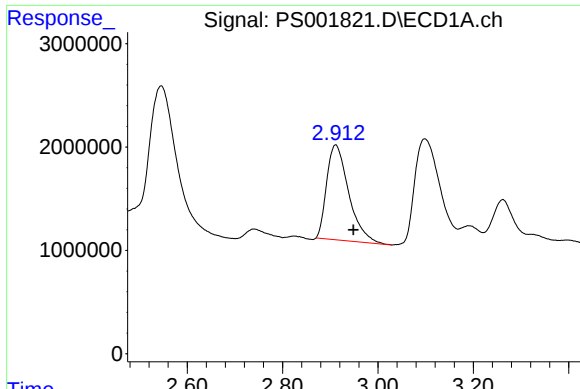

#1 Dalapon


R.T.: 2.911 min
Delta R.T.: -0.038 min
Response: 29497951
Conc: 90.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

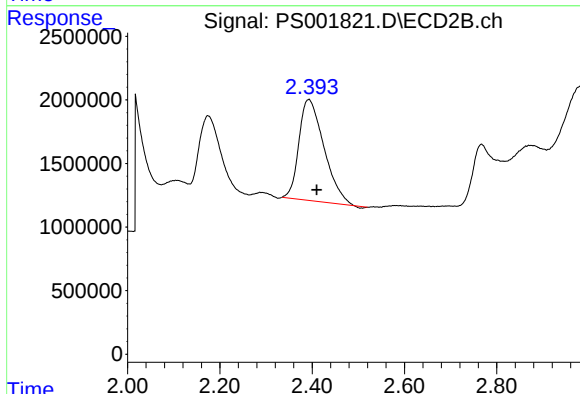


#1 Dalapon

R.T.: 2.393 min
Delta R.T.: -0.016 min
Response: 29906517
Conc: 101.23 ng/ml

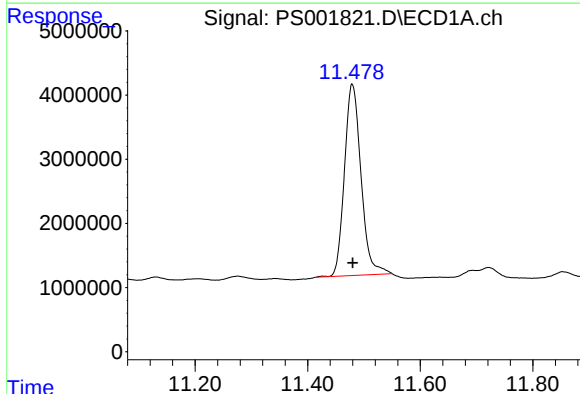


#4 2,4-DCAA

R.T.: 11.479 min
Delta R.T.: 0.000 min
Response: 60955934
Conc: 271.74 ng/ml

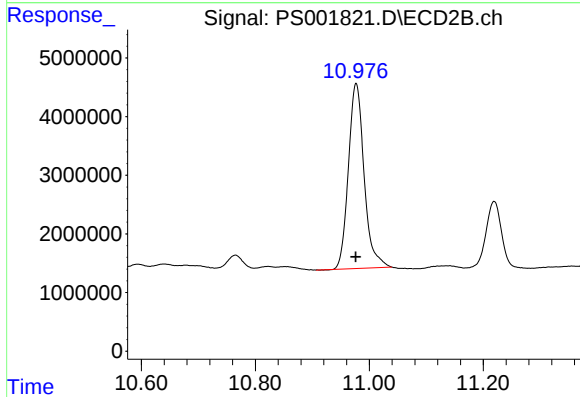

#4 2,4-DCAA


R.T.: 10.977 min
Delta R.T.: 0.000 min
Response: 60367830
Conc: 237.65 ng/ml

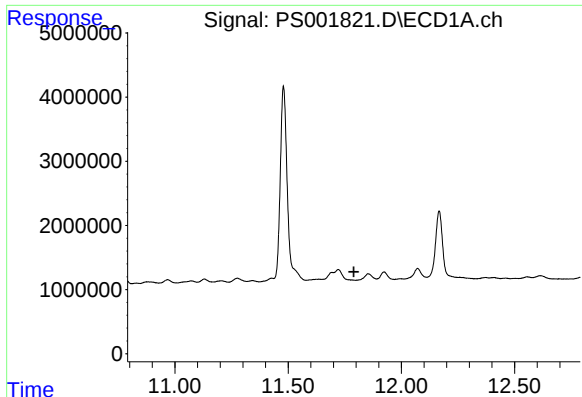

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

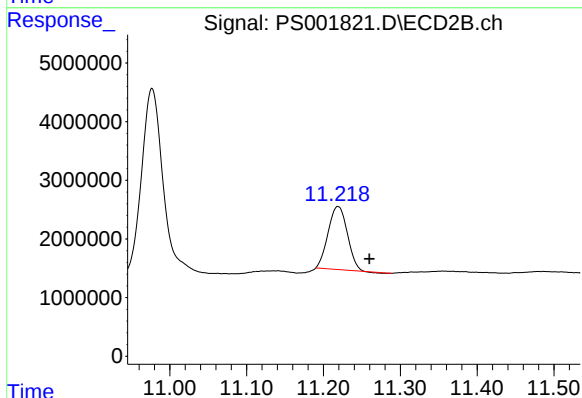


#5 DICAMBA

R.T.: 11.219 min
Delta R.T.: -0.041 min
Response: 18418115
Conc: 20.65 ng/ml

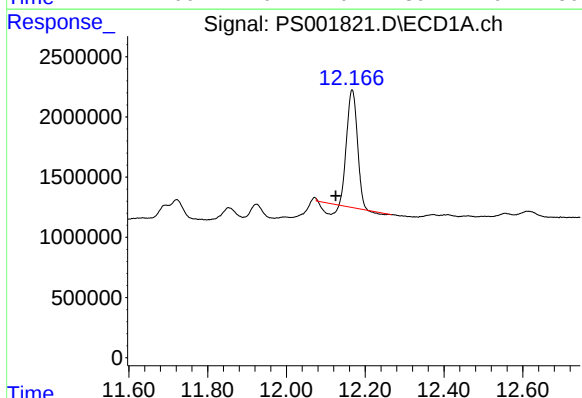


#6 MCP

R.T.: 12.167 min
Delta R.T.: 0.042 min
Response: 16672137
Conc: 26.16 ug/ml

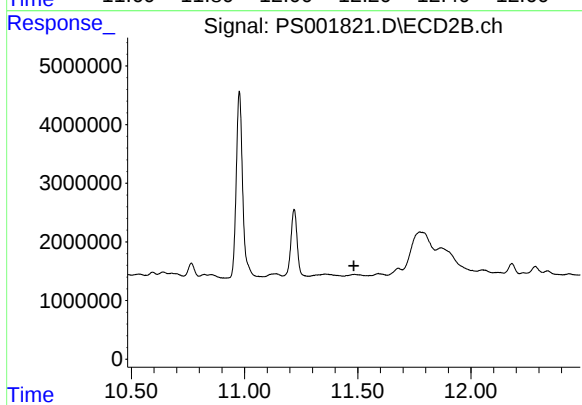

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.483 min
Response: 0
Conc: N.D.

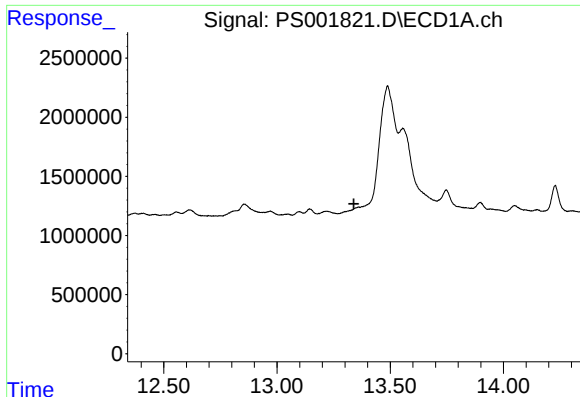

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

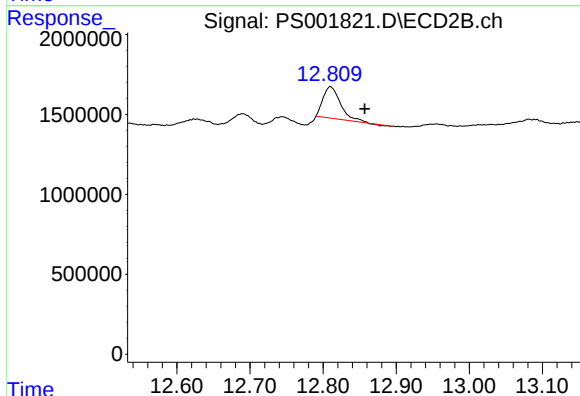


#9 2,4-D

R.T.: 12.810 min
Delta R.T.: -0.047 min
Response: 3255447
Conc: 10.46 ng/ml

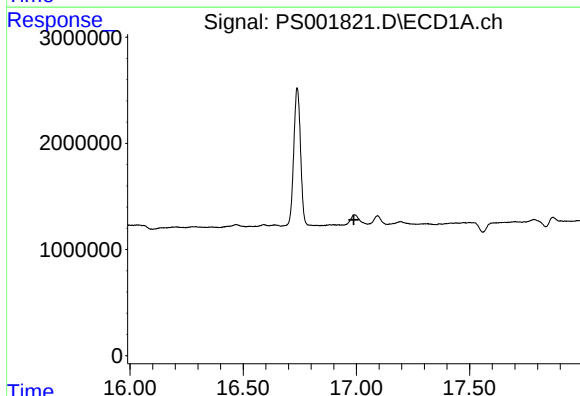


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.988 min
Response: 0
Conc: N.D.

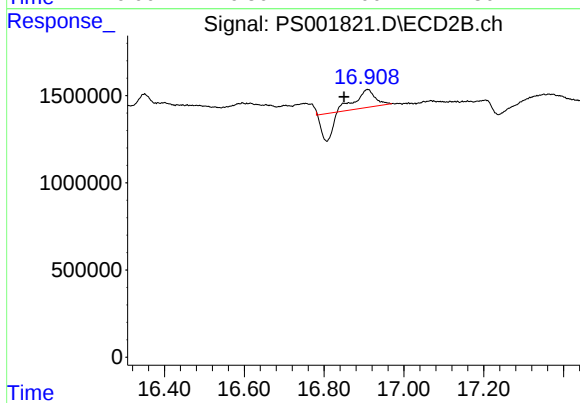

#15 Picloram


R.T.: 16.909 min
Delta R.T.: 0.059 min
Response: 1129736
Conc: 0.66 ng/ml

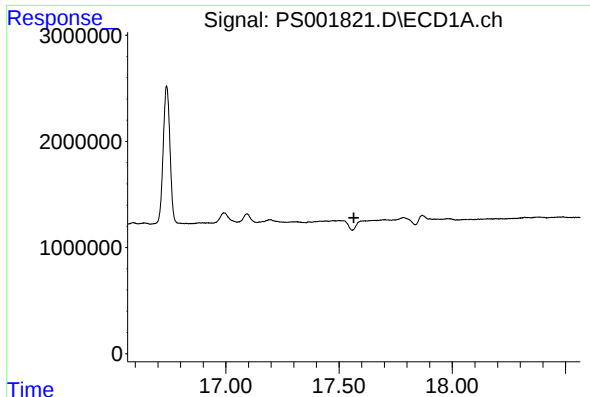

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

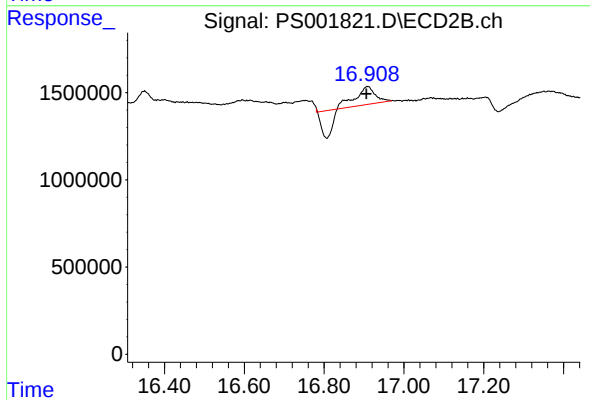

#16 DCPA

R.T.: 16.909 min
Delta R.T.: 0.003 min
Response: 1129736
Conc: 0.61 ng/ml