

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092418\  
 Data File : PS001826.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Sep 2018 04:57  
 Operator : EI\SJ  
 Sample : J5023-12  
 Misc :  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 25 06:34:29 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS091718.M  
 Quant Title : 8080.M  
 QLast Update : Tue Sep 18 03:01:16 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml     |
|-----------------------------|--------------|--------|--------|----------|----------|---------|-----------|
| -----                       |              |        |        |          |          |         |           |
| System Monitoring Compounds |              |        |        |          |          |         |           |
| 4) S                        | 2,4-DCAA     | 11.456 | 10.953 | 70060666 | 67692520 | 312.331 | 266.488   |
| Target Compounds            |              |        |        |          |          |         |           |
| 1) T                        | Dalapon      | 2.887  | 2.369  | 1425191  | 37882855 | 4.383   | 128.235 # |
| 2) T                        | 3,5-DICHL... | 0.000  | 9.110  | 0        | 1848636  | N.D.    | 5.857 #   |
| 5) T                        | DICAMBA      | 11.831 | 0.000  | 1700842  | 0        | 1.962   | N.D. #    |
| 6) T                        | MCP          | 12.143 | 0.000  | 22714186 | 0        | 35.645  | N.D. #    |
| 15) T                       | Picloram     | 0.000  | 16.886 | 0        | 9371571  | N.D.    | 5.510 #   |
| 16) T                       | DCPA         | 0.000  | 16.886 | 0        | 9371571  | N.D.    | 5.081 #   |
| -----                       |              |        |        |          |          |         |           |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092418\  
Data File : PS001826.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Sep 2018 04:57  
Operator : EI\SJ  
Sample : J5023-12  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 25 06:34:29 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS091718.M  
Quant Title : 8080.M  
QLast Update : Tue Sep 18 03:01:16 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

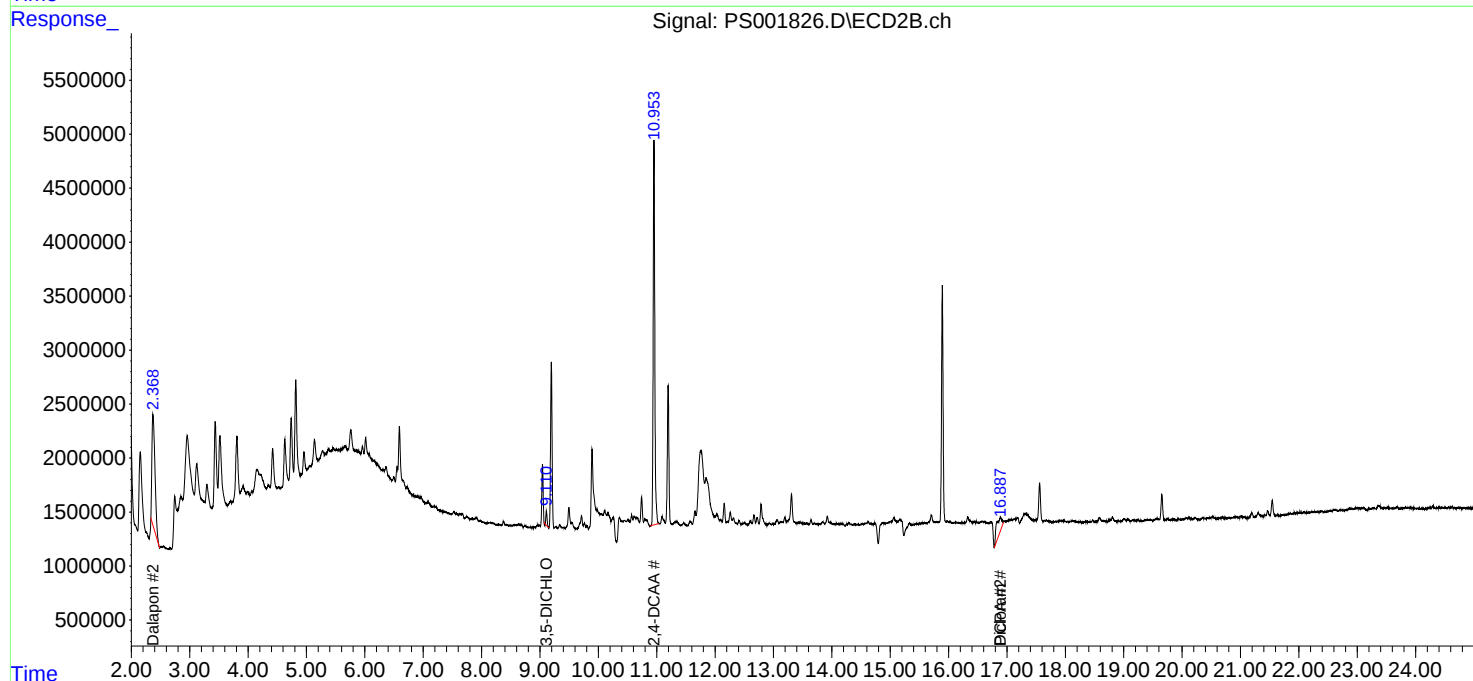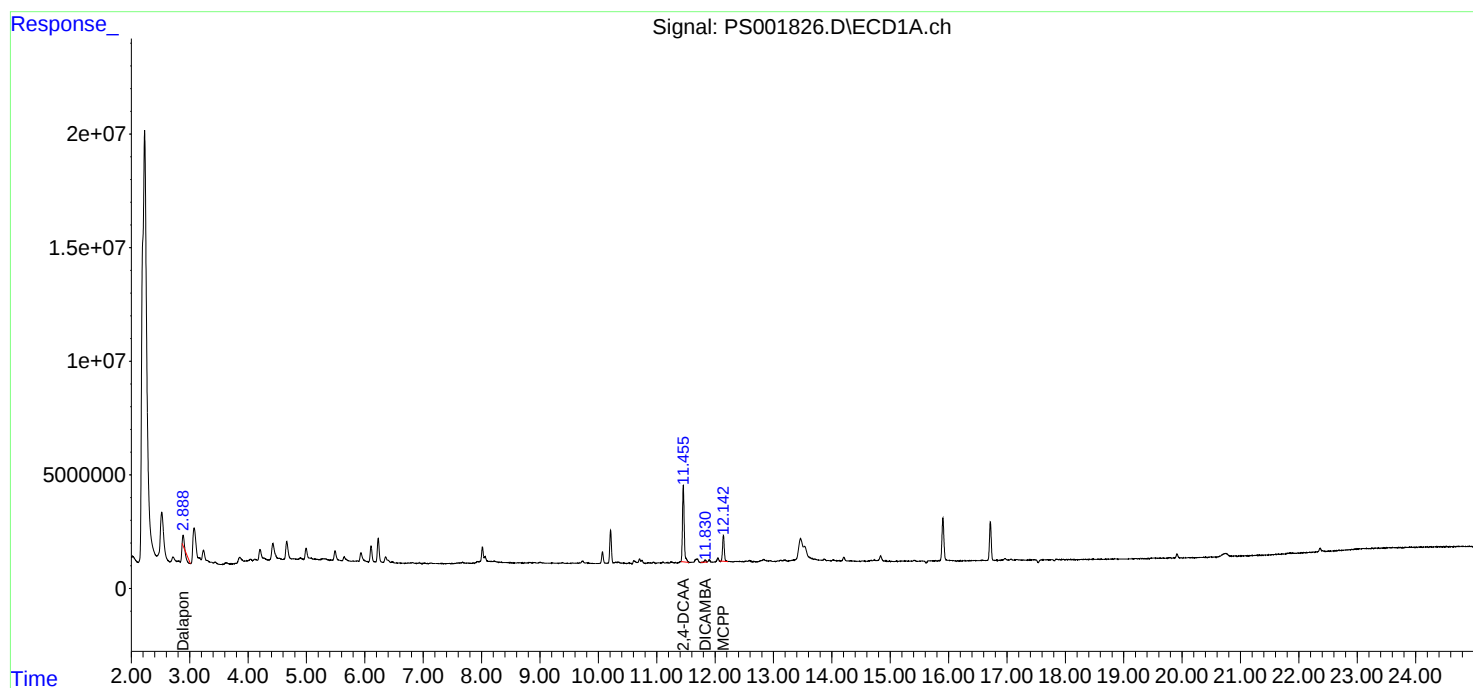


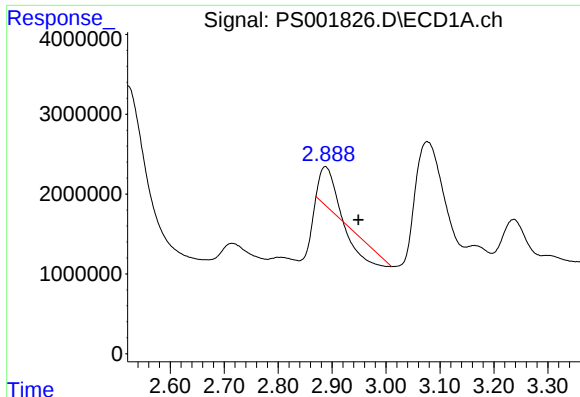

#1 Dalapon


R.T.: 2.887 min  
Delta R.T.: -0.062 min  
Response: 1425191  
Conc: 4.38 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

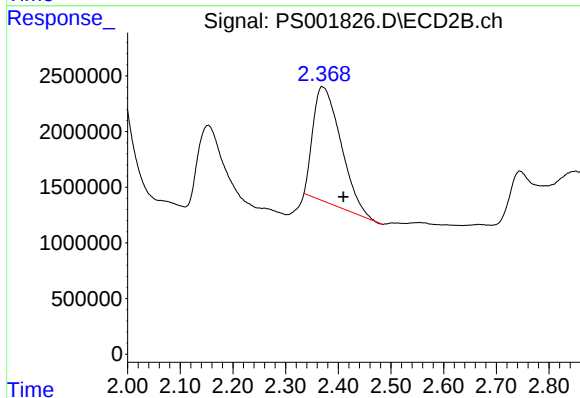


#1 Dalapon

R.T.: 2.369 min  
Delta R.T.: -0.041 min  
Response: 37882855  
Conc: 128.24 ng/ml

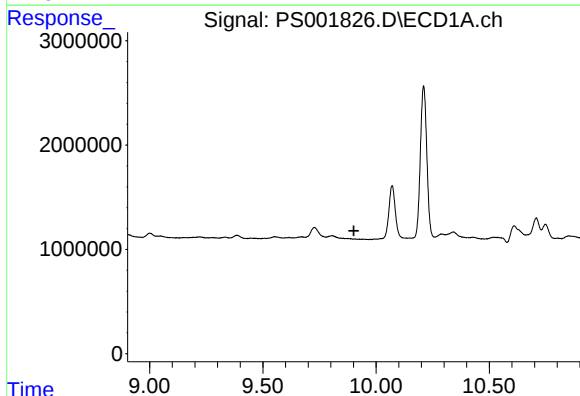


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T. : 9.902 min  
Response: 0  
Conc: N.D.

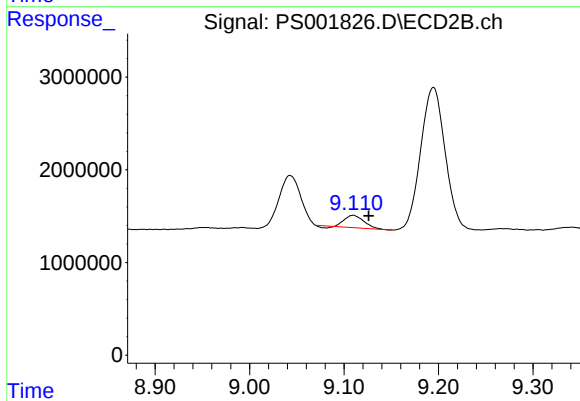

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.110 min  
Delta R.T.: -0.016 min  
Response: 1848636  
Conc: 5.86 ng/ml

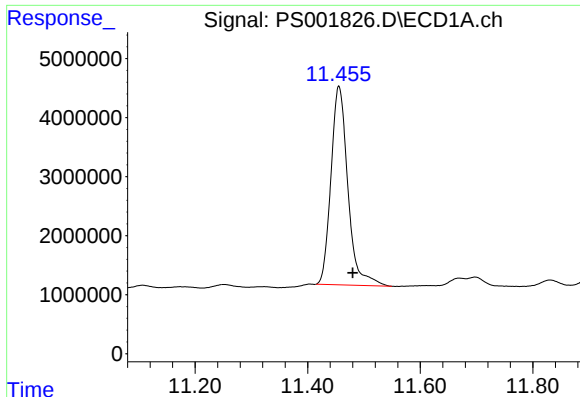

#4 2,4-DCAA


R.T.: 11.456 min  
Delta R.T.: -0.024 min  
Response: 70060666  
Conc: 312.33 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

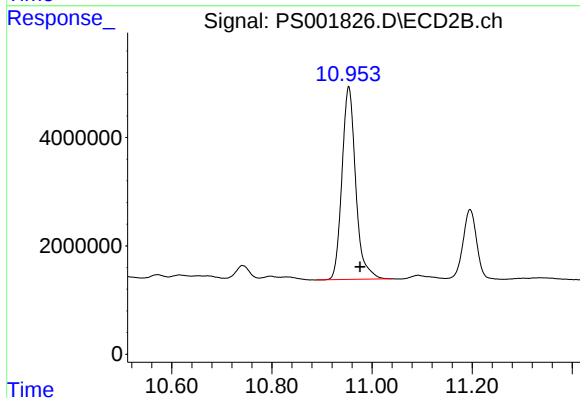


#4 2,4-DCAA

R.T.: 10.953 min  
Delta R.T.: -0.023 min  
Response: 67692520  
Conc: 266.49 ng/ml

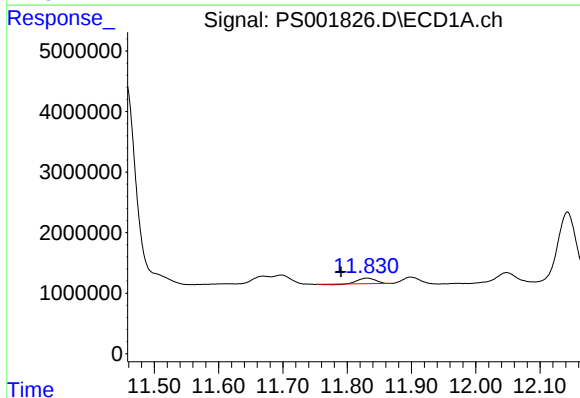


#5 DICAMBA

R.T.: 11.831 min  
Delta R.T.: 0.040 min  
Response: 1700842  
Conc: 1.96 ng/ml

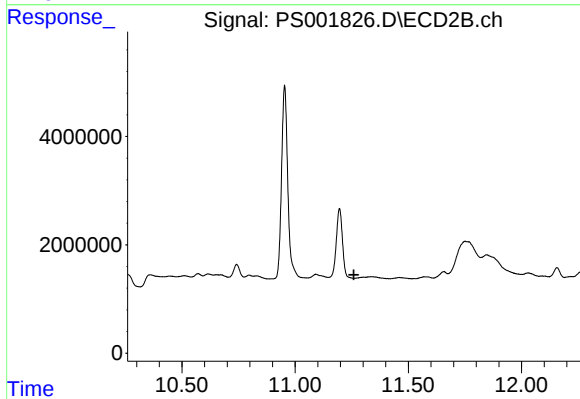

#5 DICAMBA


R.T.: 0.000 min  
Exp R.T. : 11.260 min  
Response: 0  
Conc: N.D.

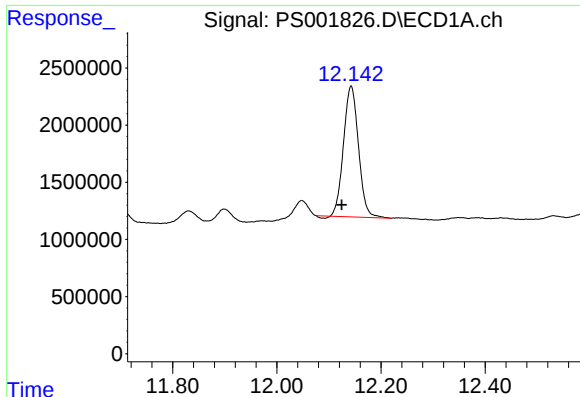

#6 MCP


R.T.: 12.143 min  
Delta R.T.: 0.018 min  
Response: 22714186  
Conc: 35.64 ug/ml

Instrument :  
ECD\_S  
ClientSampleId :

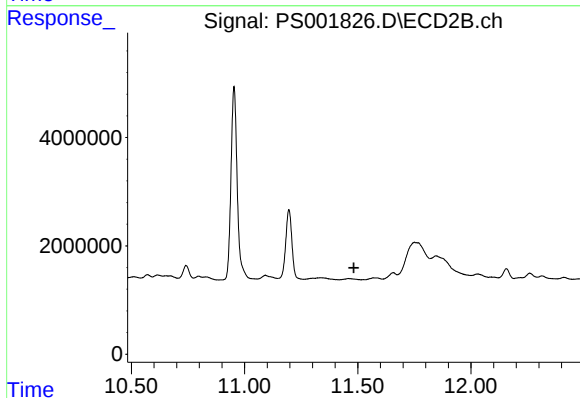


#6 MCP

R.T.: 0.000 min  
Exp R.T. : 11.483 min  
Response: 0  
Conc: N.D.

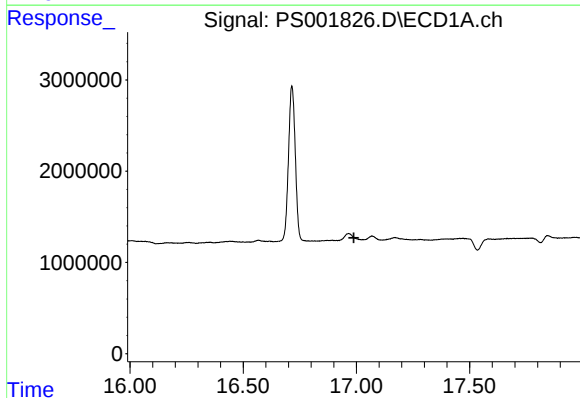


#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 16.988 min  
Response: 0  
Conc: N.D.

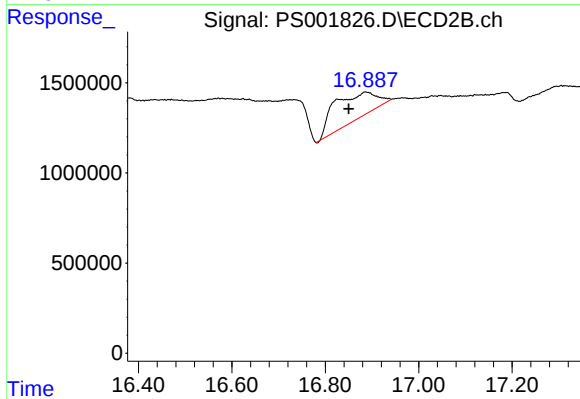

#15 Picloram


R.T.: 16.886 min  
Delta R.T.: 0.036 min  
Response: 9371571  
Conc: 5.51 ng/ml

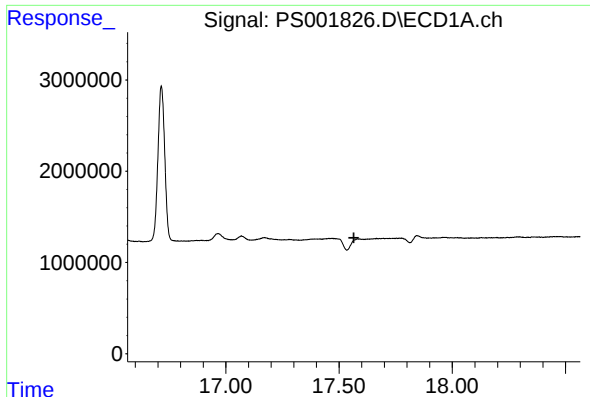

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 17.565 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

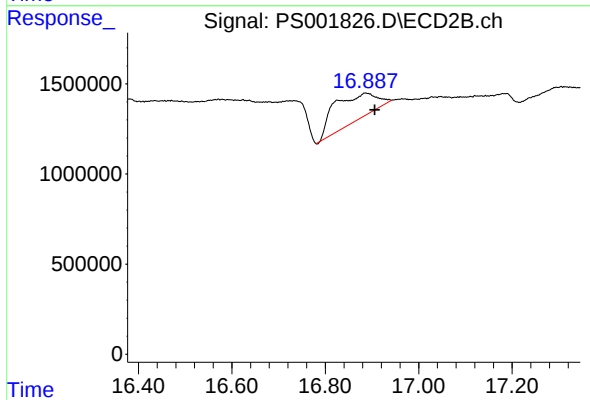

#16 DCPA

R.T.: 16.886 min  
Delta R.T.: -0.020 min  
Response: 9371571  
Conc: 5.08 ng/ml