

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092419\
 Data File : PS006874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2019 15:23
 Operator : SM\AJ
 Sample : PB123247BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:04:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.495	5.225	685.9E6	383.6E6	750.620	834.118
Target Compounds							
1) T	Dalapon	2.043	1.756	109.4E6	94515088	102.431	177.304 #
2) T	3,5-DICHL...	0.000	4.554	0	42902516	N.D.	74.631
3) T	4-Nitroph...	5.348	0.000	11048884	0	28.977	N.D. #
5) T	DICAMBA	5.590	0.000	33401733	0	10.338	N.D. #
7) T	MCPA	5.972	5.604	13528311	24546112	4.348	13.336 #
9) T	2,4-D	6.561	6.148	108.5E6	7982716	132.354	15.650 #
10) T	Pentachlo...	6.756	6.533	48896916	34485888	4.103	5.481 #
11) T	2,4,5-TP ...	0.000	6.846	0	33353315	N.D.	13.924
13) T	2,4-DB	8.073	0.000	35134103	0	60.575	N.D. #
15) T	Picloram	0.000	9.012	0	2061880	N.D.	<MDL
16) T	DCPA	0.000	9.012	0	2061880	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092419\
Data File : PS006874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2019 15:23
Operator : SM\AJ
Sample : PB123247BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:04:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

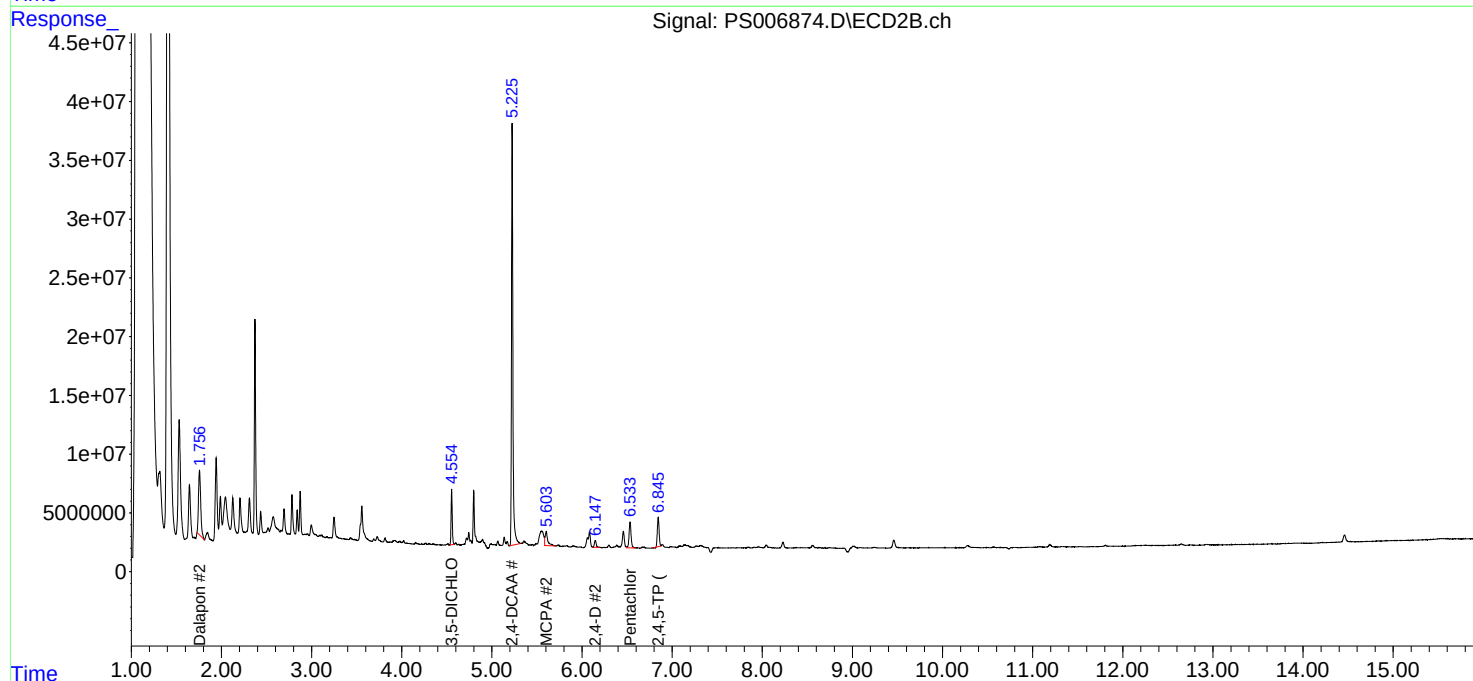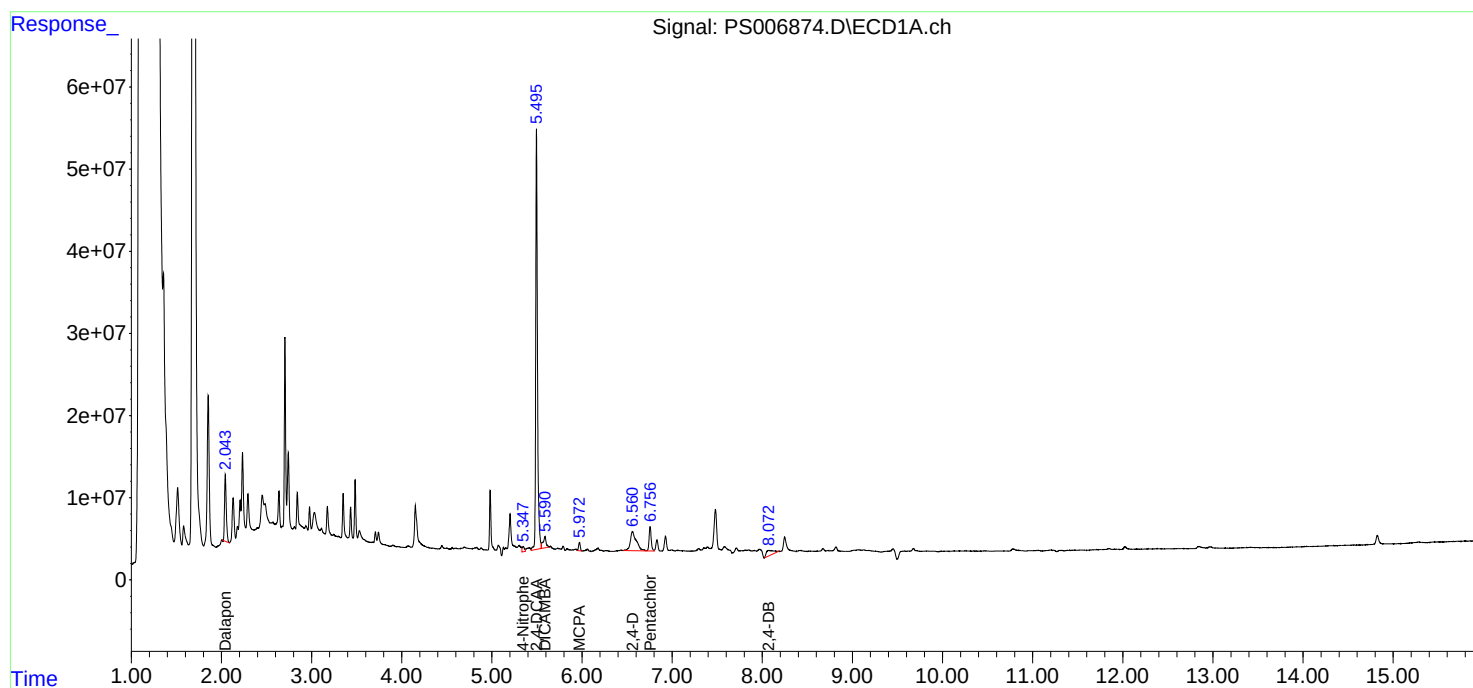


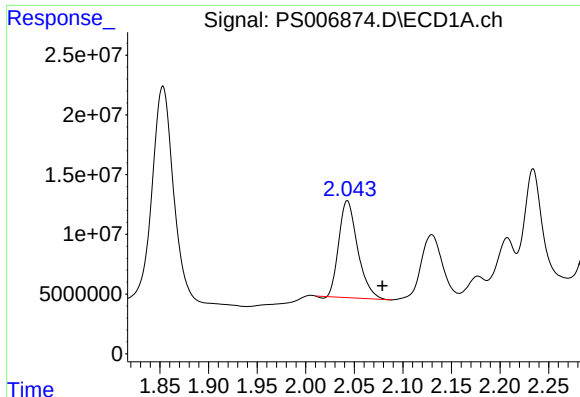

#1 Dalapon


R.T.: 2.043 min
Delta R.T.: -0.036 min
Response: 109437907
Conc: 102.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

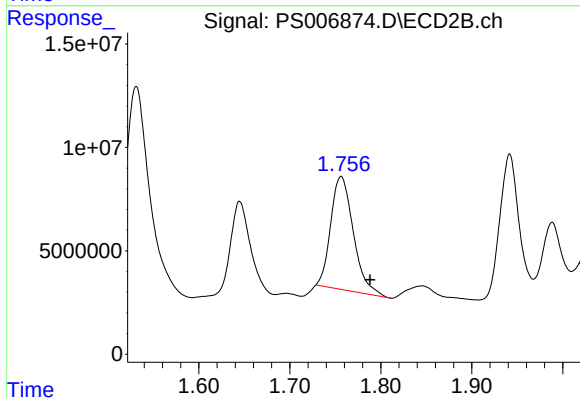


#1 Dalapon

R.T.: 1.756 min
Delta R.T.: -0.032 min
Response: 94515088
Conc: 177.30 ng/ml

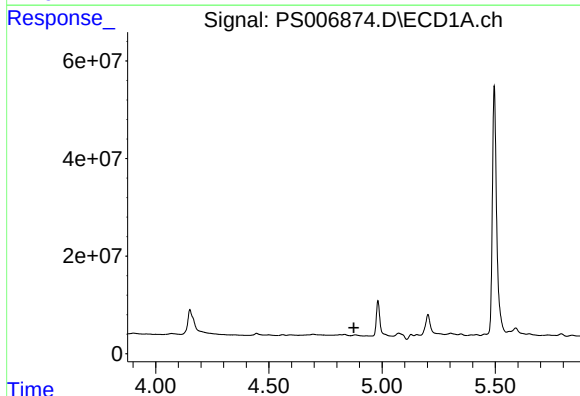


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.876 min
Response: 0
Conc: N.D.

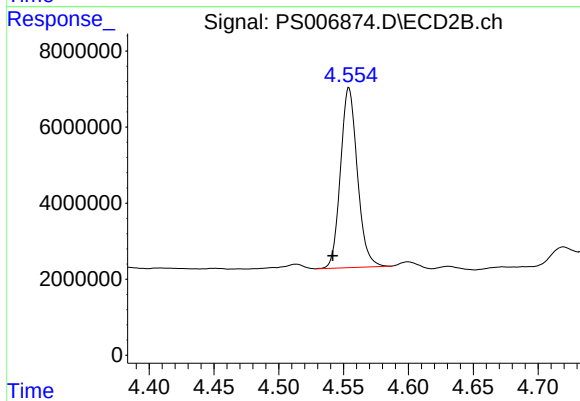

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.554 min
Delta R.T.: 0.013 min
Response: 42902516
Conc: 74.63 ng/ml

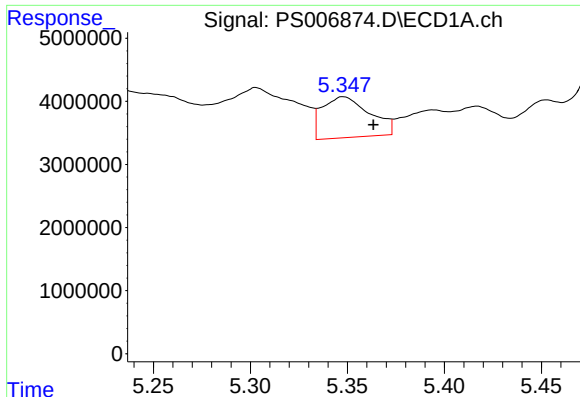

#3 4-Nitrophenol


R.T.: 5.348 min
Delta R.T.: -0.016 min
Response: 11048884
Conc: 28.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

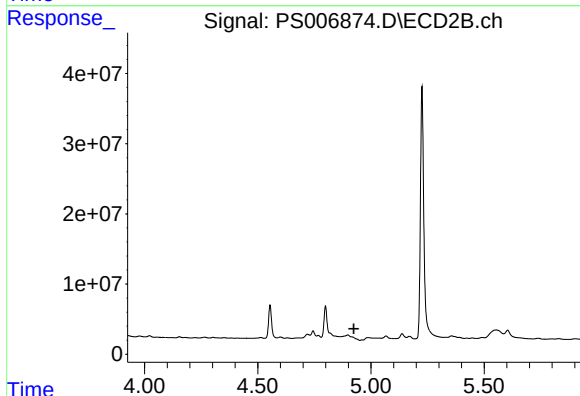


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

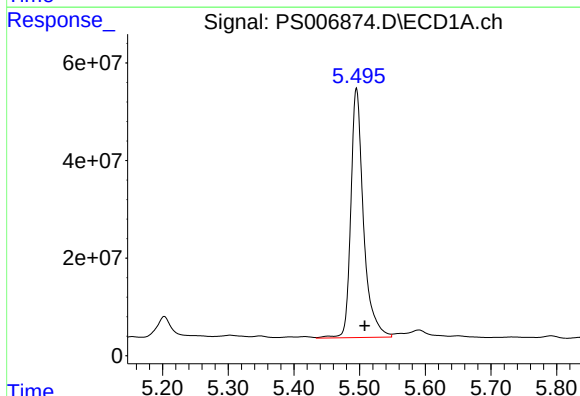


#4 2,4-DCAA

R.T.: 5.495 min
Delta R.T.: -0.013 min
Response: 685926593
Conc: 750.62 ng/ml

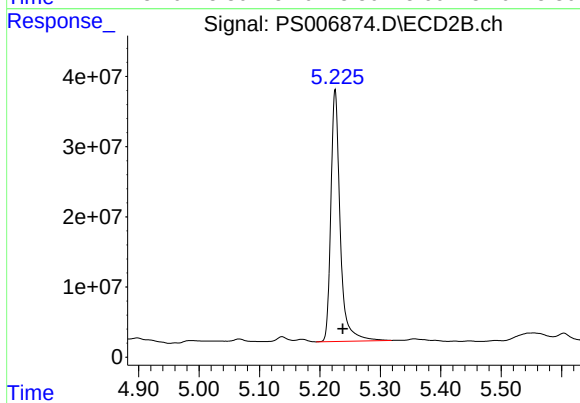

#4 2,4-DCAA


R.T.: 5.225 min
Delta R.T.: -0.013 min
Response: 383562128
Conc: 834.12 ng/ml

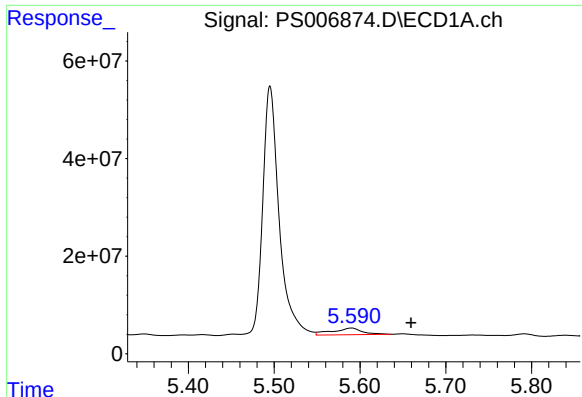

#5 DICAMBA


R.T.: 5.590 min
Delta R.T.: -0.070 min
Response: 33401733
Conc: 10.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

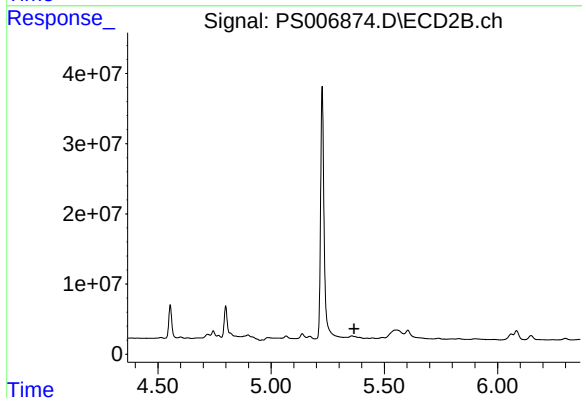


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.366 min
Response: 0
Conc: N.D.

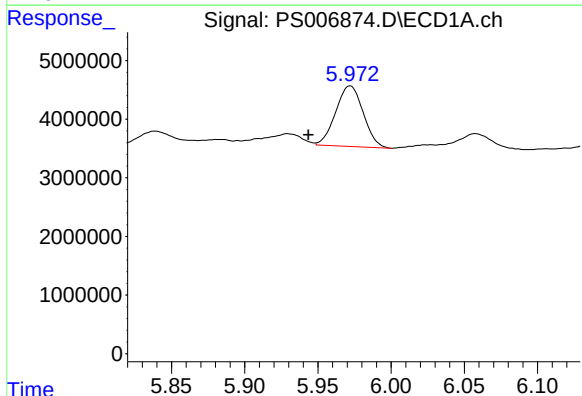


#7 MCPA

R.T.: 5.972 min
Delta R.T.: 0.028 min
Response: 13528311
Conc: 4.35 ug/ml

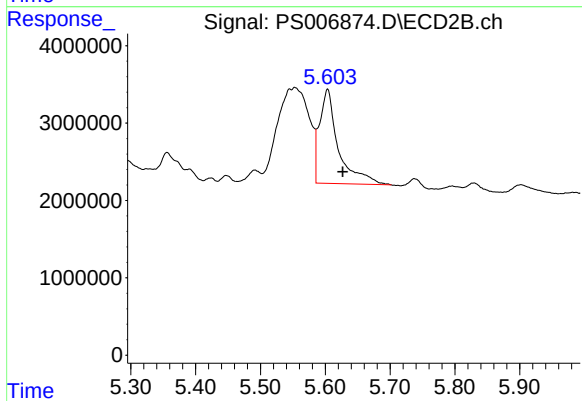

#7 MCPA


R.T.: 5.604 min
Delta R.T.: -0.024 min
Response: 24546112
Conc: 13.34 ug/ml

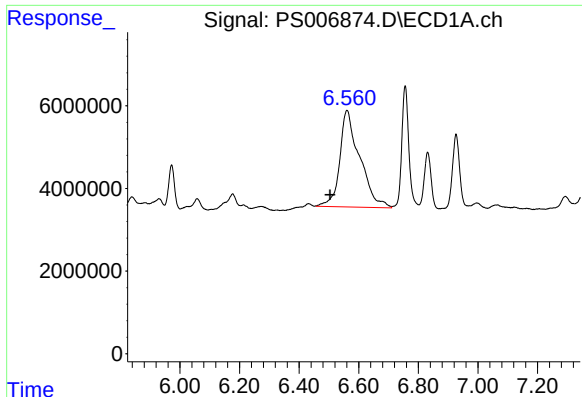

#9 2,4-D


R.T.: 6.561 min
Delta R.T.: 0.057 min
Response: 108466292
Conc: 132.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

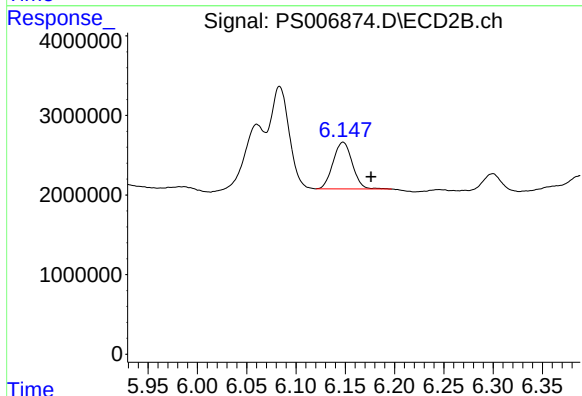


#9 2,4-D

R.T.: 6.148 min
Delta R.T.: -0.028 min
Response: 7982716
Conc: 15.65 ng/ml

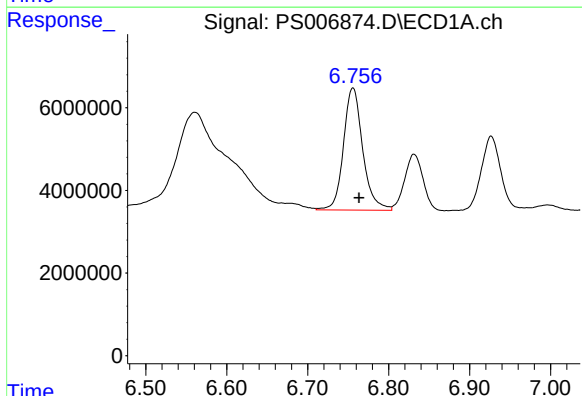


#10 Pentachlorophenol

R.T.: 6.756 min
Delta R.T.: -0.008 min
Response: 48896916
Conc: 4.10 ng/ml

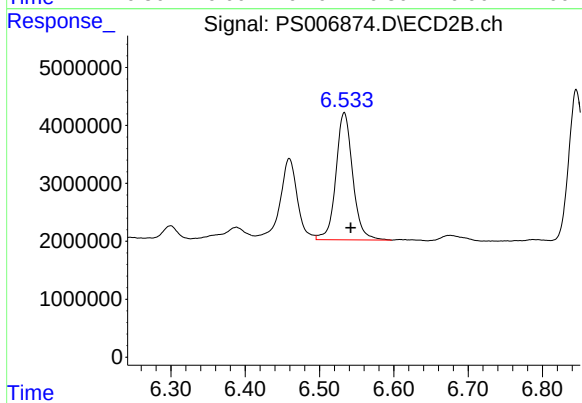

#10 Pentachlorophenol


R.T.: 6.533 min
Delta R.T.: -0.009 min
Response: 34485888
Conc: 5.48 ng/ml

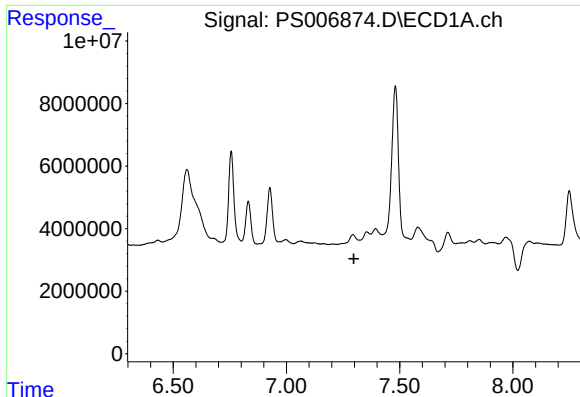

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

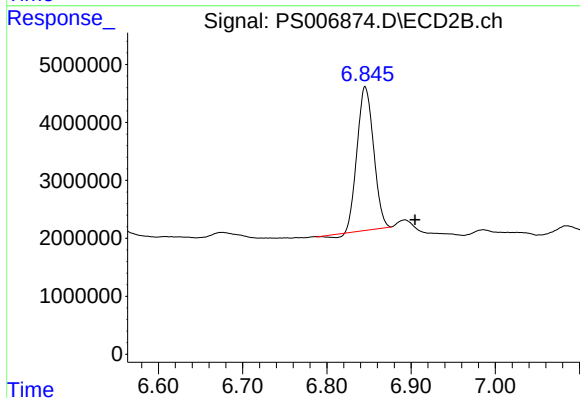


#11 2,4,5-TP (SILVEX)

R.T.: 6.846 min
Delta R.T.: -0.059 min
Response: 33353315
Conc: 13.92 ng/ml

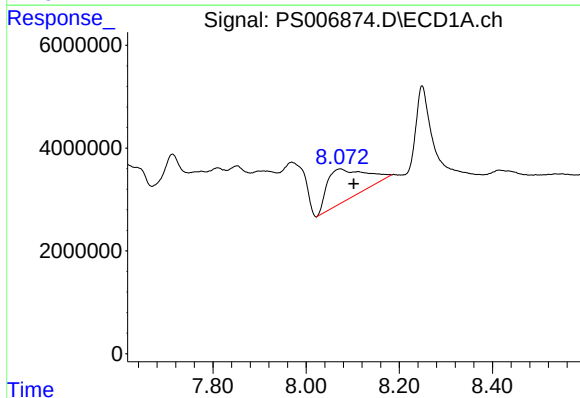

#13 2,4-DB

R.T.: 8.073 min
Delta R.T.: -0.029 min
Response: 35134103
Conc: 60.57 ng/ml

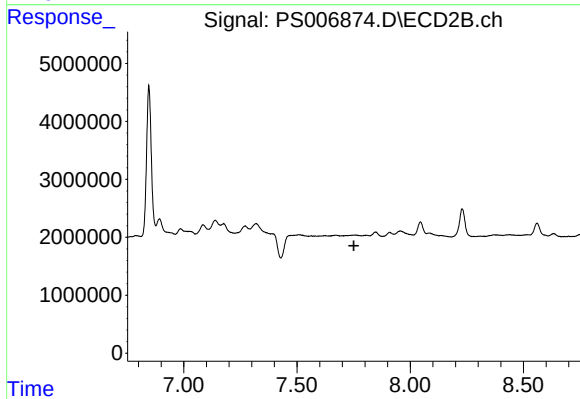

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 7.751 min
Response: 0
Conc: N.D.