

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092420\
 Data File : PS012475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 09:02
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 10:30:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) T	MCP	0.000	7.228	0	6099173	N.D.	4.032
9) T	2,4-D	8.347	7.962	155.8E6	6492031	137.190	10.367 #
13) T	2,4-DB	0.000	9.708	0	7810822	N.D.	20.864



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092420\
Data File : PS012475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 09:02
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 10:30:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

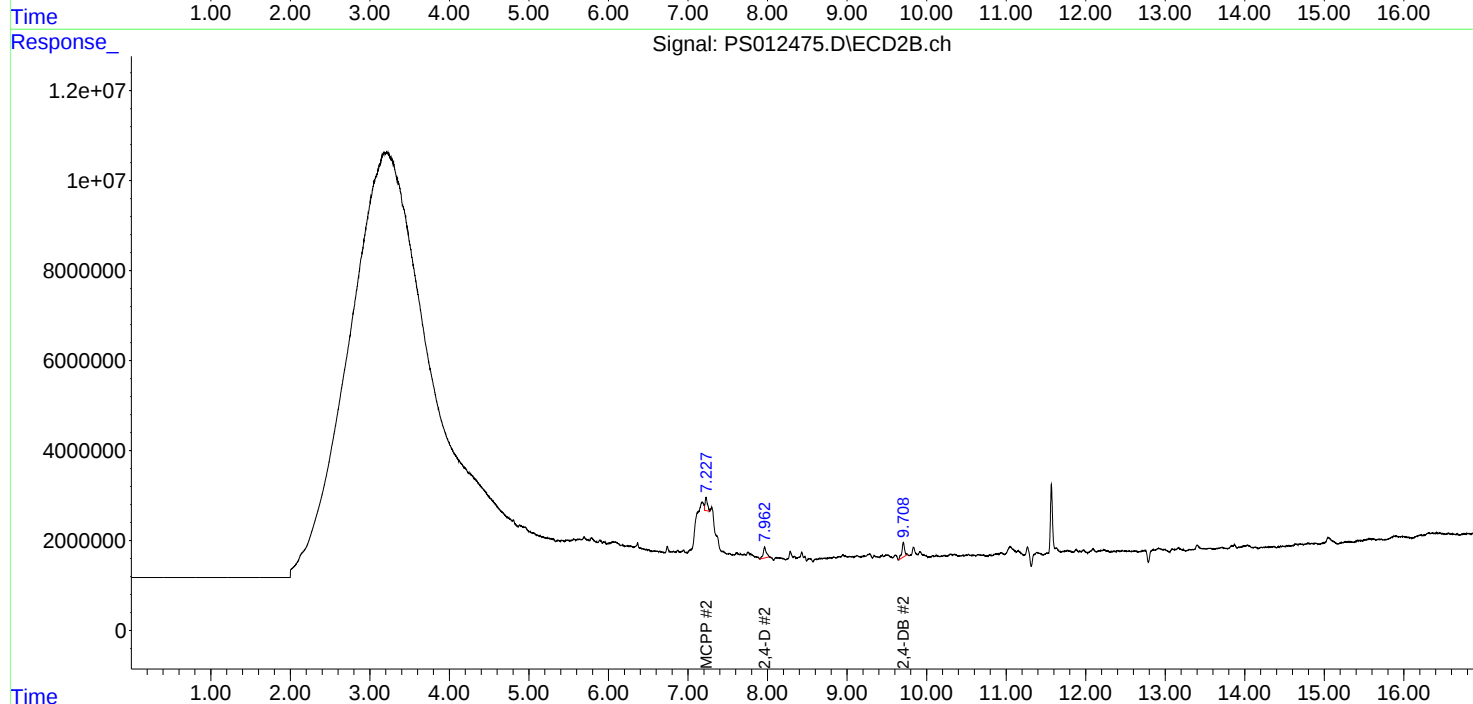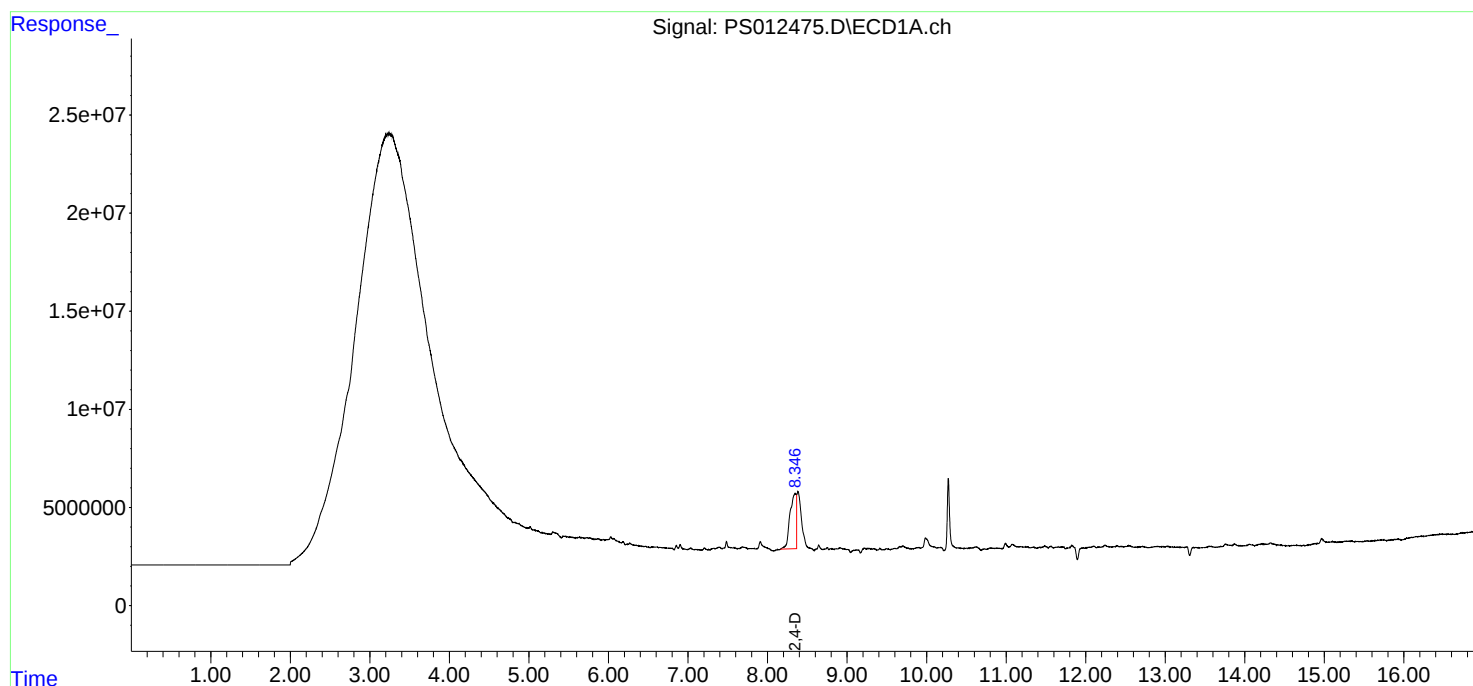


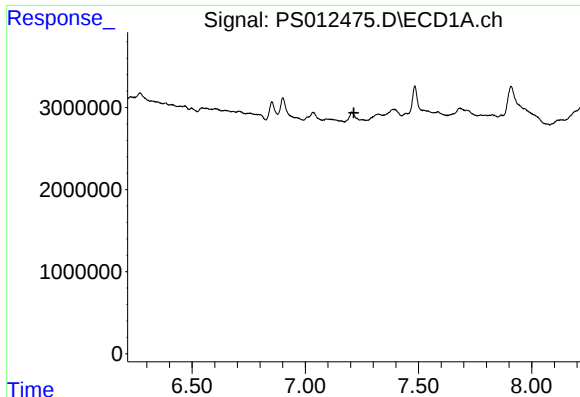

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.215 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

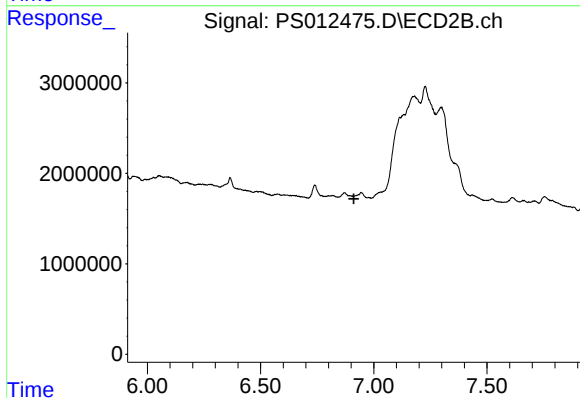


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

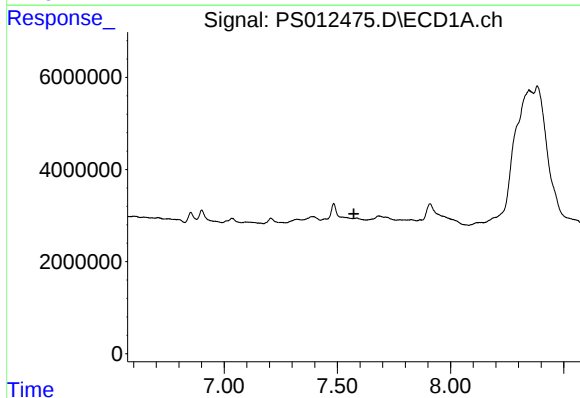


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.573 min
Response: 0
Conc: N.D.

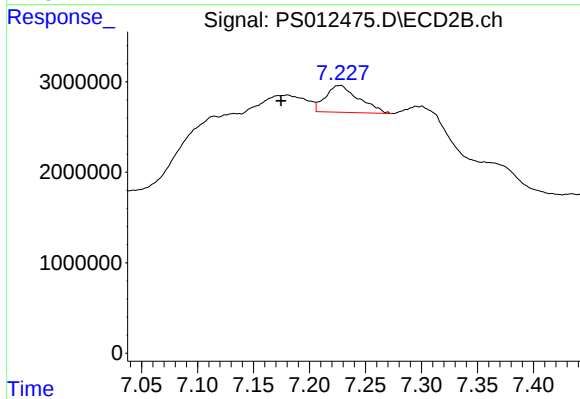

#6 MCP


R.T.: 7.228 min
Delta R.T.: 0.053 min
Response: 6099173
Conc: 4.03 ug/ml

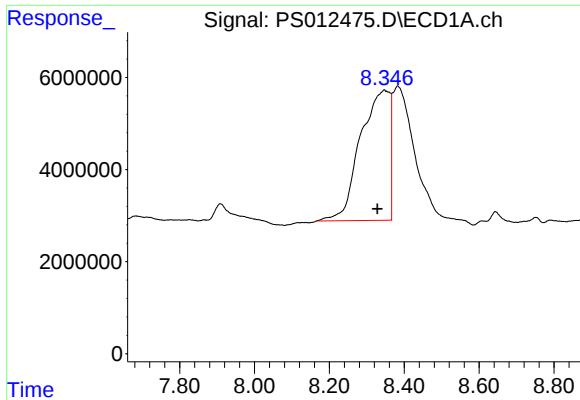

#9 2,4-D


R.T.: 8.347 min
Delta R.T.: 0.019 min
Response: 155768823
Conc: 137.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

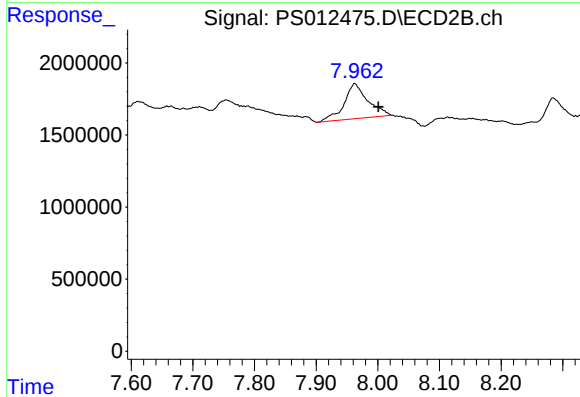


#9 2,4-D

R.T.: 7.962 min
Delta R.T.: -0.039 min
Response: 6492031
Conc: 10.37 ng/ml

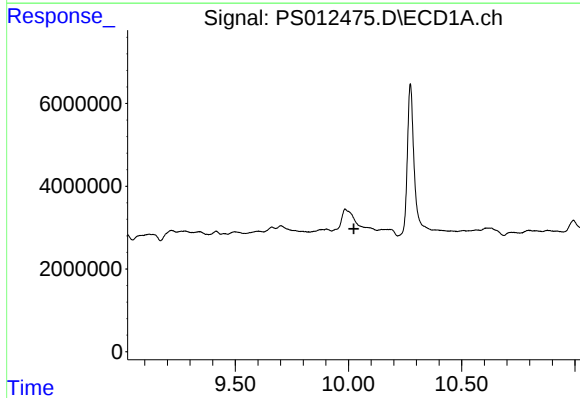

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.024 min
Response: 0
Conc: N.D.

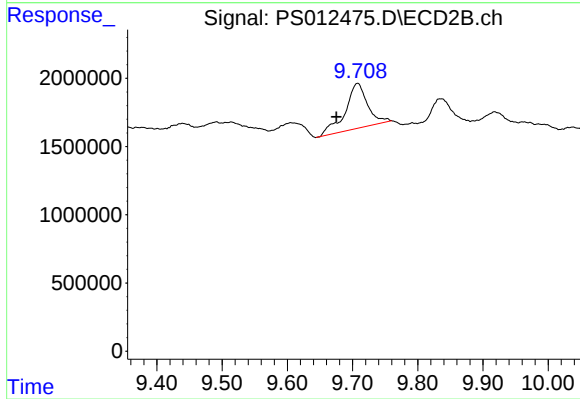

#13 2,4-DB

R.T.: 9.708 min
Delta R.T.: 0.033 min
Response: 7810822
Conc: 20.86 ng/ml