

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092425\
 Data File : PS031827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2025 12:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:57:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.748	1762.5E6	462.4E6	489.385	508.778
Target Compounds							
1) T	Dalapon	0.000	2.659f	0	52231744	N.D.	18.537
2) T	3,5-DICHL...	6.448	0.000	11440607	0	2.145	N.D. #
3) T	4-Nitroph...	7.081	0.000	5746545	0	5.209	N.D. #
6) T	MCP	7.694f	0.000	1471361	0	<MDL	N.D. #
7) T	MCPA	7.795	8.246f	2556232	51405820	<MDL	18.351 #
8) T	DICHLORPROP	8.168	0.000	92732	0	<MDL	N.D. #
10) T	Pentachlo...	8.708	9.515	10136943	42400407	<MDL	1.068 #
11) T	2,4,5-TP ...	9.292	9.914	4949157	6497838	<MDL	<MDL #
12) T	2,4,5-T	9.588	0.000	1755438	0	<MDL	N.D. #
13) T	2,4-DB	10.143	10.904	1541979	5967482	<MDL	5.577 #
14) T	DINOSEB	11.350	0.000	1924563	0	<MDL	N.D. #
15) T	Picloram	11.185	0.000	3656151	0	<MDL	N.D. #
16) T	DCPA	11.659	0.000	3680649	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092425\
Data File : PS031827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2025 12:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:57:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

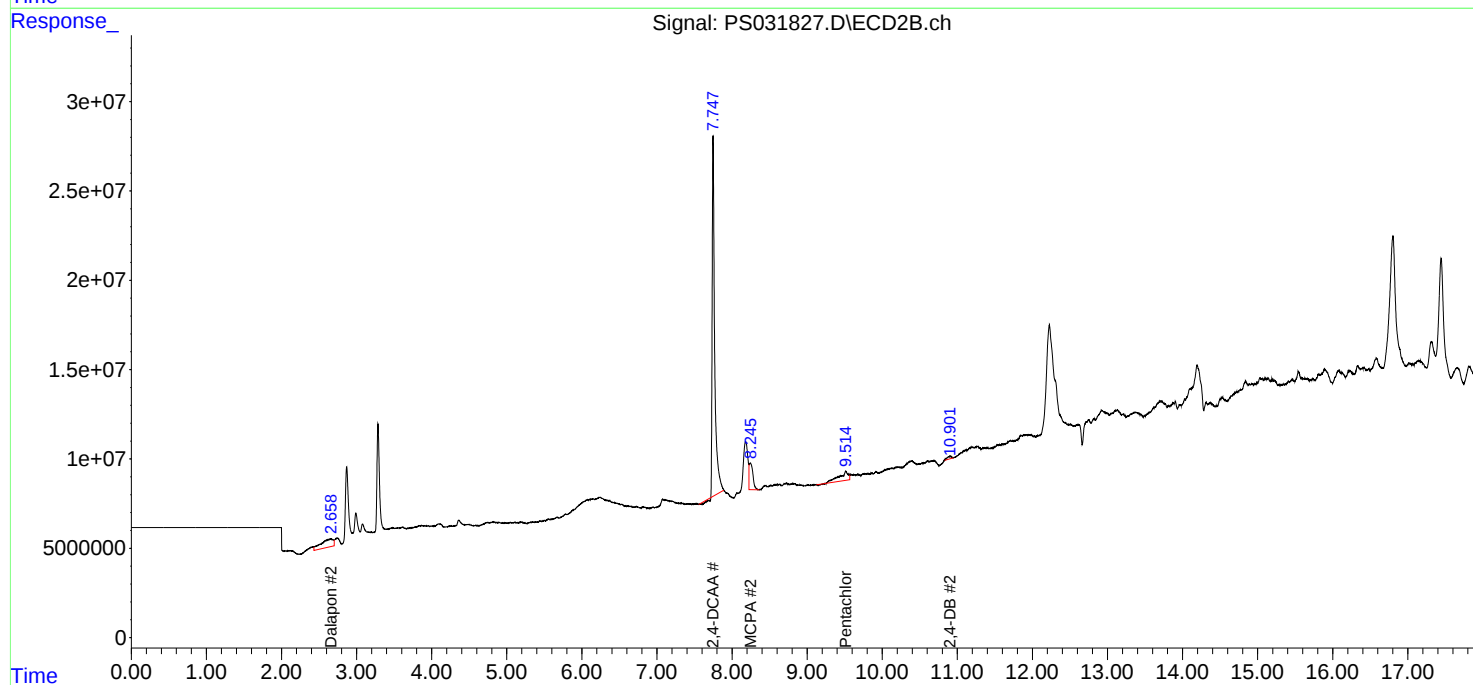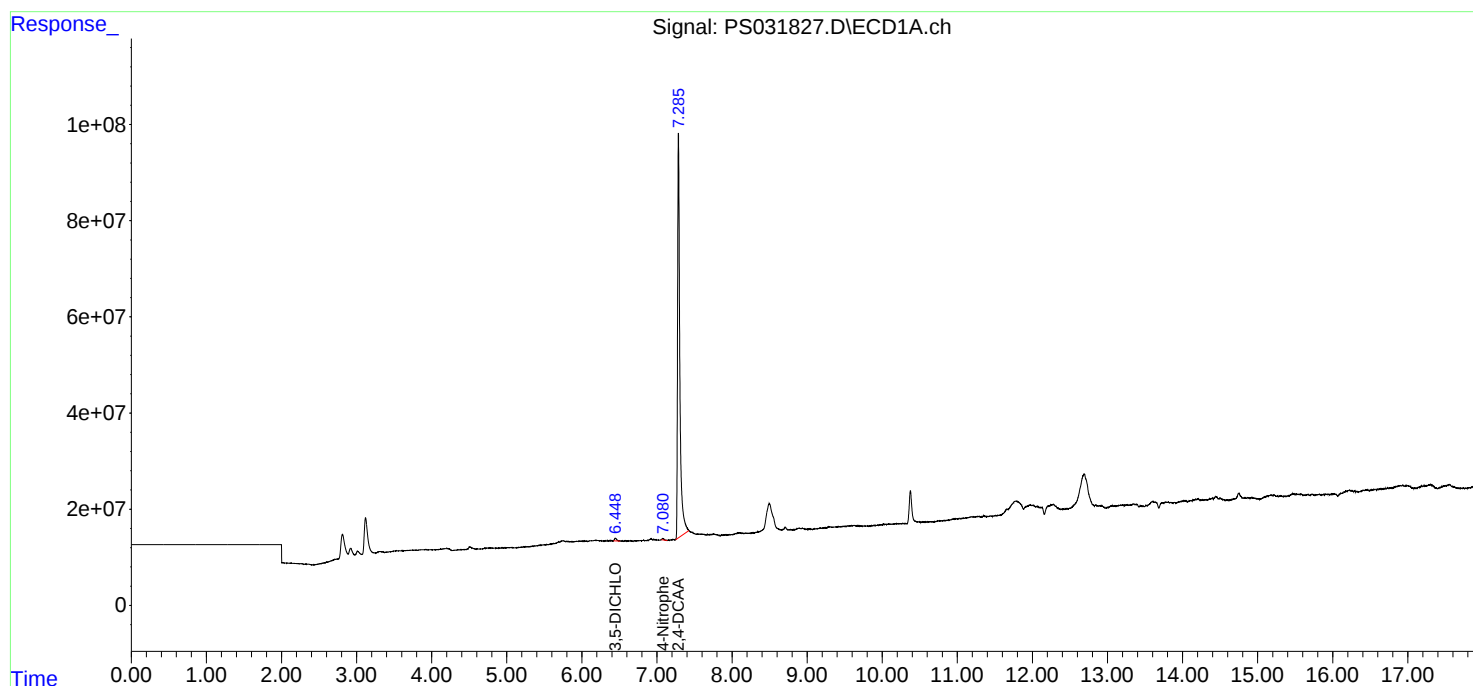


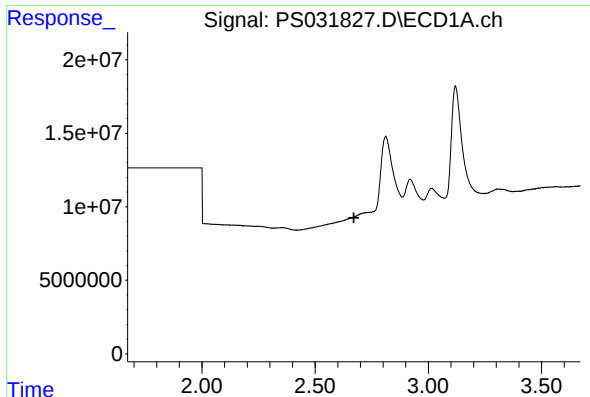

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

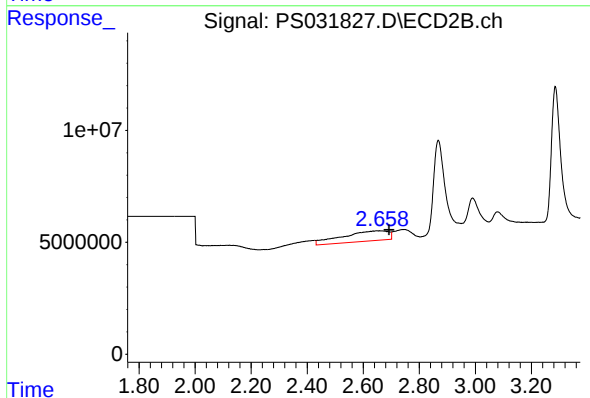


#1 Dalapon

R.T.: 2.659 min
Delta R.T.: -0.033 min
Response: 52231744
Conc: 18.54 ng/ml

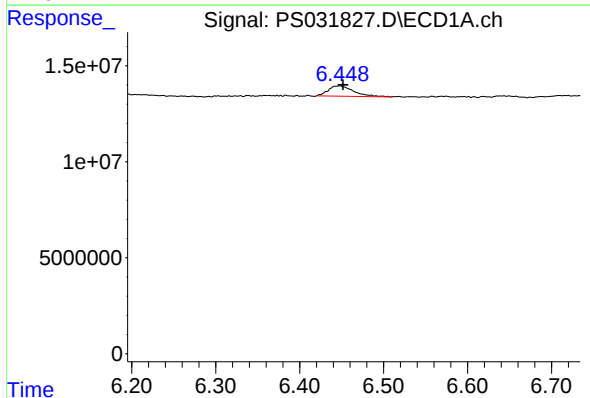


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.448 min
Delta R.T.: -0.004 min
Response: 11440607
Conc: 2.15 ng/ml

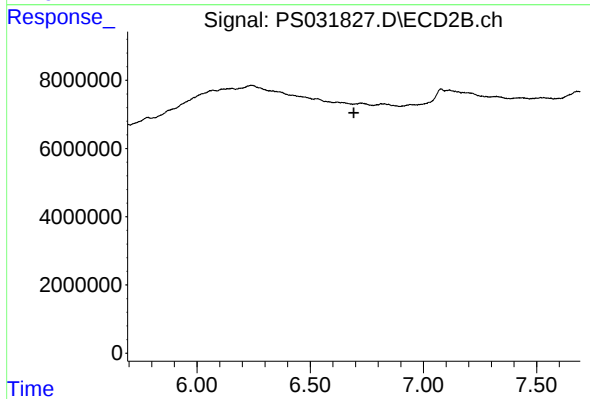

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.693 min
Response: 0
Conc: N.D.

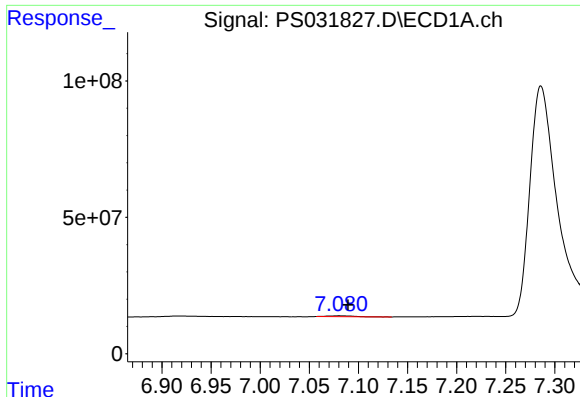

#3 4-Nitrophenol


R.T.: 7.081 min
Delta R.T.: -0.009 min
Response: 5746545
Conc: 5.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

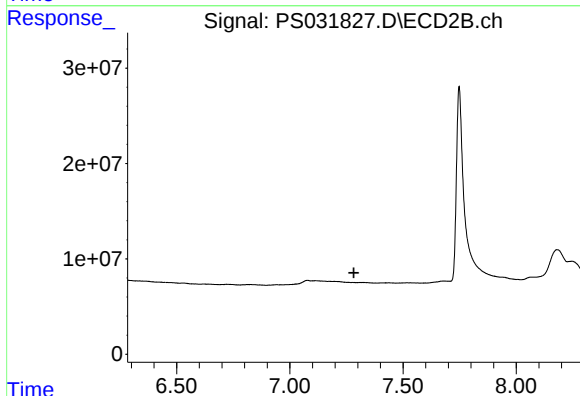


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

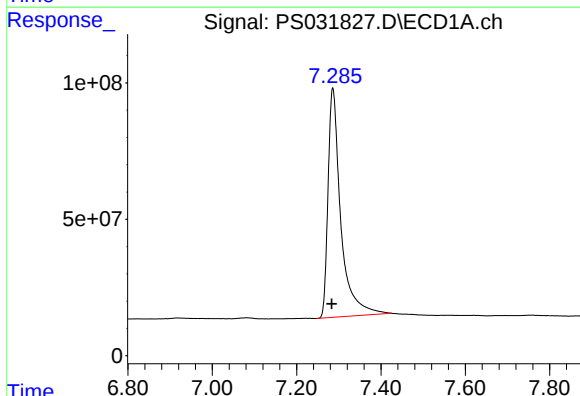


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.003 min
Response: 1762532618
Conc: 489.38 ng/ml

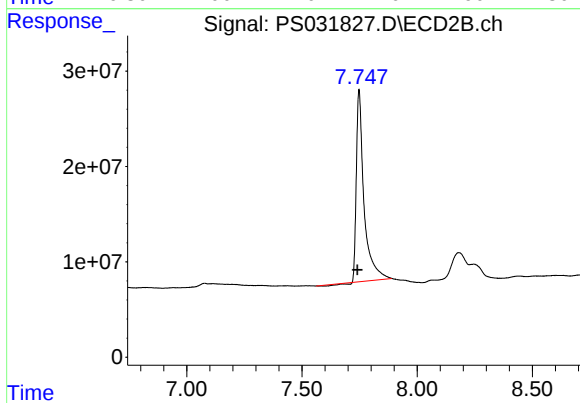

#4 2,4-DCAA


R.T.: 7.748 min
Delta R.T.: 0.007 min
Response: 462427814
Conc: 508.78 ng/ml

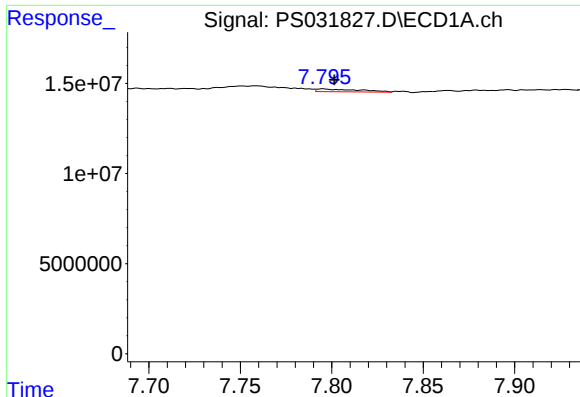

#7 MCPA


R.T.: 7.795 min
Delta R.T.: -0.006 min
Response: 2556232
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

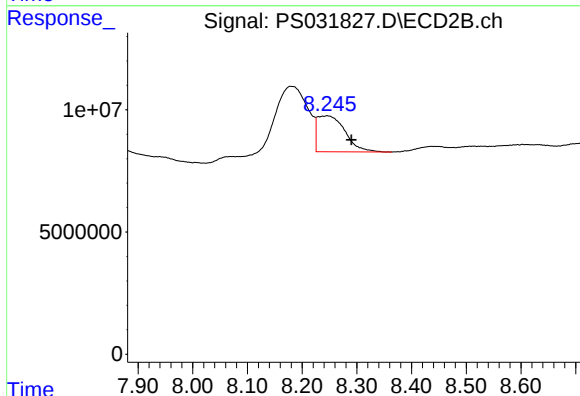


#7 MCPA

R.T.: 8.246 min
Delta R.T.: -0.044 min
Response: 51405820
Conc: 18.35 ug/ml

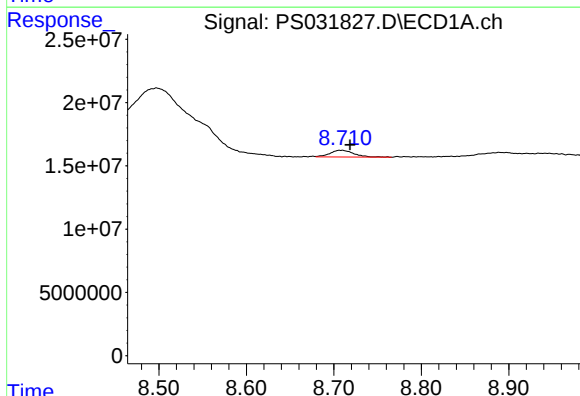


#10 Pentachlorophenol

R.T.: 8.708 min
Delta R.T.: -0.010 min
Response: 10136943
Conc: N.D.

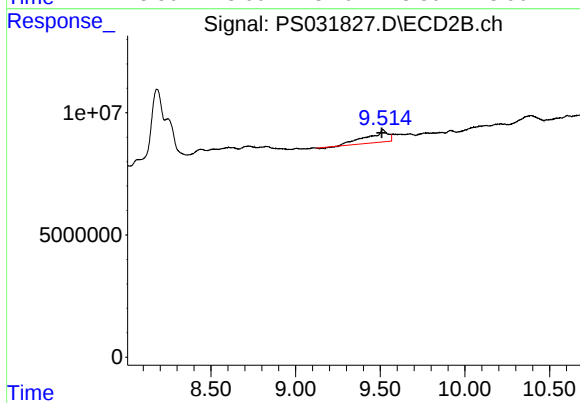

#10 Pentachlorophenol


R.T.: 9.515 min
Delta R.T.: 0.005 min
Response: 42400407
Conc: 1.07 ng/ml

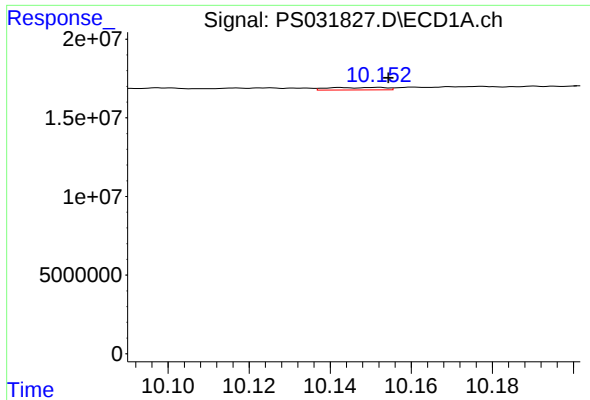

#13 2,4-DB

R.T.: 10.143 min
Delta R.T.: -0.012 min
Response: 1541979
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

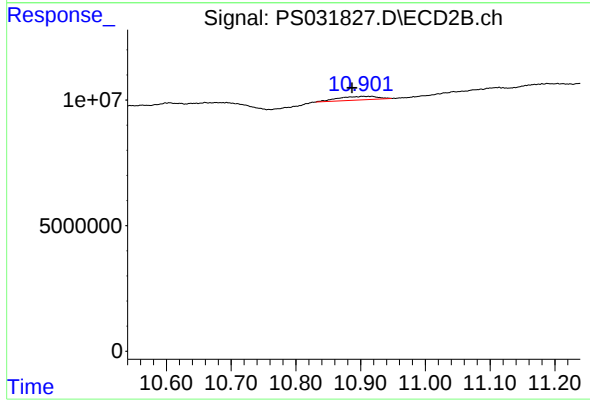

#13 2,4-DB

R.T.: 10.904 min
Delta R.T.: 0.017 min
Response: 5967482
Conc: 5.58 ng/ml