

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092425\
 Data File : PS031836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2025 20:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:58:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.283	7.744	1836.9E6	510.1E6	510.021	561.222
Target Compounds							
1) T	Dalapon	0.000	2.660f	0	71679313	N.D.	25.440
2) T	3,5-DICHL...	6.443	0.000	19215588	0	3.603	N.D. #
3) T	4-Nitroph...	7.070	0.000	5204573	0	4.718	N.D. #
5) T	DICAMBA	7.466	0.000	876639	0	<MDL	N.D. #
7) T	MCPA	7.819	8.243f	627460	52335435	<MDL	18.683 #
10) T	Pentachlo...	8.706	9.510	8254105	37892893	<MDL	<MDL #
11) T	2,4,5-TP ...	9.282	9.903	5679249	2609579	<MDL	<MDL #
12) T	2,4,5-T	9.566	0.000	434725	0	<MDL	N.D. #
13) T	2,4-DB	10.159	0.000	568429	0	<MDL	N.D. #
15) T	Picloram	11.165	0.000	9025269	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092425\
Data File : PS031836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2025 20:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:58:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

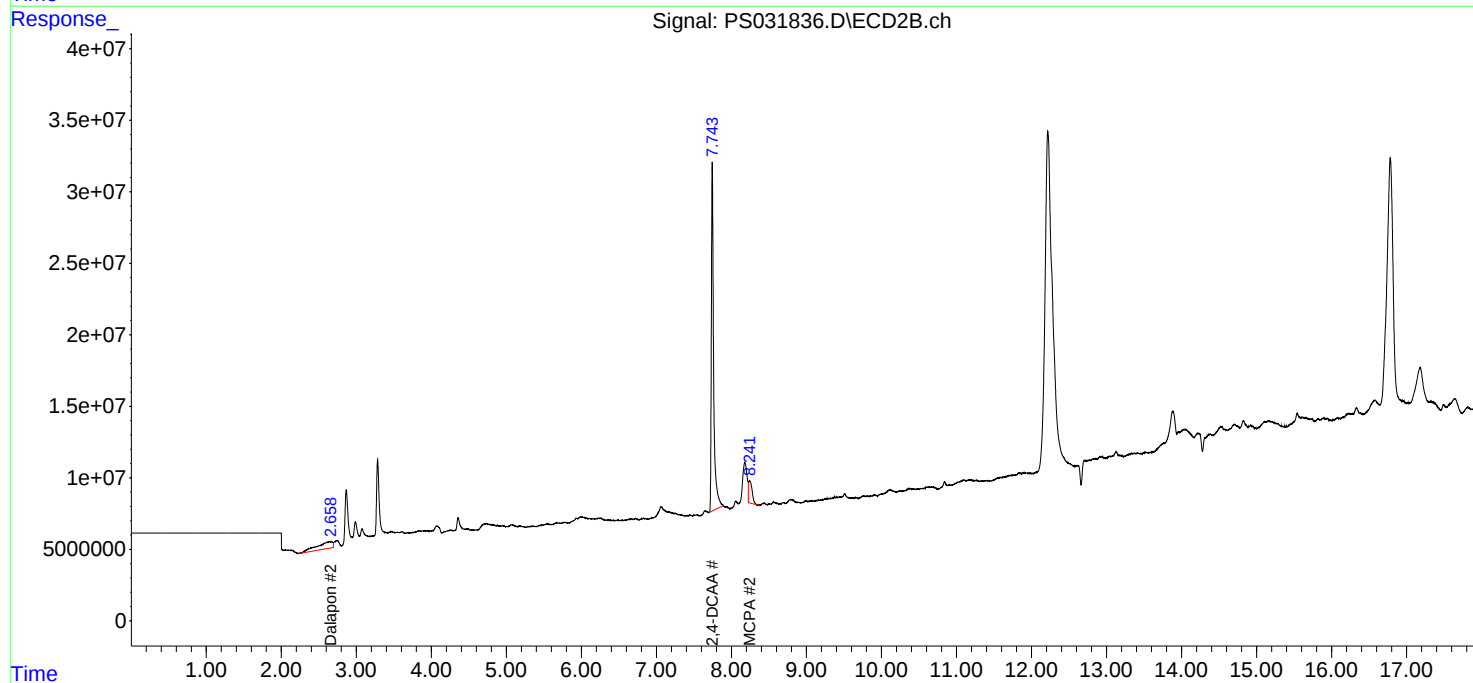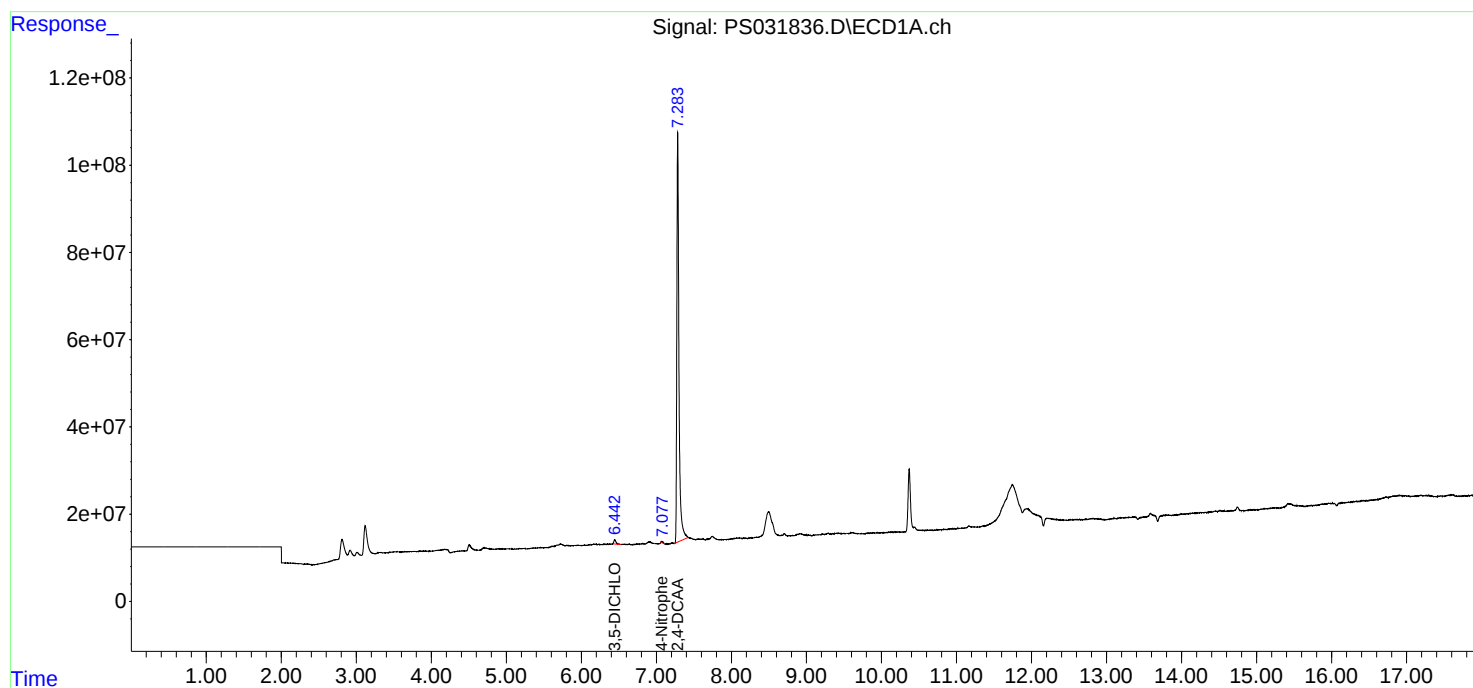


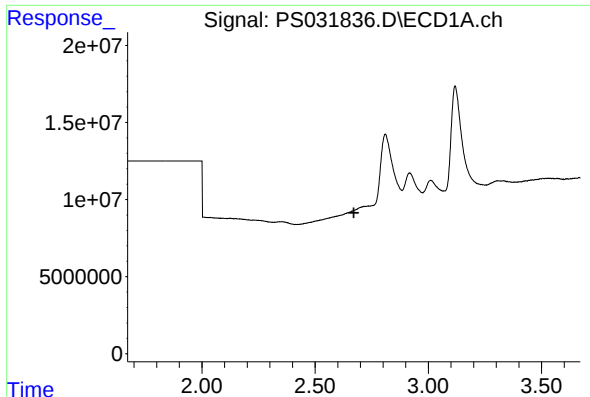

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

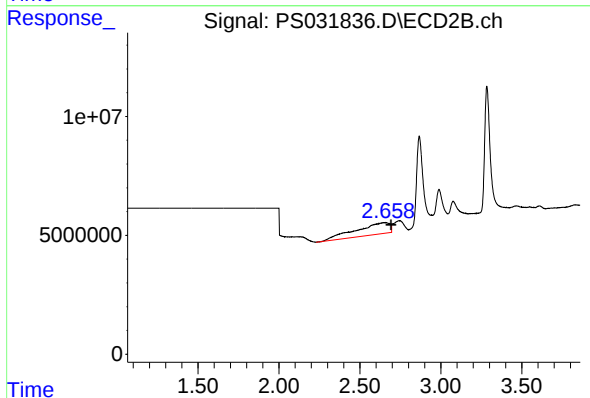


#1 Dalapon

R.T.: 2.660 min
Delta R.T.: -0.032 min
Response: 71679313
Conc: 25.44 ng/ml

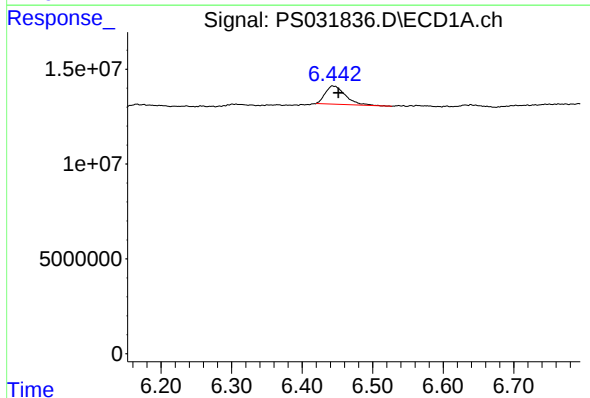


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.443 min
Delta R.T.: -0.008 min
Response: 19215588
Conc: 3.60 ng/ml

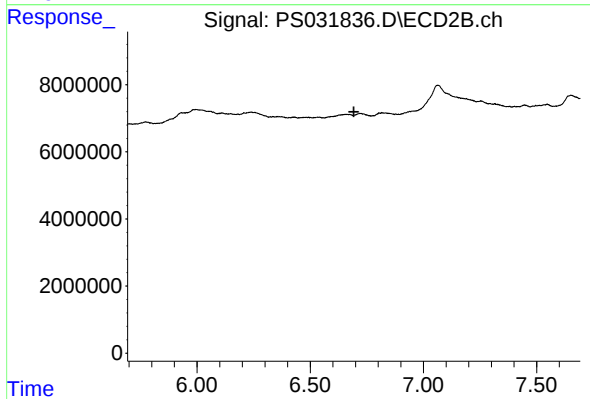

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.693 min
Response: 0
Conc: N.D.

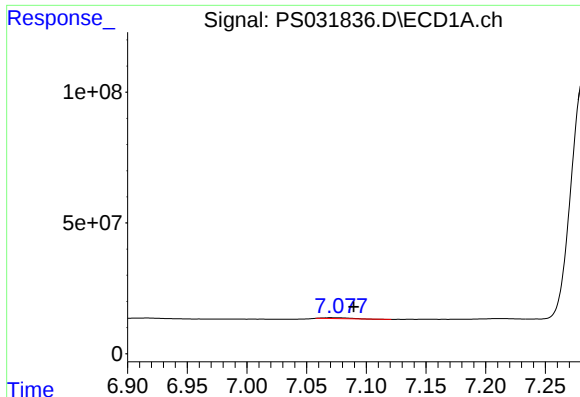

#3 4-Nitrophenol


R.T.: 7.070 min
Delta R.T.: -0.019 min
Response: 5204573
Conc: 4.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

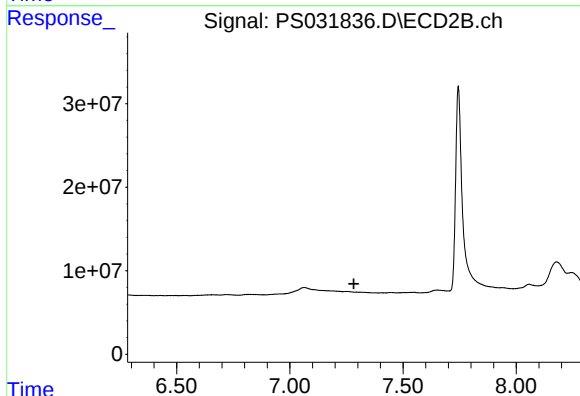


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

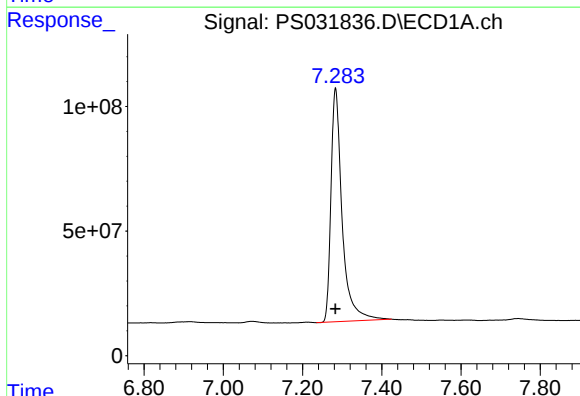


#4 2,4-DCAA

R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 1836854650
Conc: 510.02 ng/ml

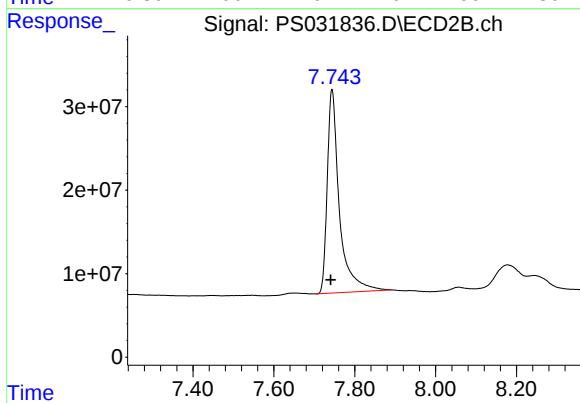

#4 2,4-DCAA


R.T.: 7.744 min
Delta R.T.: 0.003 min
Response: 510094481
Conc: 561.22 ng/ml

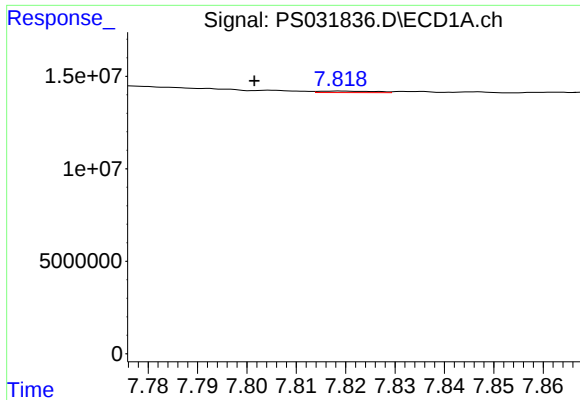

#7 MCPA

R.T.: 7.819 min
Delta R.T.: 0.017 min
Response: 627460
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

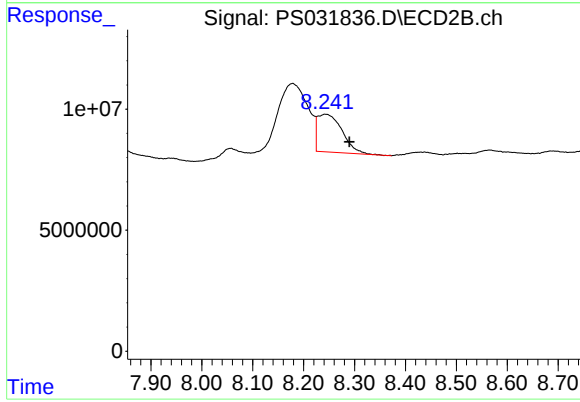

#7 MCPA

R.T.: 8.243 min
Delta R.T.: -0.047 min
Response: 52335435
Conc: 18.68 ug/ml