

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092519\
 Data File : PS006904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2019 16:37
 Operator : SM\AJ
 Sample : K5008-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SB-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:51:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.482	5.210	445.1E6	215.9E6	487.037	469.415
Target Compounds							
1) T	Dalapon	2.116	0.000	67840194	0	63.497	N.D. #
2) T	3,5-DICHL...	4.920	4.539	13663177	47179408	12.561	82.071 #
3) T	4-Nitroph...	5.336	0.000	18146655	0	47.592	N.D. #
5) T	DICAMBA	5.641	5.335	21207993	13959675	6.564	8.293 #
6) T	MCPD	5.779	0.000	14292623	0	6.718	N.D. #
7) T	MCPA	5.959	5.609	19762928	12019301	6.352	6.530
9) T	2,4-D	6.550	6.132	86801896	9356059	105.919	18.343 #
10) T	Pentachlo...	6.741	6.518	22890015	15775233	1.921	2.507 #
11) T	2,4,5-TP ...	7.341	0.000	11953866	0	2.631	N.D. #
12) T	2,4,5-T	0.000	7.285	0	43867947	N.D.	20.296
13) T	2,4-DB	8.090	0.000	56549667	0	97.497	N.D. #
15) T	Picloram	9.020	8.981	136.0E6	89105124	20.284	24.482
16) T	DCPA	0.000	8.981	0	89105124	N.D.	28.043



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092519\
Data File : PS006904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2019 16:37
Operator : SM\AJ
Sample : K5008-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
SB-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:51:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

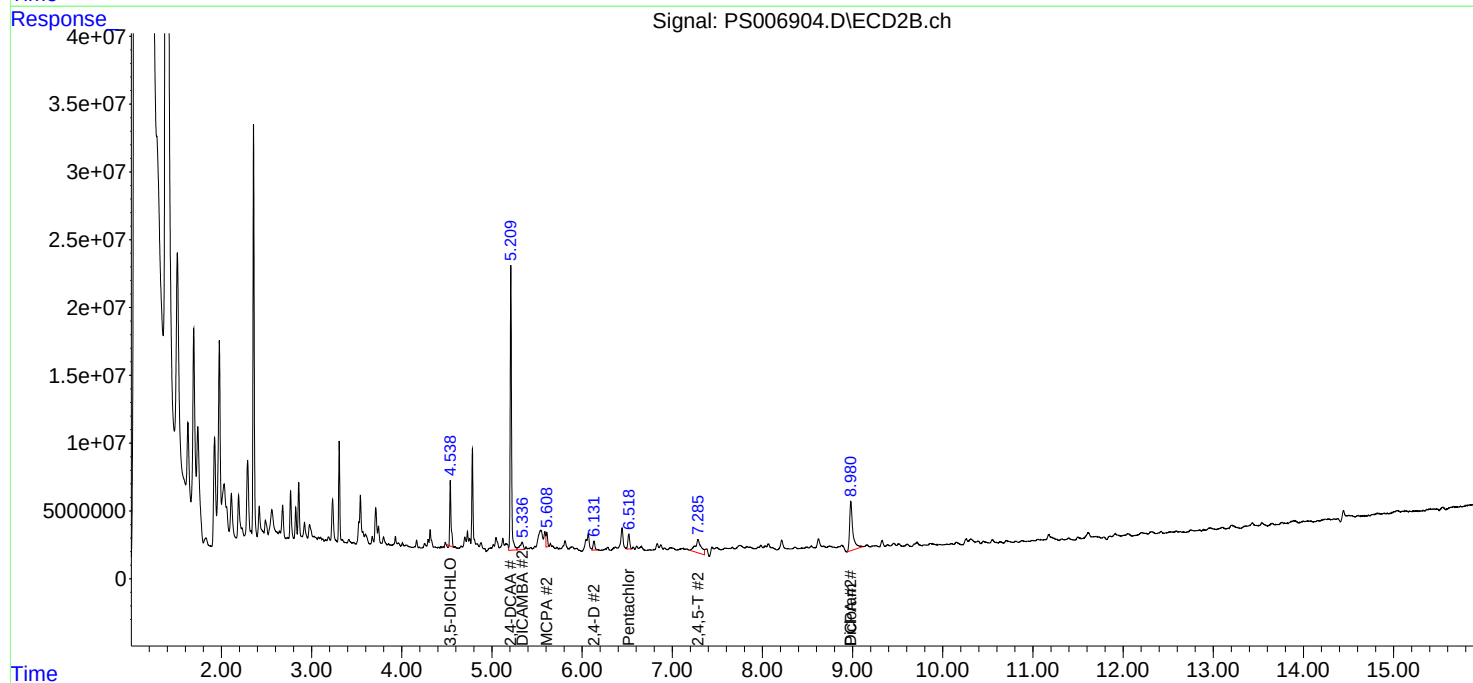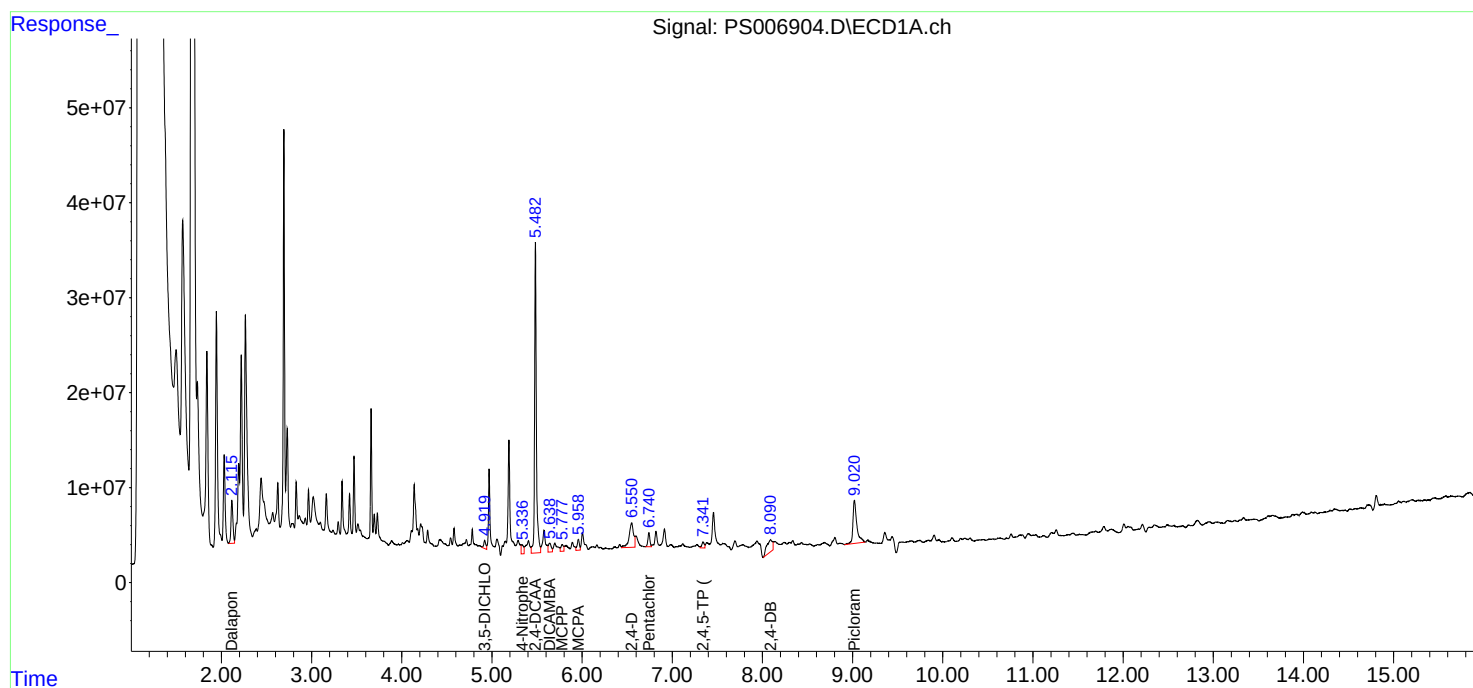


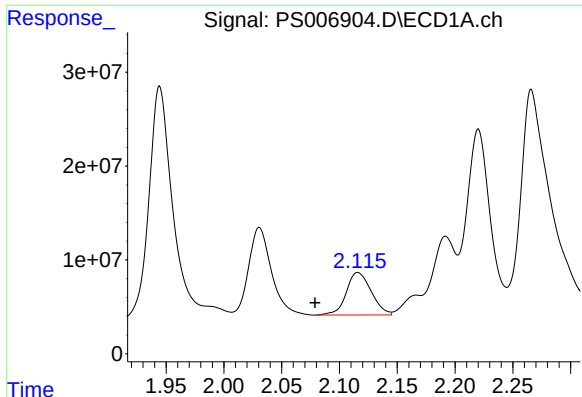

#1 Dalapon


R.T.: 2.116 min
Delta R.T.: 0.037 min
Response: 67840194
Conc: 63.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-6

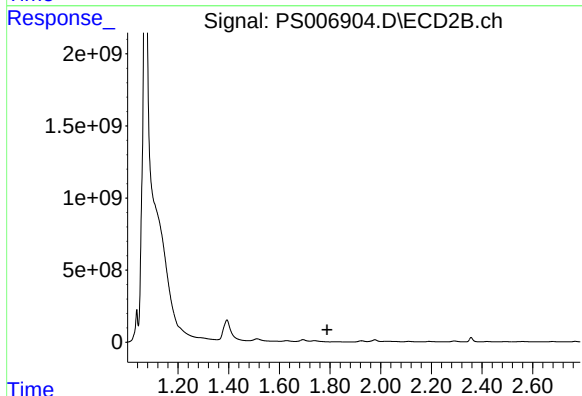


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

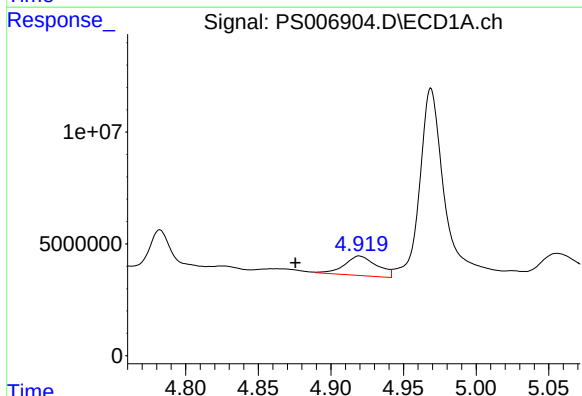


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.920 min
Delta R.T.: 0.044 min
Response: 13663177
Conc: 12.56 ng/ml

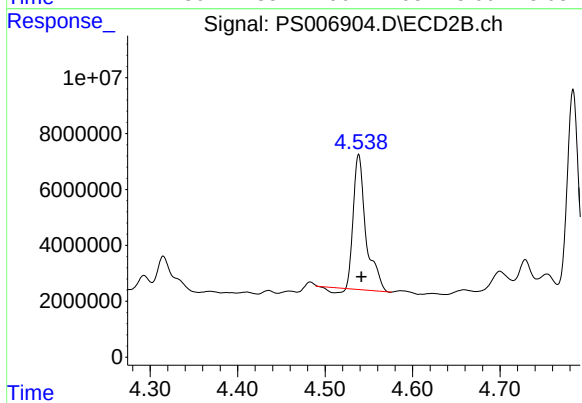

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.539 min
Delta R.T.: -0.003 min
Response: 47179408
Conc: 82.07 ng/ml

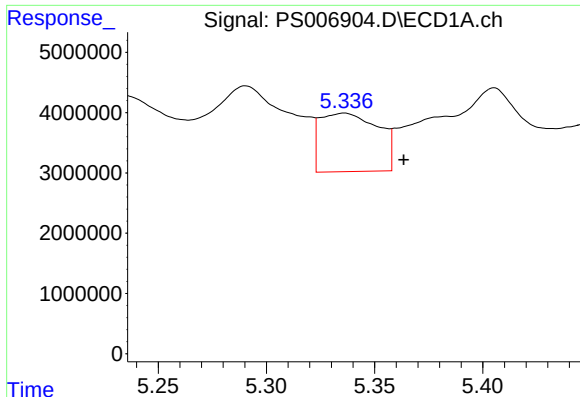

#3 4-Nitrophenol


R.T.: 5.336 min
Delta R.T.: -0.028 min
Response: 18146655
Conc: 47.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-6

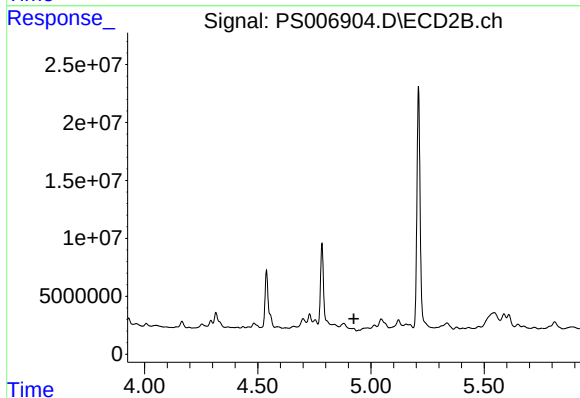


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.925 min
Response: 0
Conc: N.D.

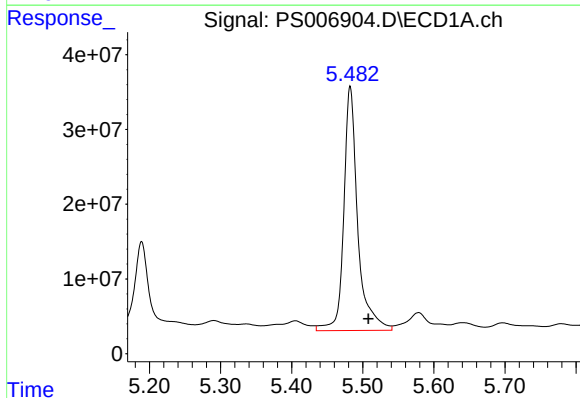


#4 2,4-DCAA

R.T.: 5.482 min
Delta R.T.: -0.025 min
Response: 445061103
Conc: 487.04 ng/ml

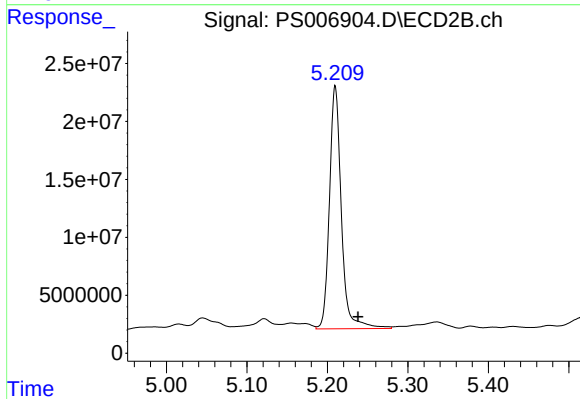

#4 2,4-DCAA


R.T.: 5.210 min
Delta R.T.: -0.028 min
Response: 215856555
Conc: 469.42 ng/ml

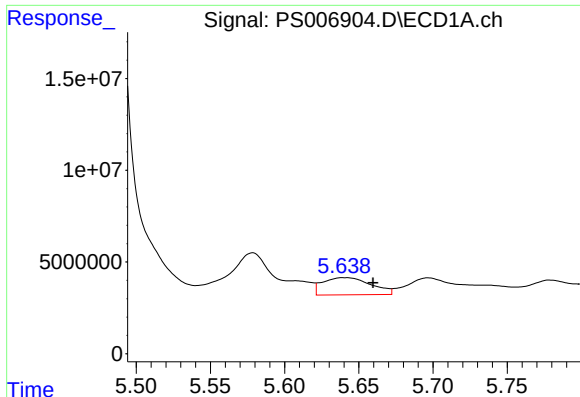

#5 DICAMBA


R.T.: 5.641 min
Delta R.T.: -0.019 min
Response: 21207993
Conc: 6.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-6

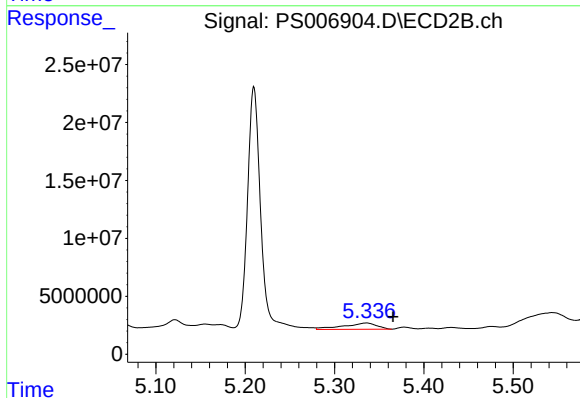


#5 DICAMBA

R.T.: 5.335 min
Delta R.T.: -0.030 min
Response: 13959675
Conc: 8.29 ng/ml

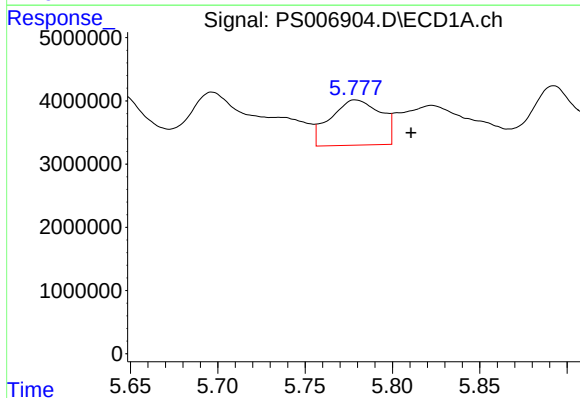


#6 MCP

R.T.: 5.779 min
Delta R.T.: -0.031 min
Response: 14292623
Conc: 6.72 ug/ml

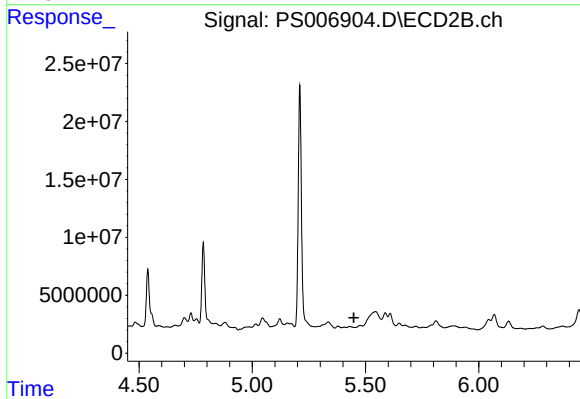

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.449 min
Response: 0
Conc: N.D.

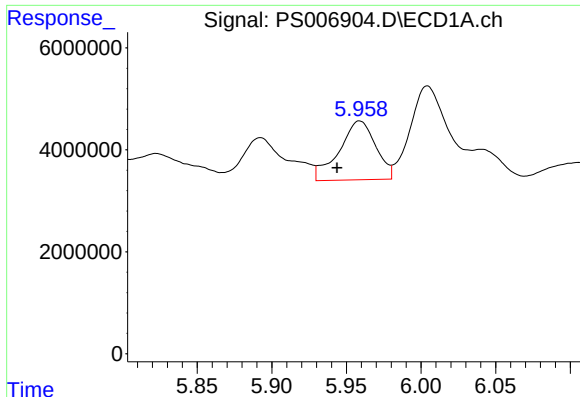

#7 MCPA


R.T.: 5.959 min
Delta R.T.: 0.015 min
Response: 19762928
Conc: 6.35 ug/ml

Instrument :
ECD_S
ClientSampleId :
SB-6

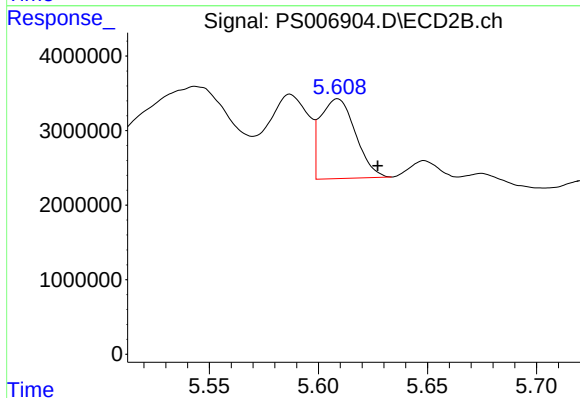


#7 MCPA

R.T.: 5.609 min
Delta R.T.: -0.019 min
Response: 12019301
Conc: 6.53 ug/ml

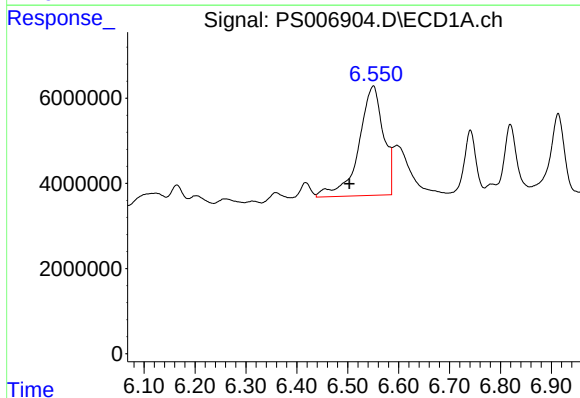


#9 2,4-D

R.T.: 6.550 min
Delta R.T.: 0.046 min
Response: 86801896
Conc: 105.92 ng/ml

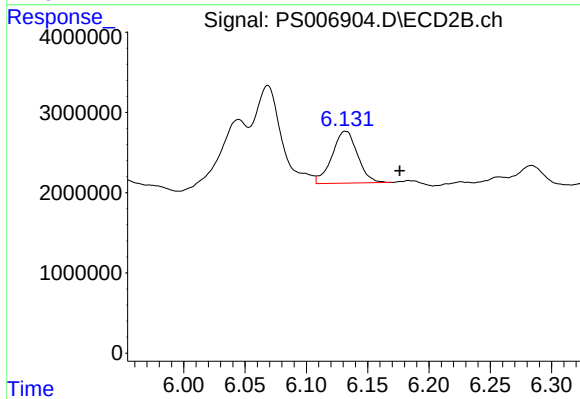

#9 2,4-D


R.T.: 6.132 min
Delta R.T.: -0.044 min
Response: 9356059
Conc: 18.34 ng/ml

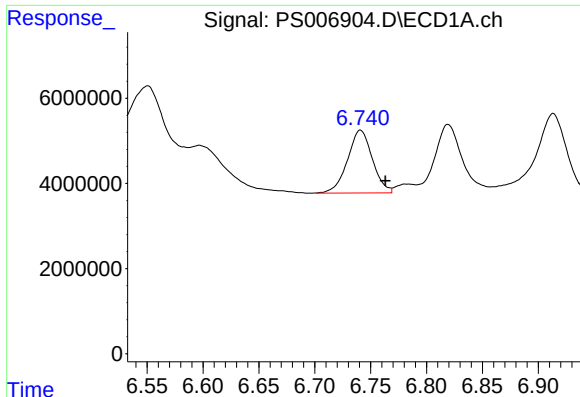

#10 Pentachlorophenol


R.T.: 6.741 min
Delta R.T.: -0.022 min
Response: 22890015
Conc: 1.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-6

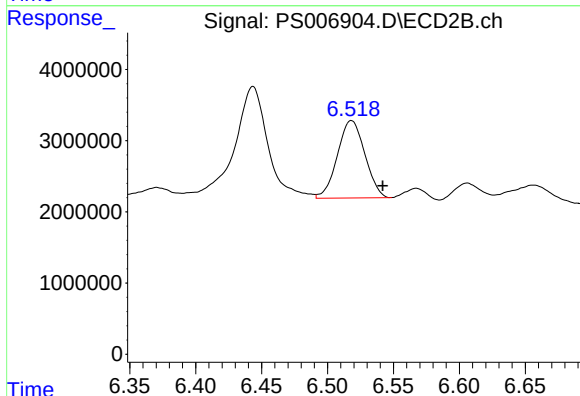


#10 Pentachlorophenol

R.T.: 6.518 min
Delta R.T.: -0.024 min
Response: 15775233
Conc: 2.51 ng/ml

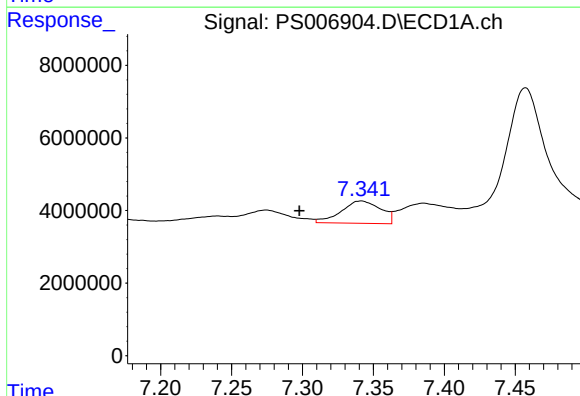


#11 2,4,5-TP (SILVEX)

R.T.: 7.341 min
Delta R.T.: 0.043 min
Response: 11953866
Conc: 2.63 ng/ml

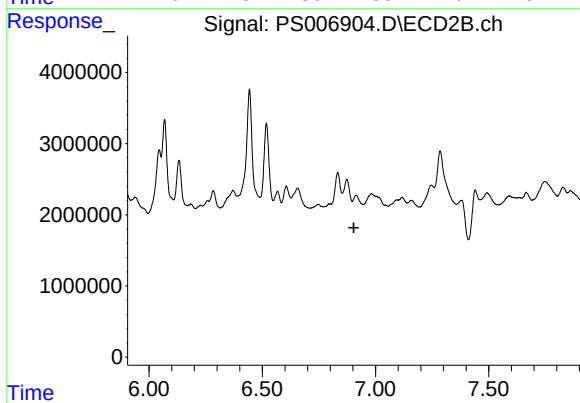

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 6.905 min
Response: 0
Conc: N.D.

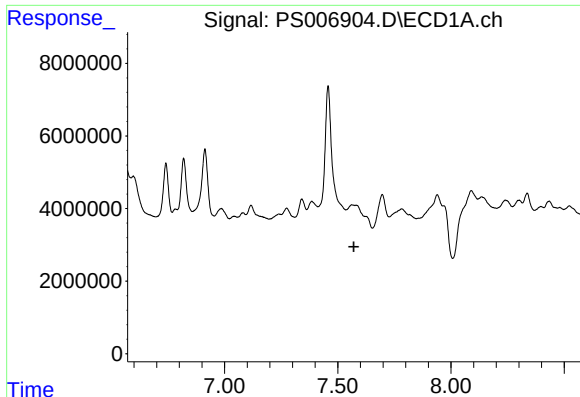

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SB-6

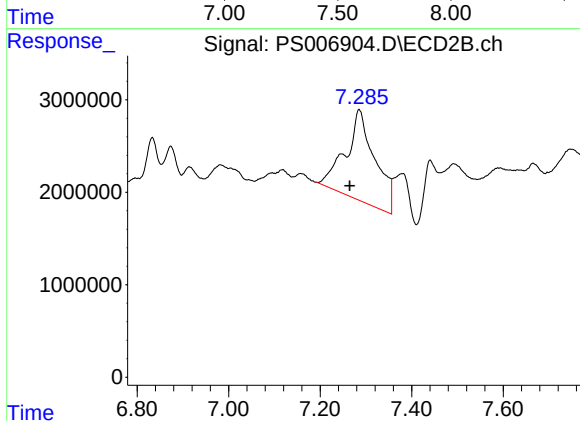


#12 2,4,5-T

R.T.: 7.285 min
Delta R.T.: 0.021 min
Response: 43867947
Conc: 20.30 ng/ml

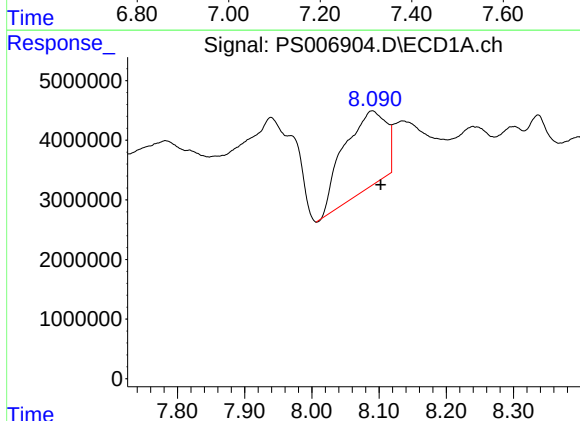


#13 2,4-DB

R.T.: 8.090 min
Delta R.T.: -0.012 min
Response: 56549667
Conc: 97.50 ng/ml

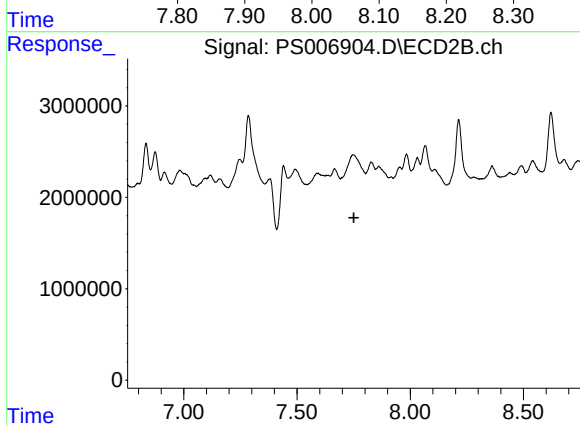

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.751 min
Response: 0
Conc: N.D.

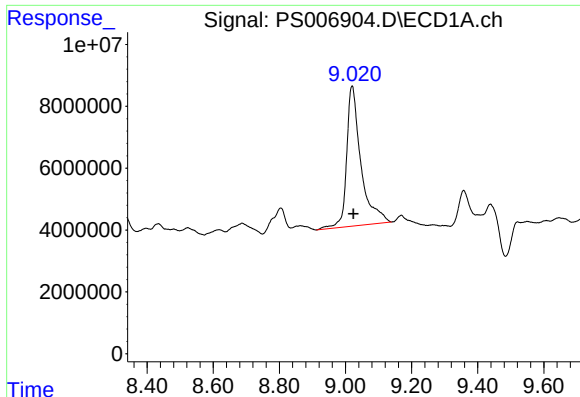

#15 Picloram


R.T.: 9.020 min
Delta R.T.: -0.005 min
Response: 136017992
Conc: 20.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-6

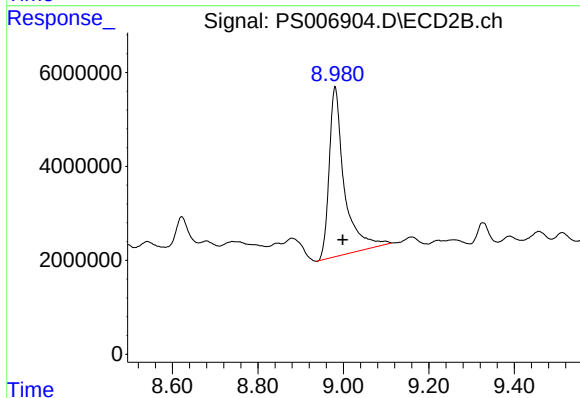


#15 Picloram

R.T.: 8.981 min
Delta R.T.: -0.018 min
Response: 89105124
Conc: 24.48 ng/ml

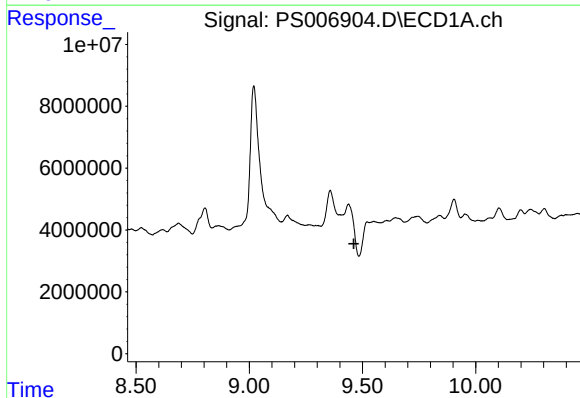

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.462 min
Response: 0
Conc: N.D.

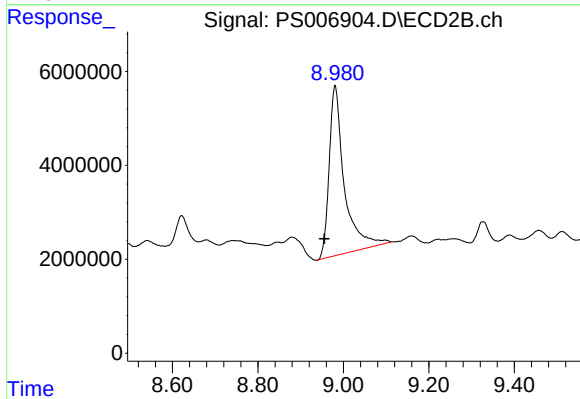

#16 DCPA

R.T.: 8.981 min
Delta R.T.: 0.025 min
Response: 89105124
Conc: 28.04 ng/ml