

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092523\
 Data File : PS024382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2023 12:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 13:33:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.363	6.784	1006.4E6	326.4E6	505.132	486.065
Target Compounds							
1) T	Dalapon	2.516	2.567	4533629	2567901	2.086	2.435
3) T	4-Nitroph...	6.204	0.000	7796992	0	6.276	N.D. #
5) T	DICAMBA	6.492	6.966	503687	4671347	<MDL	1.622 #
6) T	MCP	6.686	7.010f	950136	375622	<MDL	<MDL #
7) T	MCPA	6.848f	0.000	571346	0	<MDL	N.D. #
8) T	DICHLORPROP	7.154f	7.576	26382063	1305978	11.605	1.797 #
9) T	2,4-D	0.000	7.788f	0	978163	N.D.	1.098
11) T	2,4,5-TP ...	8.047	8.625	1418479	720072	<MDL	<MDL #
12) T	2,4,5-T	8.312	9.041	141888	1068038	<MDL	<MDL #
13) T	2,4-DB	8.746f	0.000	847875	0	<MDL	N.D. #
14) T	DINOSEB	9.875	0.000	1889966	0	<MDL	N.D. #
15) T	Picloram	9.688	10.786	10574695	7425193	<MDL	1.250 #
16) T	DCPA	0.000	10.786	0	7425193	N.D.	1.447



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092523\
Data File : PS024382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2023 12:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 13:33:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

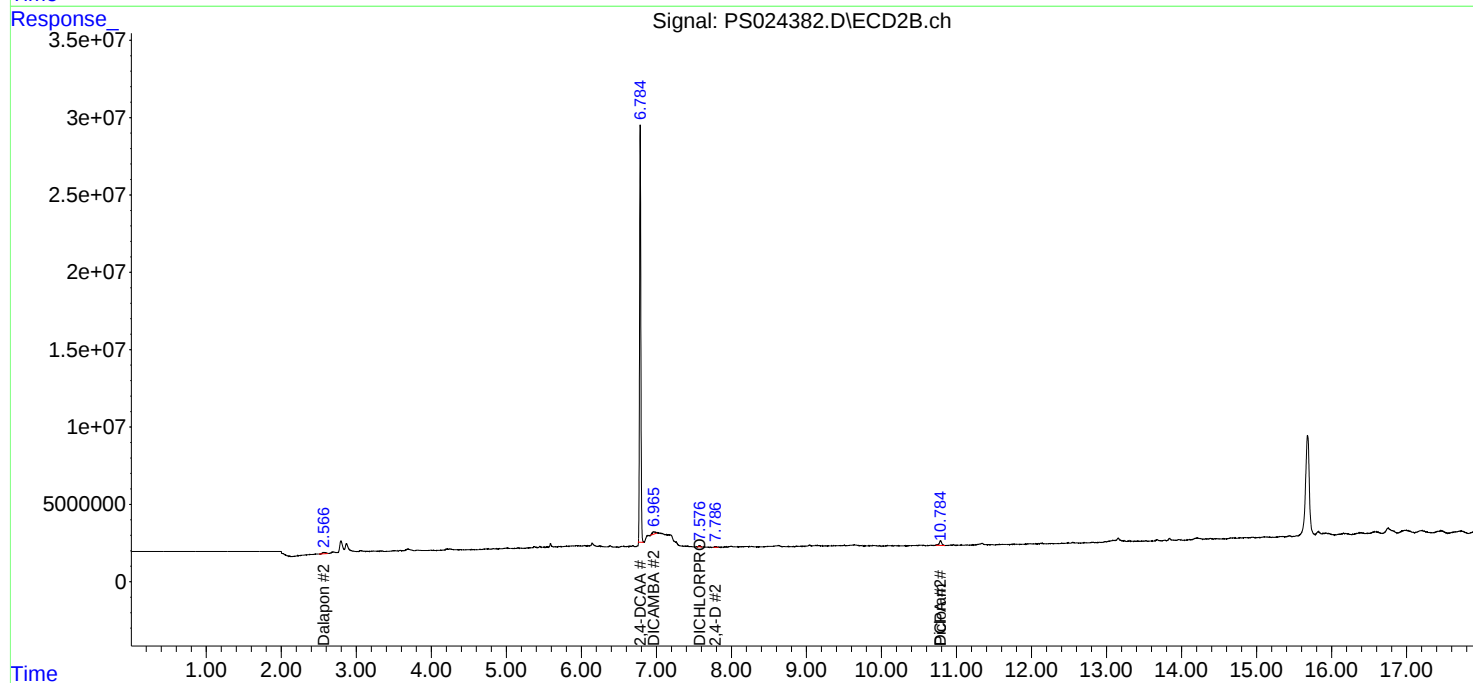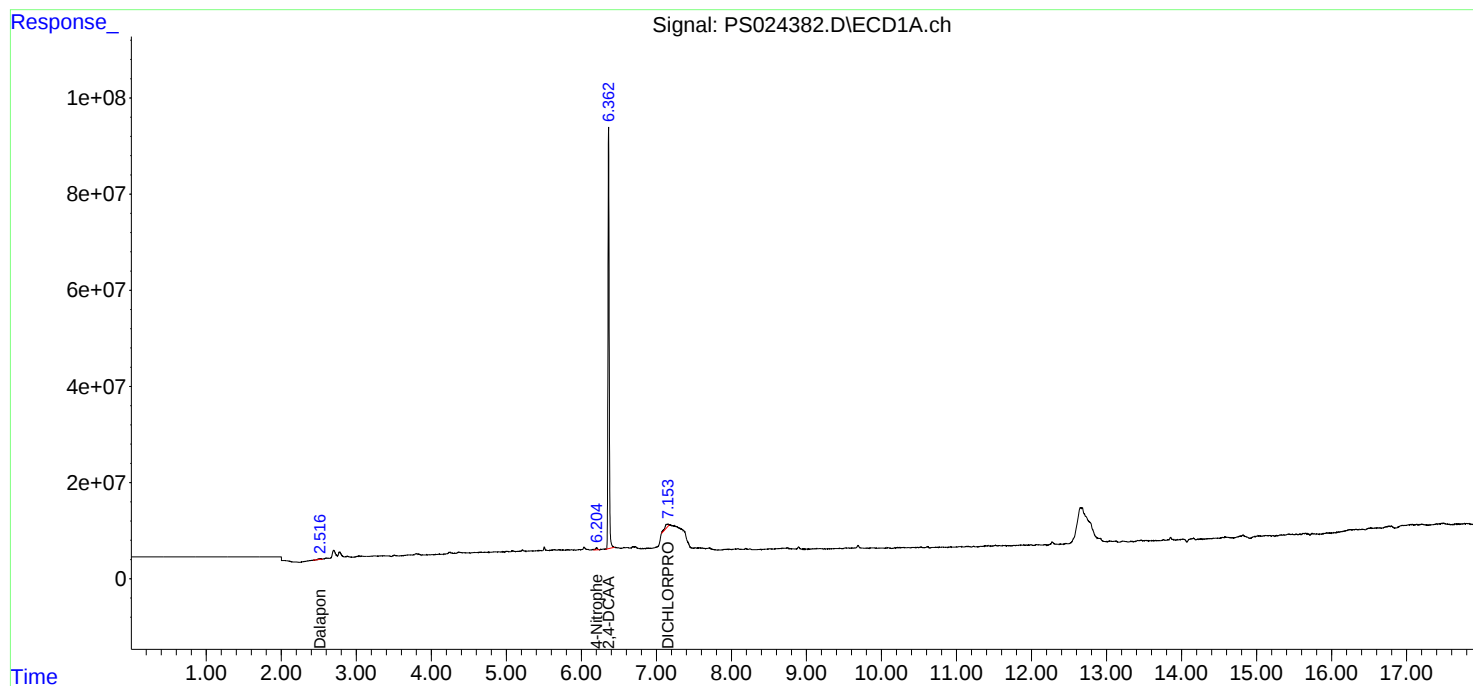


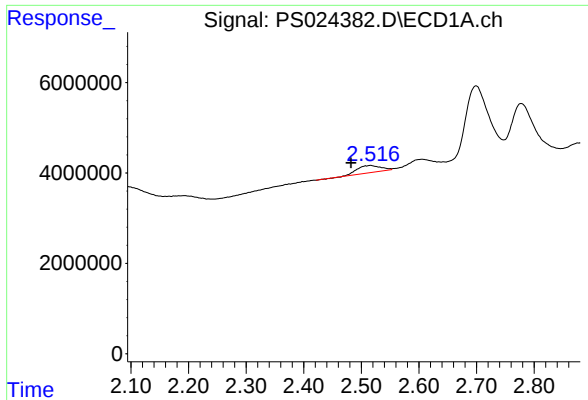

#1 Dalapon


R.T.: 2.516 min
Delta R.T.: 0.034 min
Response: 4533629
Conc: 2.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

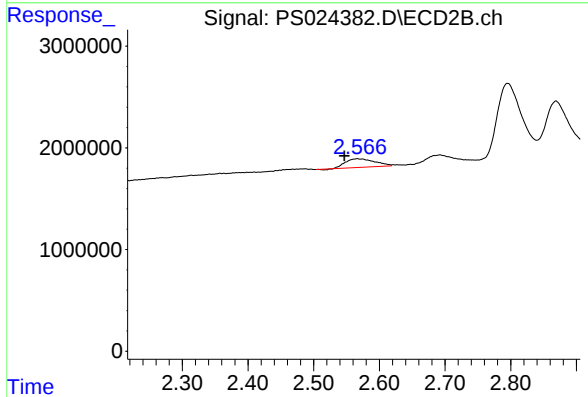


#1 Dalapon

R.T.: 2.567 min
Delta R.T.: 0.020 min
Response: 2567901
Conc: 2.44 ng/ml

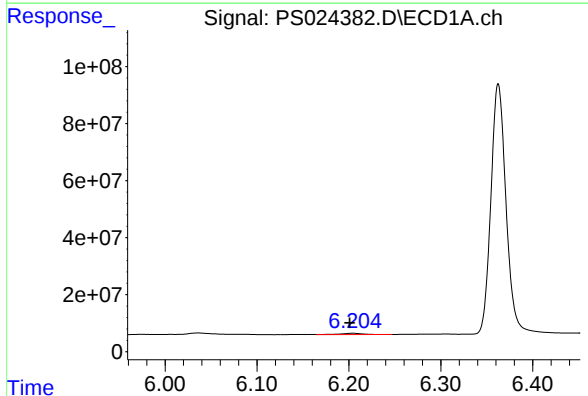


#3 4-Nitrophenol

R.T.: 6.204 min
Delta R.T.: 0.003 min
Response: 7796992
Conc: 6.28 ng/ml

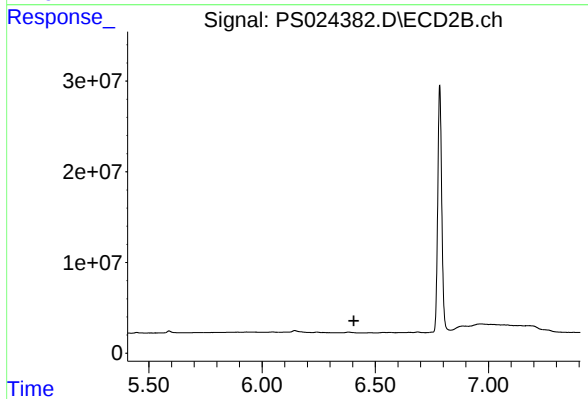

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.405 min
Response: 0
Conc: N.D.

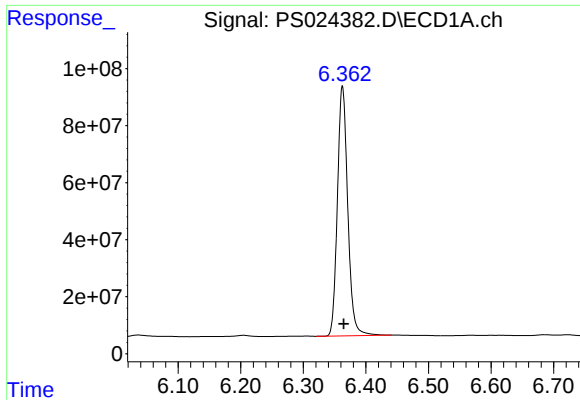

#4 2,4-DCAA


R.T.: 6.363 min
Delta R.T.: -0.002 min
Response: 1006384596
Conc: 505.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

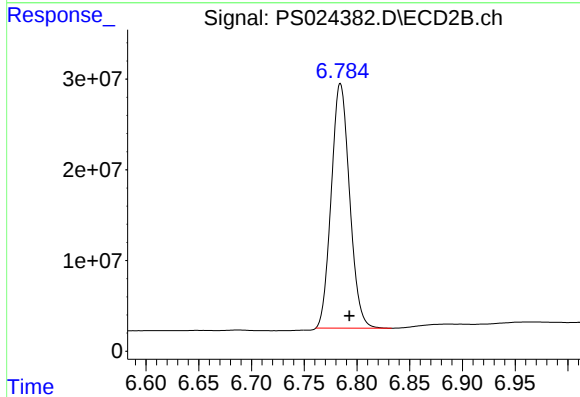


#4 2,4-DCAA

R.T.: 6.784 min
Delta R.T.: -0.009 min
Response: 326437178
Conc: 486.06 ng/ml

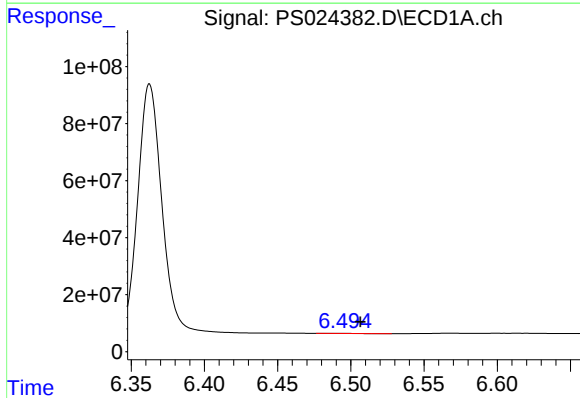


#5 DICAMBA

R.T.: 6.492 min
Delta R.T.: -0.014 min
Response: 503687
Conc: N.D.

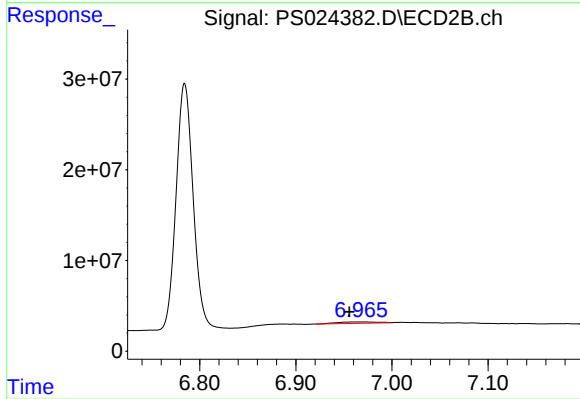

#5 DICAMBA


R.T.: 6.966 min
Delta R.T.: 0.010 min
Response: 4671347
Conc: 1.62 ng/ml

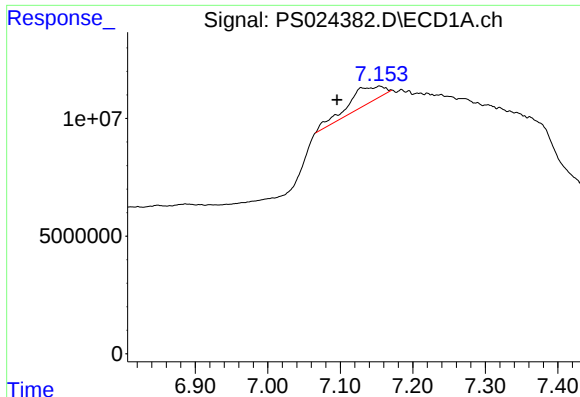

#8 DICHLORPROP


R.T.: 7.154 min
Delta R.T.: 0.059 min
Response: 26382063
Conc: 11.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

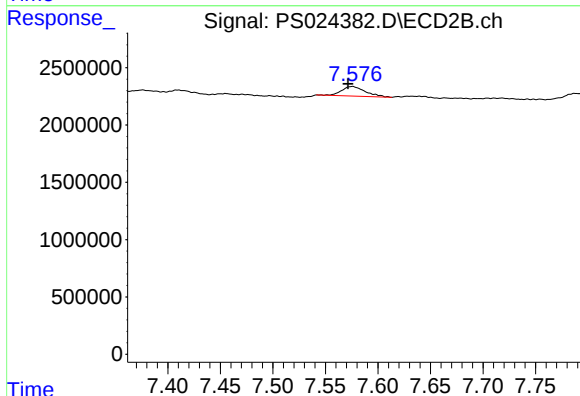


#8 DICHLORPROP

R.T.: 7.576 min
Delta R.T.: 0.004 min
Response: 1305978
Conc: 1.80 ng/ml

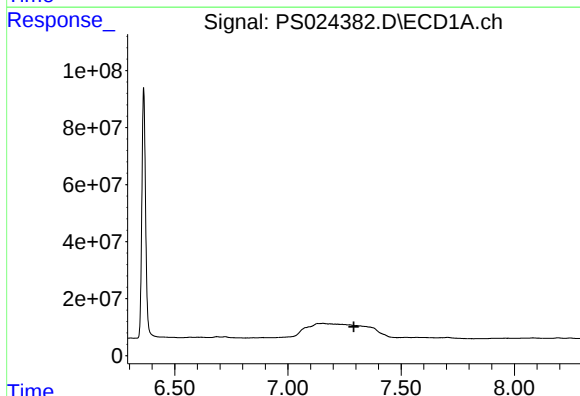


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.291 min
Response: 0
Conc: N.D.

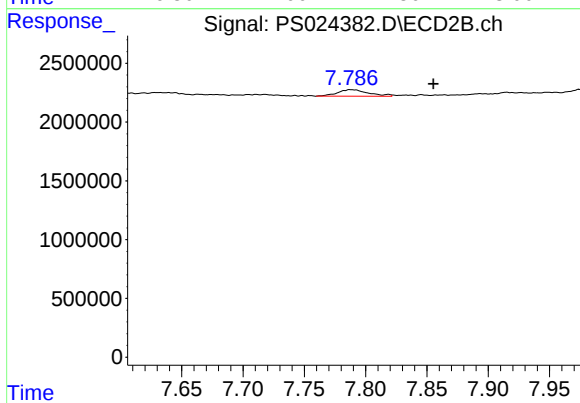

#9 2,4-D


R.T.: 7.788 min
Delta R.T.: -0.067 min
Response: 978163
Conc: 1.10 ng/ml

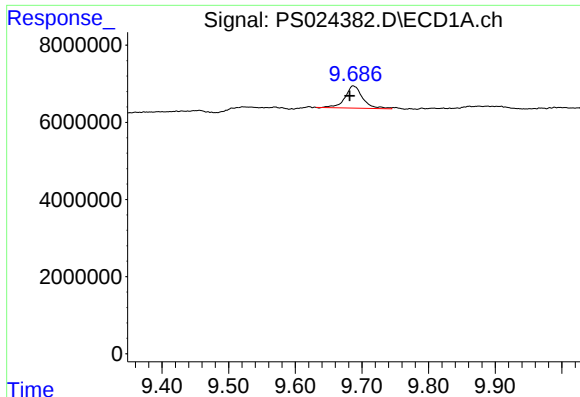

#15 Picloram


R.T.: 9.688 min
Delta R.T.: 0.006 min
Response: 10574695
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

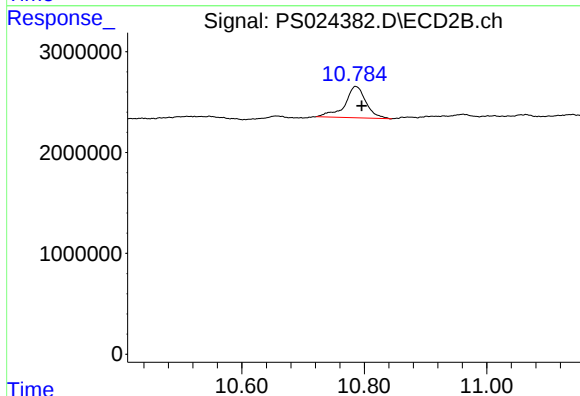


#15 Picloram

R.T.: 10.786 min
Delta R.T.: -0.010 min
Response: 7425193
Conc: 1.25 ng/ml

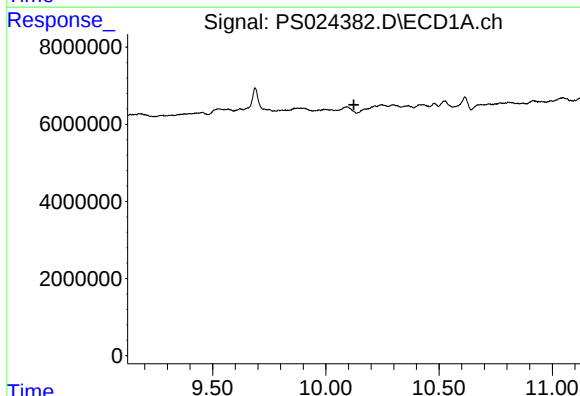

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.124 min
Response: 0
Conc: N.D.

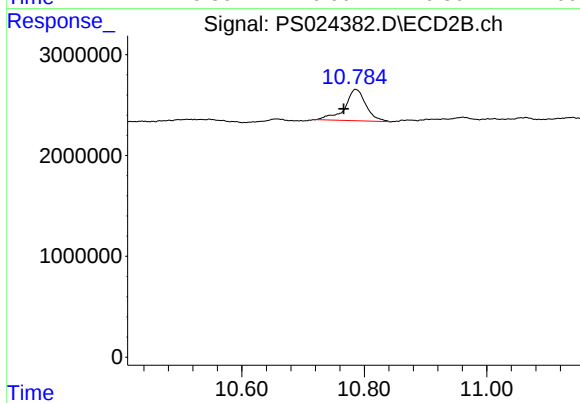

#16 DCPA

R.T.: 10.786 min
Delta R.T.: 0.020 min
Response: 7425193
Conc: 1.45 ng/ml