

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092524\
 Data File : PS027768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2024 13:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:08:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.106	7.627	1196.1E6	510.0E6	480.833	514.569
Target Compounds							
1) T	Dalapon	2.534	0.000	20141917	0	4.862	N.D. #
3) T	4-Nitroph...	6.905	0.000	30041940	0	17.743	N.D. #
6) T	MCP	0.000	7.920	0	3718147	N.D.	1.133
8) T	DICHLORPROP	0.000	8.518	0	532161	N.D.	<MDL
10) T	Pentachlo...	8.470	0.000	2743022	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.045	9.793f	34252015	1227386	2.340	<MDL #
12) T	2,4,5-T	9.360	10.148	2198805	3323330	<MDL	<MDL #
14) T	DINOSEB	11.066	0.000	1873487	0	<MDL	N.D. #
15) T	Picloram	10.911	12.180	12732773	2234826	<MDL	<MDL #
16) T	DCPA	11.352f	12.124	18157068	3835857	1.094	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092524\
Data File : PS027768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 13:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:08:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

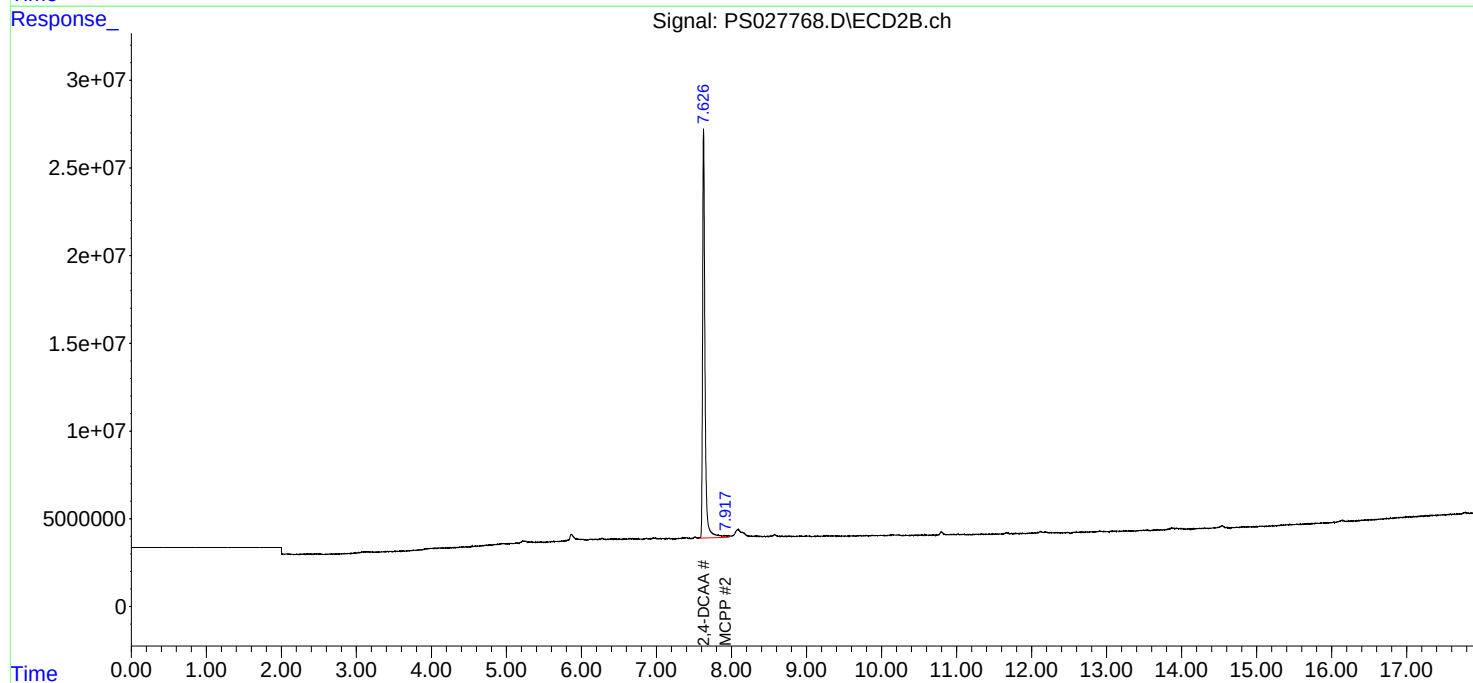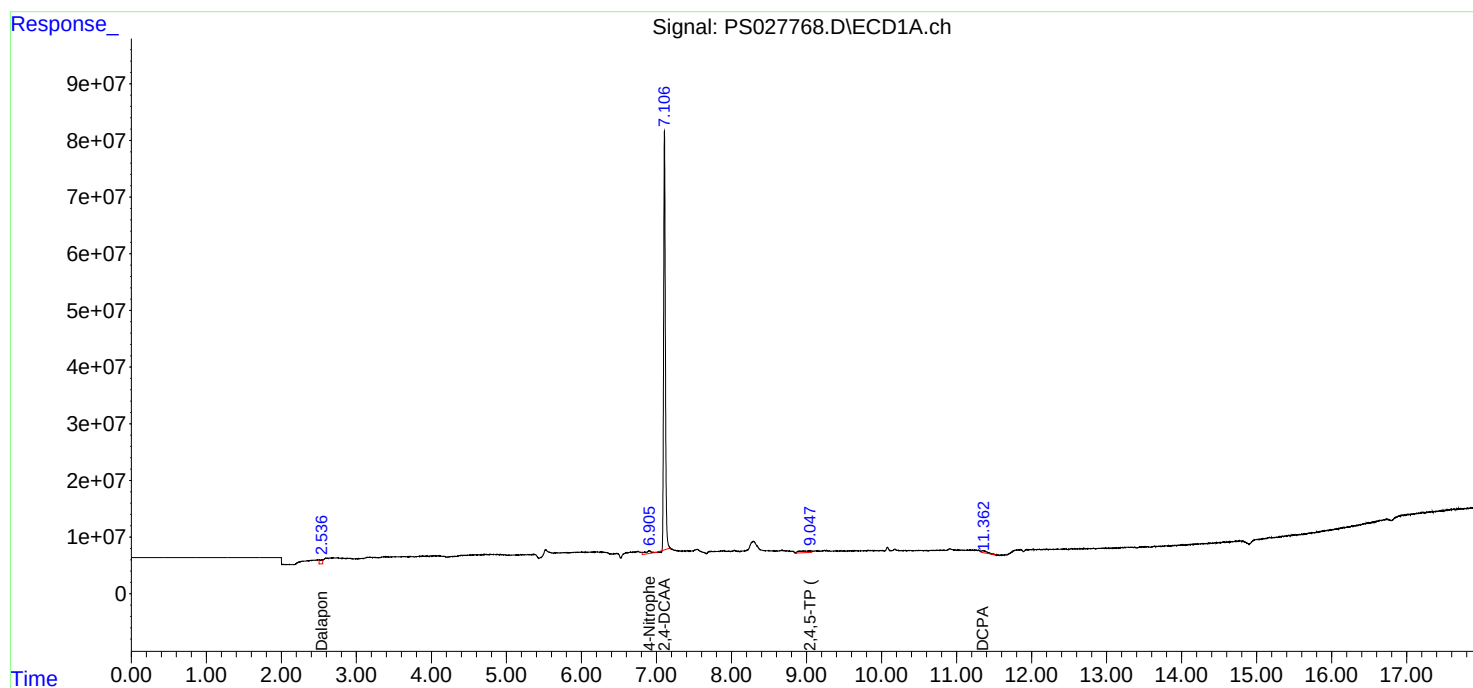


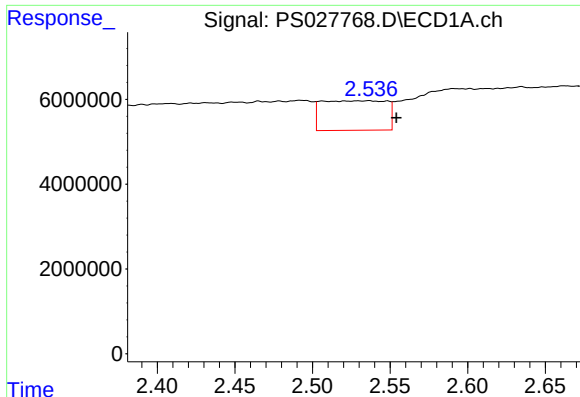

#1 Dalapon


R.T.: 2.534 min
Delta R.T.: -0.020 min
Response: 20141917
Conc: 4.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

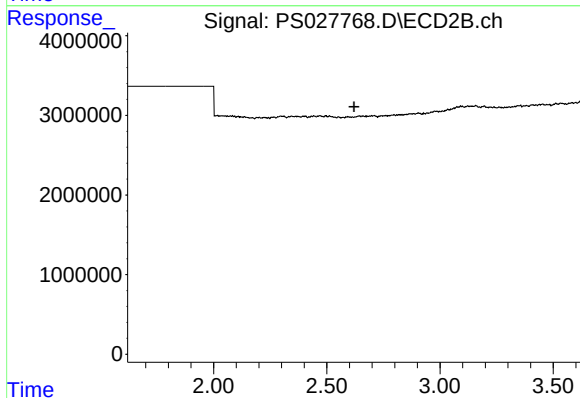


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

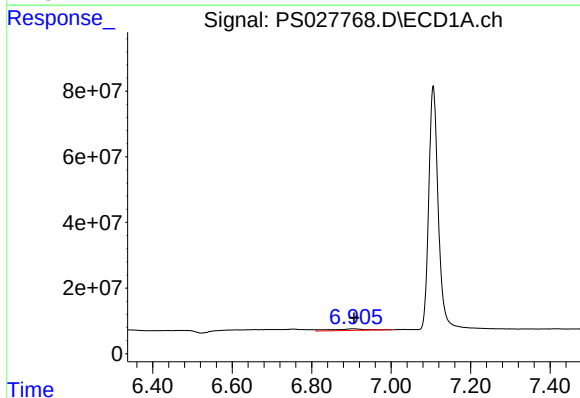


#3 4-Nitrophenol

R.T.: 6.905 min
Delta R.T.: -0.002 min
Response: 30041940
Conc: 17.74 ng/ml

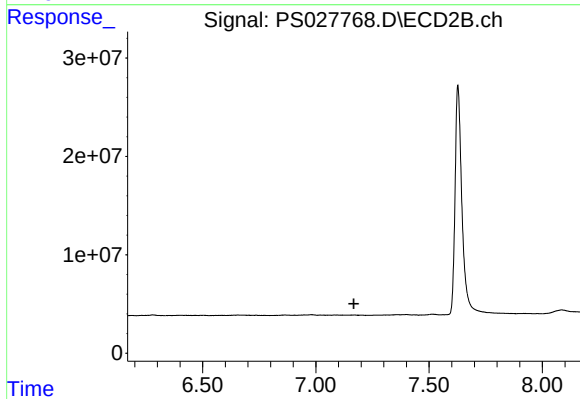

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.168 min
Response: 0
Conc: N.D.

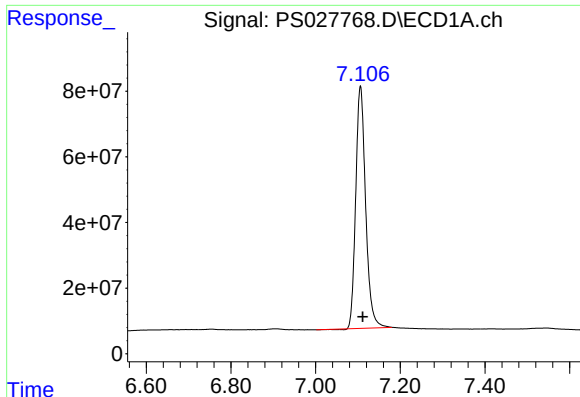

#4 2,4-DCAA


R.T.: 7.106 min
Delta R.T.: -0.005 min
Response: 1196123399
Conc: 480.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

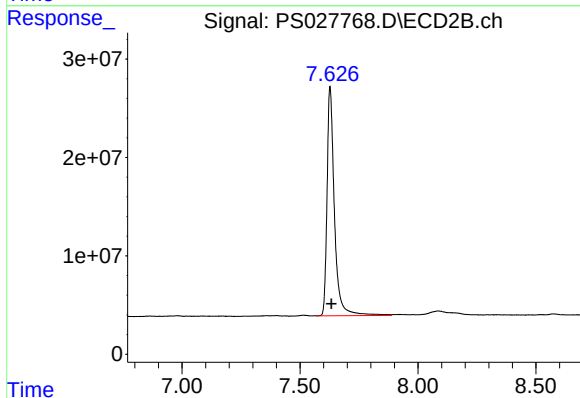


#4 2,4-DCAA

R.T.: 7.627 min
Delta R.T.: -0.006 min
Response: 509955352
Conc: 514.57 ng/ml

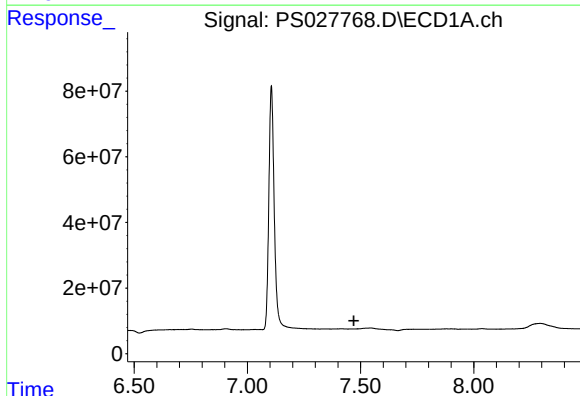


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.471 min
Response: 0
Conc: N.D.

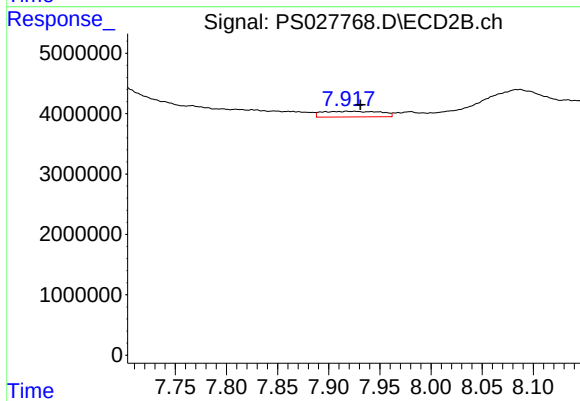

#6 MCP


R.T.: 7.920 min
Delta R.T.: -0.011 min
Response: 3718147
Conc: 1.13 ug/ml

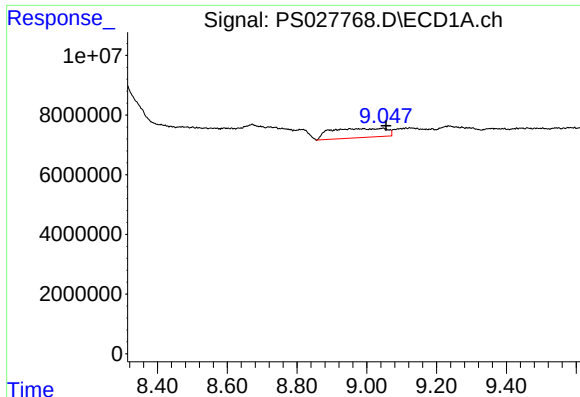

#11 2,4,5-TP (SILVEX)


R.T.: 9.045 min
Delta R.T.: -0.011 min
Response: 34252015
Conc: 2.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

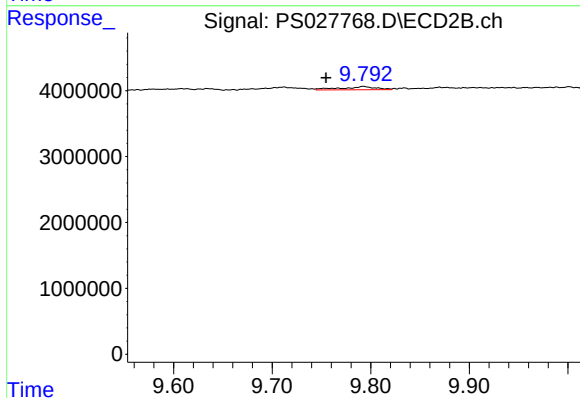


#11 2,4,5-TP (SILVEX)

R.T.: 9.793 min
Delta R.T.: 0.038 min
Response: 1227386
Conc: N.D.

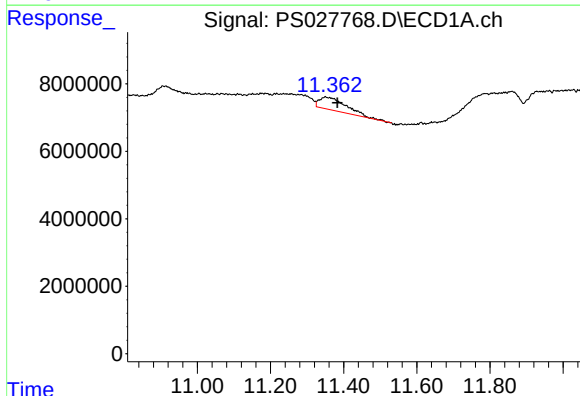

#16 DCPA

R.T.: 11.352 min
Delta R.T.: -0.032 min
Response: 18157068
Conc: 1.09 ng/ml

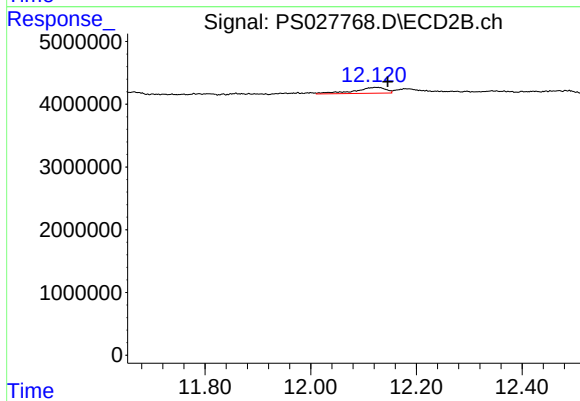

#16 DCPA

R.T.: 12.124 min
Delta R.T.: -0.021 min
Response: 3835857
Conc: N.D.