

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092524\
 Data File : PS027774.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2024 19:22
 Operator : AR\AJ
 Sample : P4148-01MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 STOCK-PILEMS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/27/2024
 Supervised By :Ankita Jodhani 09/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:13:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.102	7.627	512.9E6	147.6E6	206.177m	148.909 #
Target Compounds							
1) T	Dalapon	2.550	2.618	506.2E6	241.0E6	122.172m	147.714m
2) T	3,5-DICHL...	6.294	6.598	460.0E6	179.9E6	125.931	111.633
3) T	4-Nitroph...	6.901	7.164	114.2E6	57463561	67.449m	80.168m
5) T	DICAMBA	7.283	7.820	1334.0E6	479.1E6	132.012	108.736
6) T	MCP	7.458	7.920	55392318	24313413	8.035m	7.407
7) T	MCPA	7.602	8.159	128.5E6	75414341	12.685	14.246m
8) T	DICHLORPROP	7.969	8.527	336.5E6	112.9E6	126.932	101.045
9) T	2,4-D	8.193	8.854	424.2E6	160.3E6	138.382m	143.755
10) T	Pentachlo...	8.478	9.366	2587.5E6	860.2E6	71.141	52.031 #
11) T	2,4,5-TP ...	9.045	9.742	1431.8E6	425.8E6	97.837	71.009m#
12) T	2,4,5-T	9.331	10.161	1578.4E6	421.5E6	105.454	80.642m
13) T	2,4-DB	9.895	10.722	216.7E6	49760645	93.297m	80.872m
15) T	Picloram	10.890	12.175	2774.3E6	531.6E6	148.295	114.385
16) T	DCPA	11.370	12.127	4049.9E6	1388.3E6	244.011	215.410

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092524\
Data File : PS027774.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 19:22
Operator : AR\AJ
Sample : P4148-01MS
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
STOCK-PILEMS


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/27/2024
Supervised By : Ankita Jodhani 09/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:13:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

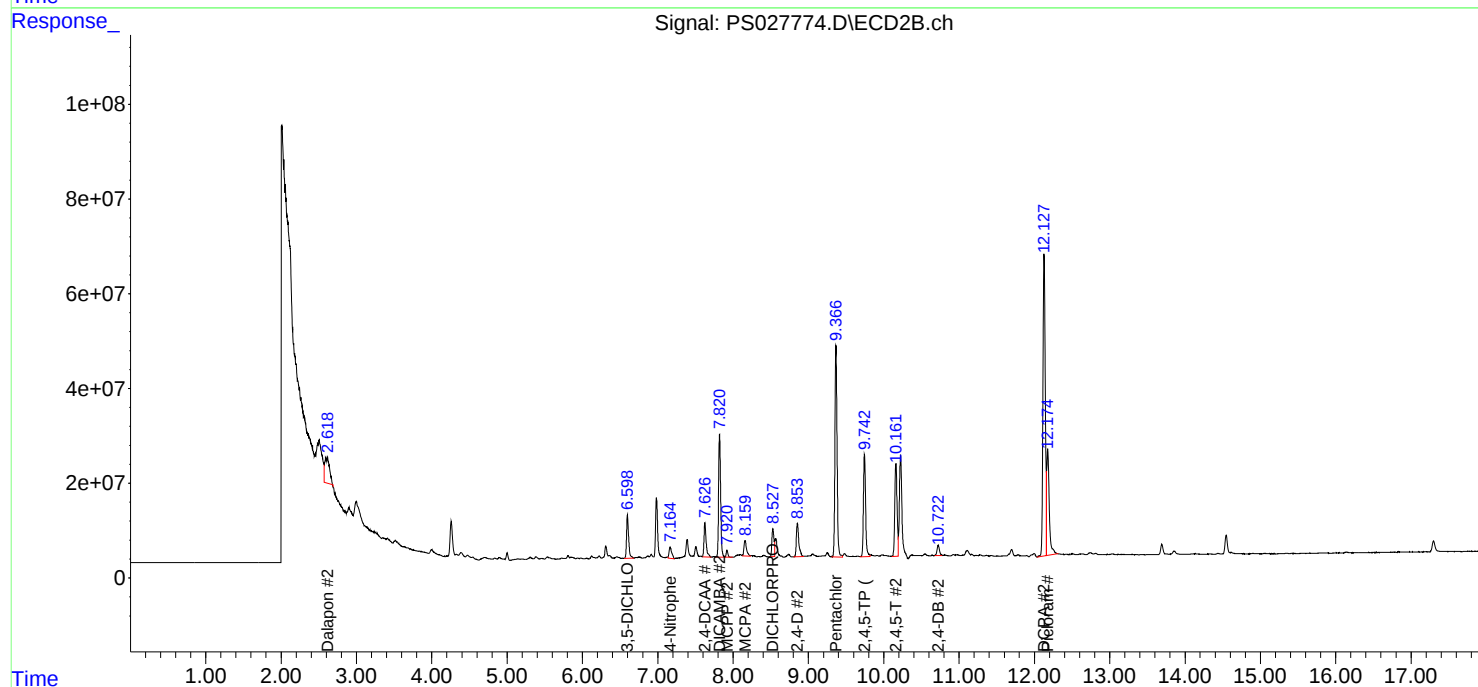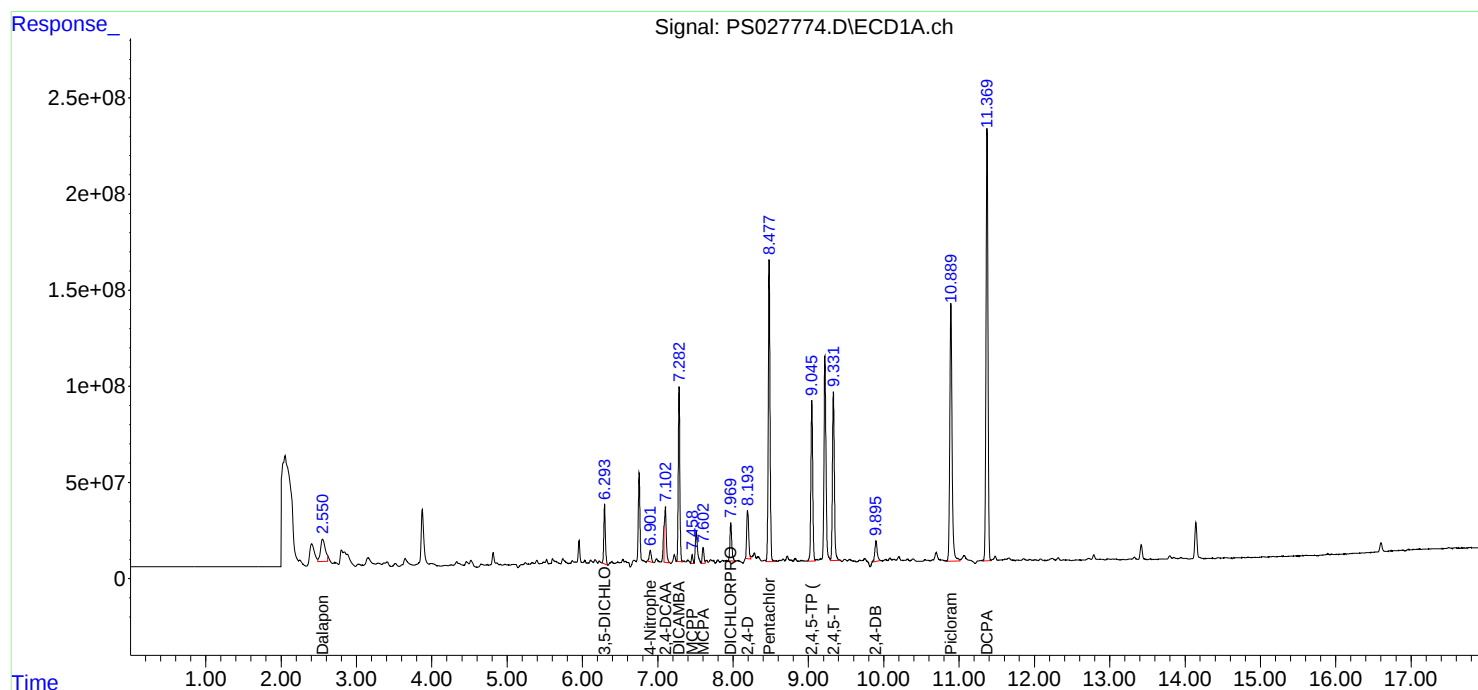

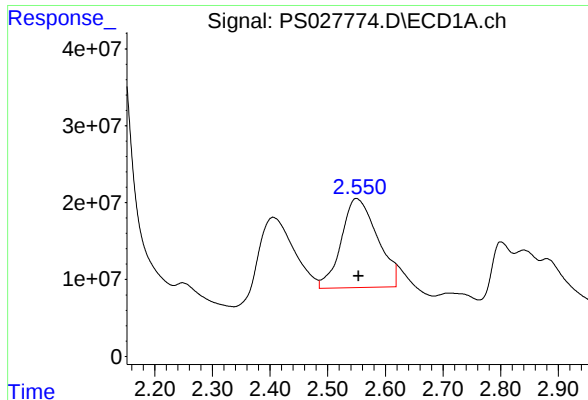


#1 Dalapon

R.T.: 2.550 min
Delta R.T.: -0.004 min
Response: 506168986
Conc: 122.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILEMS


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/27/2024
Supervised By :Ankita Jodhani 09/27/2024

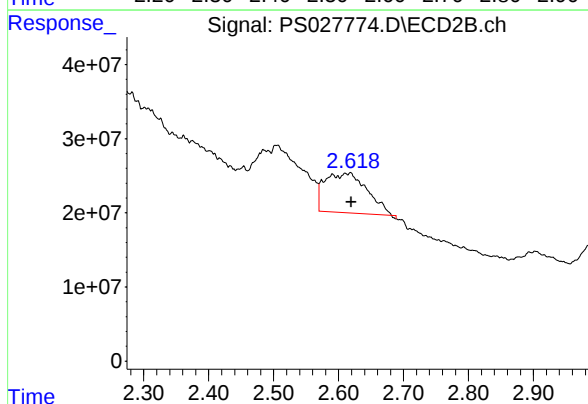


#1 Dalapon

R.T.: 2.618 min
Delta R.T.: -0.002 min
Response: 241049048
Conc: 147.71 ng/ml

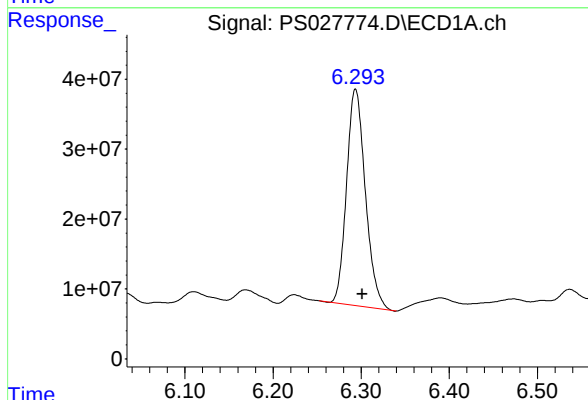


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.294 min
Delta R.T.: -0.008 min
Response: 460008119
Conc: 125.93 ng/ml

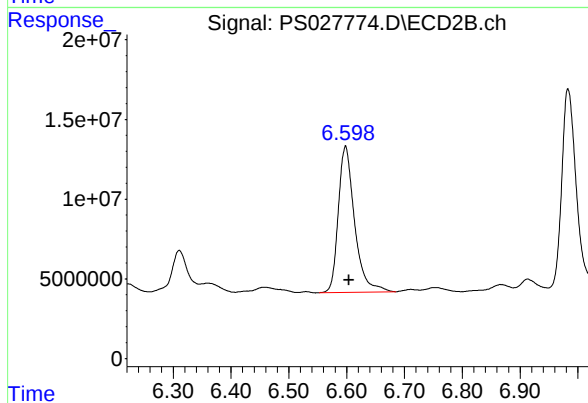

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.598 min
Delta R.T.: -0.006 min
Response: 179887799
Conc: 111.63 ng/ml

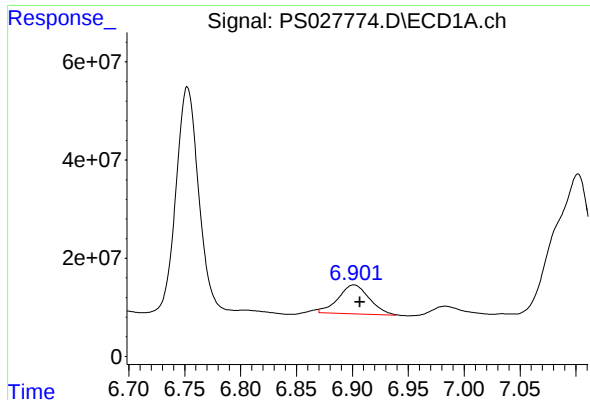


#3 4-Nitrophenol

R.T.: 6.901 min
Delta R.T.: -0.006 min
Response: 114200132
Conc: 67.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILEMS


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/27/2024
Supervised By :Ankita Jodhani 09/27/2024

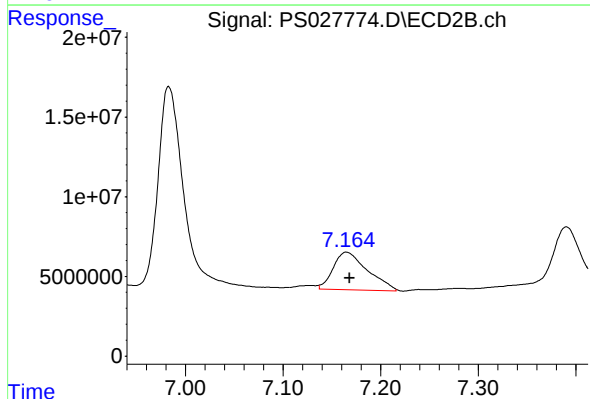


#3 4-Nitrophenol

R.T.: 7.164 min
Delta R.T.: -0.004 min
Response: 57463561
Conc: 80.17 ng/ml m

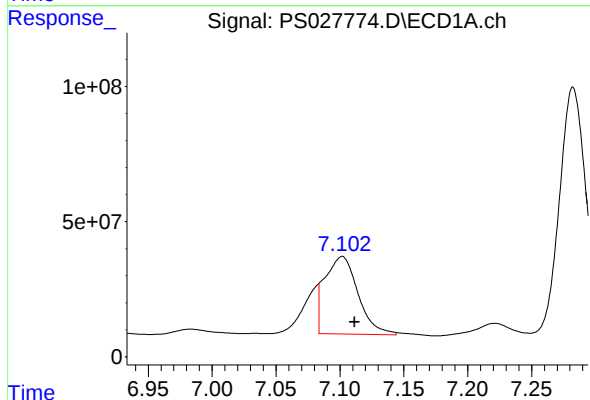


#4 2,4-DCAA

R.T.: 7.102 min
Delta R.T.: -0.010 min
Response: 512888254
Conc: 206.18 ng/ml m

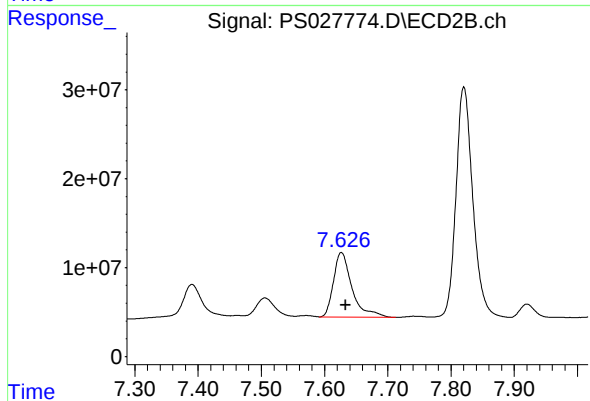

#4 2,4-DCAA

R.T.: 7.627 min
Delta R.T.: -0.007 min
Response: 147573348
Conc: 148.91 ng/ml

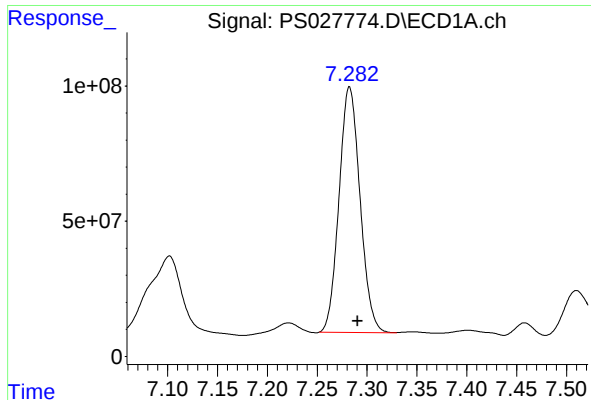


#5 DICAMBA

R.T.: 7.283 min
Delta R.T.: -0.008 min
Response: 1334000812
Conc: 132.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILEMS


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/27/2024
Supervised By :Ankita Jodhani 09/27/2024

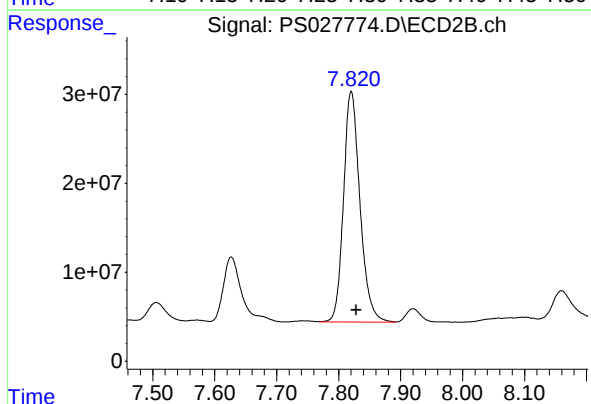


#5 DICAMBA

R.T.: 7.820 min
Delta R.T.: -0.008 min
Response: 479132177
Conc: 108.74 ng/ml

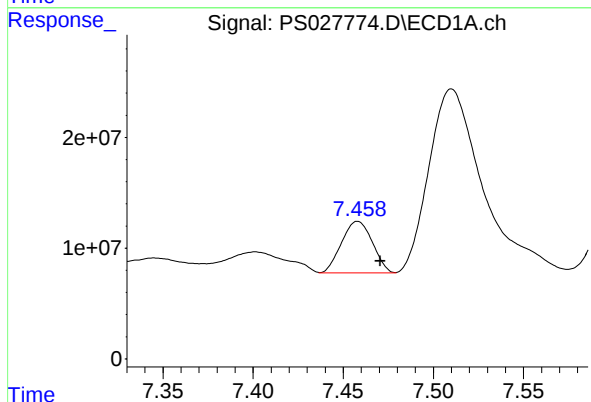


#6 MCPP

R.T.: 7.458 min
Delta R.T.: -0.013 min
Response: 55392318
Conc: 8.04 ug/ml m

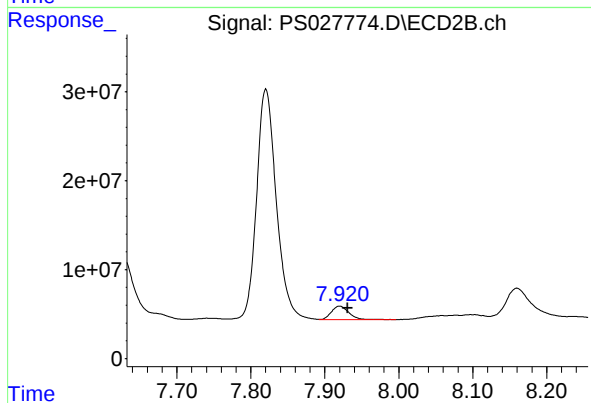

#6 MCPP

R.T.: 7.920 min
Delta R.T.: -0.011 min
Response: 24313413
Conc: 7.41 ug/ml

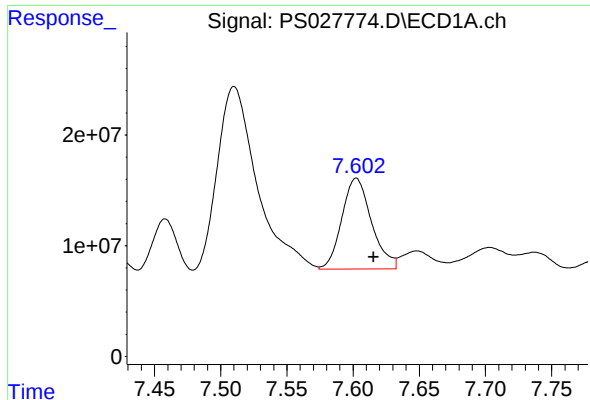


#7 MCPA

R.T.: 7.602 min
Delta R.T.: -0.013 min
Response: 128498863
Conc: 12.69 ug/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILEMS


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/27/2024
Supervised By :Ankita Jodhani 09/27/2024

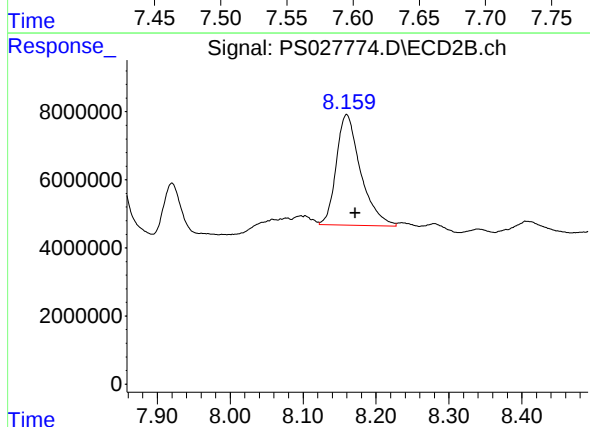


#7 MCPA

R.T.: 8.159 min
Delta R.T.: -0.012 min
Response: 75414341
Conc: 14.25 ug/ml

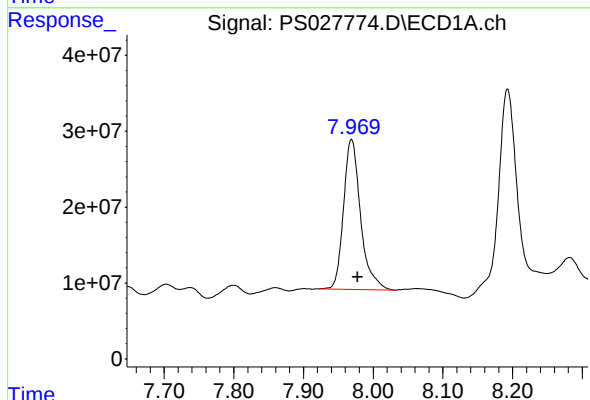


#8 DICHLORPROP

R.T.: 7.969 min
Delta R.T.: -0.009 min
Response: 336481480
Conc: 126.93 ng/ml

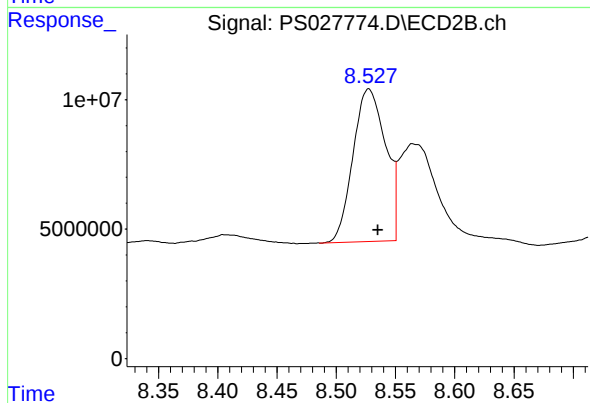

#8 DICHLORPROP

R.T.: 8.527 min
Delta R.T.: -0.008 min
Response: 112889424
Conc: 101.04 ng/ml

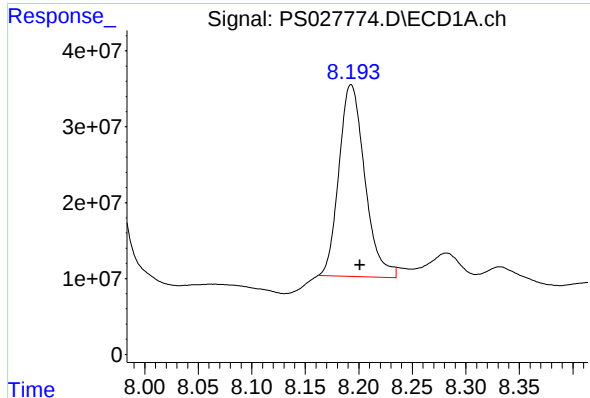


#9 2,4-D

R.T.: 8.193 min
Delta R.T.: -0.008 min
Response: 424173874
Conc: 138.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILEMS


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/27/2024
Supervised By :Ankita Jodhani 09/27/2024

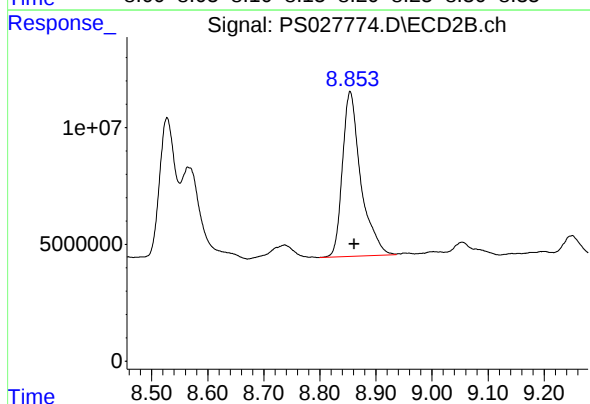


#9 2,4-D

R.T.: 8.854 min
Delta R.T.: -0.007 min
Response: 160289172
Conc: 143.76 ng/ml

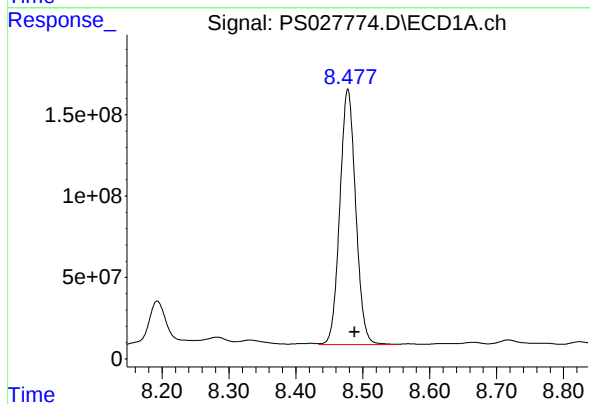


#10 Pentachlorophenol

R.T.: 8.478 min
Delta R.T.: -0.010 min
Response: 2587497286
Conc: 71.14 ng/ml

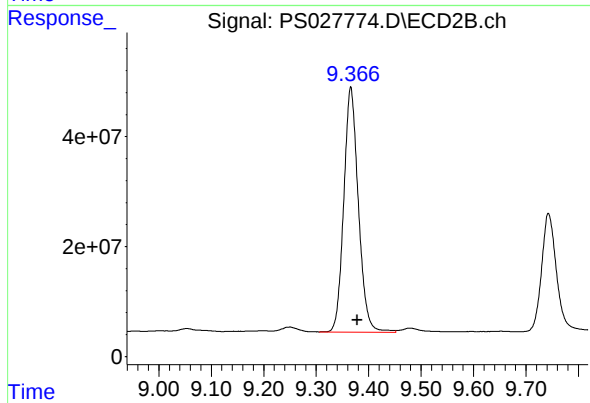

#10 Pentachlorophenol

R.T.: 9.366 min
Delta R.T.: -0.012 min
Response: 860201039
Conc: 52.03 ng/ml

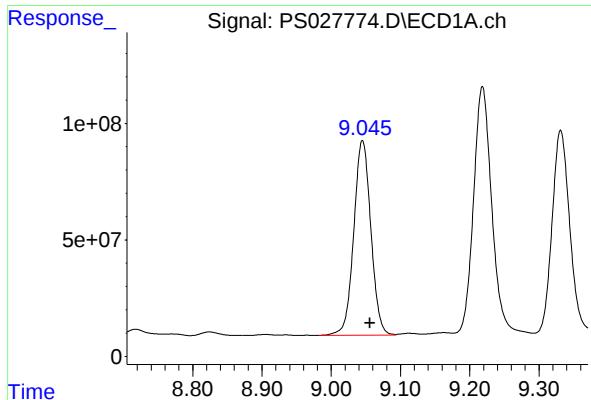


#11 2,4,5-TP (SILVEX)

R.T.: 9.045 min
Delta R.T.: -0.011 min
Response: 1431841780
Conc: 97.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILEMS


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/27/2024
Supervised By :Ankita Jodhani 09/27/2024

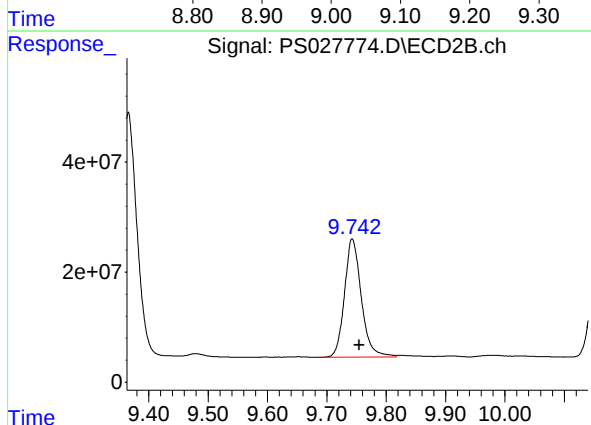


#11 2,4,5-TP (SILVEX)

R.T.: 9.742 min
Delta R.T.: -0.013 min
Response: 425763152
Conc: 71.01 ng/ml m

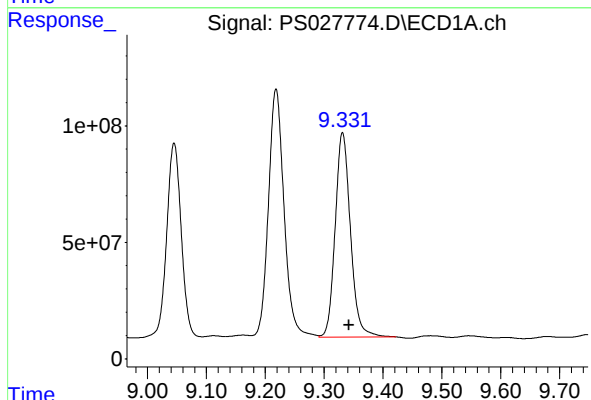


#12 2,4,5-T

R.T.: 9.331 min
Delta R.T.: -0.010 min
Response: 1578416925
Conc: 105.45 ng/ml

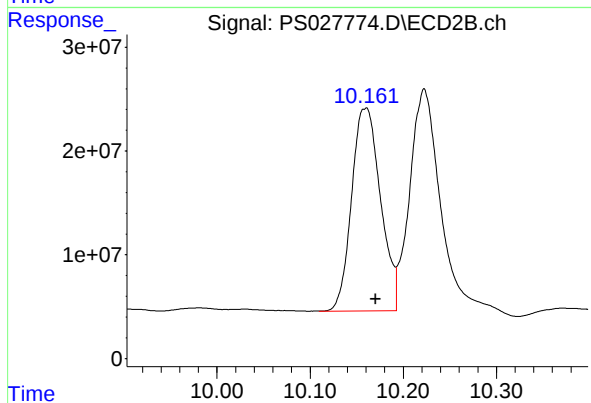

#12 2,4,5-T

R.T.: 10.161 min
Delta R.T.: -0.010 min
Response: 421500553
Conc: 80.64 ng/ml m

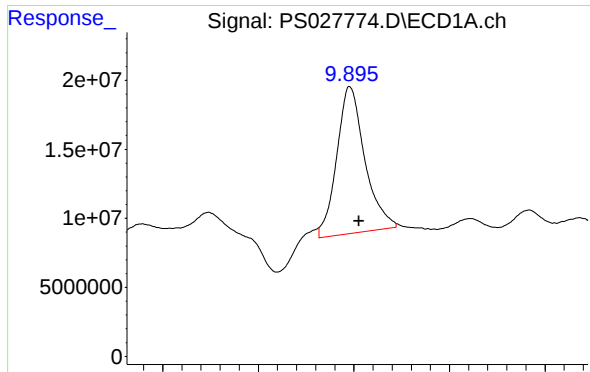


#13 2,4-DB

R.T.: 9.895 min
Delta R.T.: -0.011 min
Response: 216656715
Conc: 93.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILEMS


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/27/2024
Supervised By :Ankita Jodhani 09/27/2024

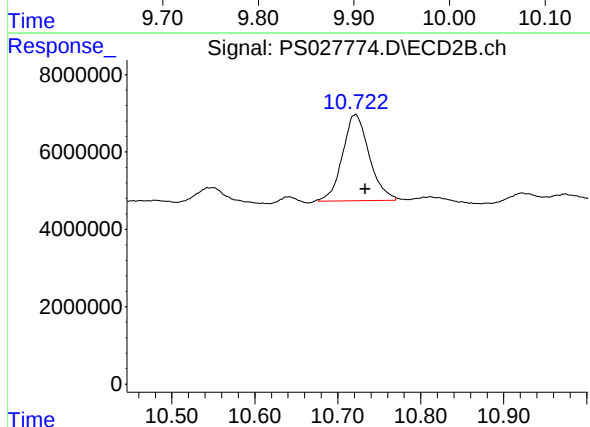


#13 2,4-DB

R.T.: 10.722 min
Delta R.T.: -0.011 min
Response: 49760645
Conc: 80.87 ng/ml

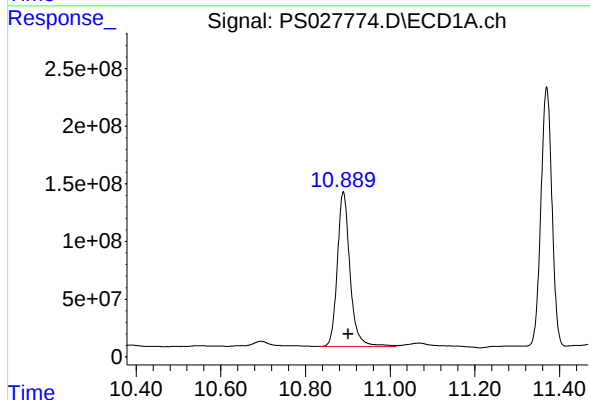


#15 Picloram

R.T.: 10.890 min
Delta R.T.: -0.011 min
Response: 2774270037
Conc: 148.30 ng/ml

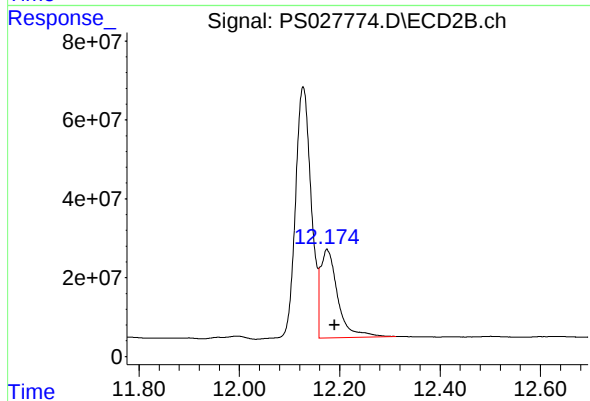

#15 Picloram

R.T.: 12.175 min
Delta R.T.: -0.015 min
Response: 531587289
Conc: 114.39 ng/ml

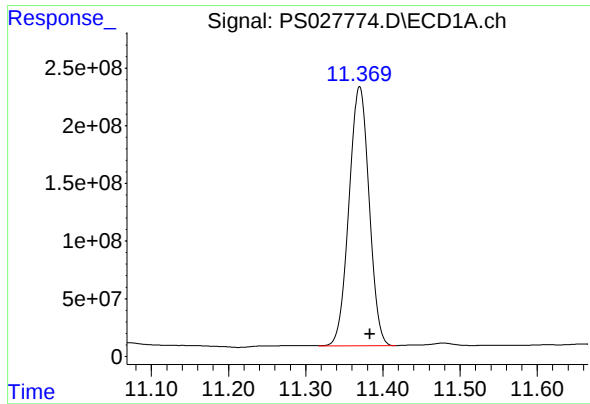


#16 DCPA

R.T.: 11.370 min
Delta R.T.: -0.014 min
Response: 4049940756
Conc: 244.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILEMS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/27/2024
Supervised By :Ankita Jodhani 09/27/2024

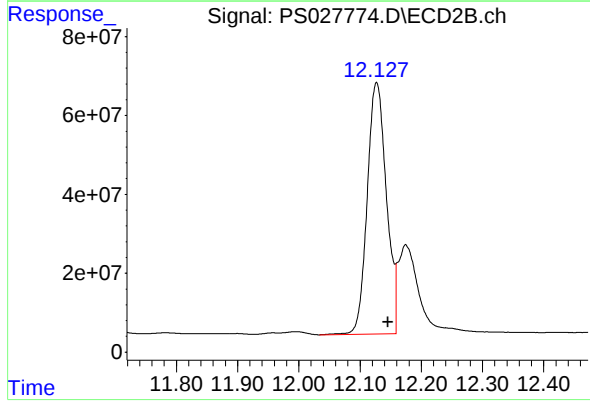

#16 DCPA

R.T.: 12.127 min
Delta R.T.: -0.018 min
Response: 1388341232
Conc: 215.41 ng/ml