

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092525\
 Data File : PS031839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2025 11:19
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 06:58:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.747	1825.0E6	500.8E6	506.735	550.974
Target Compounds							
1) T	Dalapon	0.000	2.663f	0	57166868	N.D.	20.289
2) T	3,5-DICHL...	6.447	0.000	9218408	0	1.728	N.D. #
3) T	4-Nitroph...	7.078	0.000	9378611	0	8.501	N.D. #
7) T	MCPA	7.755f	0.000	6941836	0	<MDL	N.D. #
9) T	2,4-D	0.000	9.008	0	2412720	N.D.	1.467
10) T	Pentachlo...	8.710	9.513	10375340	10048091	<MDL	<MDL #
11) T	2,4,5-TP ...	9.298	9.917f	4643351	2955536	<MDL	<MDL #
12) T	2,4,5-T	9.622f	0.000	9866949	0	<MDL	N.D. #
14) T	DINOSEB	11.356	0.000	7858042	0	<MDL	N.D. #
15) T	Picloram	11.184	0.000	9679998	0	<MDL	N.D. #
16) T	DCPA	11.655	12.322	9610258	19750205	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092525\
Data File : PS031839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2025 11:19
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 06:58:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

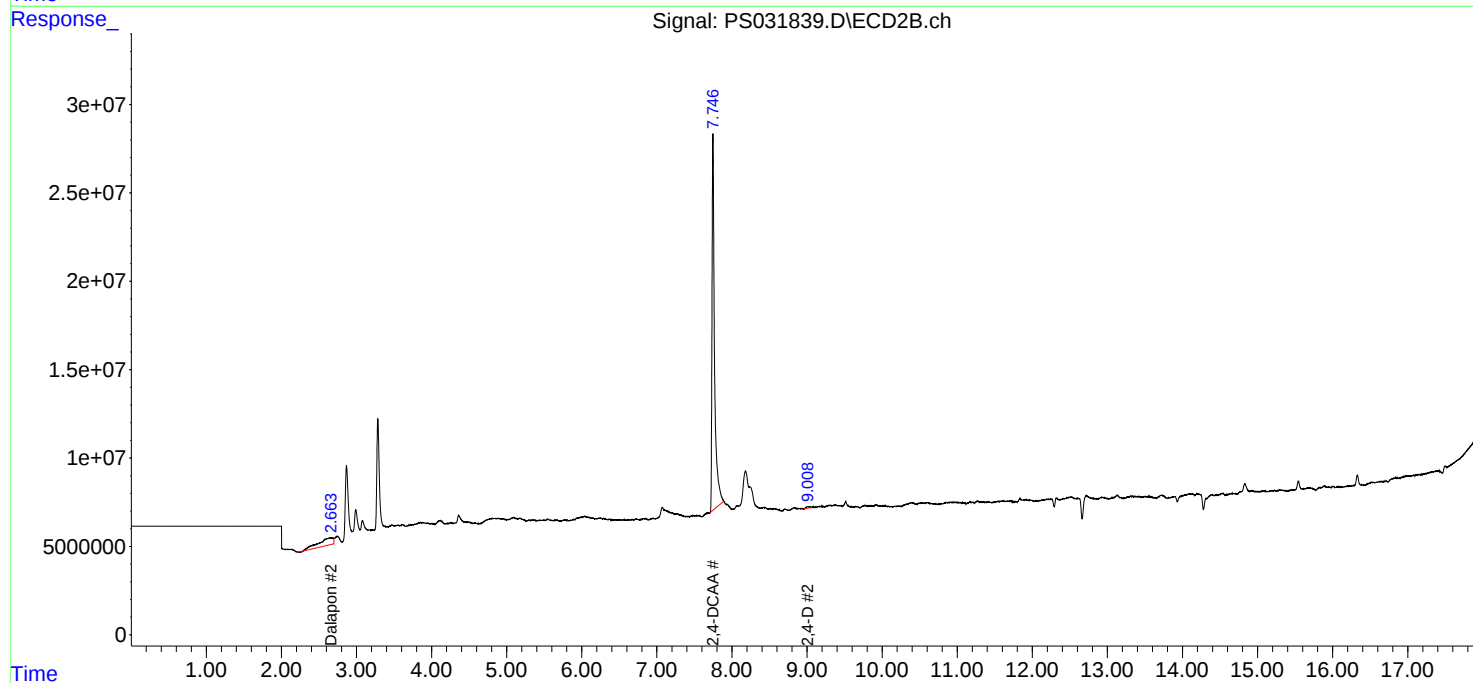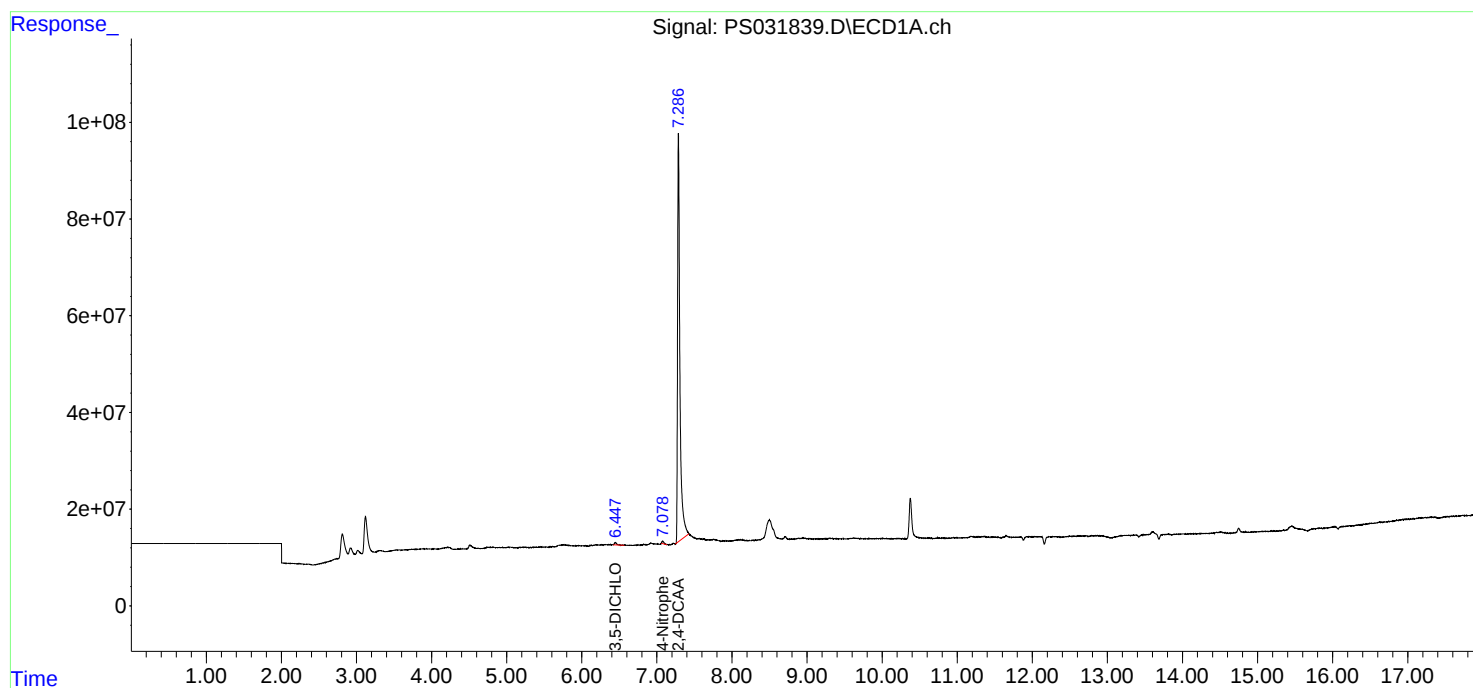


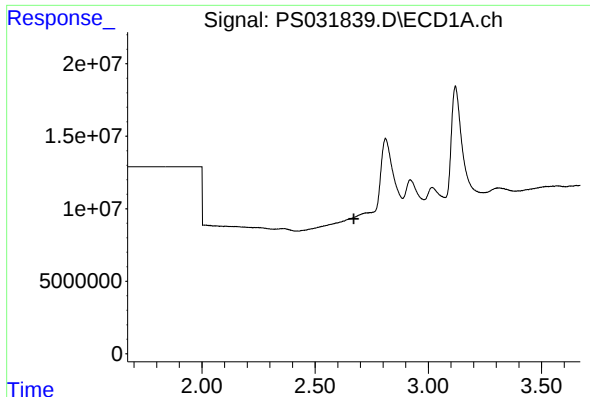

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

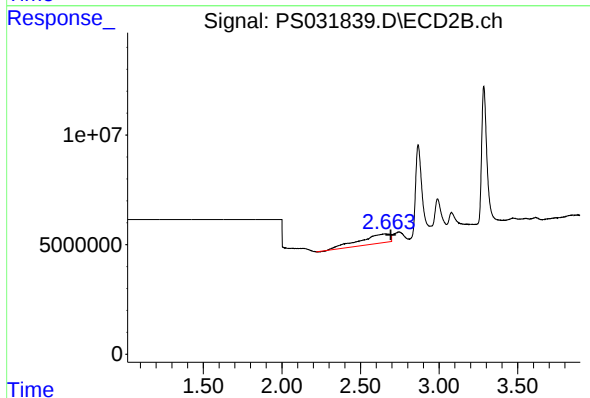


#1 Dalapon

R.T.: 2.663 min
Delta R.T.: -0.028 min
Response: 57166868
Conc: 20.29 ng/ml

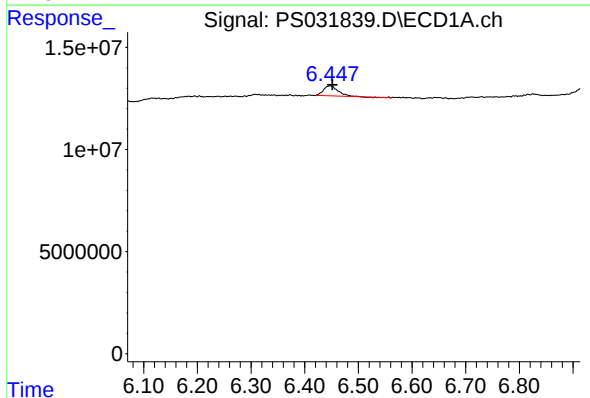


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.447 min
Delta R.T.: -0.004 min
Response: 9218408
Conc: 1.73 ng/ml

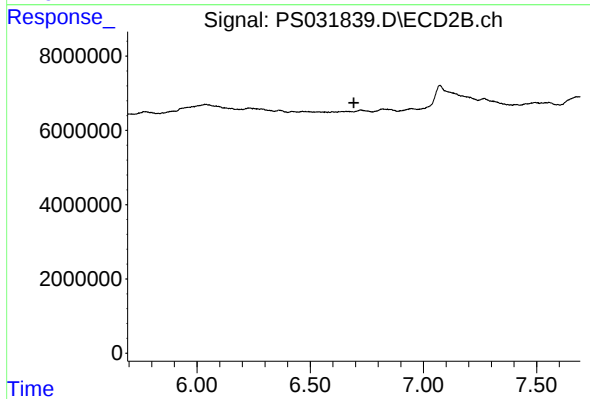

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.693 min
Response: 0
Conc: N.D.

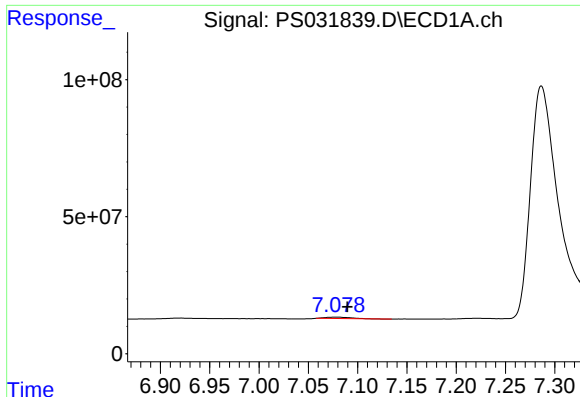

#3 4-Nitrophenol


R.T.: 7.078 min
Delta R.T.: -0.011 min
Response: 9378611
Conc: 8.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

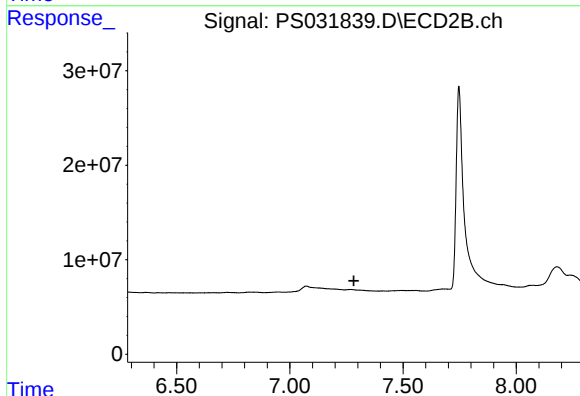


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

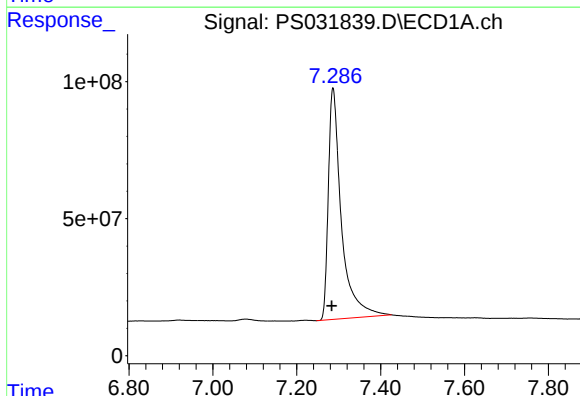


#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: 0.004 min
Response: 1825021311
Conc: 506.74 ng/ml

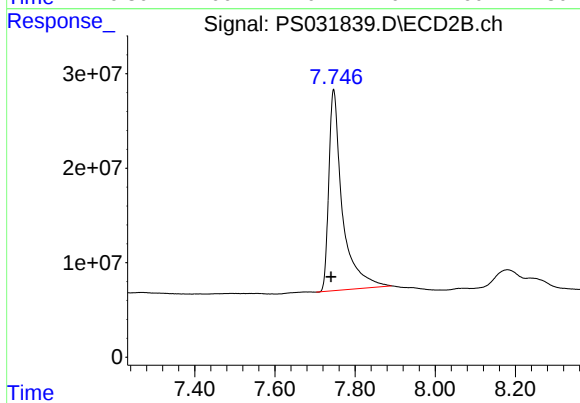

#4 2,4-DCAA


R.T.: 7.747 min
Delta R.T.: 0.006 min
Response: 500780136
Conc: 550.97 ng/ml

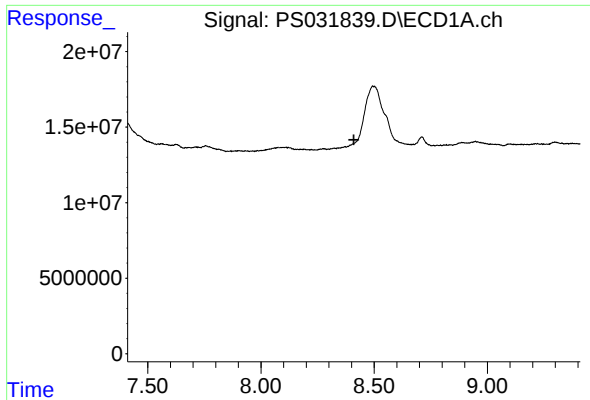

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

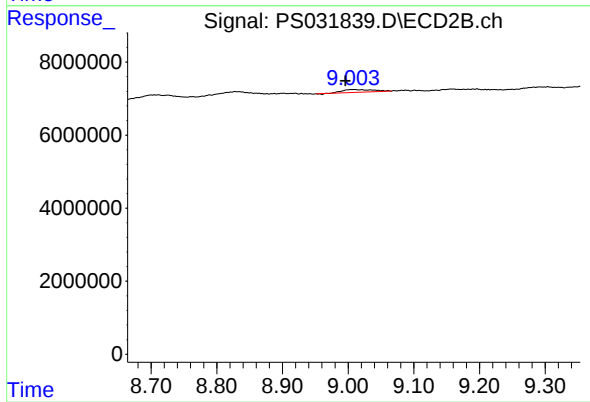

#9 2,4-D

R.T.: 9.008 min
Delta R.T.: 0.012 min
Response: 2412720
Conc: 1.47 ng/ml