

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092619\
 Data File : PS006921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2019 16:41
 Operator : SM\AJ
 Sample : K4657-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 00:48:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.483	5.214	517.0E6	286.8E6	565.790	623.744
Target Compounds							
1) T	Dalapon	2.117	1.745	126.6E6	80013013	118.521	150.099 #
2) T	3,5-DICHL...	4.868	4.542	8552989	62386216	7.863	108.524 #
5) T	DICAMBA	0.000	5.357	0	15516878	N.D.	9.218
6) T	MCP	5.777	0.000	14293314	0	6.719	N.D. #
9) T	2,4-D	6.550	6.136	109.9E6	6689424	134.142	13.115 #
10) T	Pentachlo...	6.743	6.522	13892575	10240764	1.166	1.628 #
11) T	2,4,5-TP ...	7.277	6.835	8247383	71112486	1.815	29.688 #
14) T	DINOSEB	0.000	8.064	0	24445123	N.D.	14.190
15) T	Picloram	8.991	0.000	6435475	0	<MDL	N.D. #
16) T	DCPA	9.438	0.000	17698344	0	3.033	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092619\
Data File : PS006921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2019 16:41
Operator : SM\AJ
Sample : K4657-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 00:48:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

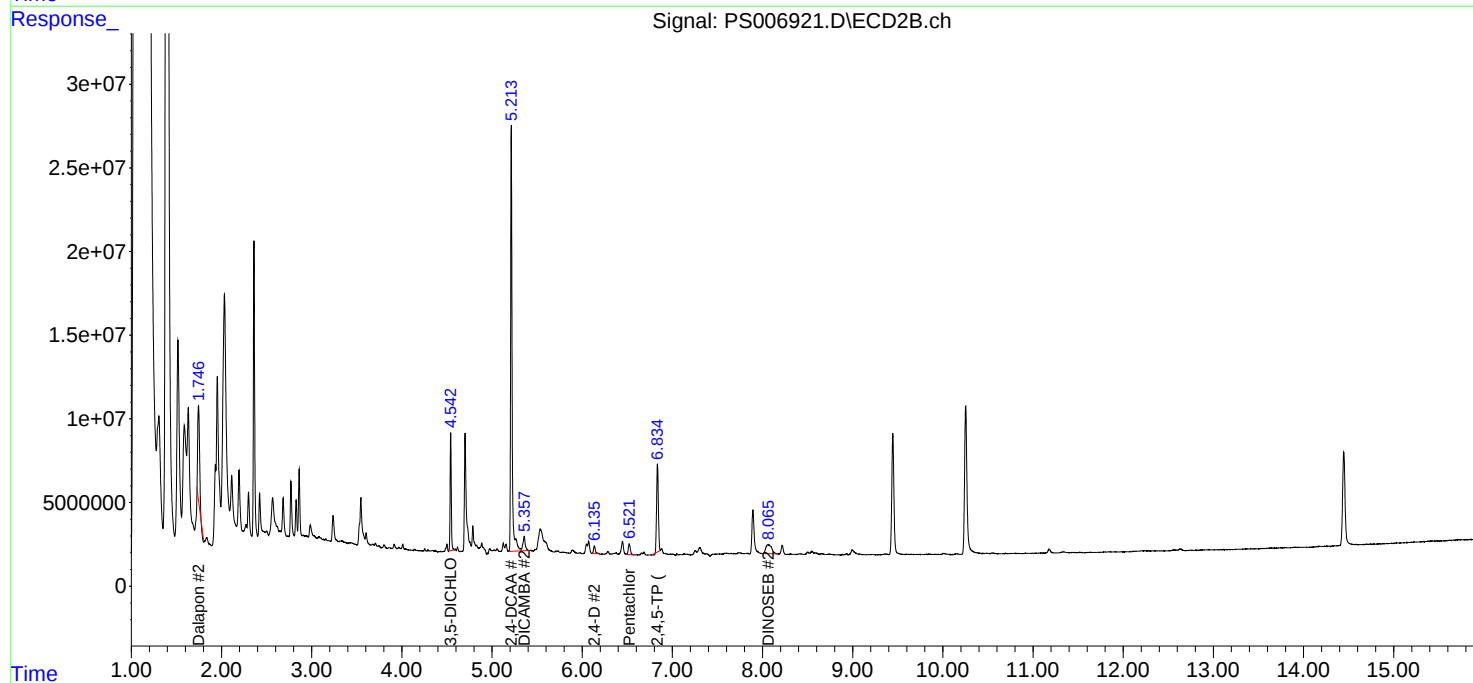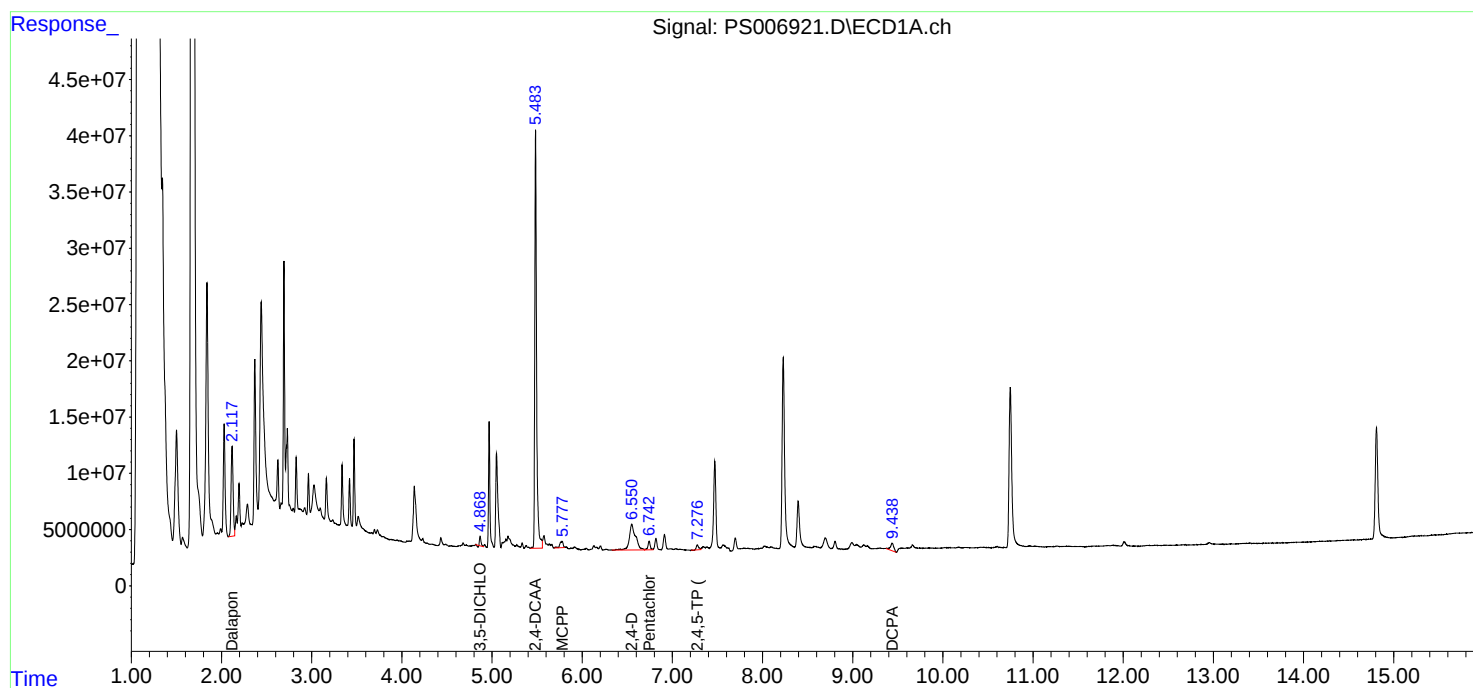


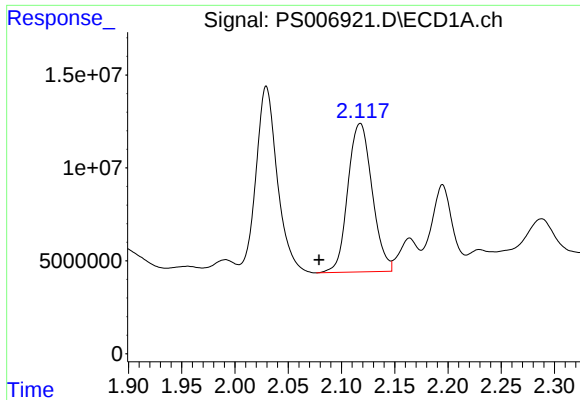

#1 Dalapon


R.T.: 2.117 min
Delta R.T.: 0.038 min
Response: 126628136
Conc: 118.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

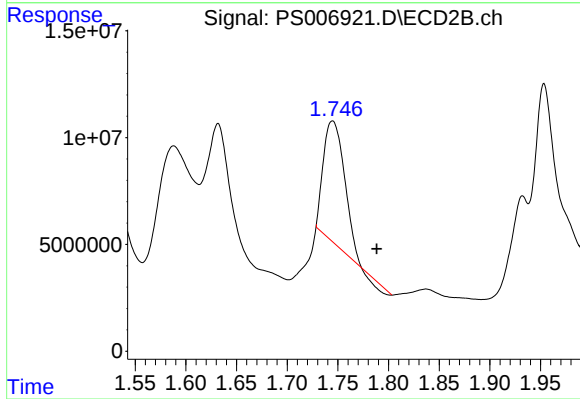


#1 Dalapon

R.T.: 1.745 min
Delta R.T.: -0.043 min
Response: 80013013
Conc: 150.10 ng/ml

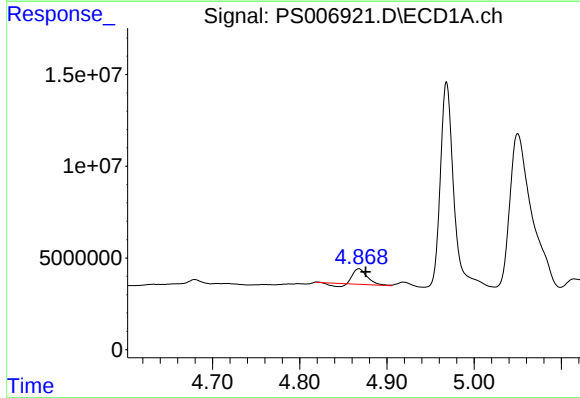


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.868 min
Delta R.T.: -0.008 min
Response: 8552989
Conc: 7.86 ng/ml

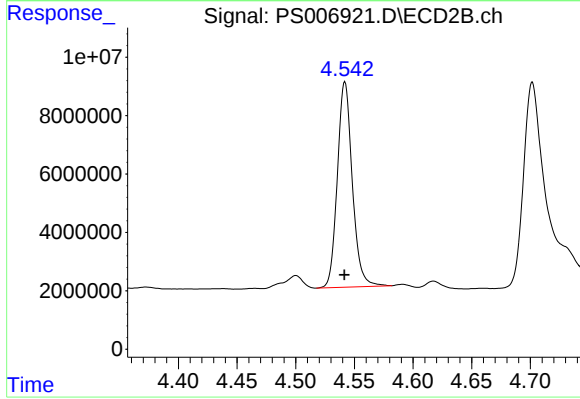

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.542 min
Delta R.T.: 0.000 min
Response: 62386216
Conc: 108.52 ng/ml

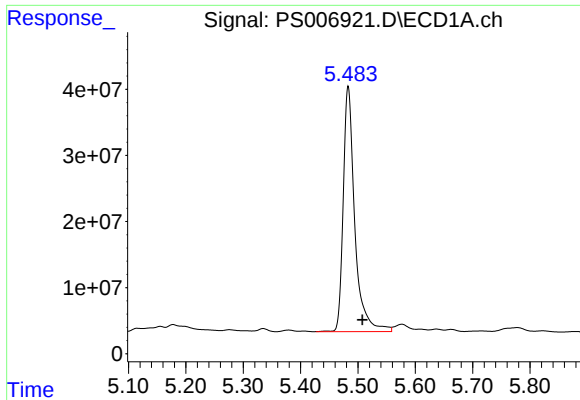

#4 2,4-DCAA


R.T.: 5.483 min
Delta R.T.: -0.025 min
Response: 517026940
Conc: 565.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

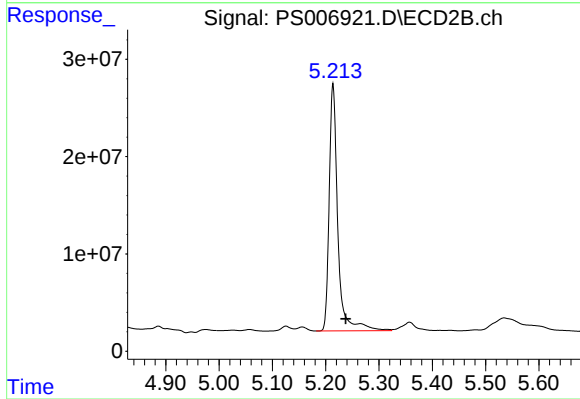


#4 2,4-DCAA

R.T.: 5.214 min
Delta R.T.: -0.024 min
Response: 286823479
Conc: 623.74 ng/ml

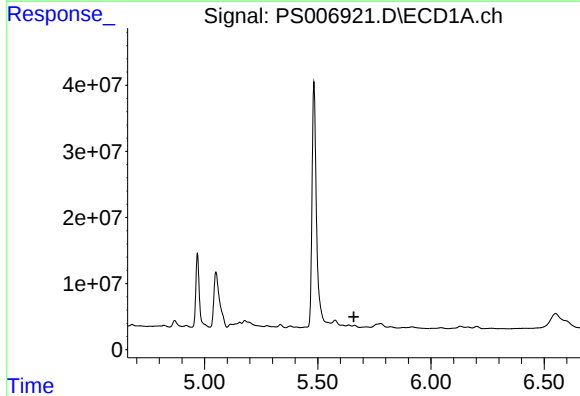


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.660 min
Response: 0
Conc: N.D.

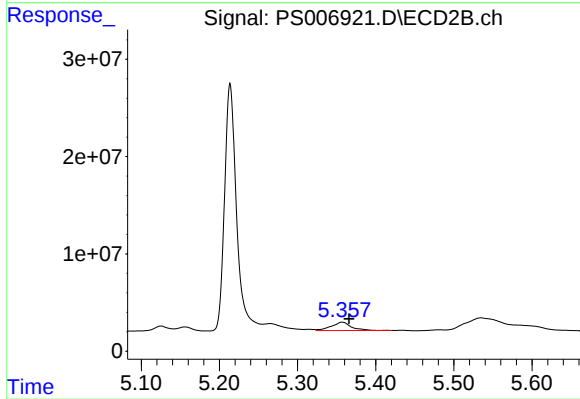

#5 DICAMBA


R.T.: 5.357 min
Delta R.T.: -0.009 min
Response: 15516878
Conc: 9.22 ng/ml

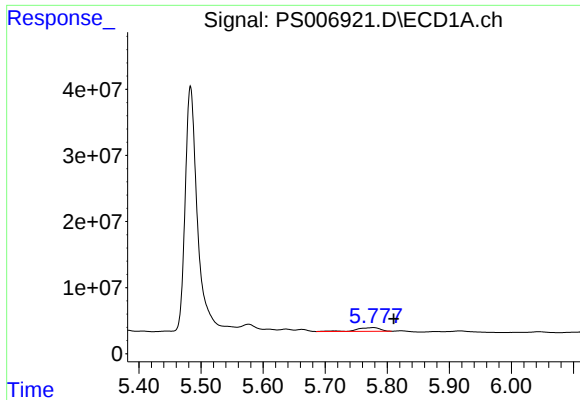

#6 MCP


R.T.: 5.777 min
Delta R.T.: -0.034 min
Response: 14293314
Conc: 6.72 ug/ml

Instrument :
ECD_S
ClientSampleId :

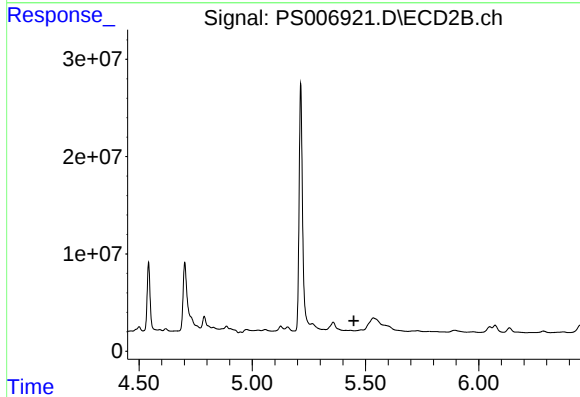


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.449 min
Response: 0
Conc: N.D.

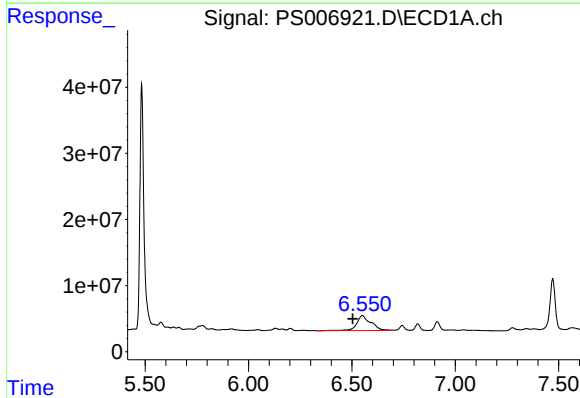


#9 2,4-D

R.T.: 6.550 min
Delta R.T.: 0.046 min
Response: 109931273
Conc: 134.14 ng/ml

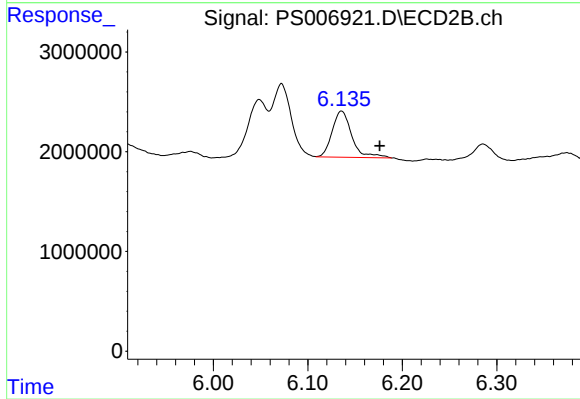

#9 2,4-D


R.T.: 6.136 min
Delta R.T.: -0.040 min
Response: 6689424
Conc: 13.11 ng/ml

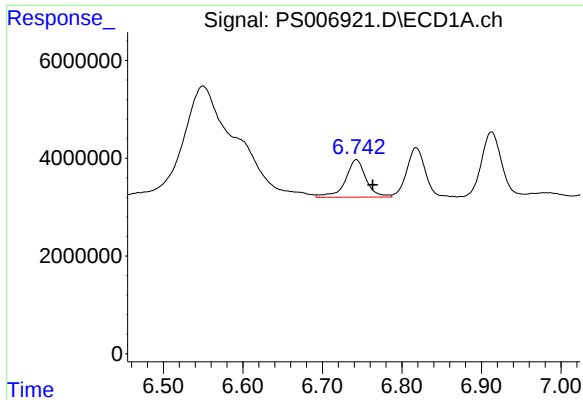

#10 Pentachlorophenol


R.T.: 6.743 min
Delta R.T.: -0.021 min
Response: 13892575
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

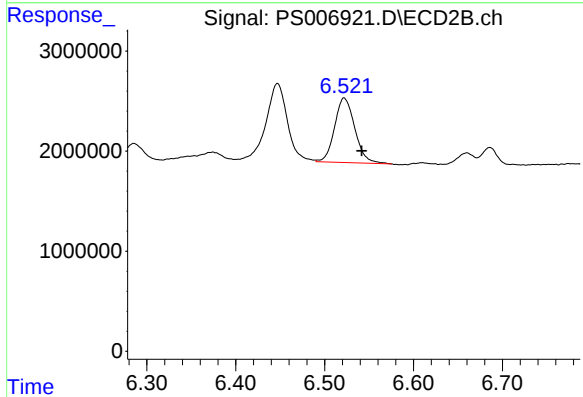


#10 Pentachlorophenol

R.T.: 6.522 min
Delta R.T.: -0.020 min
Response: 10240764
Conc: 1.63 ng/ml

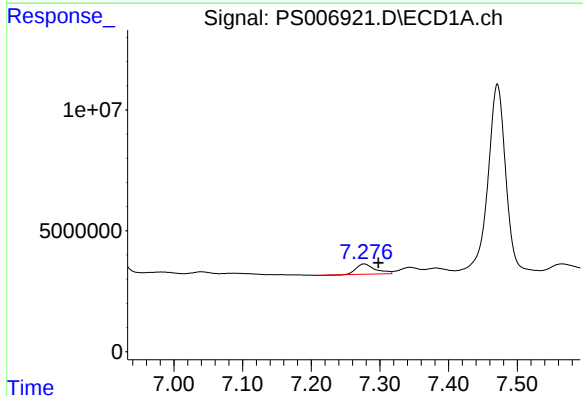


#11 2,4,5-TP (SILVEX)

R.T.: 7.277 min
Delta R.T.: -0.021 min
Response: 8247383
Conc: 1.82 ng/ml

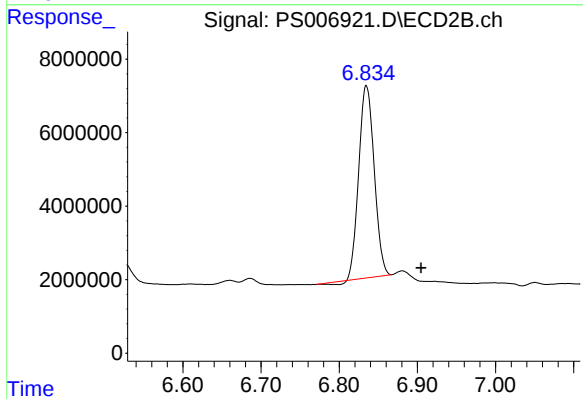

#11 2,4,5-TP (SILVEX)


R.T.: 6.835 min
Delta R.T.: -0.070 min
Response: 71112486
Conc: 29.69 ng/ml

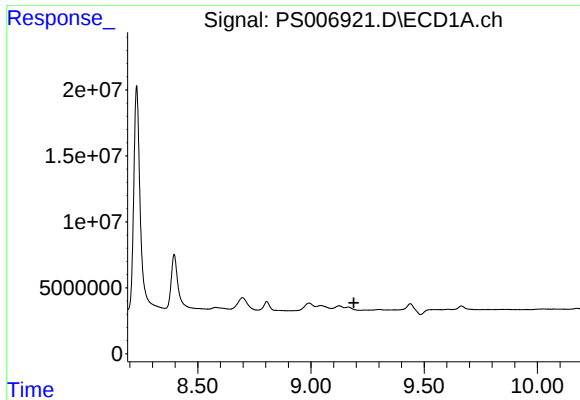

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

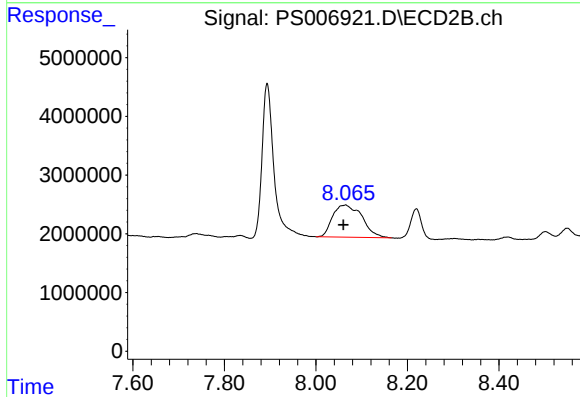


#14 DINOSEB

R.T.: 8.064 min
Delta R.T.: 0.004 min
Response: 24445123
Conc: 14.19 ng/ml

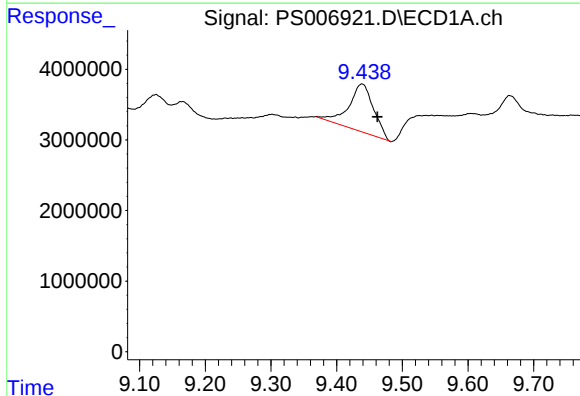

#16 DCPA

R.T.: 9.438 min
Delta R.T.: -0.024 min
Response: 17698344
Conc: 3.03 ng/ml

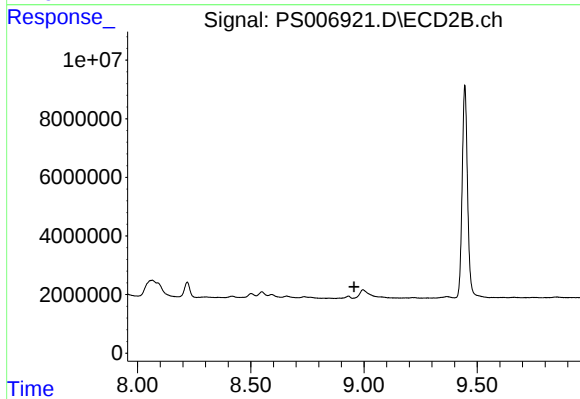

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 8.956 min
Response: 0
Conc: N.D.