

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092619\
 Data File : PS006925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2019 18:09
 Operator : SM\AJ
 Sample : K4663-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 00:49:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.508	5.239	535.5E6	289.8E6	586.010	630.264
Target Compounds							
1) T	Dalapon	2.055	1.770	124.1E6	122.6E6	116.181	230.026 #
2) T	3,5-DICHL...	0.000	4.526	0	4723376	N.D.	8.217
5) T	DICAMBA	5.602	0.000	30361068	0	9.397	N.D. #
6) T	MCPD	5.803	0.000	13327015	0	6.264	N.D. #
7) T	MCPA	0.000	5.560	0	59166222	N.D.	32.145
9) T	2,4-D	0.000	6.161	0	6626195	N.D.	12.991
11) T	2,4,5-TP ...	0.000	6.860	0	74043803	N.D.	30.912
14) T	DINOSEB	0.000	8.091	0	28121088	N.D.	16.323
15) T	Picloram	9.017	0.000	14883384	0	2.220	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092619\
Data File : PS006925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2019 18:09
Operator : SM\AJ
Sample : K4663-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 00:49:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

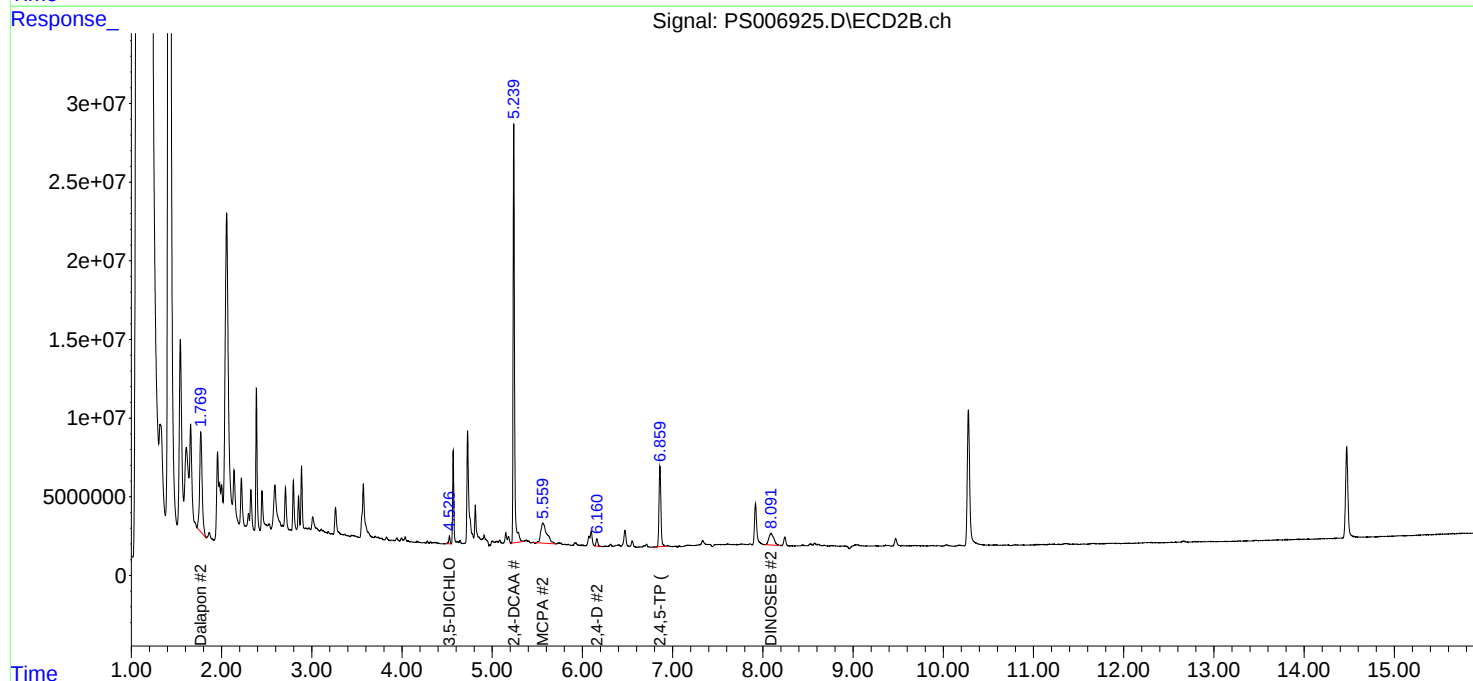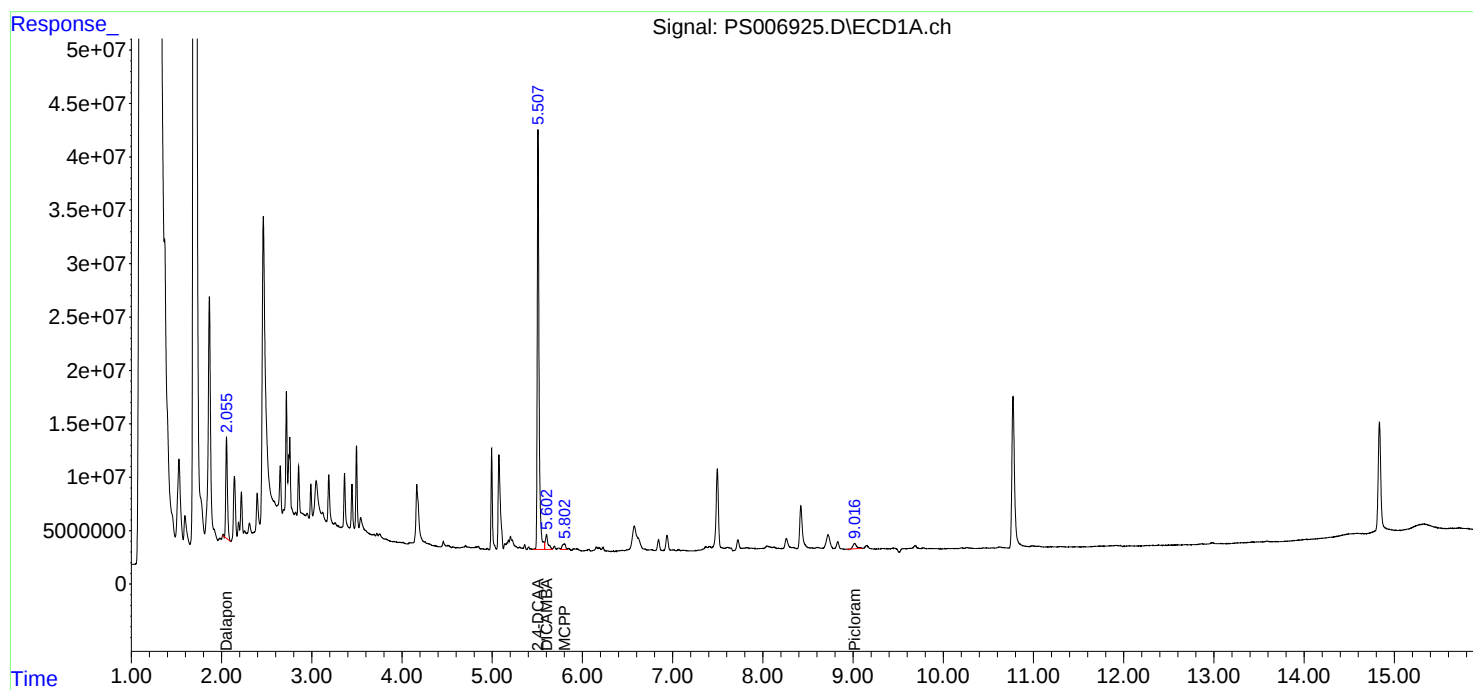


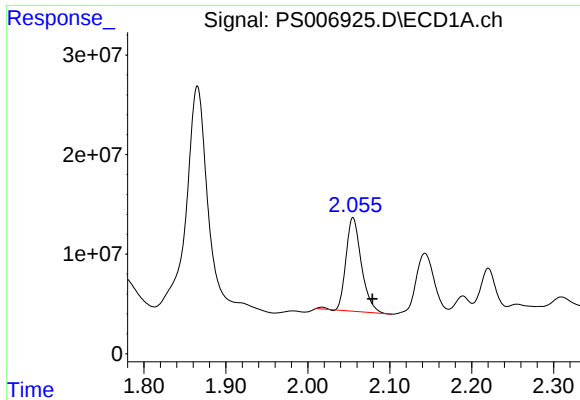

#1 Dalapon


R.T.: 2.055 min
Delta R.T.: -0.024 min
Response: 124128434
Conc: 116.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

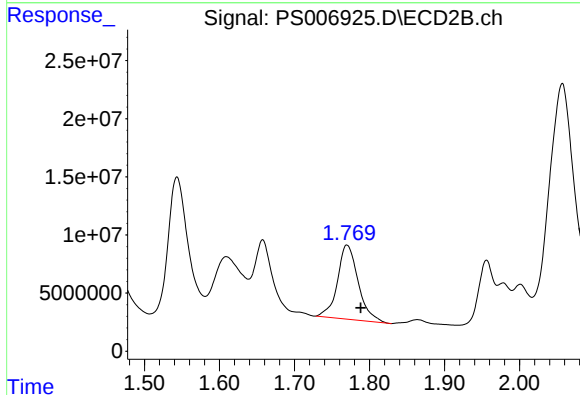


#1 Dalapon

R.T.: 1.770 min
Delta R.T.: -0.018 min
Response: 122619589
Conc: 230.03 ng/ml

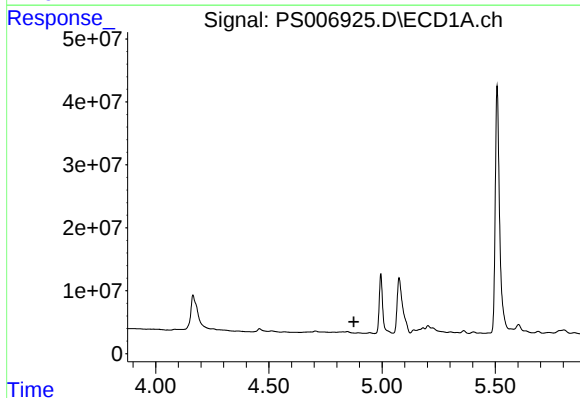


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.876 min
Response: 0
Conc: N.D.

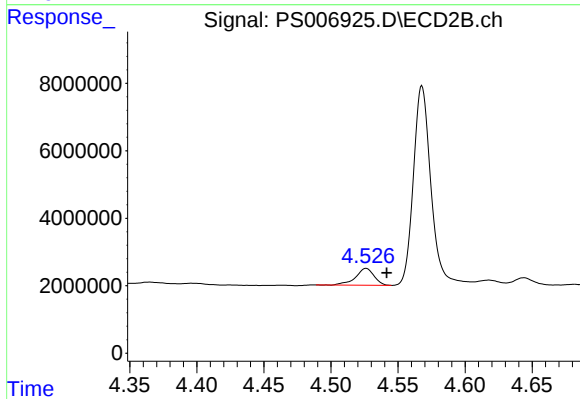

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.526 min
Delta R.T.: -0.015 min
Response: 4723376
Conc: 8.22 ng/ml

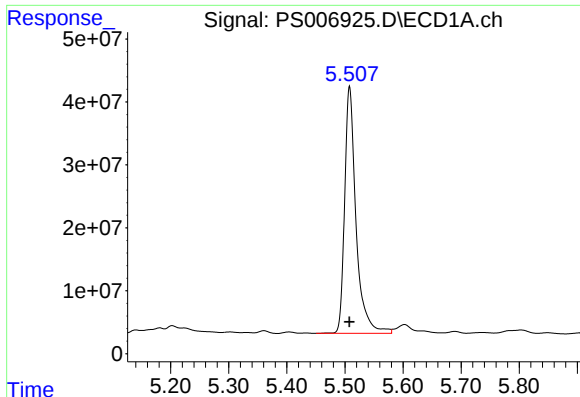

#4 2,4-DCAA


R.T.: 5.508 min
Delta R.T.: 0.000 min
Response: 535504184
Conc: 586.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

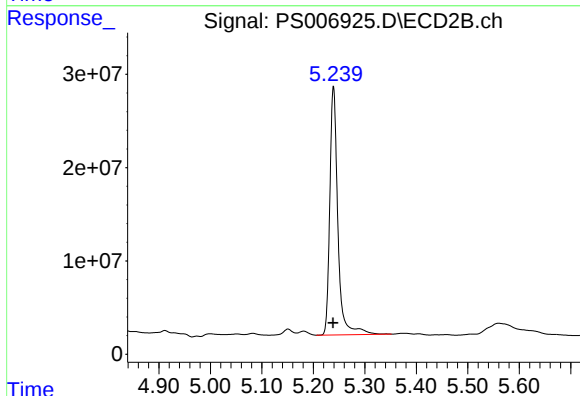


#4 2,4-DCAA

R.T.: 5.239 min
Delta R.T.: 0.001 min
Response: 289821613
Conc: 630.26 ng/ml

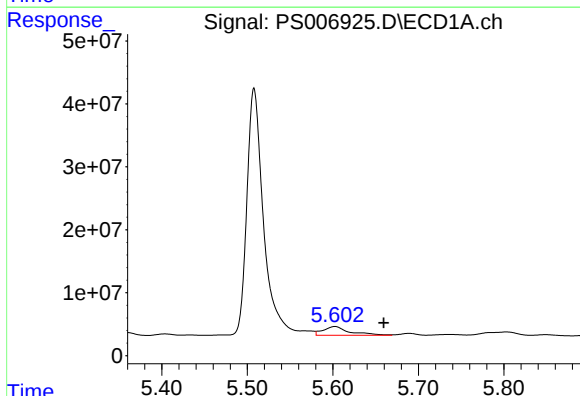


#5 DICAMBA

R.T.: 5.602 min
Delta R.T.: -0.057 min
Response: 30361068
Conc: 9.40 ng/ml

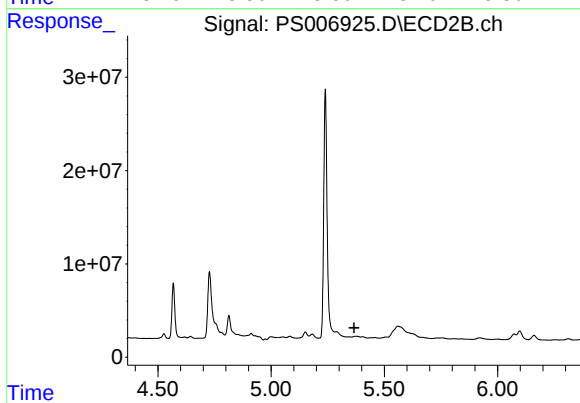

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

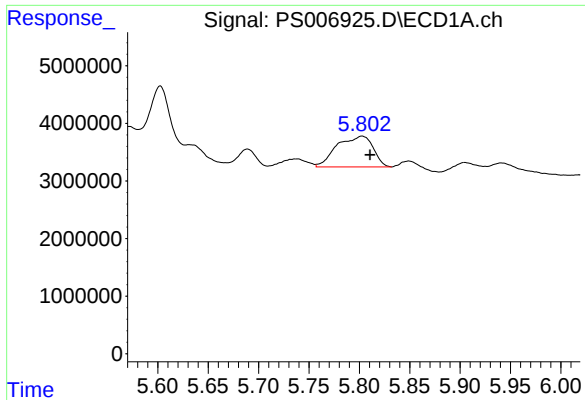

#6 MCPP


R.T.: 5.803 min
Delta R.T.: -0.008 min
Response: 13327015
Conc: 6.26 ug/ml

Instrument :
ECD_S
ClientSampleId :

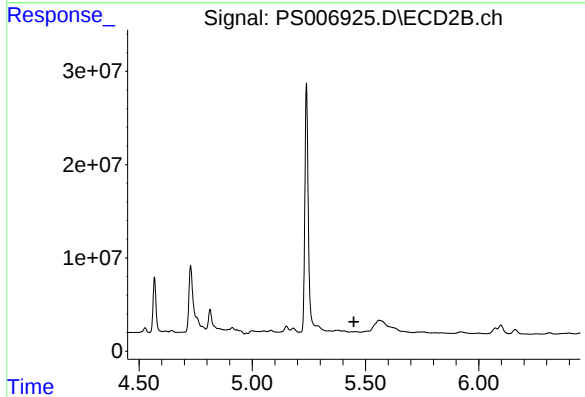


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.449 min
Response: 0
Conc: N.D.

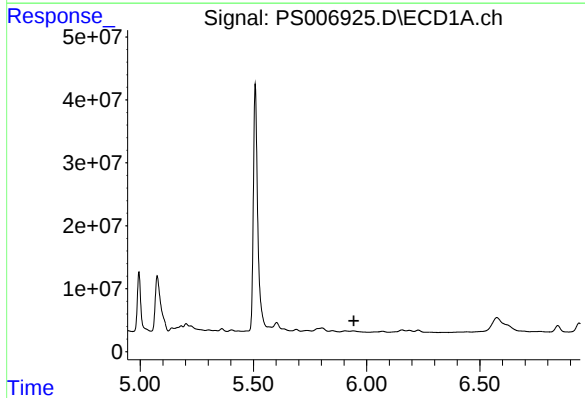


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.944 min
Response: 0
Conc: N.D.

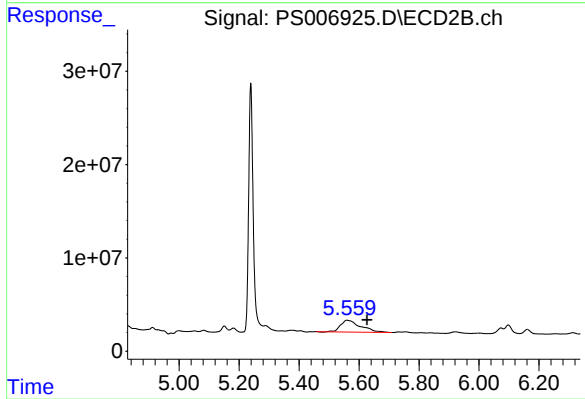

#7 MCPA


R.T.: 5.560 min
Delta R.T.: -0.067 min
Response: 59166222
Conc: 32.15 ug/ml

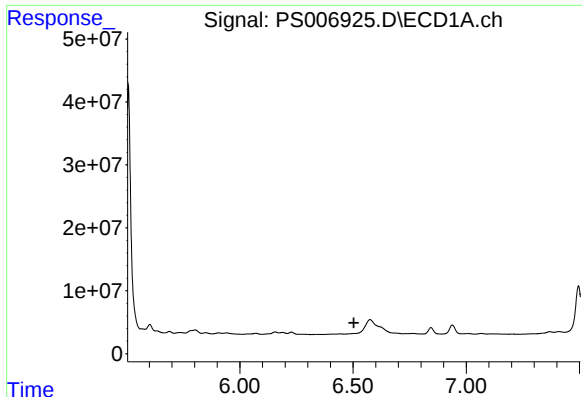

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.504 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

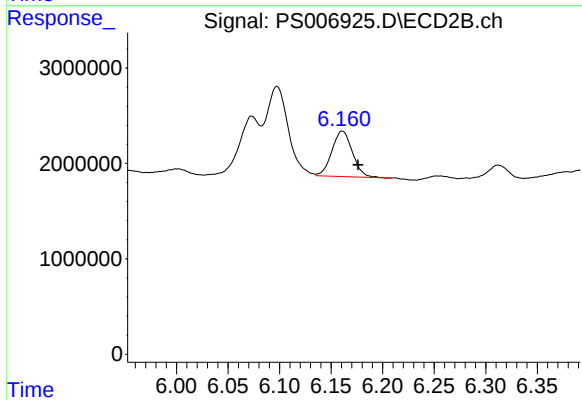


#9 2,4-D

R.T.: 6.161 min
Delta R.T.: -0.015 min
Response: 6626195
Conc: 12.99 ng/ml

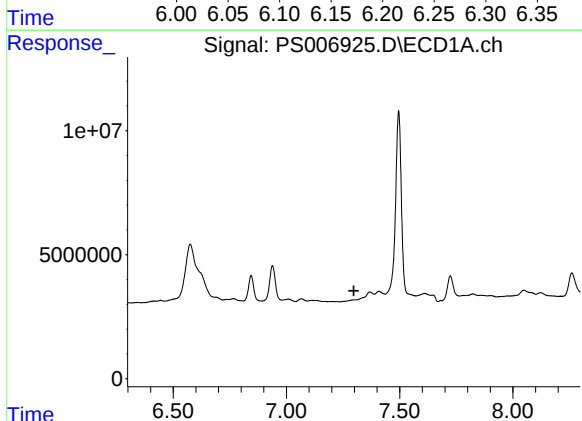


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.298 min
Response: 0
Conc: N.D.

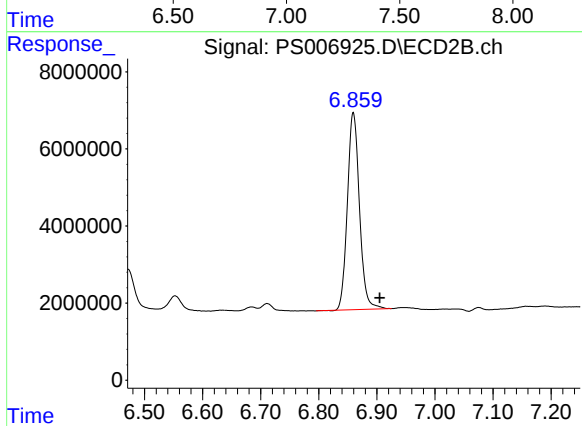

#11 2,4,5-TP (SILVEX)


R.T.: 6.860 min
Delta R.T.: -0.045 min
Response: 74043803
Conc: 30.91 ng/ml

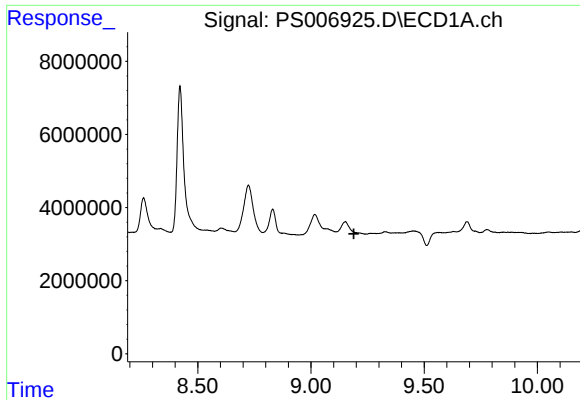

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

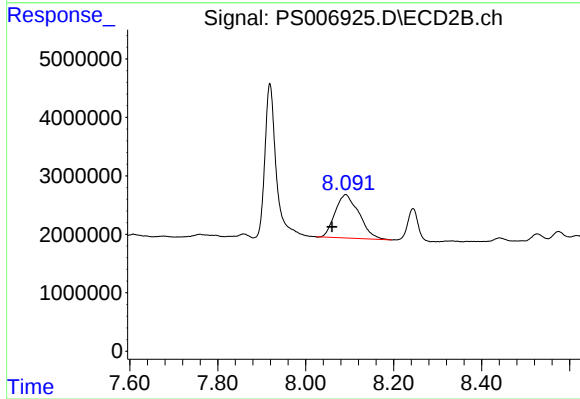


#14 DINOSEB

R.T.: 8.091 min
Delta R.T.: 0.031 min
Response: 28121088
Conc: 16.32 ng/ml

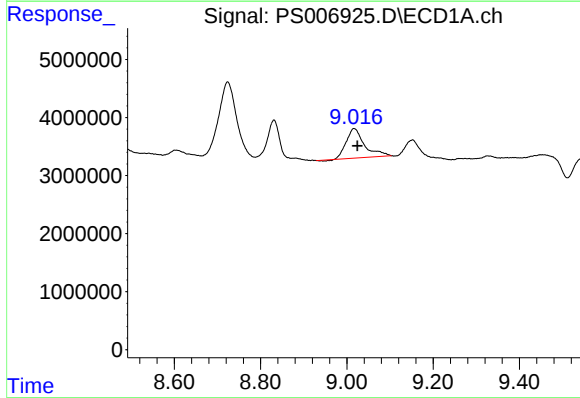

#15 Picloram

R.T.: 9.017 min
Delta R.T.: -0.008 min
Response: 14883384
Conc: 2.22 ng/ml

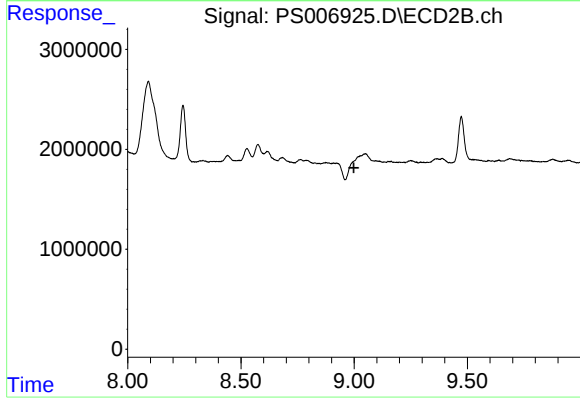

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.999 min
Response: 0
Conc: N.D.