

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092622\
 Data File : PS020653.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2022 13:54
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 00:12:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.181	6.761	1673.8E6	466.3E6	486.362	547.501
Target Compounds							
1) T	Dalapon	3.042f	0.000	1502837	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.451f	0.000	1138305	0	<MDL	N.D. #
3) T	4-Nitroph...	6.990	0.000	1804602	0	128.041	N.D. #
9) T	2,4-D	8.356f	0.000	238.5E6	0	51.304	N.D. #
10) T	Pentachlo...	8.600	0.000	284259	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.106	0.000	6347007	0	<MDL	N.D. #
12) T	2,4,5-T	9.490f	0.000	13358547	0	<MDL	N.D. #
14) T	DINOSEB	11.138	0.000	13679410	0	<MDL	N.D. #
15) T	Picloram	0.000	10.785	0	7188369	N.D.	<MDL
16) T	DCPA	11.442f	10.785	-35486	7188369	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092622\
Data File : PS020653.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2022 13:54
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 00:12:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

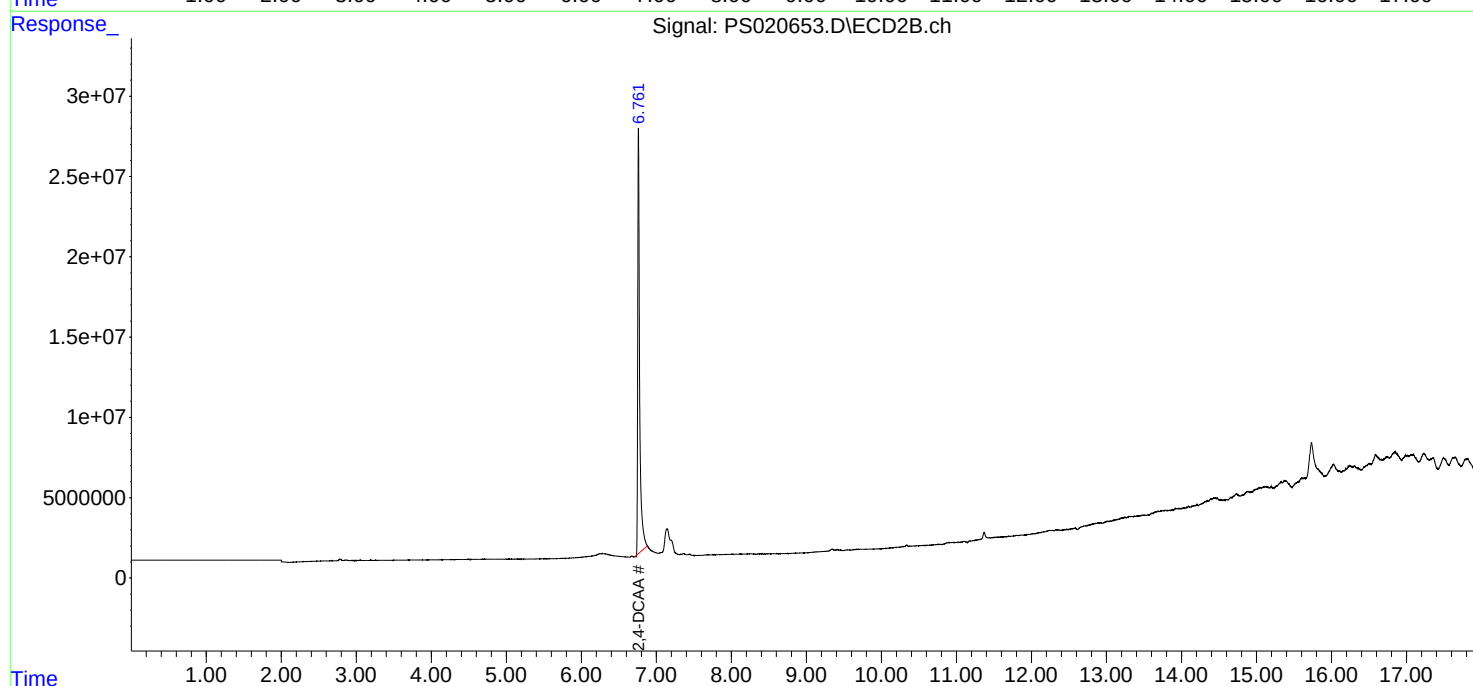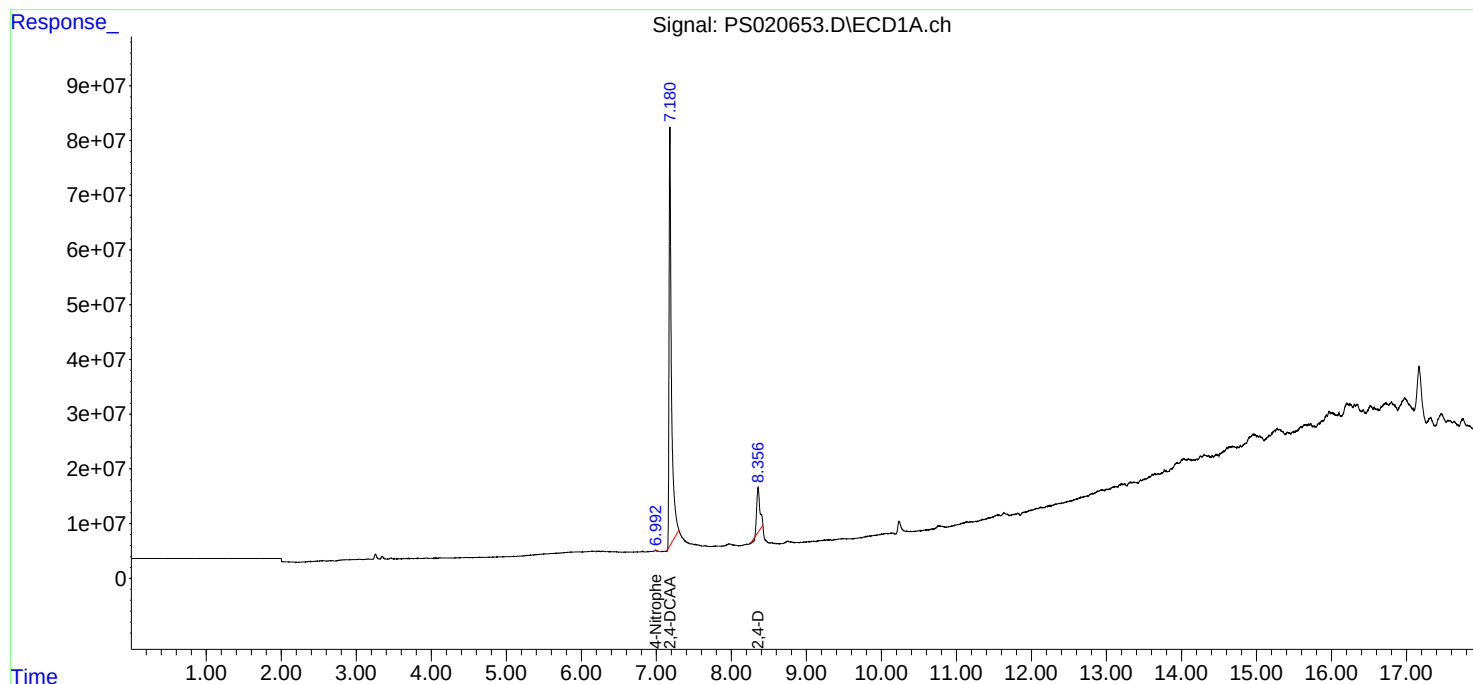


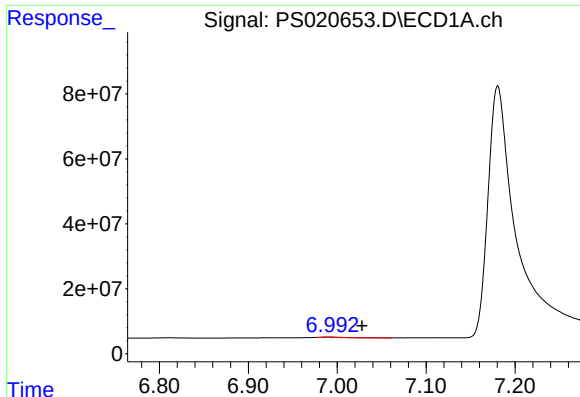

#3 4-Nitrophenol


R.T.: 6.990 min
Delta R.T.: -0.038 min
Response: 1804602
Conc: 128.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

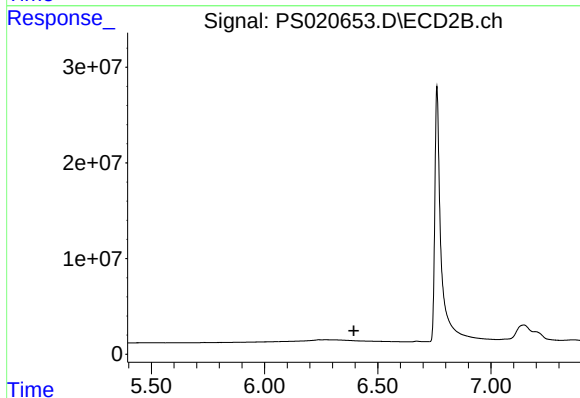


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

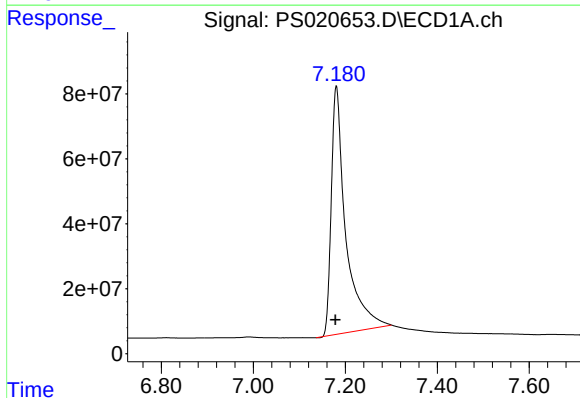


#4 2,4-DCAA

R.T.: 7.181 min
Delta R.T.: 0.002 min
Response: 1673808568
Conc: 486.36 ng/ml

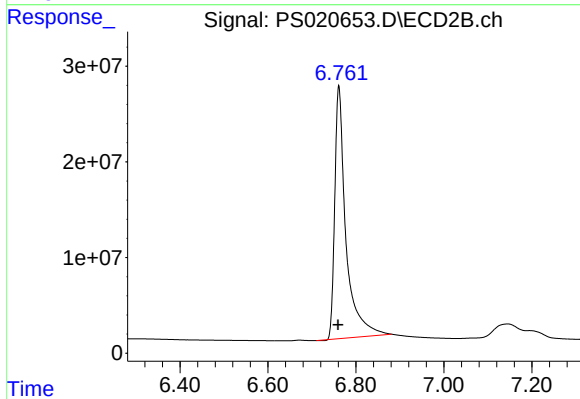

#4 2,4-DCAA


R.T.: 6.761 min
Delta R.T.: 0.002 min
Response: 466303588
Conc: 547.50 ng/ml

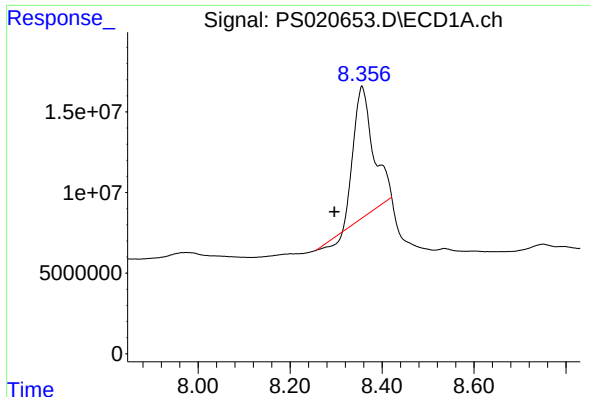

#9 2,4-D

R.T.: 8.356 min
Delta R.T.: 0.060 min
Response: 238462556
Conc: 51.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

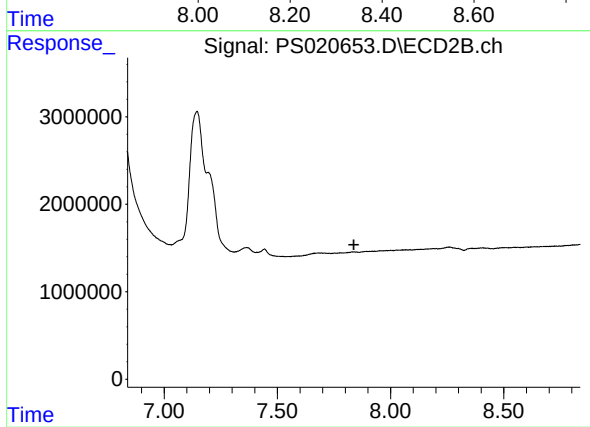

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.