

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092624\
 Data File : PS027779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2024 11:33
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 04:01:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.105	7.627	1225.9E6	492.9E6	492.783	497.375
Target Compounds							
1) T	Dalapon	2.512f	0.000	98984166	0	23.891	N.D. #
3) T	4-Nitroph...	6.904	0.000	14769191	0	8.723	N.D. #
5) T	DICAMBA	0.000	7.868f	0	4035412	N.D.	<MDL
6) T	MCP	0.000	7.973f	0	2381190	N.D.	<MDL
8) T	DICHLORPROP	7.992	8.523	378408	365138	<MDL	<MDL #
10) T	Pentachlo...	8.482	9.329f	1074623	1213732	<MDL	<MDL #
11) T	2,4,5-TP ...	9.038	9.745	5603998	569928	<MDL	<MDL #
12) T	2,4,5-T	9.351	10.164	1255930	663012	<MDL	<MDL #
13) T	2,4-DB	9.908	0.000	2165568	0	<MDL	N.D. #
14) T	DINOSEB	11.070	0.000	2556056	0	<MDL	N.D. #
15) T	Picloram	10.909	12.189	22779763	3914577	1.218	<MDL #
16) T	DCPA	11.366	12.121	17264620	3221389	1.040	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092624\
Data File : PS027779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2024 11:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 04:01:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

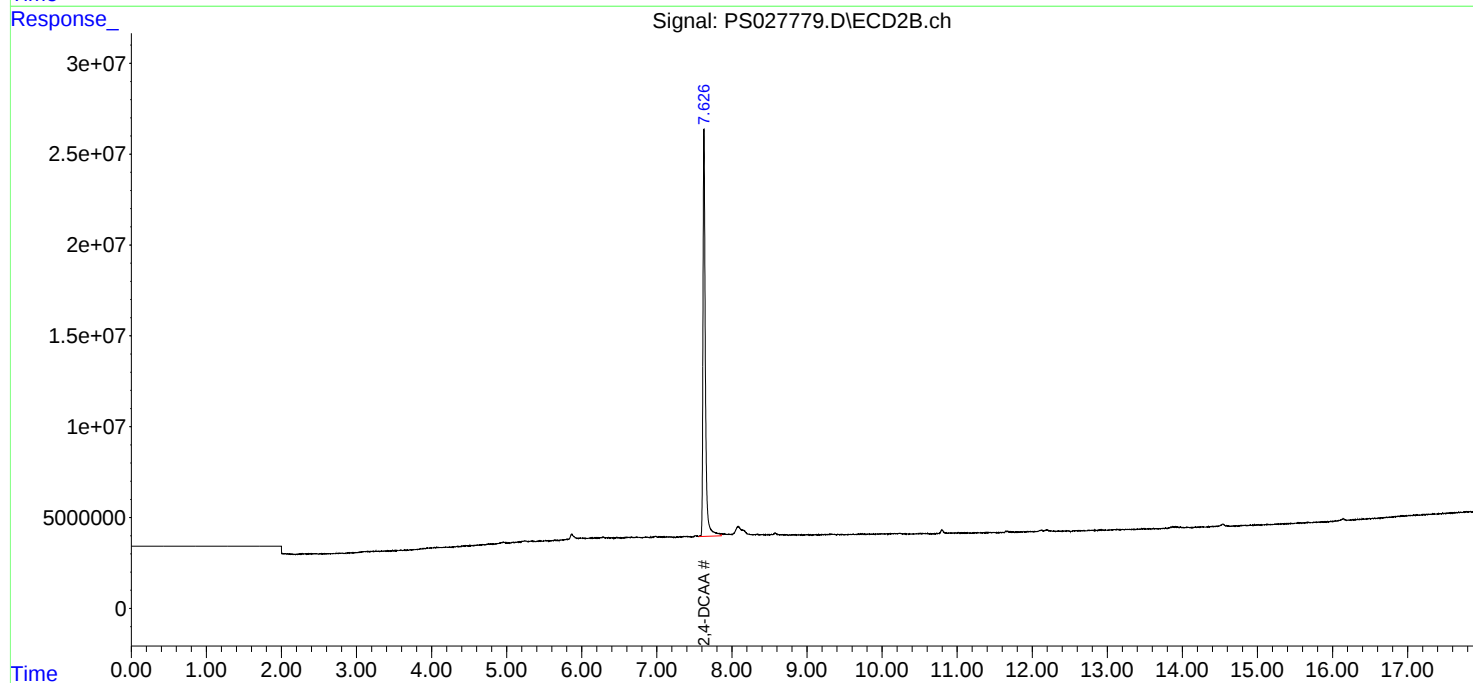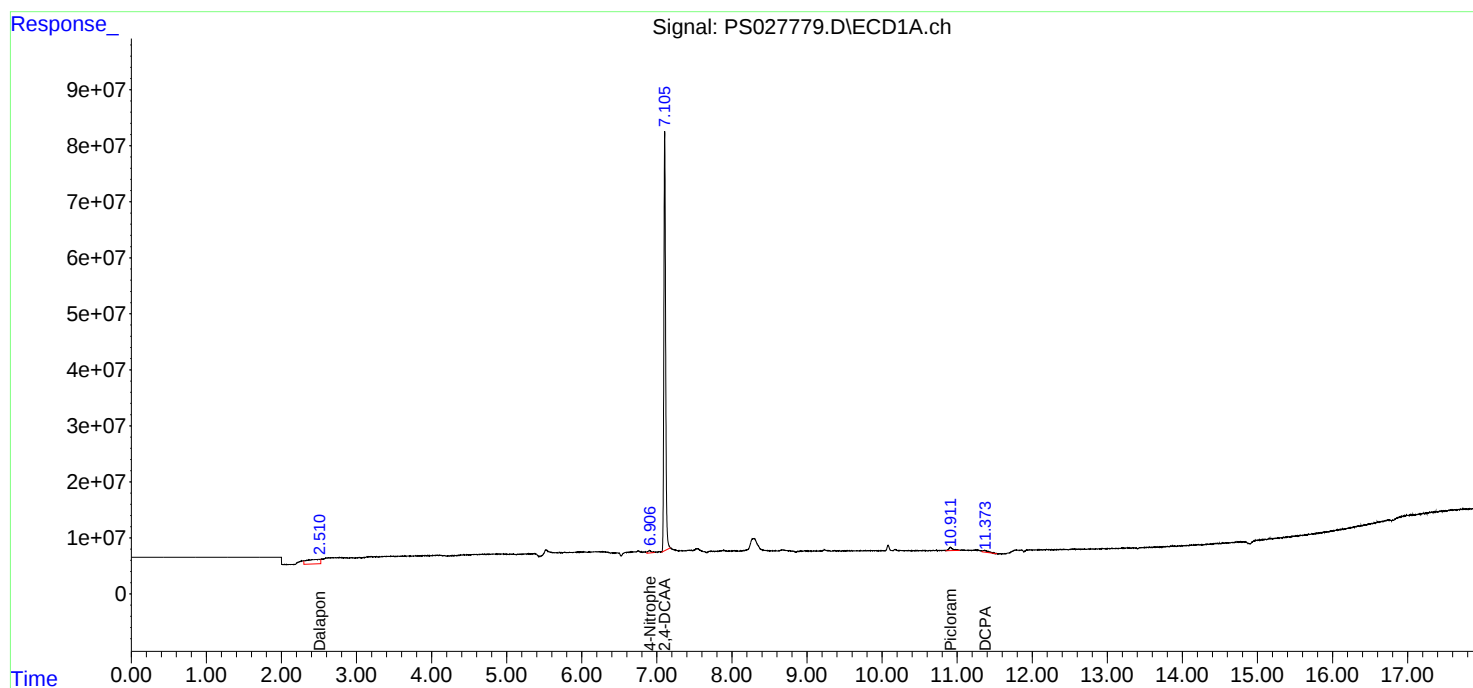


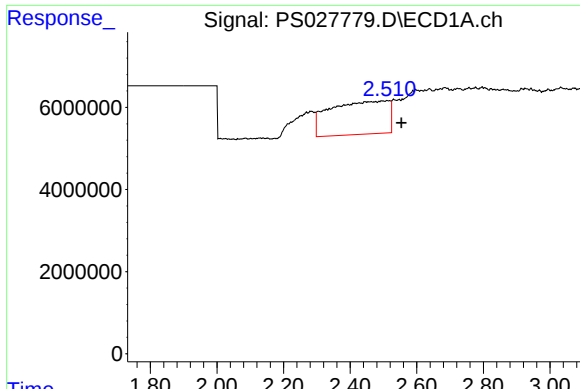

#1 Dalapon


R.T.: 2.512 min
Delta R.T.: -0.042 min
Response: 98984166
Conc: 23.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

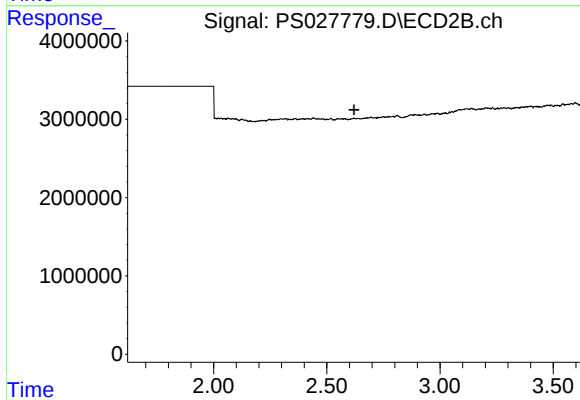


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

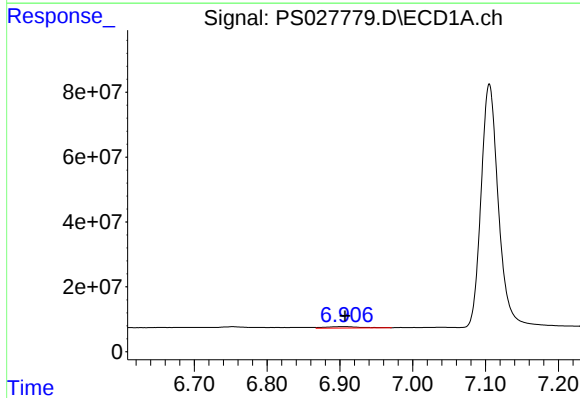


#3 4-Nitrophenol

R.T.: 6.904 min
Delta R.T.: -0.002 min
Response: 14769191
Conc: 8.72 ng/ml

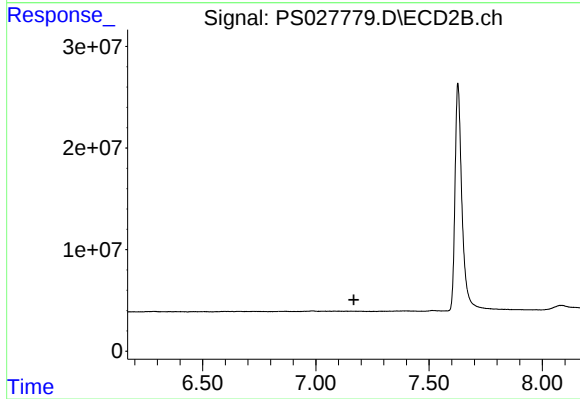

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.168 min
Response: 0
Conc: N.D.

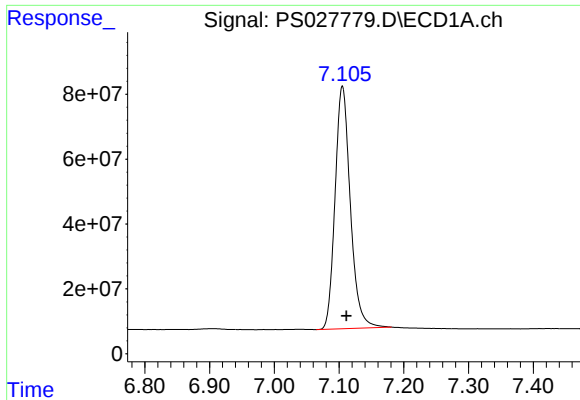

#4 2,4-DCAA


R.T.: 7.105 min
Delta R.T.: -0.006 min
Response: 1225850107
Conc: 492.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

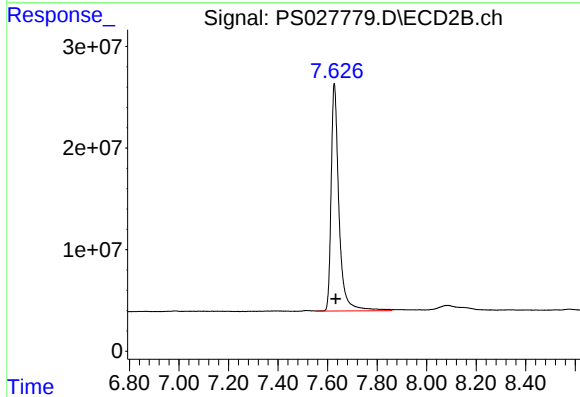


#4 2,4-DCAA

R.T.: 7.627 min
Delta R.T.: -0.006 min
Response: 492915206
Conc: 497.37 ng/ml

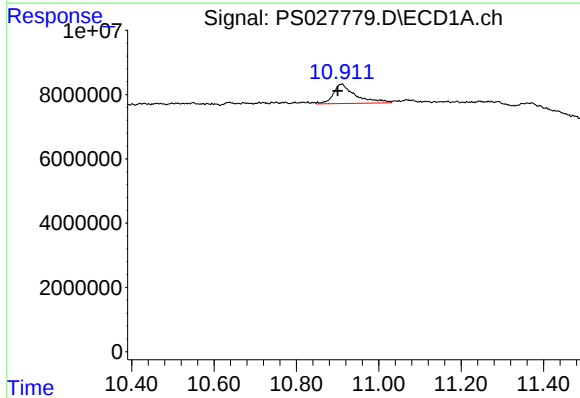


#15 Picloram

R.T.: 10.909 min
Delta R.T.: 0.009 min
Response: 22779763
Conc: 1.22 ng/ml

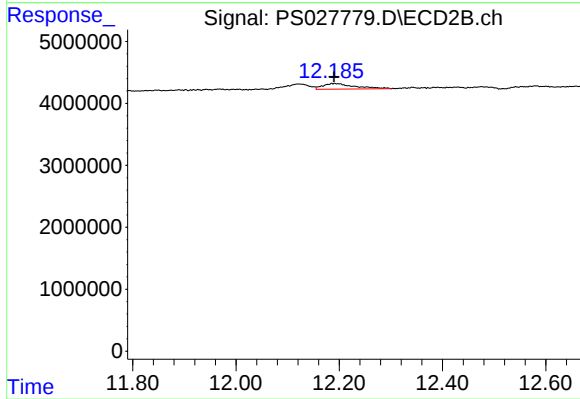

#15 Picloram


R.T.: 12.189 min
Delta R.T.: 0.000 min
Response: 3914577
Conc: N.D.

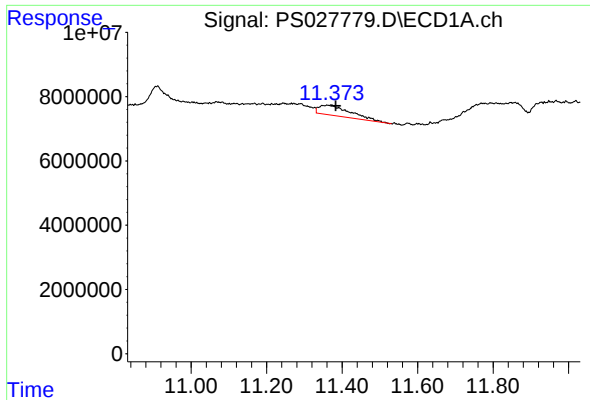

#16 DCPA

R.T.: 11.366 min
Delta R.T.: -0.018 min
Response: 17264620
Conc: 1.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

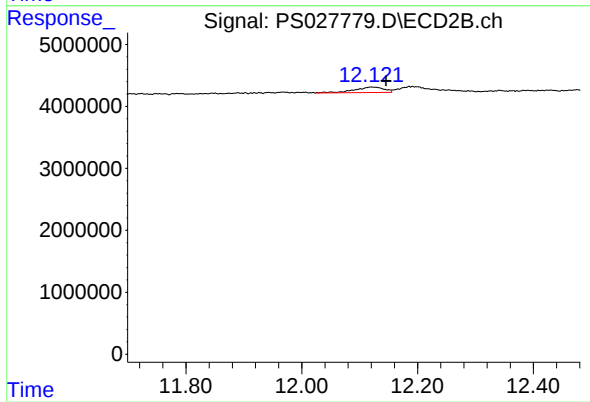

#16 DCPA

R.T.: 12.121 min
Delta R.T.: -0.024 min
Response: 3221389
Conc: N.D.