

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092718\
 Data File : PS001838.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2018 18:56
 Operator : EI\SJ
 Sample : J5097-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 02:00:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.478	10.975	80665249	81566610	359.606	321.107
Target Compounds							
1) T	Dalapon	2.910	2.392	47687434	76885504	146.655	260.261 #
5) T	DICAMBA	0.000	11.217	0	18613796	N.D.	20.870 #
6) T	MCPD	12.165	0.000	19134284	0	30.027	N.D. #
9) T	2,4-D	0.000	12.809	0	3116497	N.D.	10.017 #
15) T	Picloram	0.000	16.909	0	71347	N.D.	0.042 #
16) T	DCPA	0.000	16.909	0	71347	N.D.	0.039 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092718\
Data File : PS001838.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2018 18:56
Operator : EI\SJ
Sample : J5097-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 02:00:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

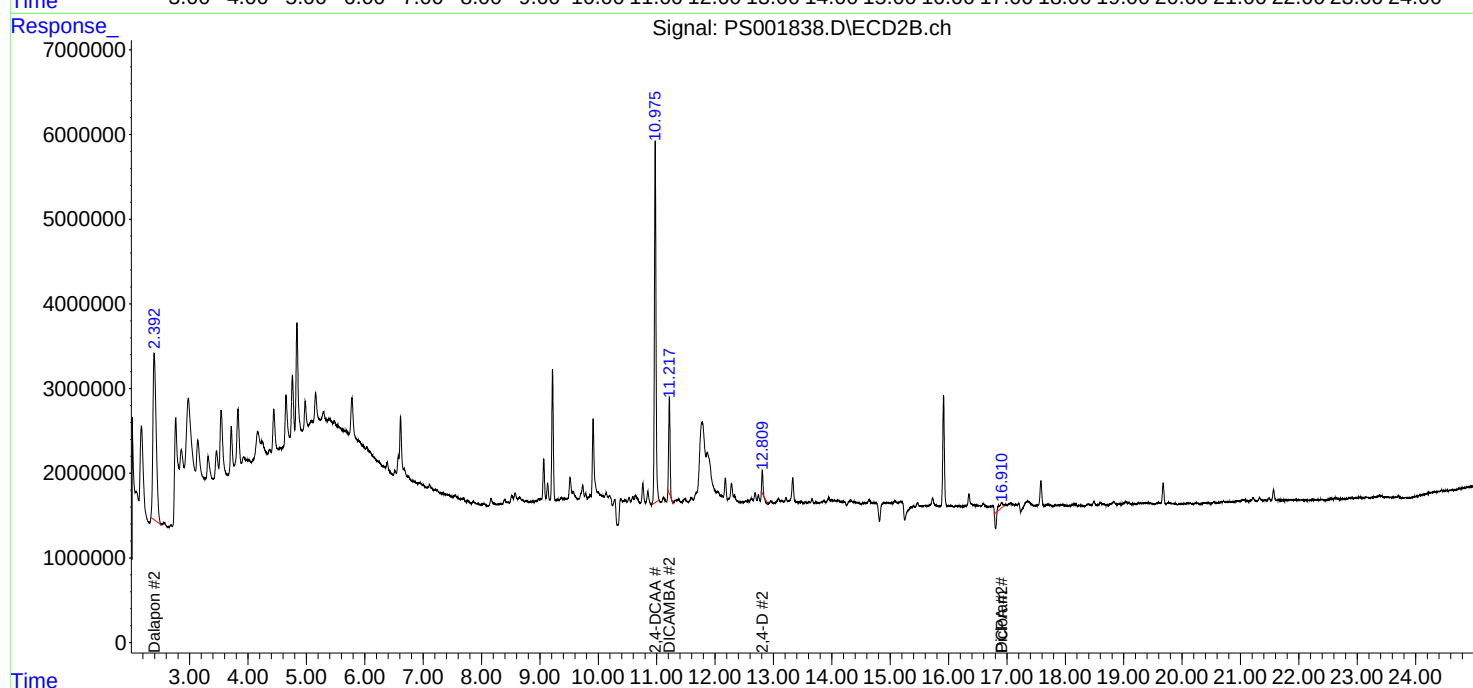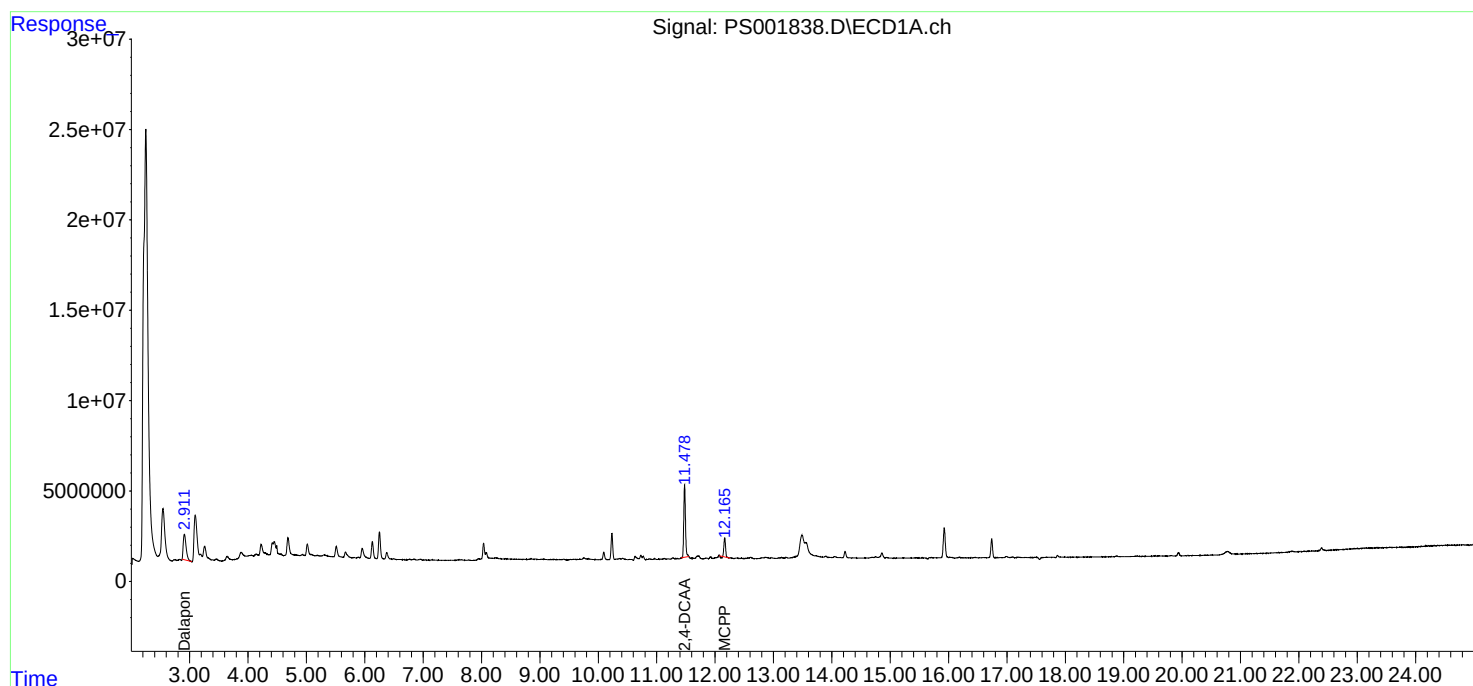


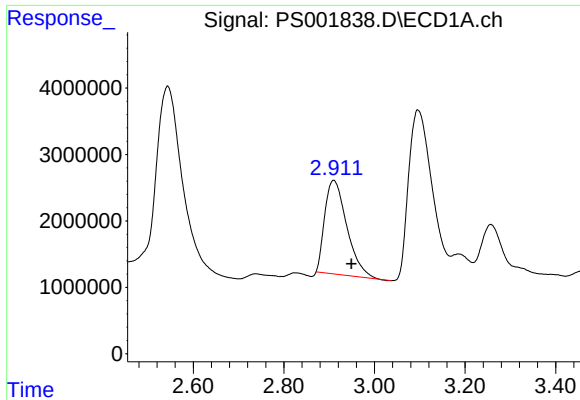

#1 Dalapon


R.T.: 2.910 min
Delta R.T.: -0.039 min
Response: 47687434
Conc: 146.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

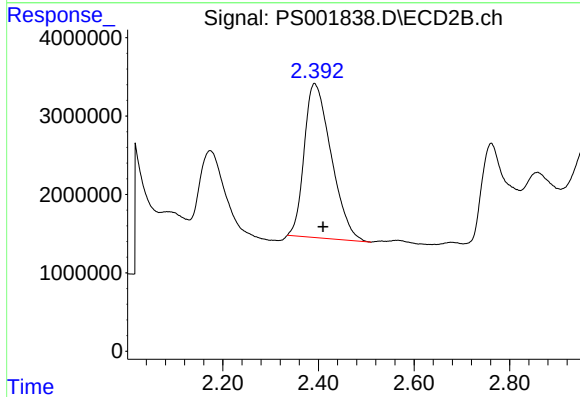


#1 Dalapon

R.T.: 2.392 min
Delta R.T.: -0.018 min
Response: 76885504
Conc: 260.26 ng/ml

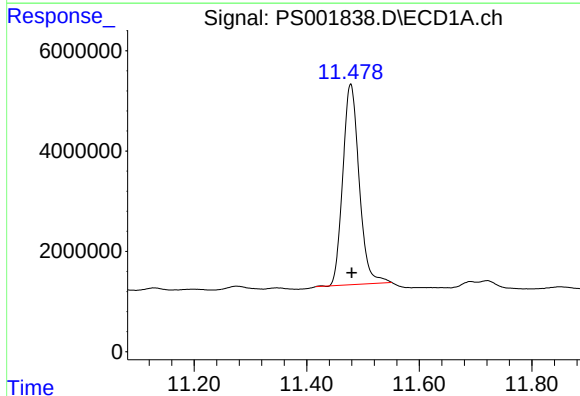


#4 2,4-DCAA

R.T.: 11.478 min
Delta R.T.: -0.002 min
Response: 80665249
Conc: 359.61 ng/ml

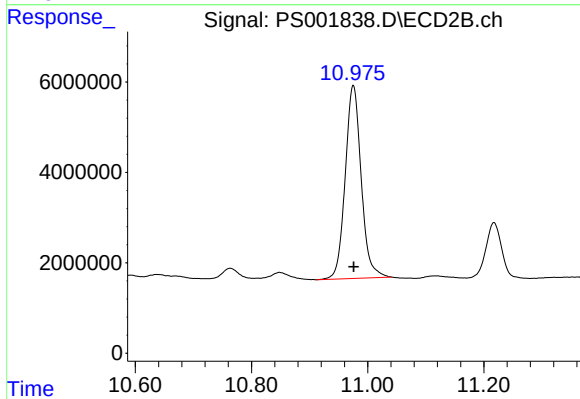

#4 2,4-DCAA


R.T.: 10.975 min
Delta R.T.: 0.000 min
Response: 81566610
Conc: 321.11 ng/ml

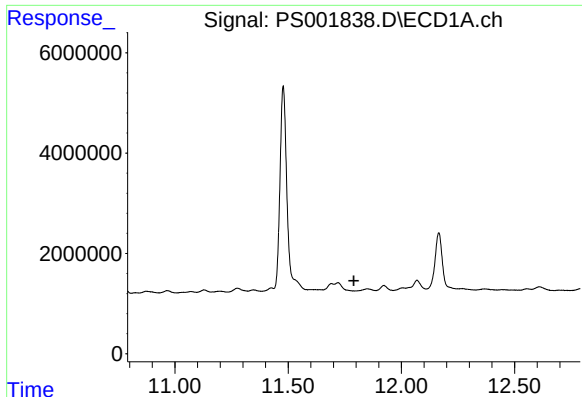

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

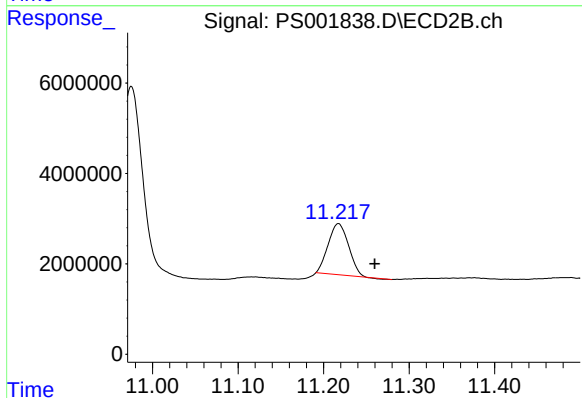


#5 DICAMBA

R.T.: 11.217 min
Delta R.T.: -0.042 min
Response: 18613796
Conc: 20.87 ng/ml

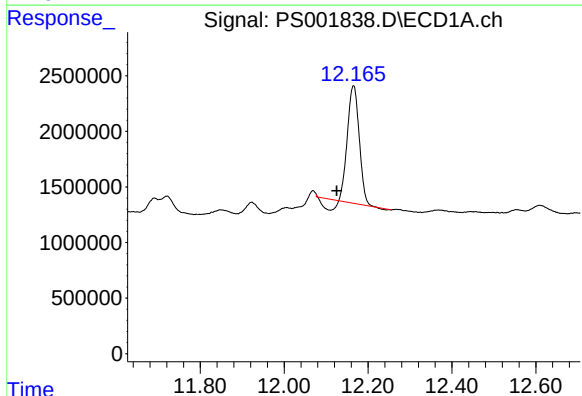


#6 MCP

R.T.: 12.165 min
Delta R.T.: 0.040 min
Response: 19134284
Conc: 30.03 ug/ml

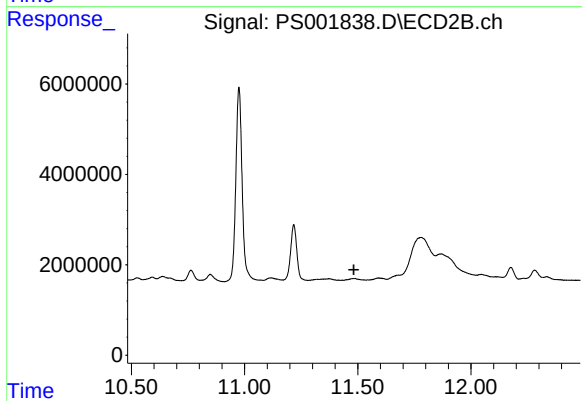

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.483 min
Response: 0
Conc: N.D.

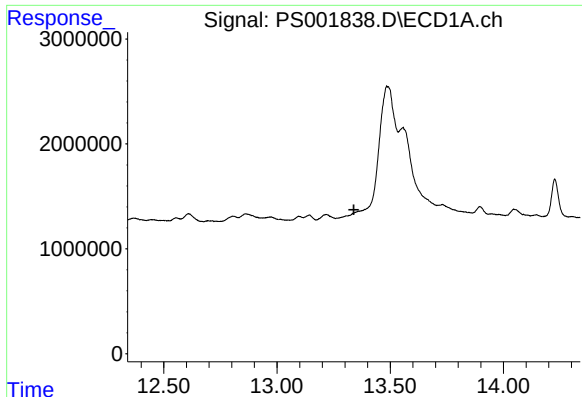

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

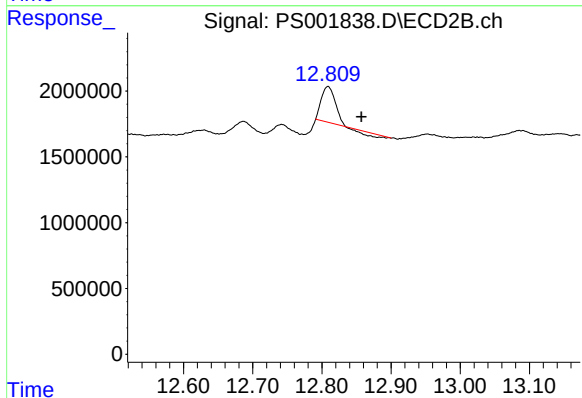


#9 2,4-D

R.T.: 12.809 min
Delta R.T.: -0.048 min
Response: 3116497
Conc: 10.02 ng/ml

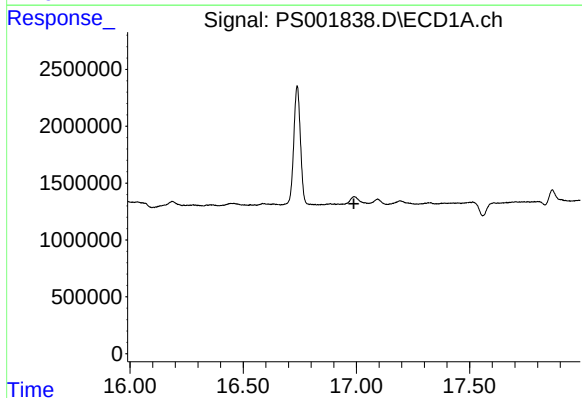


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.988 min
Response: 0
Conc: N.D.

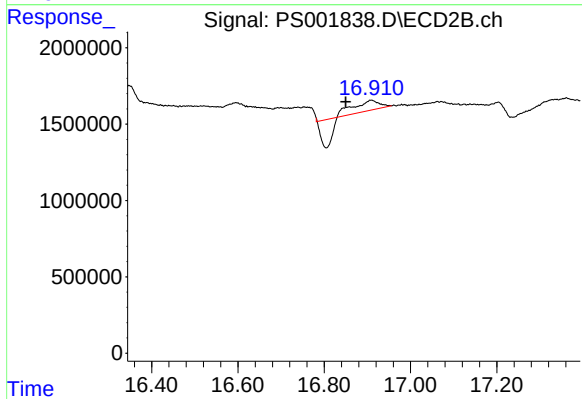

#15 Picloram


R.T.: 16.909 min
Delta R.T.: 0.059 min
Response: 71347
Conc: 0.04 ng/ml

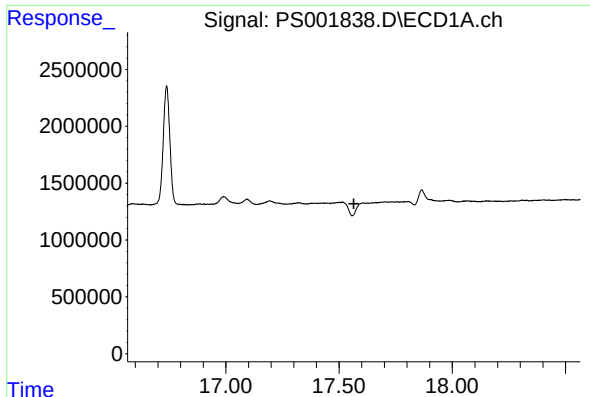

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

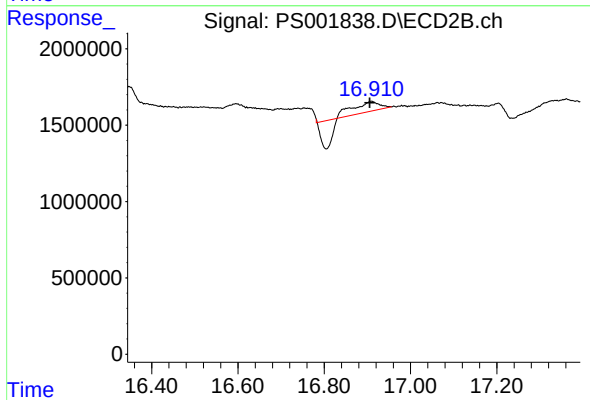

#16 DCPA

R.T.: 16.909 min
Delta R.T.: 0.003 min
Response: 71347
Conc: 0.04 ng/ml