

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092719\
 Data File : PS006929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2019 08:50
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:08:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.506	5.244	418.1E6	208.6E6	457.533	453.529
Target Compounds							
7) T	MCPA	0.000	5.576	0	39522446	N.D.	21.473
9) T	2,4-D	6.572	0.000	72027533	0	87.891	N.D. #
14) T	DINOSEB	9.122	0.000	44144008	0	11.623	N.D. #
15) T	Picloram	0.000	9.046	0	19047986	N.D.	5.233



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092719\
Data File : PS006929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2019 08:50
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:08:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

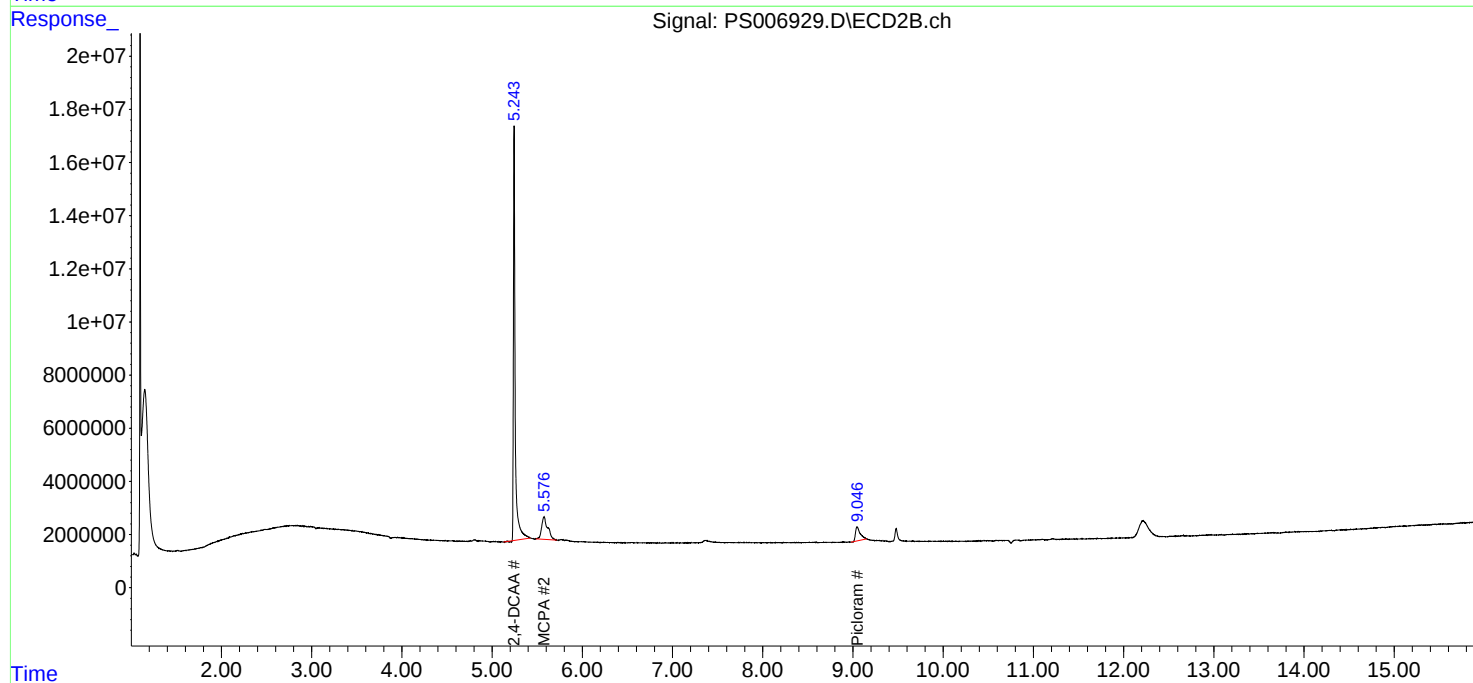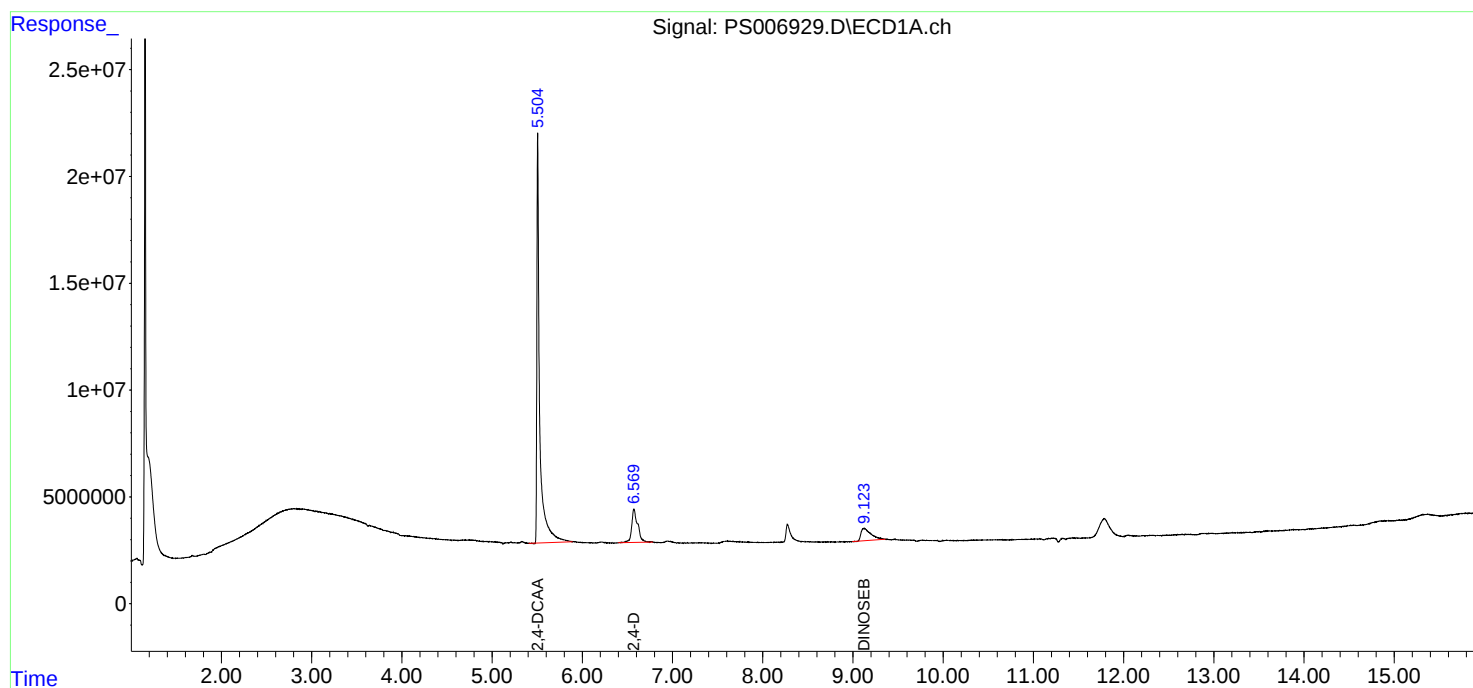


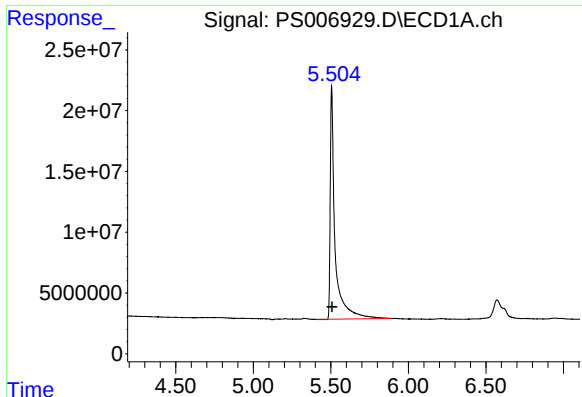

#4 2,4-DCAA


R.T.: 5.506 min
Delta R.T.: -0.002 min
Response: 418100405
Conc: 457.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

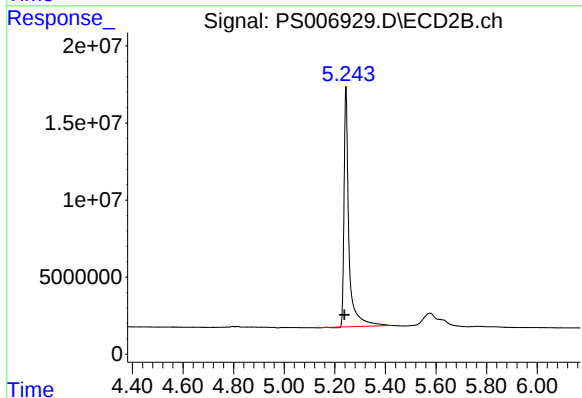


#4 2,4-DCAA

R.T.: 5.244 min
Delta R.T.: 0.006 min
Response: 208551472
Conc: 453.53 ng/ml

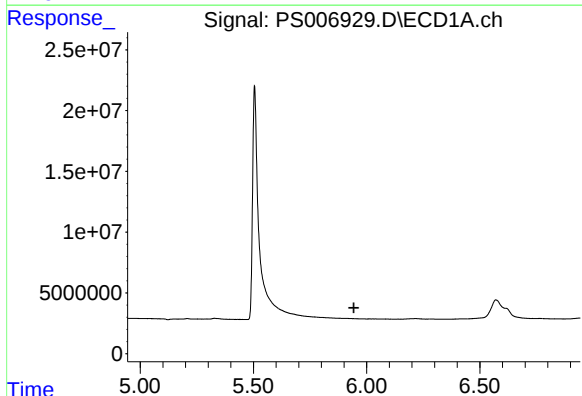


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.944 min
Response: 0
Conc: N.D.

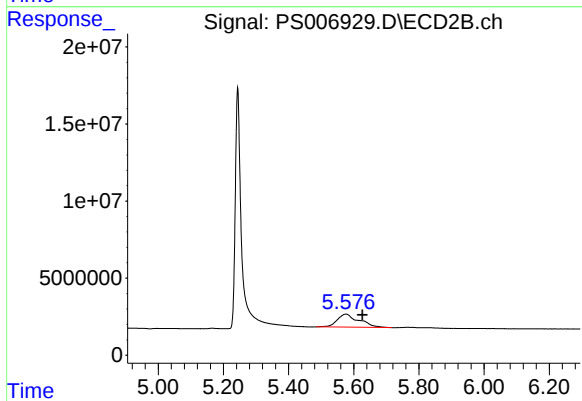

#7 MCPA


R.T.: 5.576 min
Delta R.T.: -0.051 min
Response: 39522446
Conc: 21.47 ug/ml

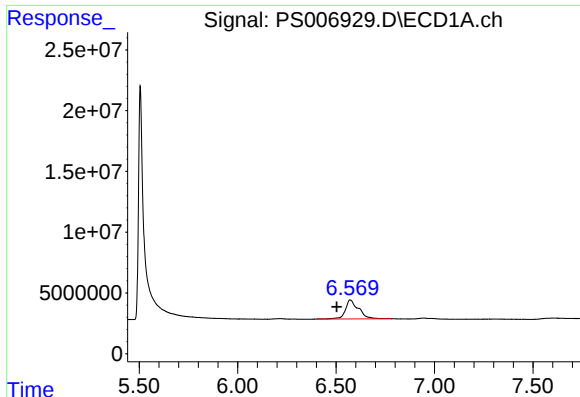

#9 2,4-D


R.T.: 6.572 min
Delta R.T.: 0.068 min
Response: 72027533
Conc: 87.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

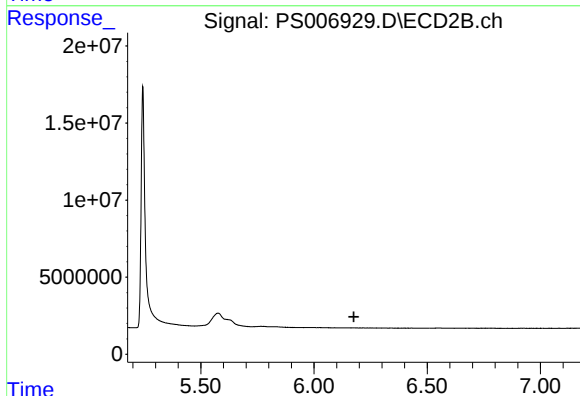


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

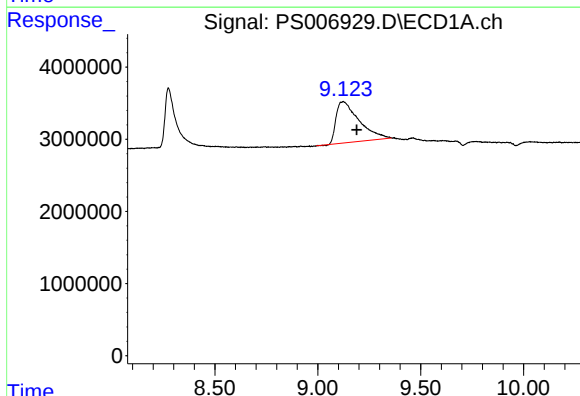


#14 DINOSEB

R.T.: 9.122 min
Delta R.T.: -0.067 min
Response: 44144008
Conc: 11.62 ng/ml

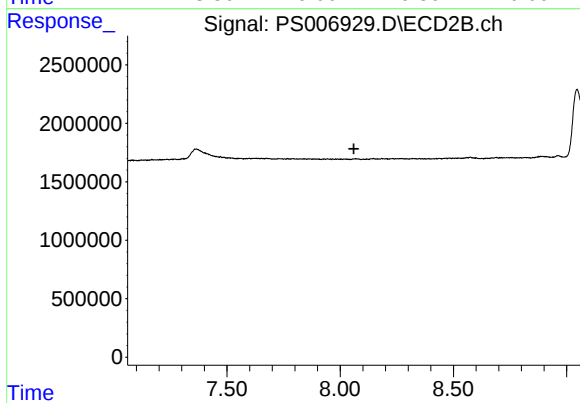

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.060 min
Response: 0
Conc: N.D.

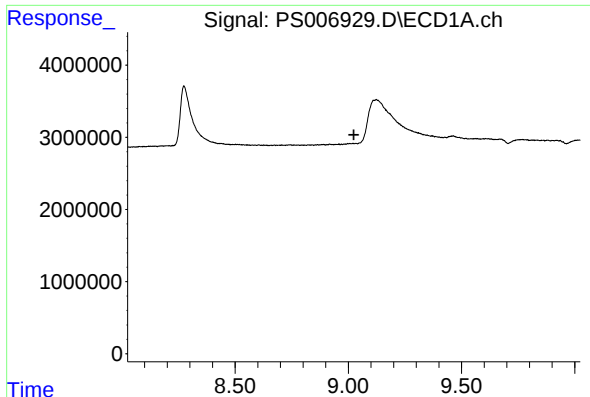

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.025 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

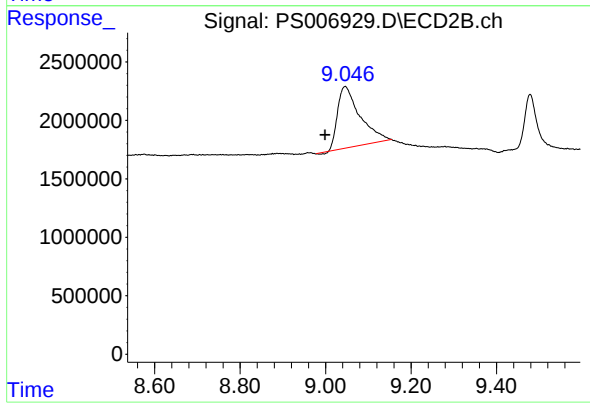

#15 Picloram

R.T.: 9.046 min
Delta R.T.: 0.047 min
Response: 19047986
Conc: 5.23 ng/ml