

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092719\
 Data File : PS006935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2019 13:05
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:10:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.502	5.232	401.3E6	202.6E6	439.103	440.684
Target Compounds							
7) T	MCPA	0.000	5.559	0	49578043	N.D.	26.936
9) T	2,4-D	6.565	0.000	90926775	0	110.952	N.D. #
10) T	Pentachlo...	6.762	0.000	8077050	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092719\
Data File : PS006935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2019 13:05
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:10:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

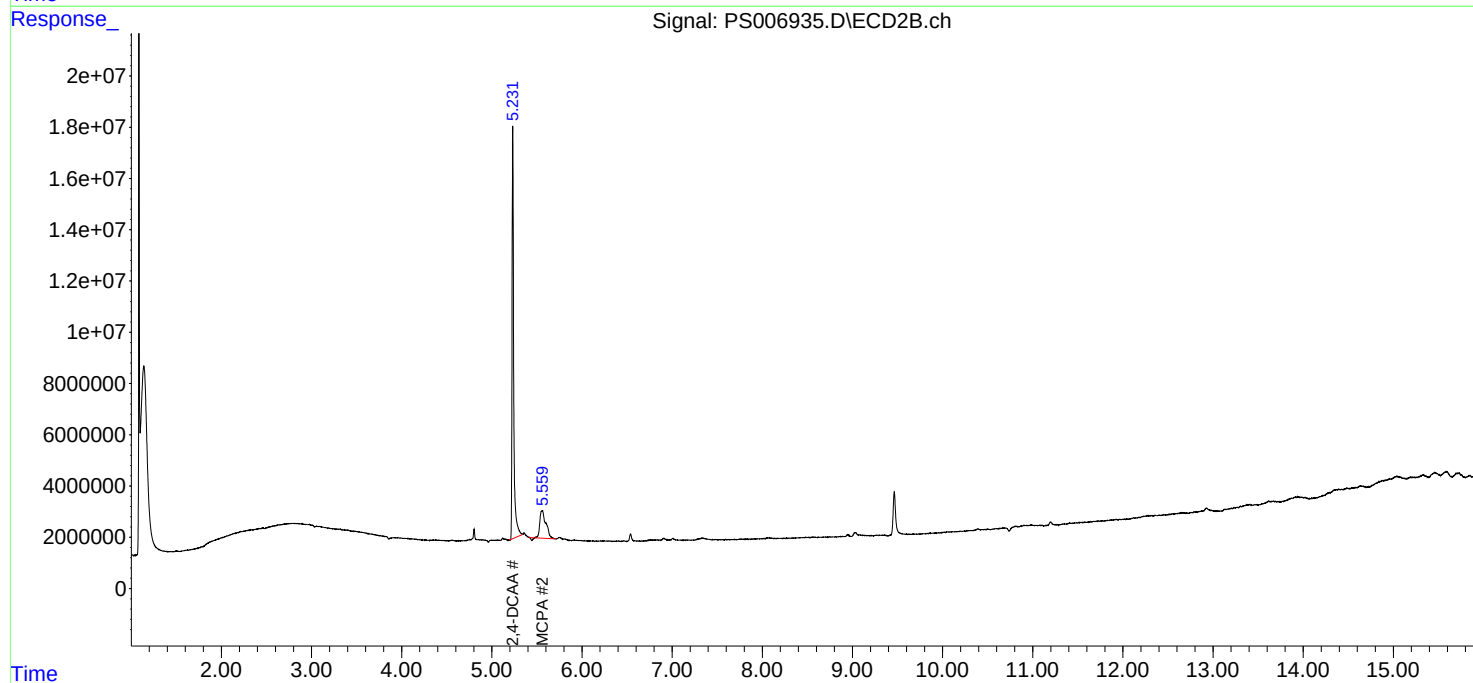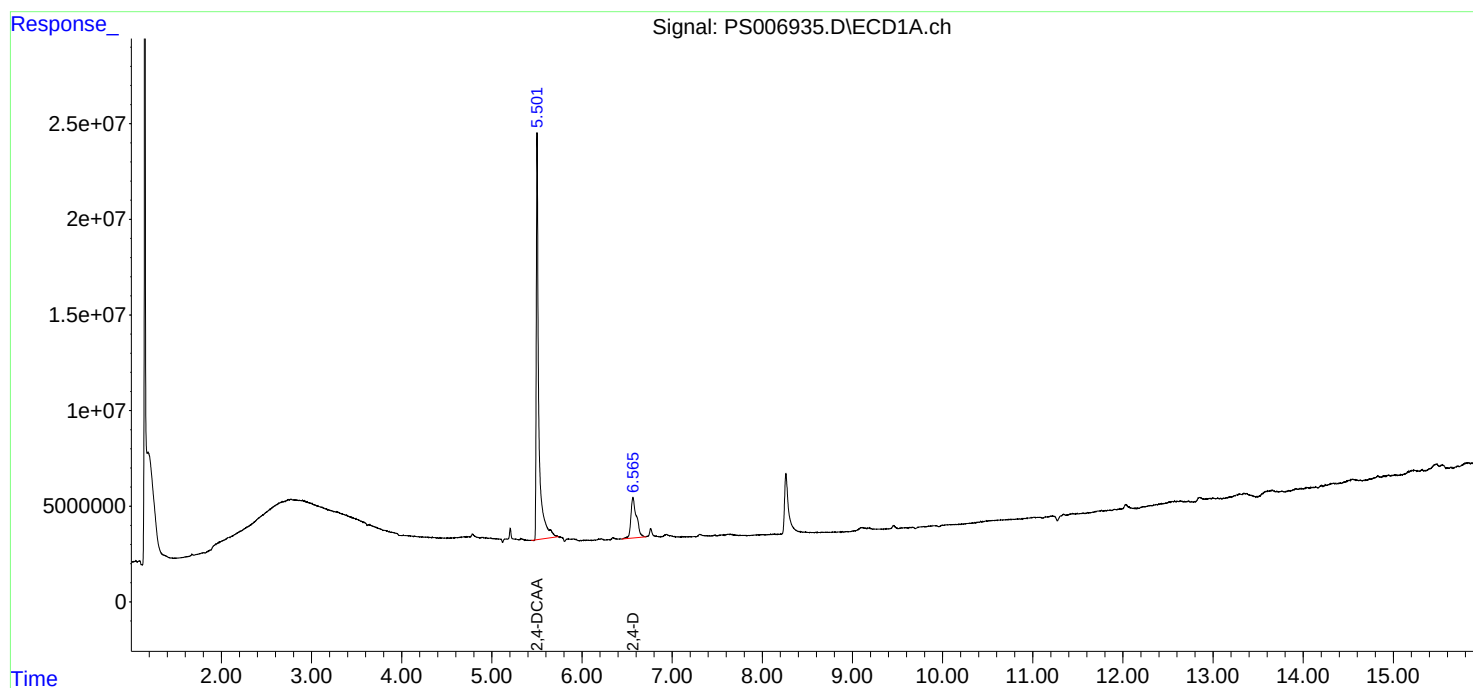


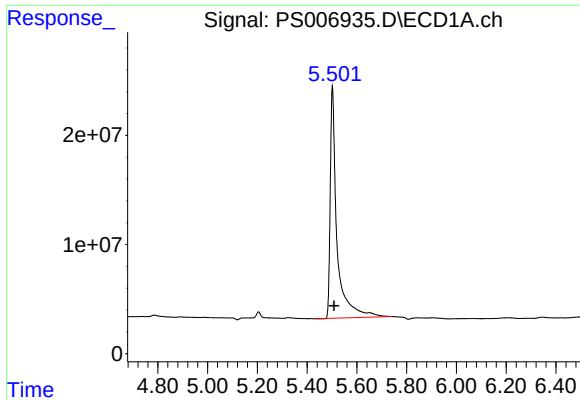

#4 2,4-DCAA


R.T.: 5.502 min
Delta R.T.: -0.006 min
Response: 401258399
Conc: 439.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

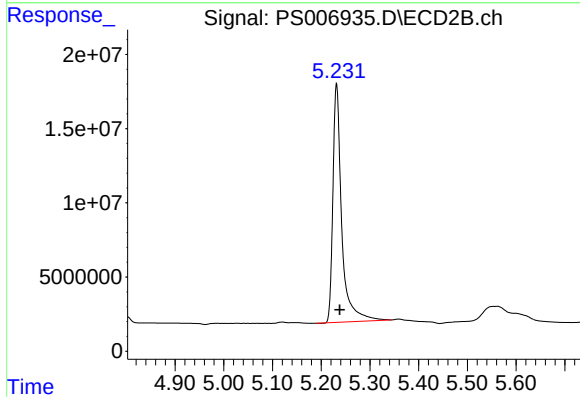


#4 2,4-DCAA

R.T.: 5.232 min
Delta R.T.: -0.006 min
Response: 202644938
Conc: 440.68 ng/ml

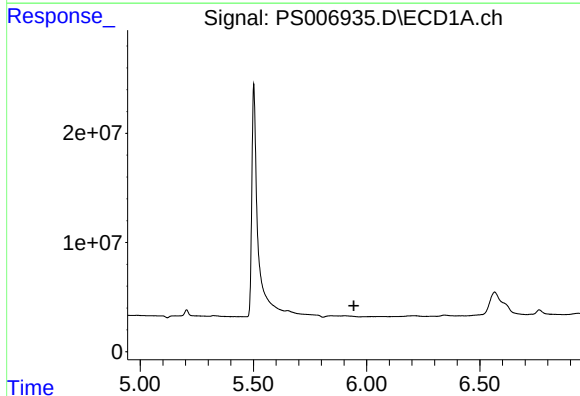


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.944 min
Response: 0
Conc: N.D.

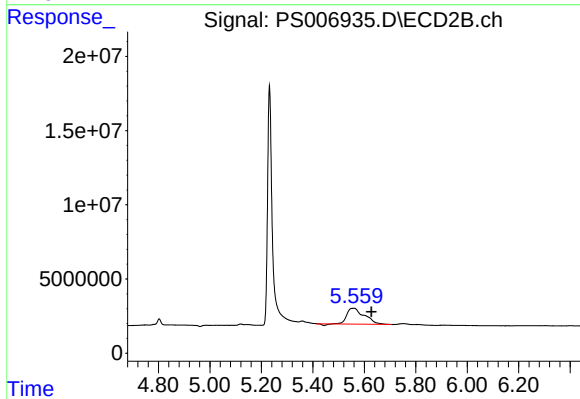

#7 MCPA


R.T.: 5.559 min
Delta R.T.: -0.068 min
Response: 49578043
Conc: 26.94 ug/ml

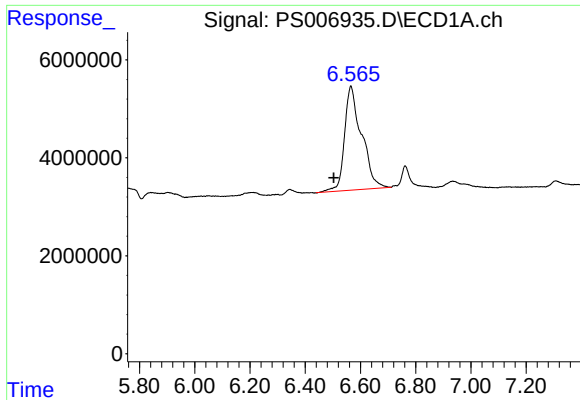

#9 2,4-D

R.T.: 6.565 min
Delta R.T.: 0.062 min
Response: 90926775
Conc: 110.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

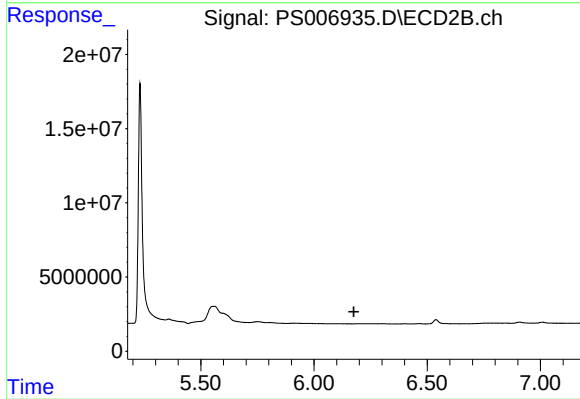

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.