

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092721\
 Data File : PS016899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2021 09:01
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:37:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.237f	0.000	5911252	0	3.880	N.D. #
Target Compounds							
13) T	2,4-DB	9.956	0.000	4742013	0	2.869	N.D. #
15) T	Picloram	10.937	10.787	40429547	12878541	3.397	3.002
16) T	DCPA	0.000	10.787	0	12878541	N.D.	2.955



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092721\
Data File : PS016899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2021 09:01
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:37:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

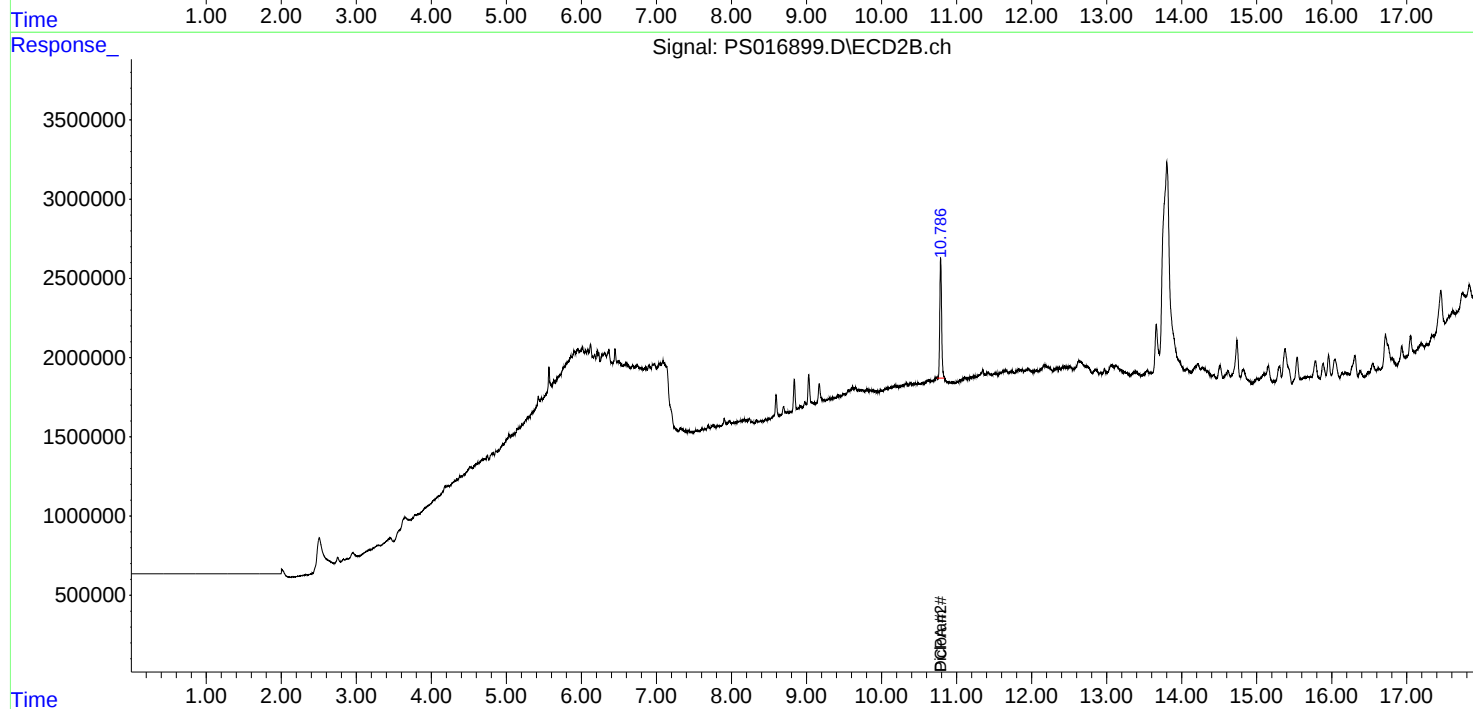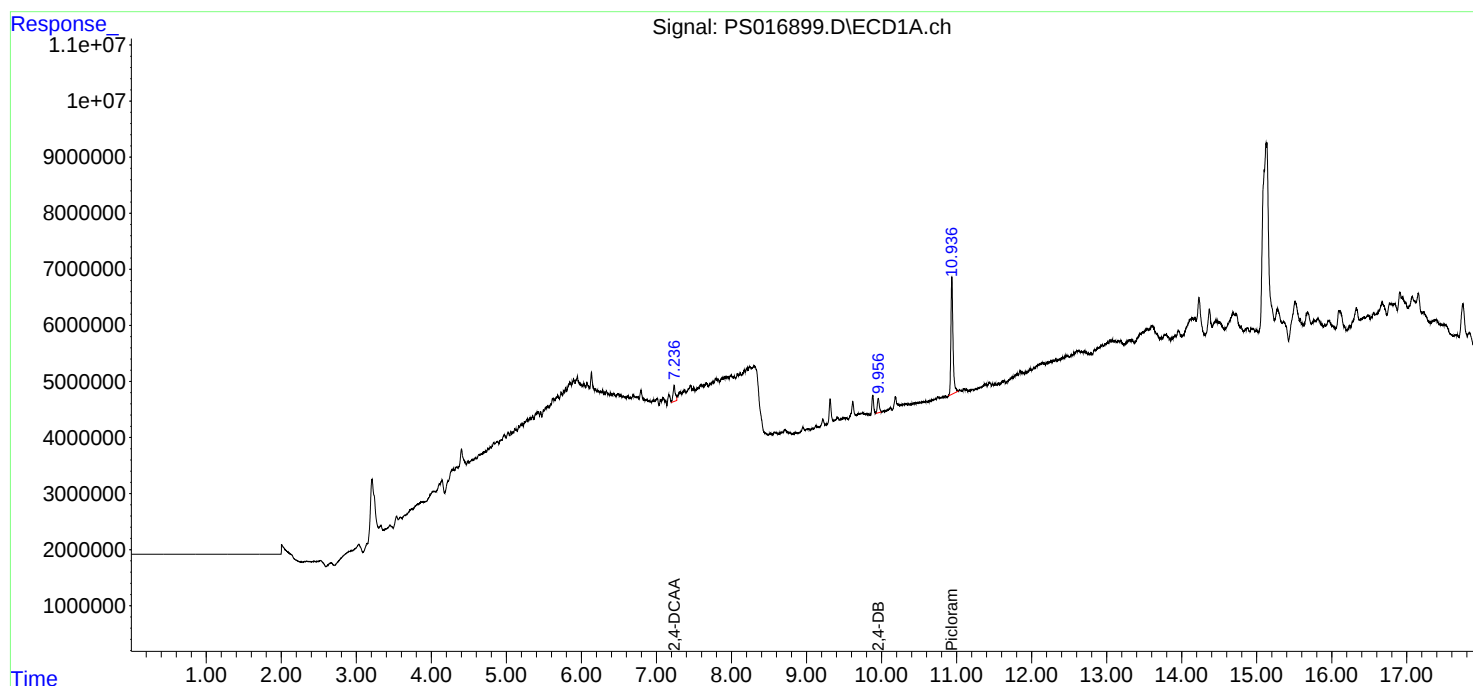


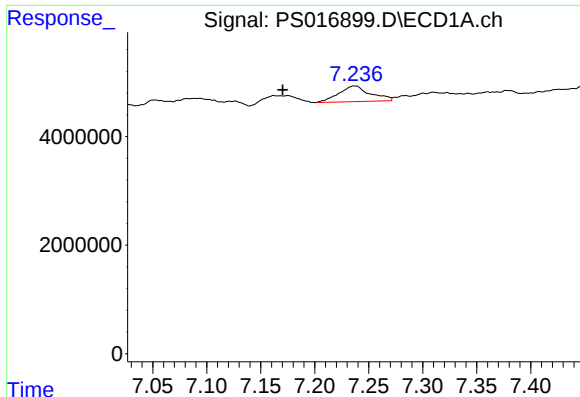

#4 2,4-DCAA


R.T.: 7.237 min
Delta R.T.: 0.067 min
Response: 5911252
Conc: 3.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

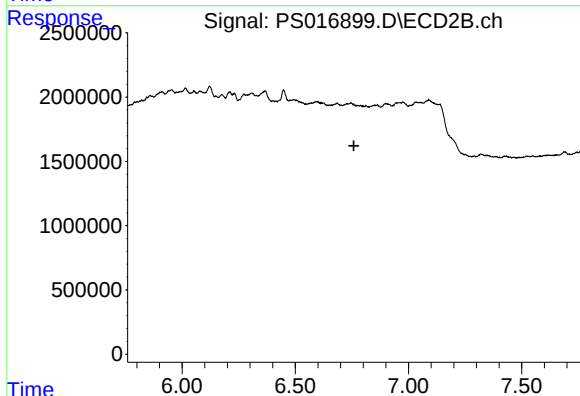


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

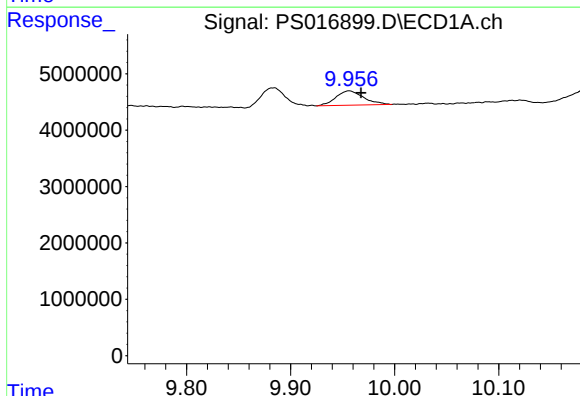


#13 2,4-DB

R.T.: 9.956 min
Delta R.T.: -0.011 min
Response: 4742013
Conc: 2.87 ng/ml

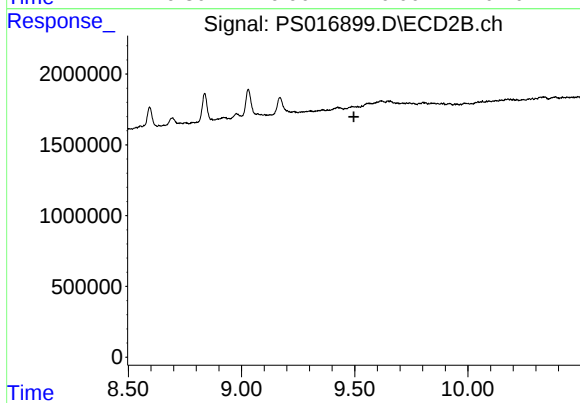

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.496 min
Response: 0
Conc: N.D.

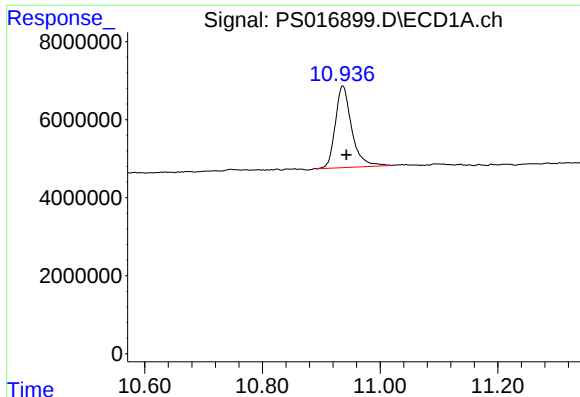

#15 Picloram


R.T.: 10.937 min
Delta R.T.: -0.006 min
Response: 40429547
Conc: 3.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

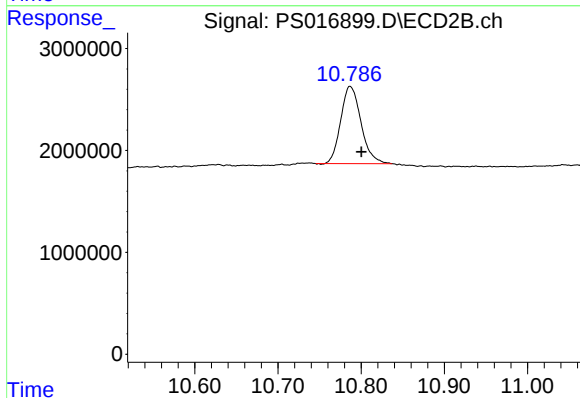


#15 Picloram

R.T.: 10.787 min
Delta R.T.: -0.014 min
Response: 12878541
Conc: 3.00 ng/ml

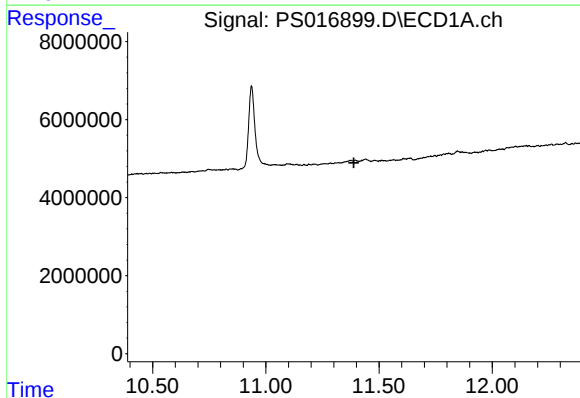

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.389 min
Response: 0
Conc: N.D.

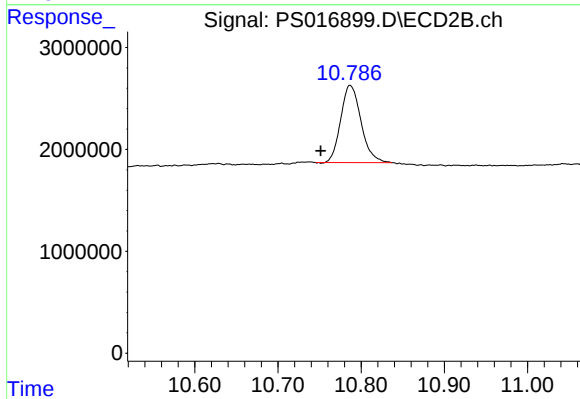

#16 DCPA

R.T.: 10.787 min
Delta R.T.: 0.035 min
Response: 12878541
Conc: 2.95 ng/ml