

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092723\
 Data File : PS024394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2023 12:55
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 00:34:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.350	6.829	1813777	593848	<MDL	<MDL	#
Target Compounds								
1) T	Dalapon	2.515	2.568	3824147	2887312	1.759	2.738	#
3) T	4-Nitroph...	6.198	0.000	6632351	0	5.338	N.D.	#
5) T	DICAMBA	6.491	6.990	934022	6214645	<MDL	2.158	#
6) T	MCP	6.659	6.990f	633697	6214645	<MDL	3.244	#
8) T	DICHLORPROP	7.093	7.571	1755914	1227122	<MDL	1.689	#
9) T	2,4-D	7.254	7.789f	94275714	940447	35.444	1.056	#
10) T	Pentachlo...	7.513	8.277	880567	94626	<MDL	<MDL	#
11) T	2,4,5-TP ...	8.019	8.622	158089	797336	<MDL	<MDL	#
12) T	2,4,5-T	8.299	9.039	483320	1903771	<MDL	<MDL	#
13) T	2,4-DB	8.792	9.491	-85785	148308	N.D.	<MDL	#
14) T	DINOSEB	9.873	9.841	2450598	54776	<MDL	<MDL	#
15) T	Picloram	9.660	10.784	80884483	20261818	4.953	3.412	#
16) T	DCPA	10.112	10.784	898846	20261818	<MDL	3.950	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092723\
Data File : PS024394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2023 12:55
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 00:34:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

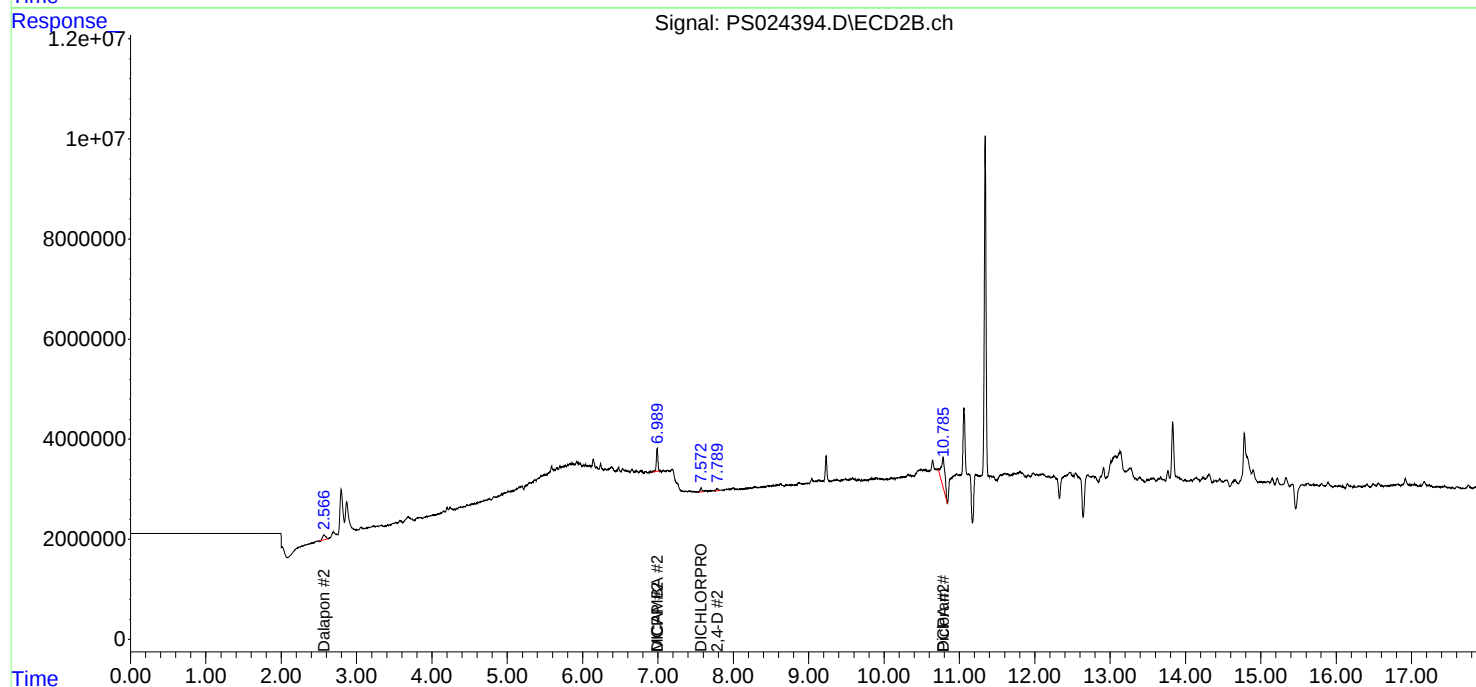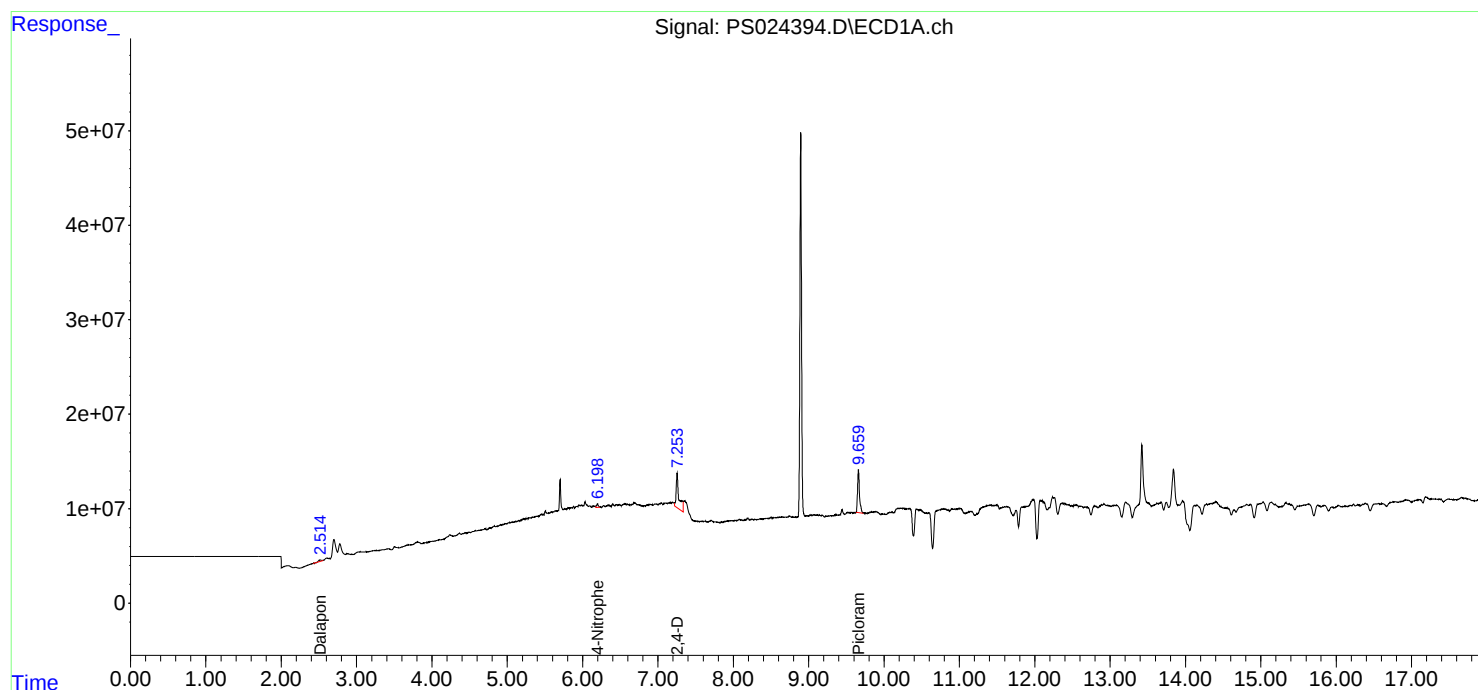


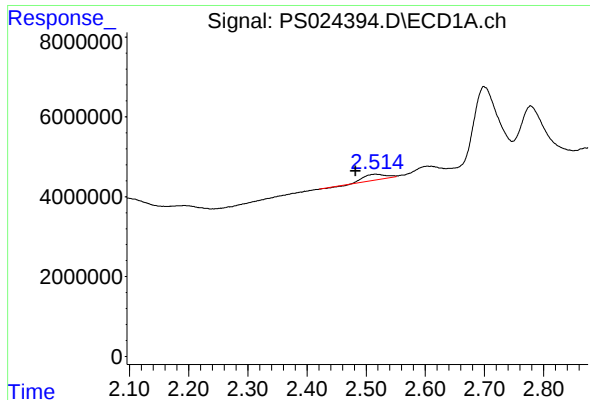

#1 Dalapon


R.T.: 2.515 min
Delta R.T.: 0.033 min
Response: 3824147
Conc: 1.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

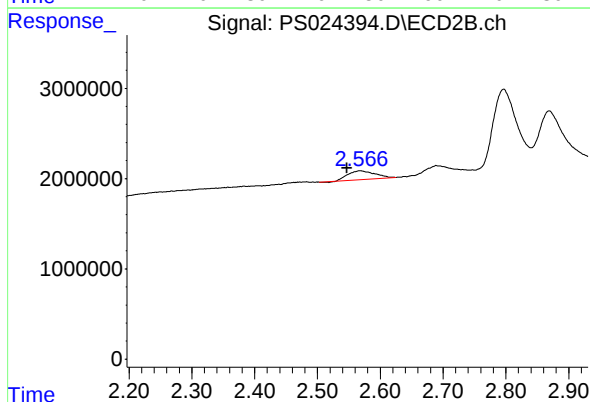


#1 Dalapon

R.T.: 2.568 min
Delta R.T.: 0.021 min
Response: 2887312
Conc: 2.74 ng/ml

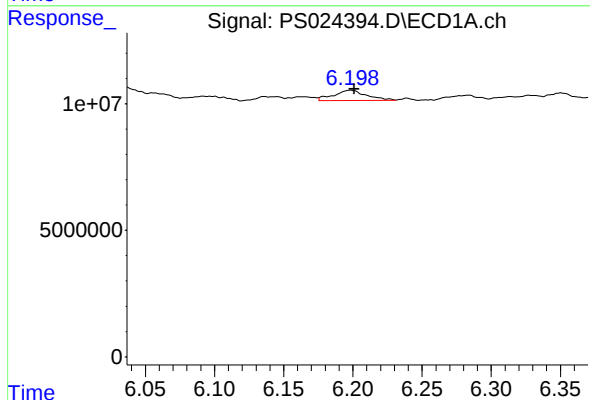


#3 4-Nitrophenol

R.T.: 6.198 min
Delta R.T.: -0.003 min
Response: 6632351
Conc: 5.34 ng/ml

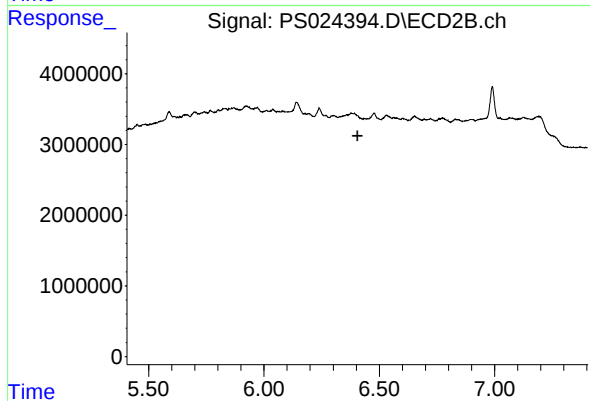

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.405 min
Response: 0
Conc: N.D.

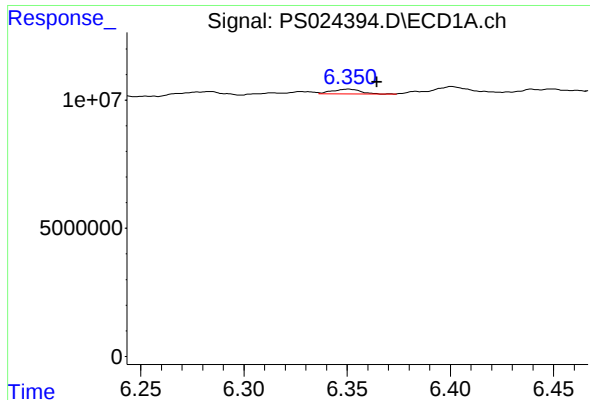

#4 2,4-DCAA


R.T.: 6.350 min
Delta R.T.: -0.014 min
Response: 1813777
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

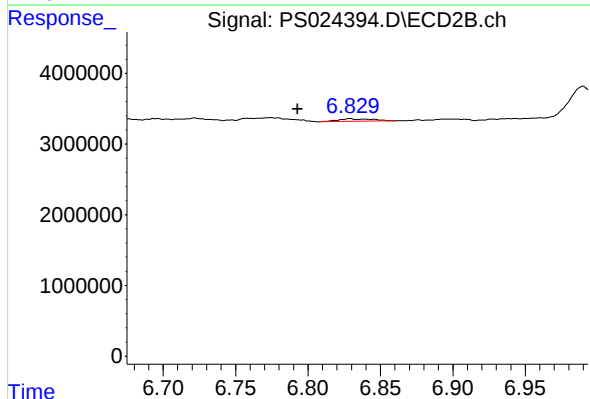


#4 2,4-DCAA

R.T.: 6.829 min
Delta R.T.: 0.036 min
Response: 593848
Conc: N.D.

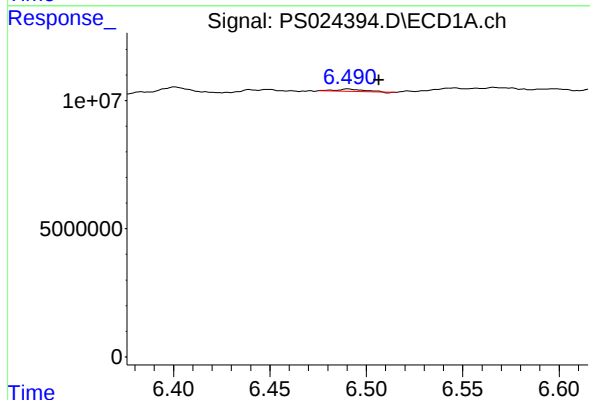


#5 DICAMBA

R.T.: 6.491 min
Delta R.T.: -0.016 min
Response: 934022
Conc: N.D.

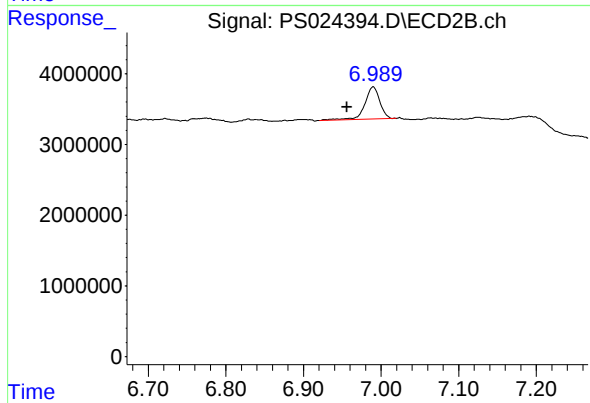

#5 DICAMBA


R.T.: 6.990 min
Delta R.T.: 0.034 min
Response: 6214645
Conc: 2.16 ng/ml

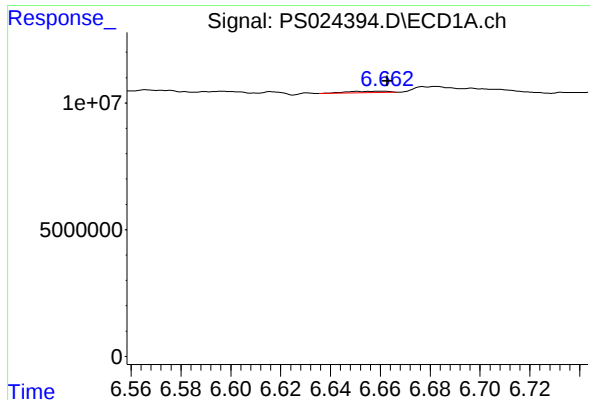

#6 MCPP


R.T.: 6.659 min
Delta R.T.: -0.003 min
Response: 633697
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

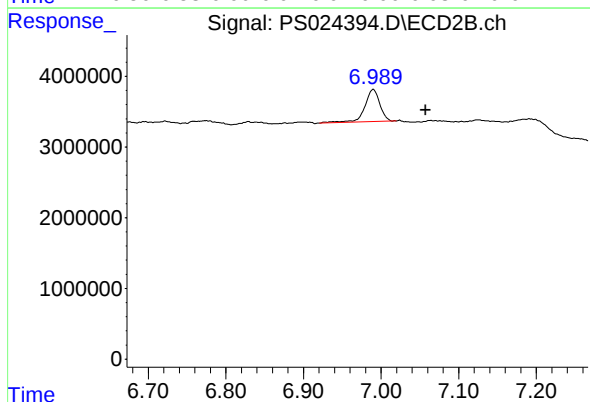


#6 MCPP

R.T.: 6.990 min
Delta R.T.: -0.007 min
Response: 6214645
Conc: 3.24 ug/ml

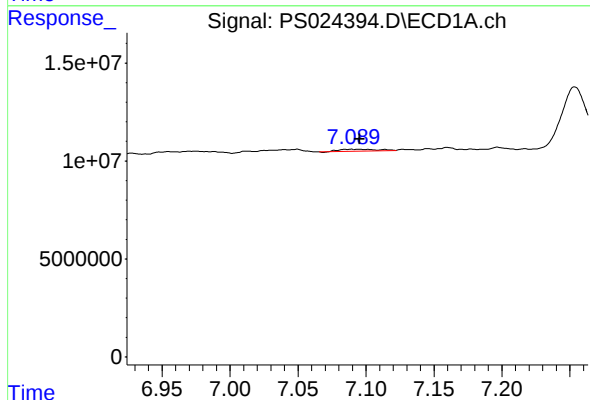


#8 DICHLORPROP

R.T.: 7.093 min
Delta R.T.: -0.002 min
Response: 1755914
Conc: N.D.

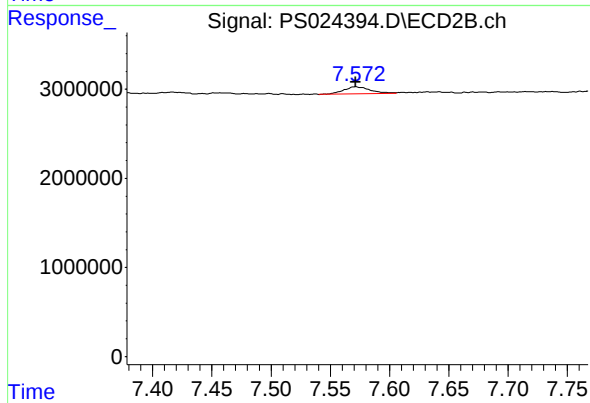

#8 DICHLORPROP


R.T.: 7.571 min
Delta R.T.: 0.000 min
Response: 1227122
Conc: 1.69 ng/ml

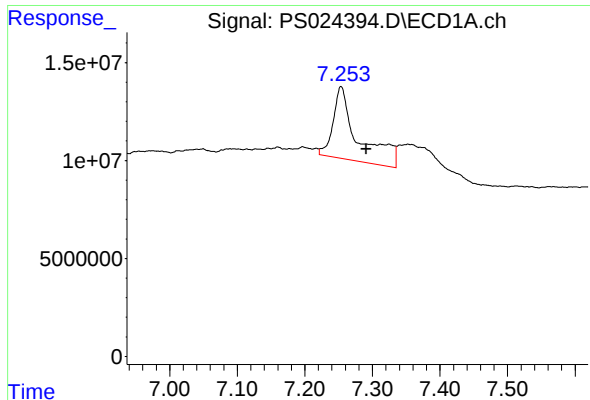

#9 2,4-D


R.T.: 7.254 min
Delta R.T.: -0.038 min
Response: 94275714
Conc: 35.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

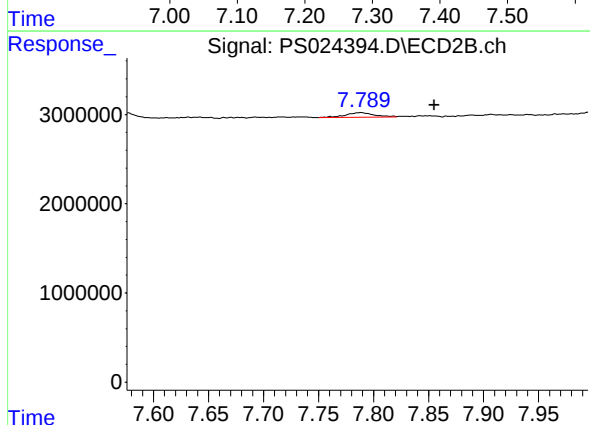


#9 2,4-D

R.T.: 7.789 min
Delta R.T.: -0.067 min
Response: 940447
Conc: 1.06 ng/ml

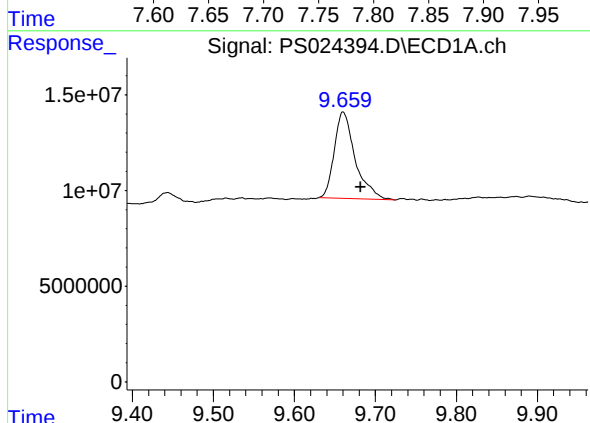


#15 Picloram

R.T.: 9.660 min
Delta R.T.: -0.021 min
Response: 80884483
Conc: 4.95 ng/ml

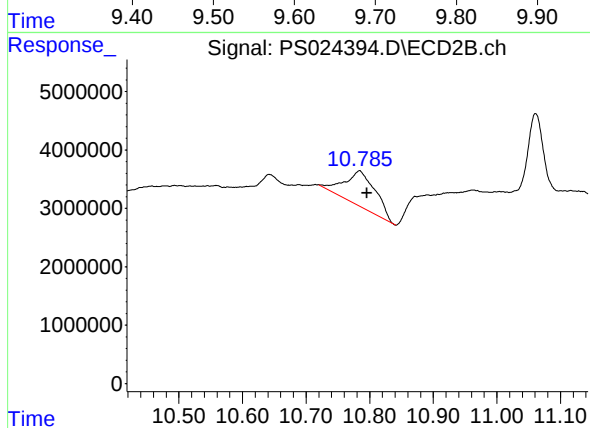

#15 Picloram


R.T.: 10.784 min
Delta R.T.: -0.012 min
Response: 20261818
Conc: 3.41 ng/ml

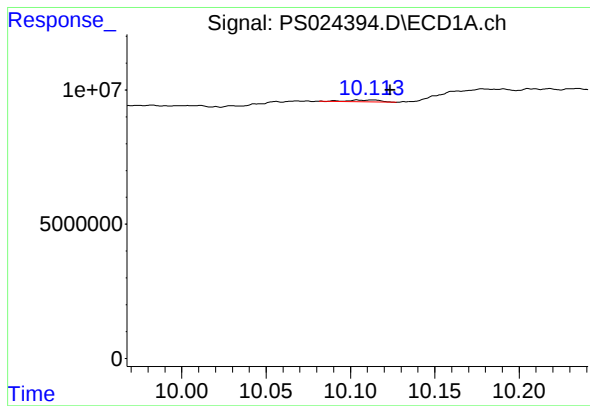

#16 DCPA

R.T.: 10.112 min
Delta R.T.: -0.012 min
Response: 898846
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

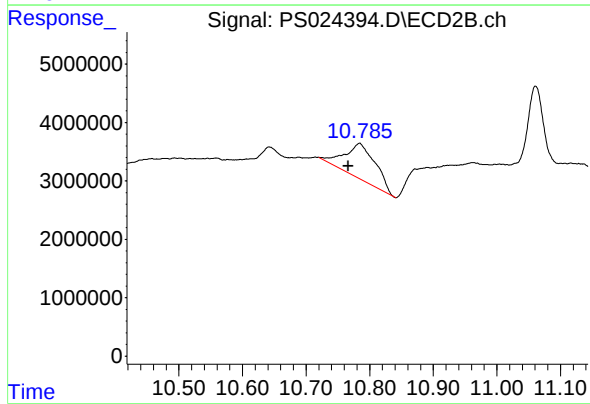

#16 DCPA

R.T.: 10.784 min
Delta R.T.: 0.018 min
Response: 20261818
Conc: 3.95 ng/ml