

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092724\
 Data File : PS027785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2024 11:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 22:34:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.104	7.628	1279.3E6	472.4E6	514.277	476.653
Target Compounds							
1) T	Dalapon	2.536	0.000	29644665	0	7.155	N.D. #
2) T	3,5-DICHL...	6.313	0.000	1216789	0	<MDL	N.D. #
3) T	4-Nitroph...	6.908	0.000	10020408	0	5.918	N.D. #
6) T	MCP	7.476	7.972f	1775728	1192327	<MDL	<MDL #
8) T	DICHLORPROP	0.000	8.528	0	951432	N.D.	<MDL
11) T	2,4,5-TP ...	9.045	9.707f	4633802	1786495	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.151	0	2031986	N.D.	<MDL
13) T	2,4-DB	9.948f	0.000	3048799	0	1.313	N.D. #
14) T	DINOSEB	11.128f	0.000	1001600	0	<MDL	N.D. #
15) T	Picloram	10.908	12.191	17479292	2139710	<MDL	<MDL #
16) T	DCPA	11.370	12.127	14583290	4109277	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092724\
Data File : PS027785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2024 11:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 22:34:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

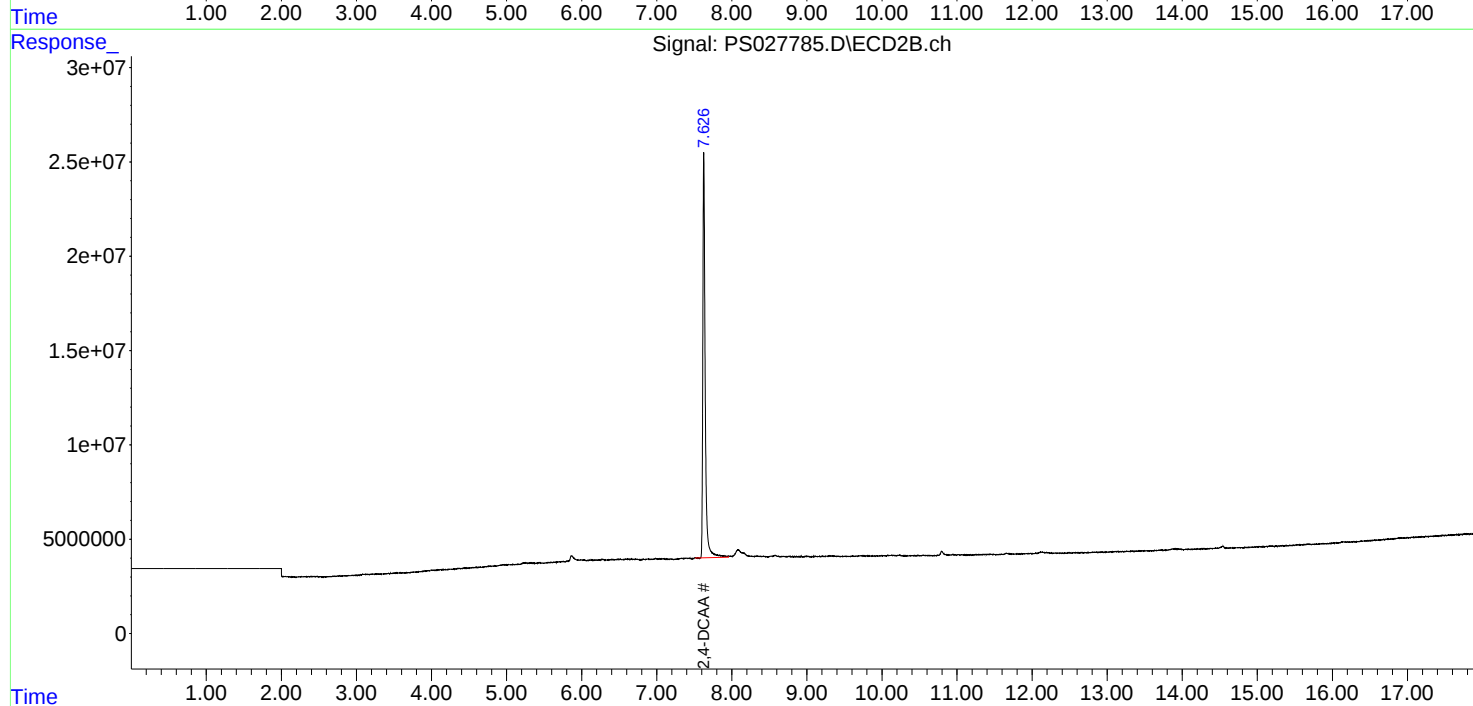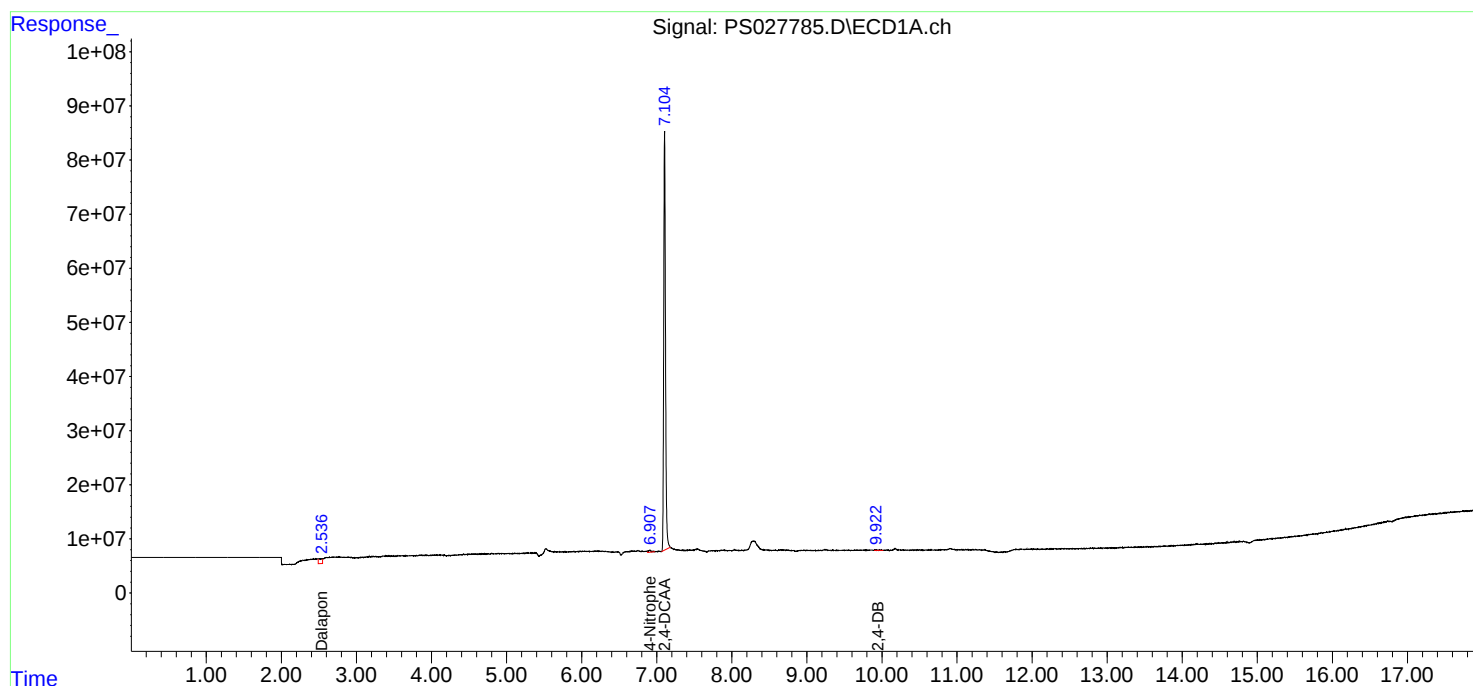


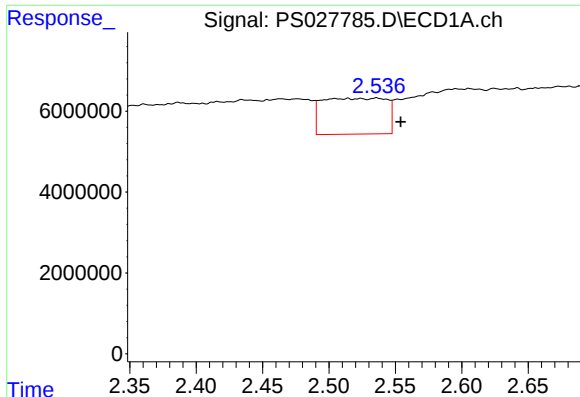

#1 Dalapon


R.T.: 2.536 min
Delta R.T.: -0.018 min
Response: 29644665
Conc: 7.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

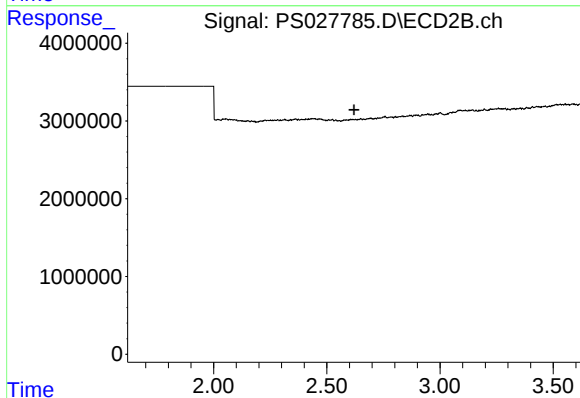


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

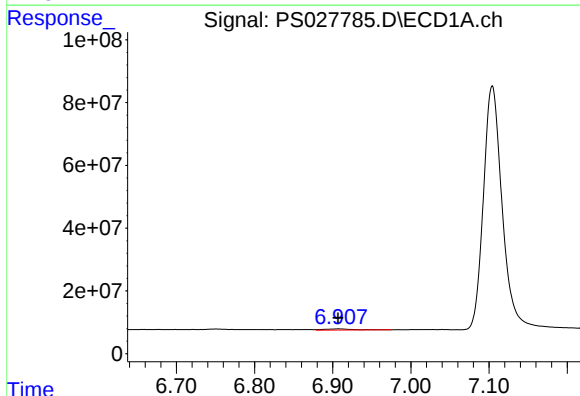


#3 4-Nitrophenol

R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 10020408
Conc: 5.92 ng/ml

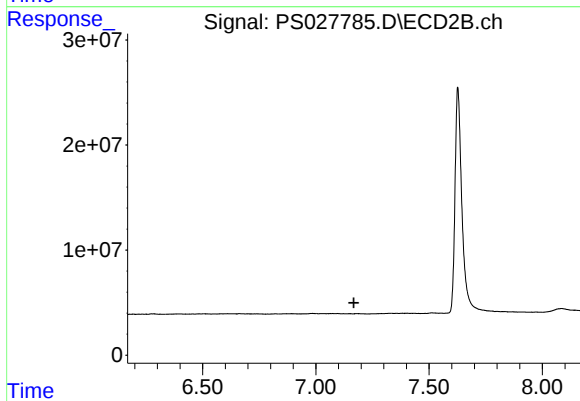

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.168 min
Response: 0
Conc: N.D.

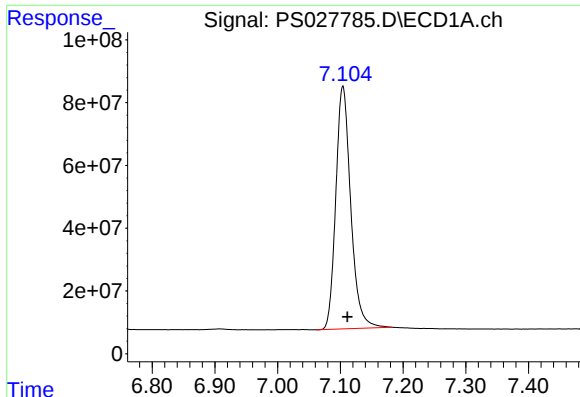

#4 2,4-DCAA


R.T.: 7.104 min
Delta R.T.: -0.007 min
Response: 1279318802
Conc: 514.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

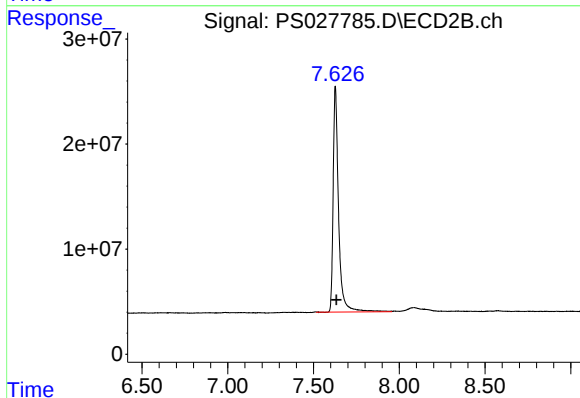


#4 2,4-DCAA

R.T.: 7.628 min
Delta R.T.: -0.006 min
Response: 472378594
Conc: 476.65 ng/ml

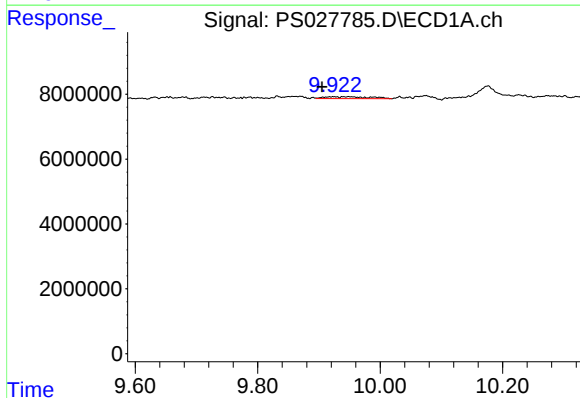

#13 2,4-DB

R.T.: 9.948 min
Delta R.T.: 0.043 min
Response: 3048799
Conc: 1.31 ng/ml

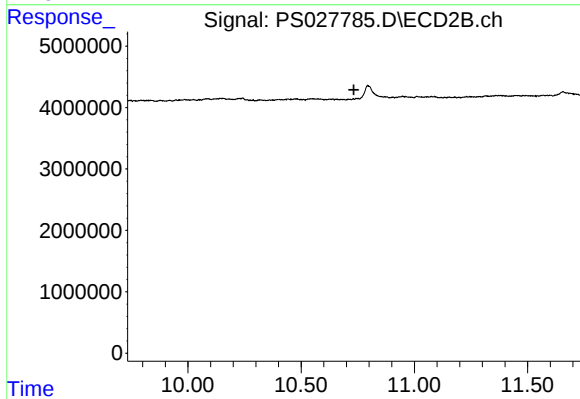

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.733 min
Response: 0
Conc: N.D.