

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092821\
 Data File : PS016932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2021 23:52
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 03:21:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.160	6.748	647.4E6	280.1E6	424.909	477.731
Target Compounds							
2) T	3,5-DICHL...	6.420	0.000	3064188	0	1.440	N.D. #
9) T	2,4-D	8.339f	0.000	96289980	0	54.765	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092821\
Data File : PS016932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2021 23:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 03:21:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

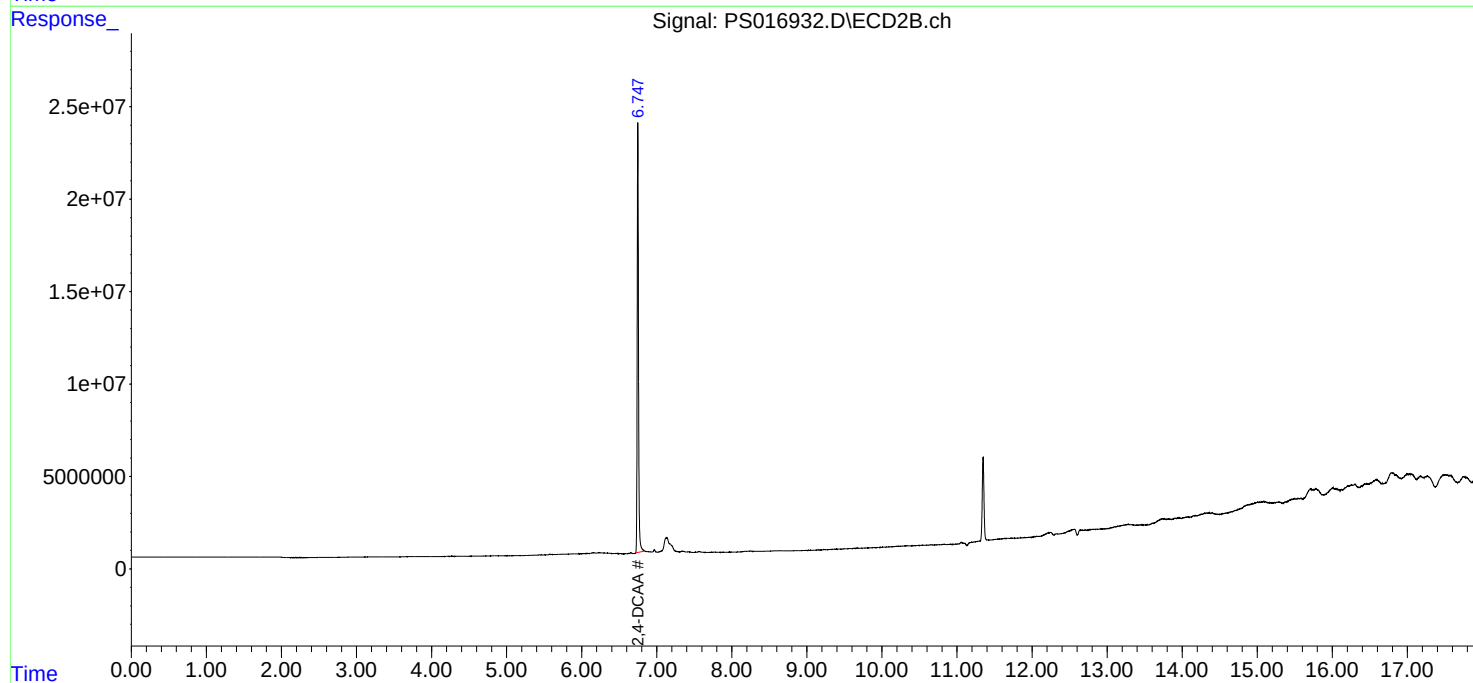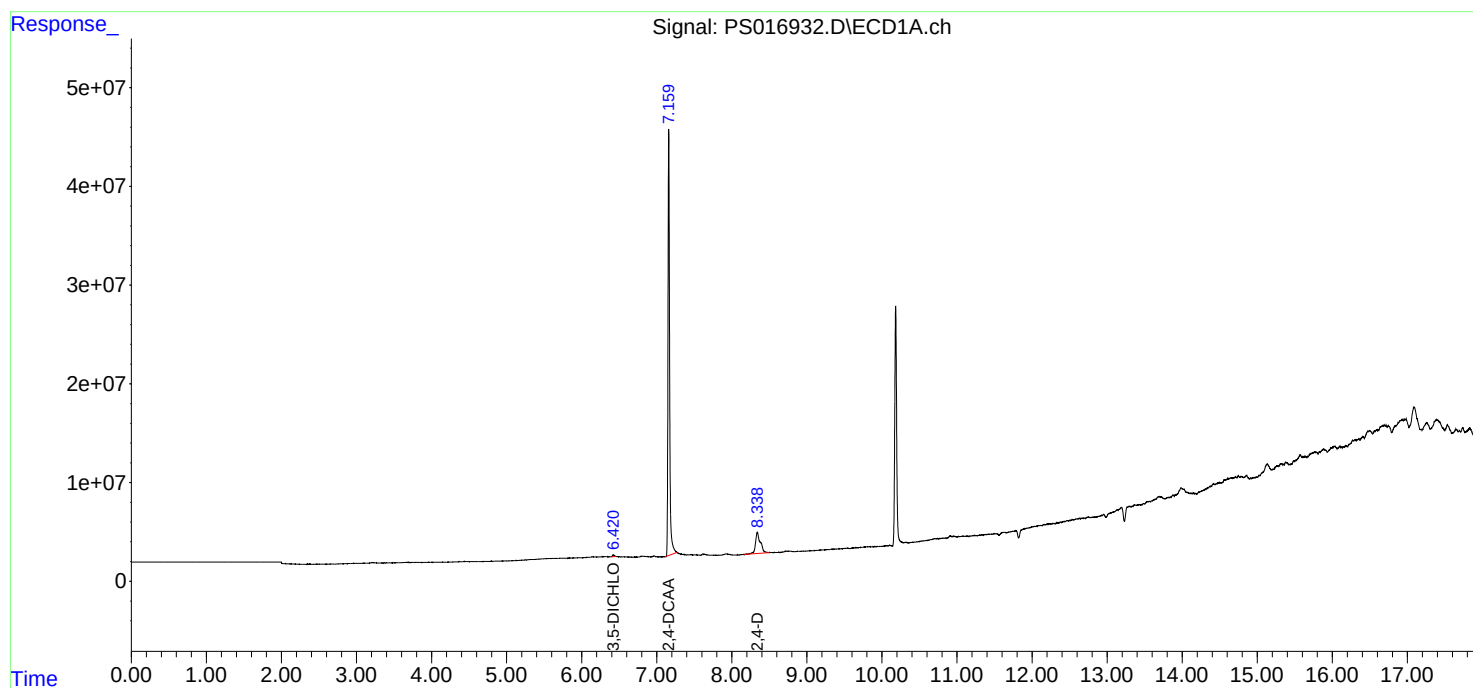


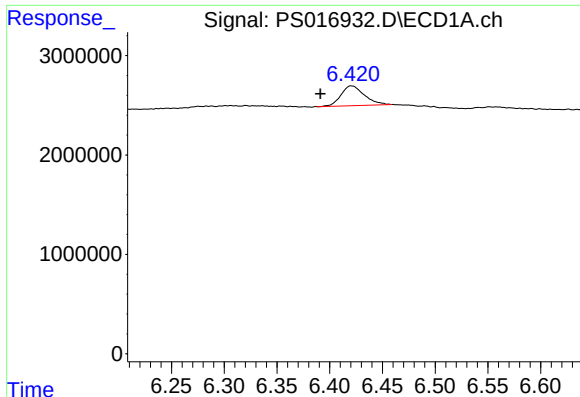

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.420 min
Delta R.T.: 0.029 min
Response: 3064188
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

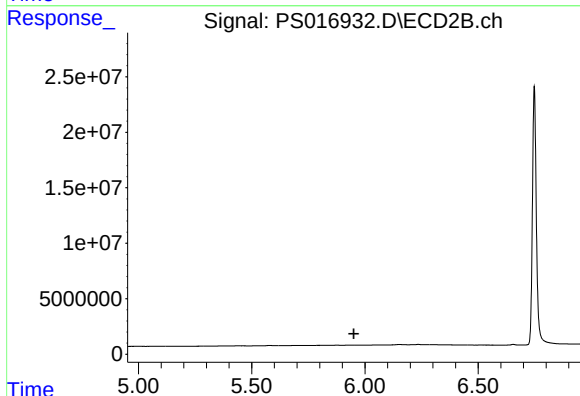


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.951 min
Response: 0
Conc: N.D.

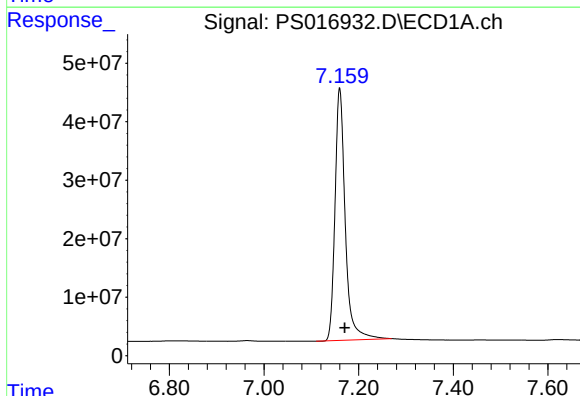


#4 2,4-DCAA

R.T.: 7.160 min
Delta R.T.: -0.011 min
Response: 647370074
Conc: 424.91 ng/ml

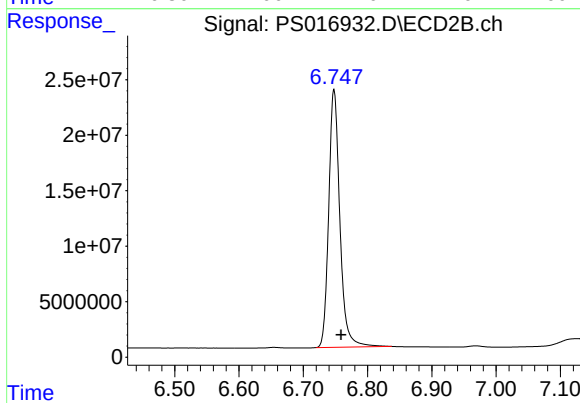

#4 2,4-DCAA


R.T.: 6.748 min
Delta R.T.: -0.011 min
Response: 280123997
Conc: 477.73 ng/ml

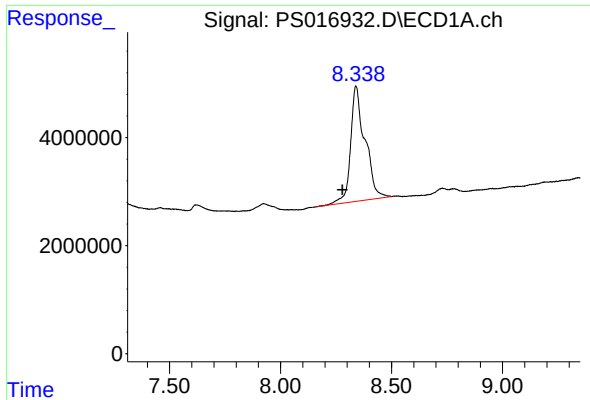

#9 2,4-D

R.T.: 8.339 min
Delta R.T.: 0.061 min
Response: 96289980
Conc: 54.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

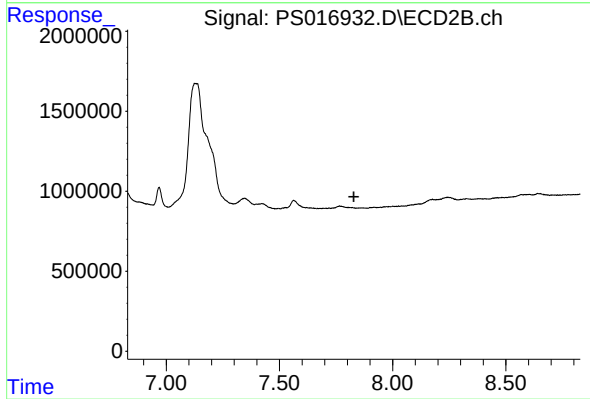

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.829 min
Response: 0
Conc: N.D.