

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092823\
 Data File : PS024420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2023 07:57
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 18:07:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.352	0.000	2512165	0	1.261	N.D. #
Target Compounds							
1) T	Dalapon	2.516	2.563	5778507	3838600	2.659	3.640 #
2) T	3,5-DICHL...	5.702	6.015	6737993	2080209	2.217	1.995
3) T	4-Nitroph...	6.199	0.000	49041947	0	39.475	N.D. #
5) T	DICAMBA	6.497	6.937	1209377	492913	<MDL	<MDL #
6) T	MCP	6.683	6.989f	4277560	8164977	<MDL	4.262 #
7) T	MCPA	6.805	0.000	1001365	0	<MDL	N.D. #
8) T	DICHLORPROP	7.089	7.573	1172111	4011496	<MDL	5.521 #
9) T	2,4-D	7.322	7.788f	12480003	695008	4.692	<MDL #
10) T	Pentachlo...	7.521	8.266	2499614	747358	<MDL	<MDL #
11) T	2,4,5-TP ...	8.043	8.625	1724062	1095086	<MDL	<MDL #
12) T	2,4,5-T	8.302	8.998	2464492	743233	<MDL	<MDL #
13) T	2,4-DB	8.793	9.504	2460274	760881	1.141	1.655 #
14) T	DINOSEB	9.861	9.830	1395016	464525	<MDL	<MDL #
15) T	Picloram	9.660	10.784	158.2E6	34123650	9.687	5.746 #
16) T	DCPA	0.000	10.784	0	34123650	N.D.	6.652



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092823\
Data File : PS024420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2023 07:57
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 18:07:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

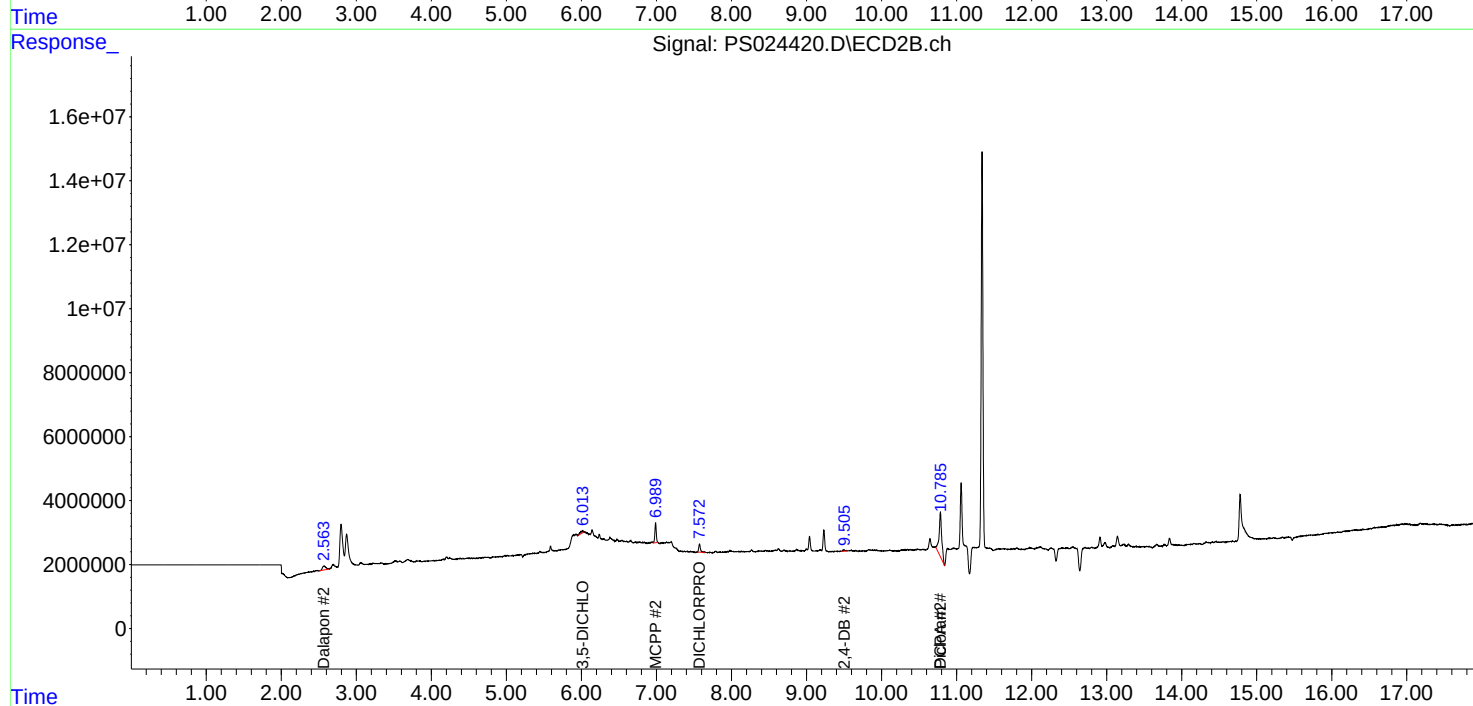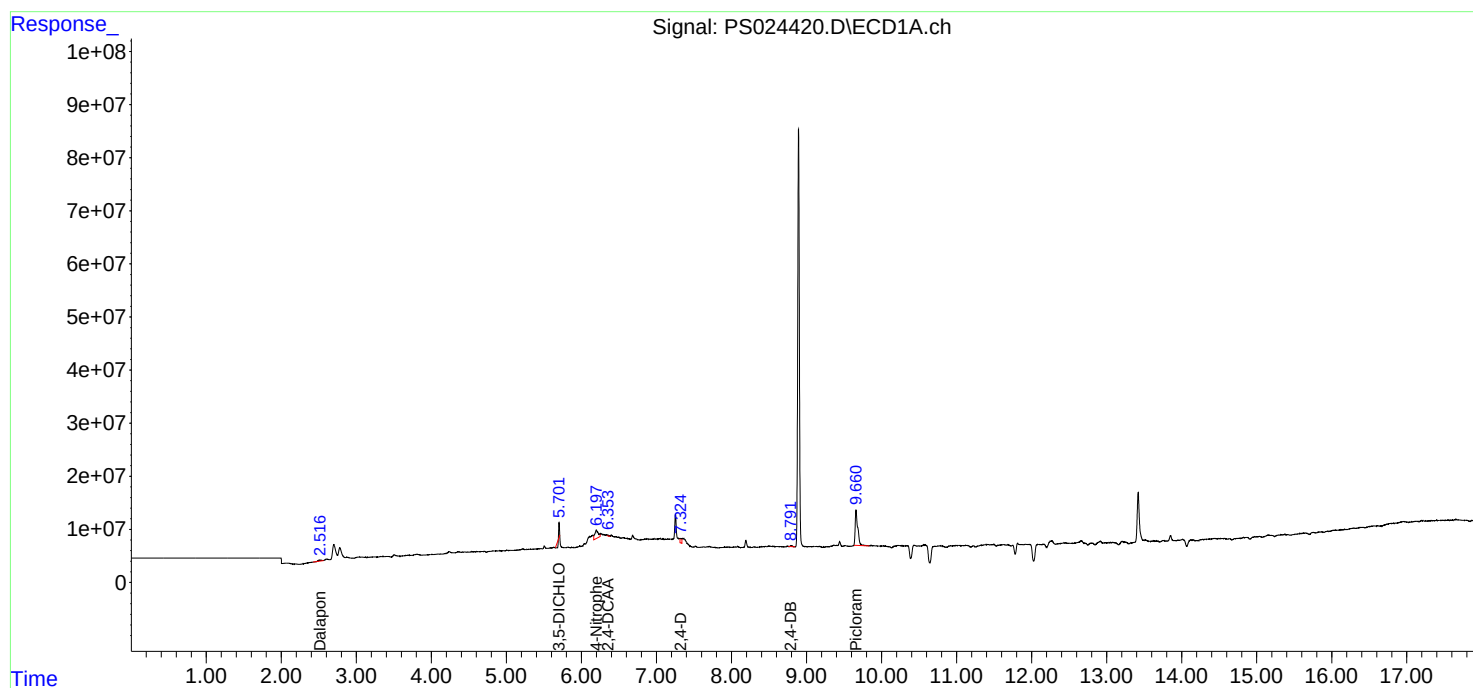


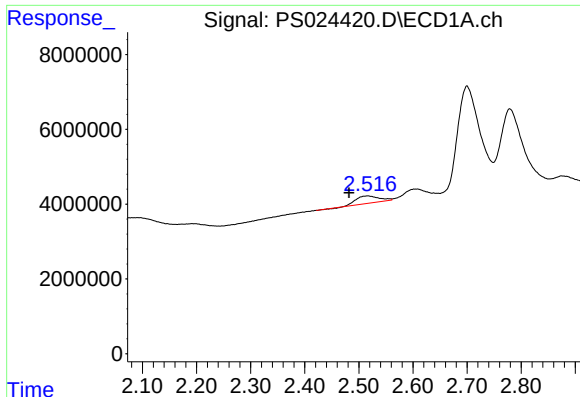

#1 Dalapon


R.T.: 2.516 min
Delta R.T.: 0.034 min
Response: 5778507
Conc: 2.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

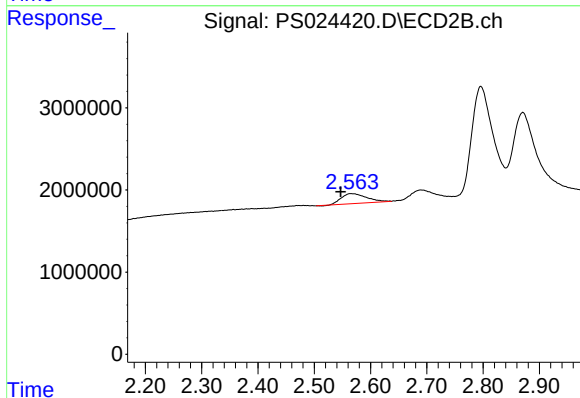


#1 Dalapon

R.T.: 2.563 min
Delta R.T.: 0.017 min
Response: 3838600
Conc: 3.64 ng/ml

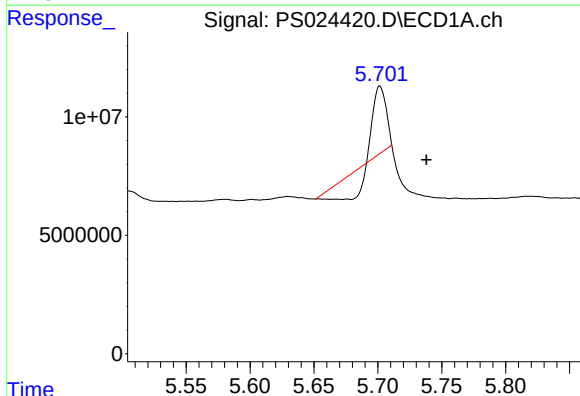


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.702 min
Delta R.T.: -0.036 min
Response: 6737993
Conc: 2.22 ng/ml

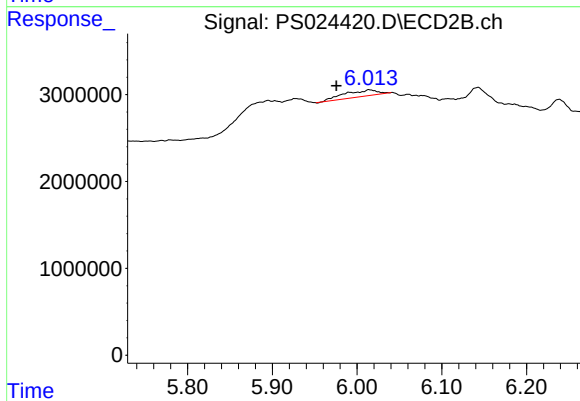

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.015 min
Delta R.T.: 0.040 min
Response: 2080209
Conc: 2.00 ng/ml

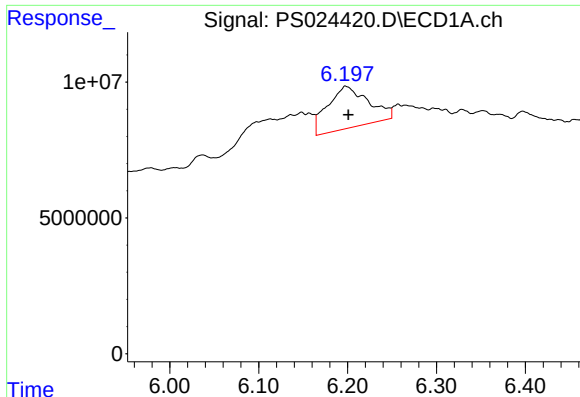

#3 4-Nitrophenol


R.T.: 6.199 min
Delta R.T.: -0.002 min
Response: 49041947
Conc: 39.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

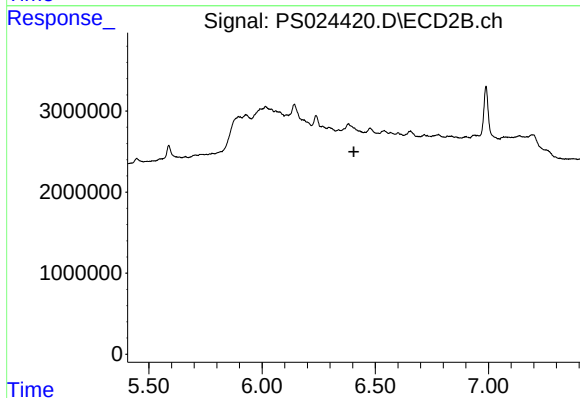


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.405 min
Response: 0
Conc: N.D.

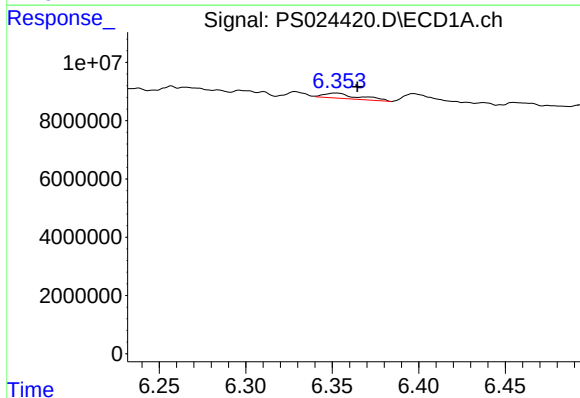


#4 2,4-DCAA

R.T.: 6.352 min
Delta R.T.: -0.013 min
Response: 2512165
Conc: 1.26 ng/ml

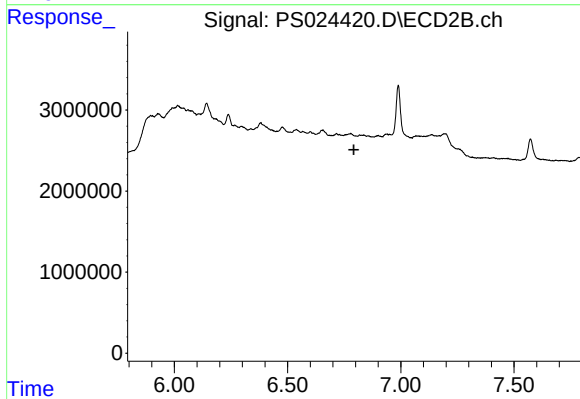

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.793 min
Response: 0
Conc: N.D.

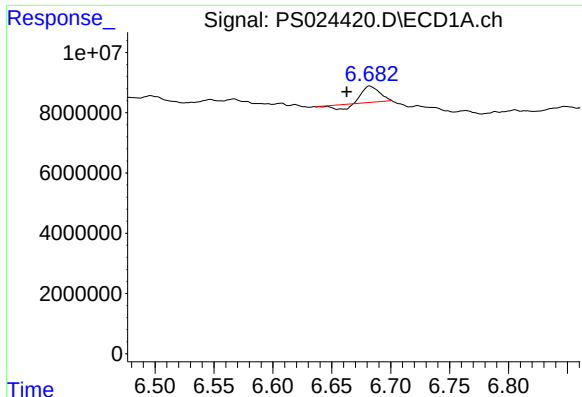

#6 MCP


R.T.: 6.683 min
Delta R.T.: 0.020 min
Response: 4277560
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

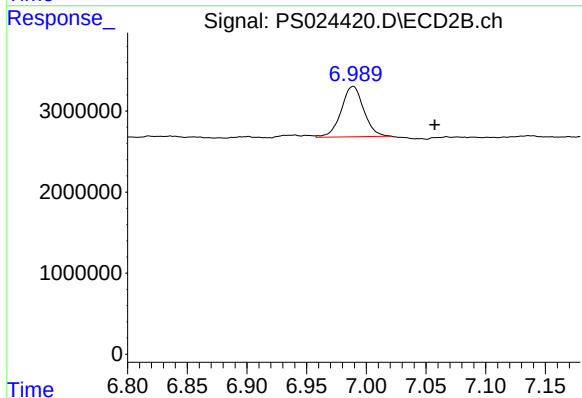


#6 MCP

R.T.: 6.989 min
Delta R.T.: -0.069 min
Response: 8164977
Conc: 4.26 ug/ml

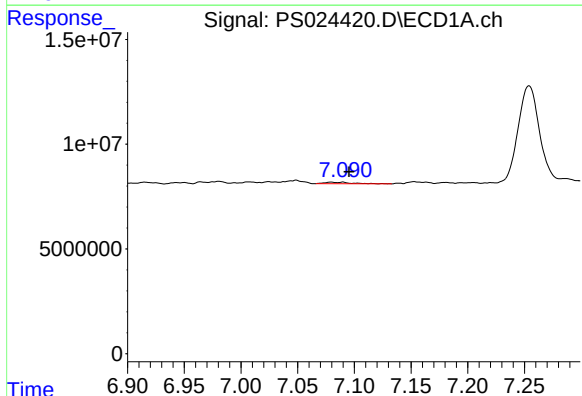


#8 DICHLORPROP

R.T.: 7.089 min
Delta R.T.: -0.006 min
Response: 1172111
Conc: N.D.

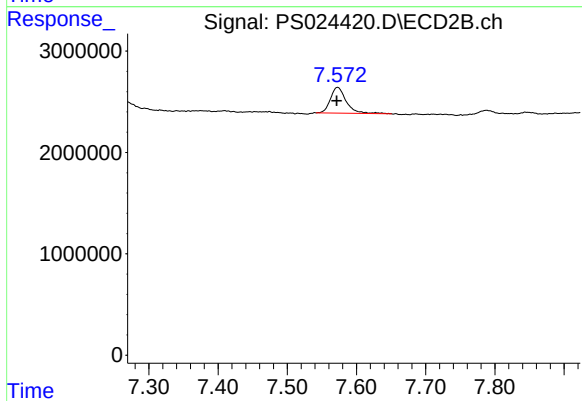

#8 DICHLORPROP


R.T.: 7.573 min
Delta R.T.: 0.001 min
Response: 4011496
Conc: 5.52 ng/ml

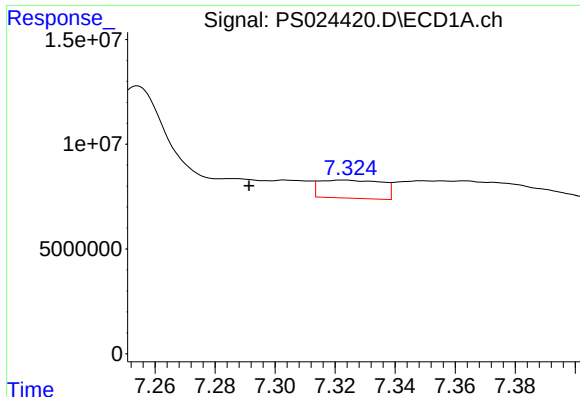

#9 2,4-D


R.T.: 7.322 min
Delta R.T.: 0.031 min
Response: 12480003
Conc: 4.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

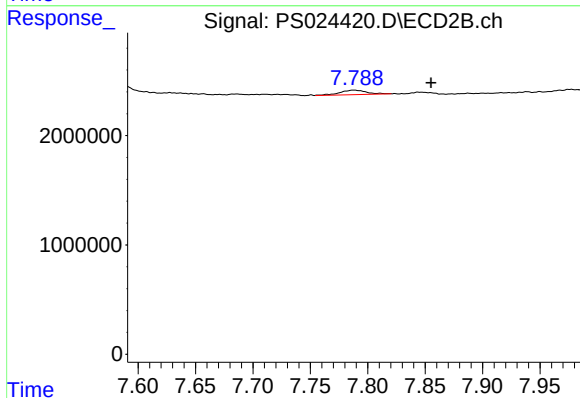


#9 2,4-D

R.T.: 7.788 min
Delta R.T.: -0.067 min
Response: 695008
Conc: N.D.

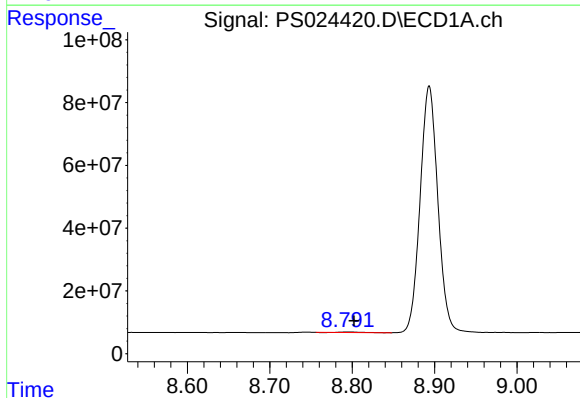


#13 2,4-DB

R.T.: 8.793 min
Delta R.T.: -0.010 min
Response: 2460274
Conc: 1.14 ng/ml

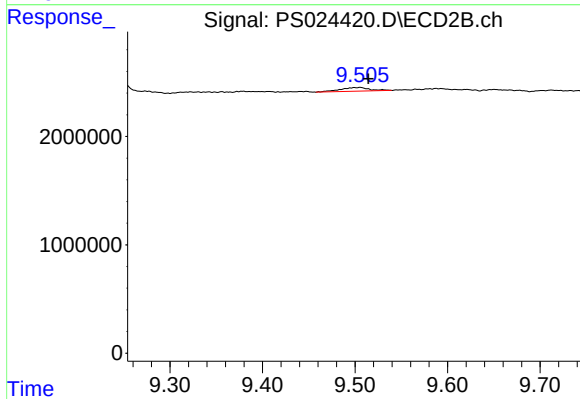

#13 2,4-DB


R.T.: 9.504 min
Delta R.T.: -0.010 min
Response: 760881
Conc: 1.66 ng/ml

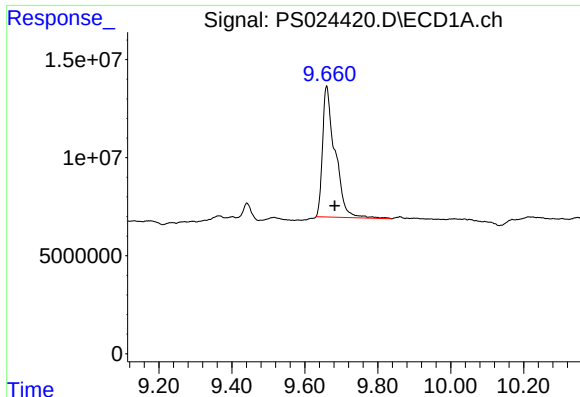

#15 Picloram


R.T.: 9.660 min
Delta R.T.: -0.022 min
Response: 158194504
Conc: 9.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

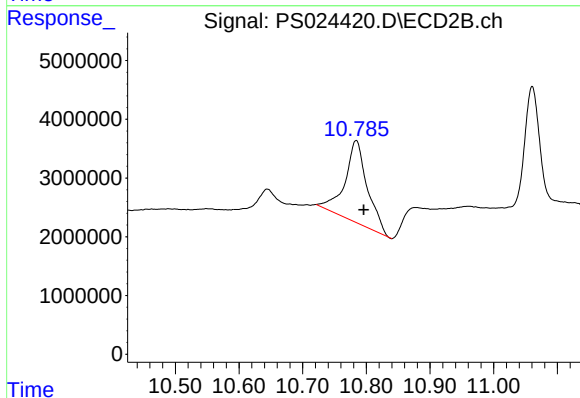


#15 Picloram

R.T.: 10.784 min
Delta R.T.: -0.012 min
Response: 34123650
Conc: 5.75 ng/ml

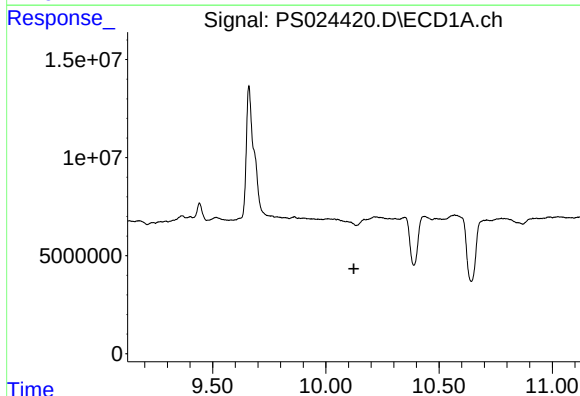

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.124 min
Response: 0
Conc: N.D.

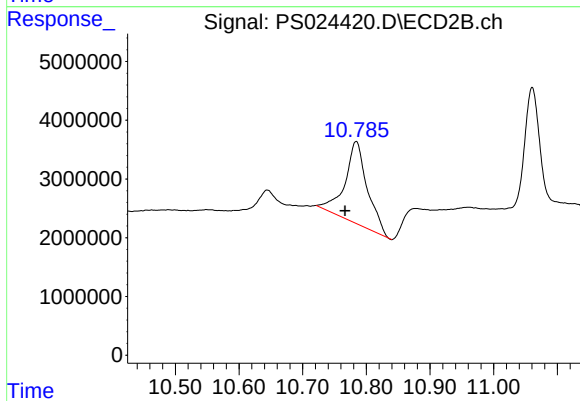

#16 DCPA

R.T.: 10.784 min
Delta R.T.: 0.018 min
Response: 34123650
Conc: 6.65 ng/ml