

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092823\
 Data File : PS024421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2023 08:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 18:07:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.361	6.785	1049.2E6	350.9E6	526.597	522.492
Target Compounds							
1) T	Dalapon	2.512	2.572	3819034	2864141	1.757	2.716 #
2) T	3,5-DICHL...	5.701	0.000	676055	0	<MDL	N.D. #
3) T	4-Nitroph...	6.202	0.000	8828183	0	7.106	N.D. #
5) T	DICAMBA	6.492	6.990	506823	2058538	<MDL	<MDL #
6) T	MCP	6.684	6.990f	1771350	2058538	<MDL	1.075 #
7) T	MCPA	6.812	0.000	33341	0	<MDL	N.D. #
8) T	DICHLORPROP	7.144f	7.576	905946	2016624	<MDL	2.776 #
9) T	2,4-D	7.253	7.791f	9932533	483732	3.734	<MDL #
10) T	Pentachlo...	7.515	0.000	2378292	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.036	8.630	975181	741589	<MDL	<MDL #
12) T	2,4,5-T	8.295	9.042	1952563	4364970	<MDL	1.088 #
13) T	2,4-DB	8.797	0.000	272860	0	<MDL	N.D. #
14) T	DINOSEB	9.849	0.000	1021665	0	<MDL	N.D. #
15) T	Picloram	9.684	10.786	37434670	15848539	2.292	2.669
16) T	DCPA	10.114	10.786	1173706	15848539	<MDL	3.089 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092823\
Data File : PS024421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2023 08:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 18:07:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

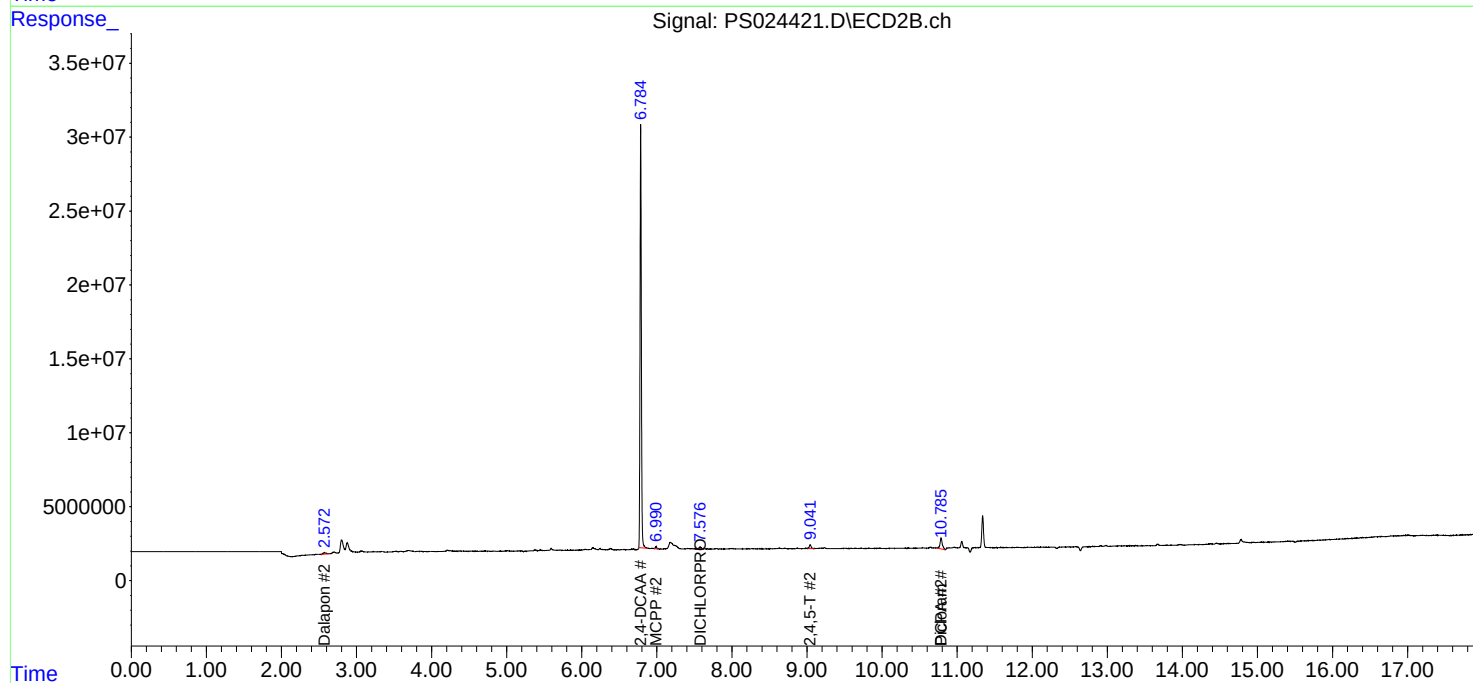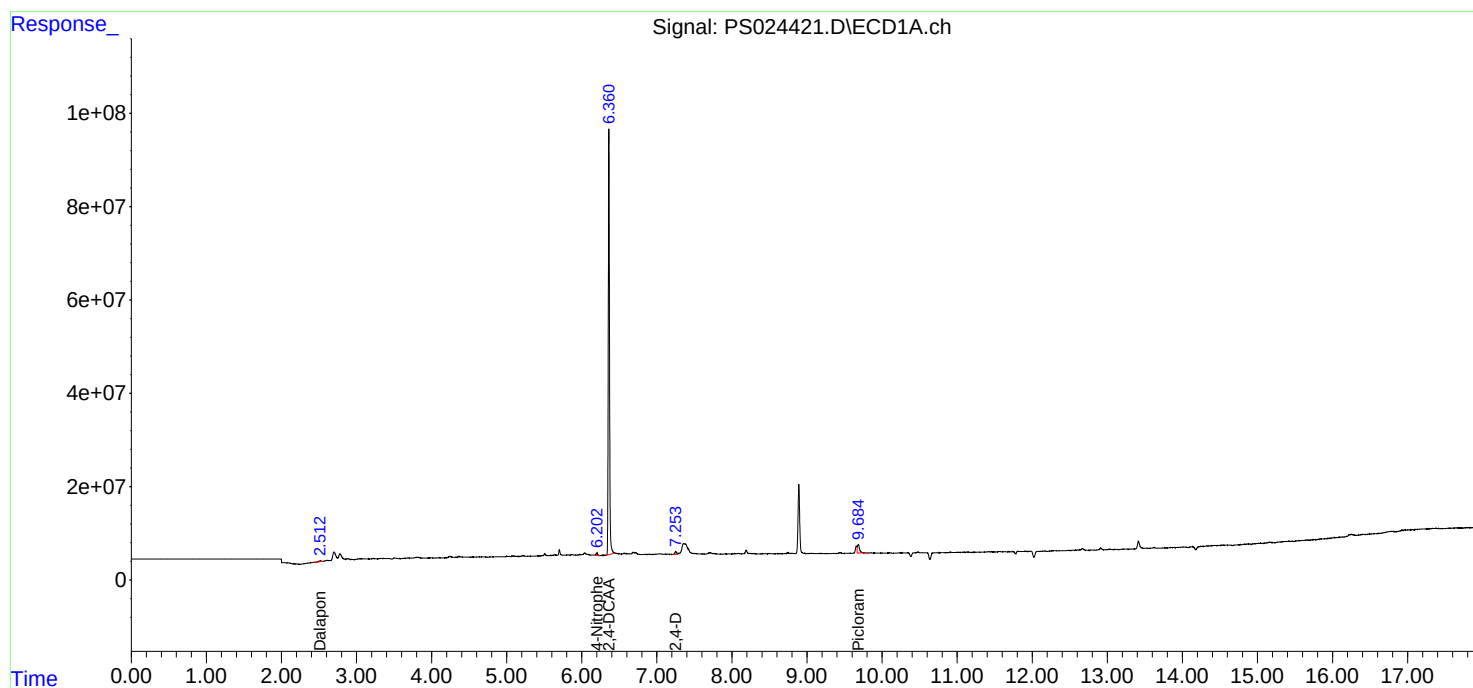


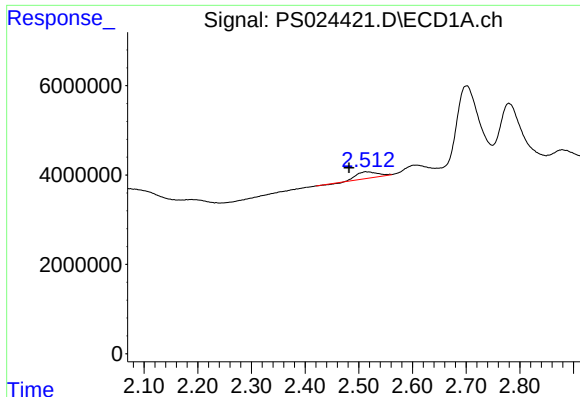

#1 Dalapon


R.T.: 2.512 min
Delta R.T.: 0.030 min
Response: 3819034
Conc: 1.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

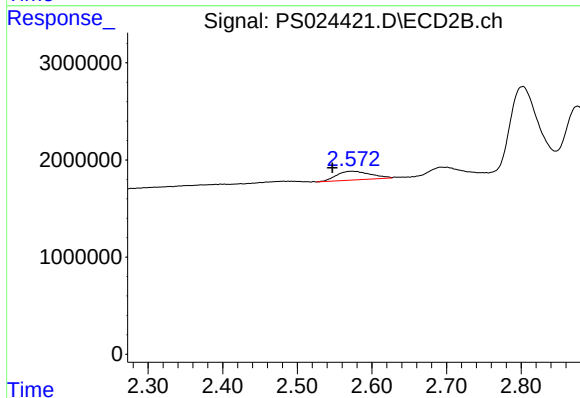


#1 Dalapon

R.T.: 2.572 min
Delta R.T.: 0.026 min
Response: 2864141
Conc: 2.72 ng/ml

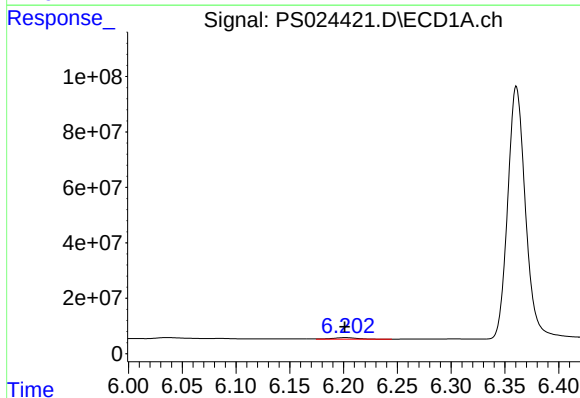


#3 4-Nitrophenol

R.T.: 6.202 min
Delta R.T.: 0.000 min
Response: 8828183
Conc: 7.11 ng/ml

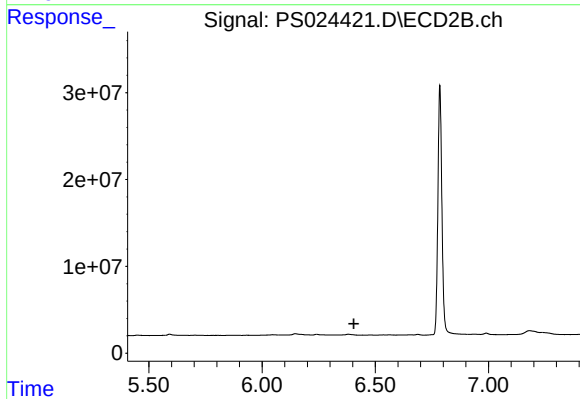

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.405 min
Response: 0
Conc: N.D.

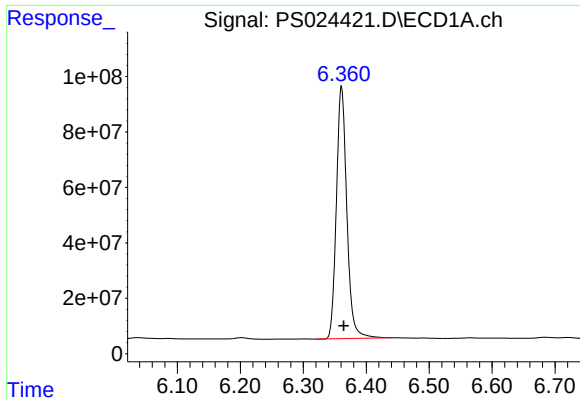

#4 2,4-DCAA


R.T.: 6.361 min
Delta R.T.: -0.004 min
Response: 1049150925
Conc: 526.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

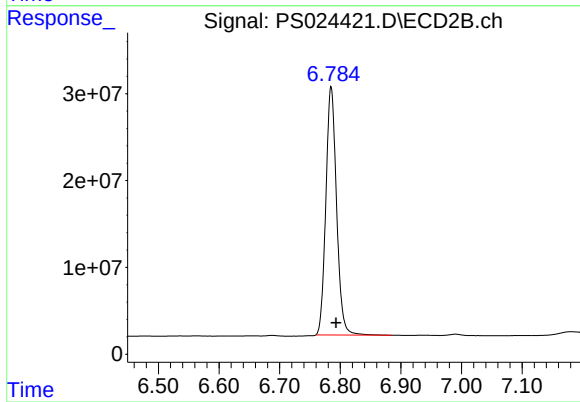


#4 2,4-DCAA

R.T.: 6.785 min
Delta R.T.: -0.008 min
Response: 350901539
Conc: 522.49 ng/ml

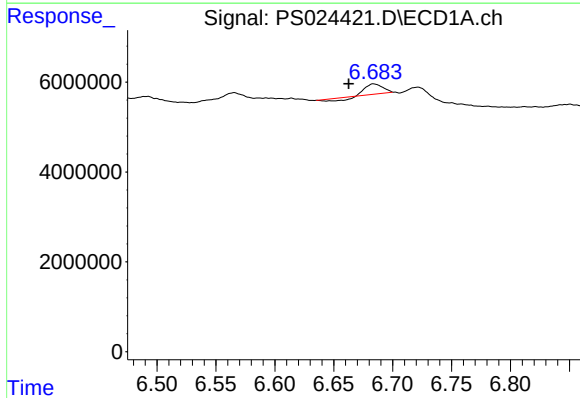


#6 MCP

R.T.: 6.684 min
Delta R.T.: 0.021 min
Response: 1771350
Conc: N.D.

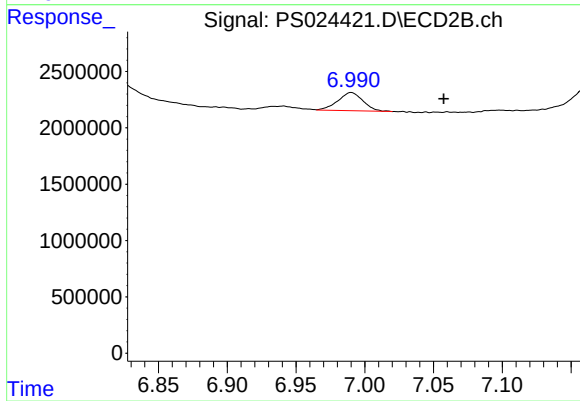

#6 MCP


R.T.: 6.990 min
Delta R.T.: -0.067 min
Response: 2058538
Conc: 1.07 ug/ml

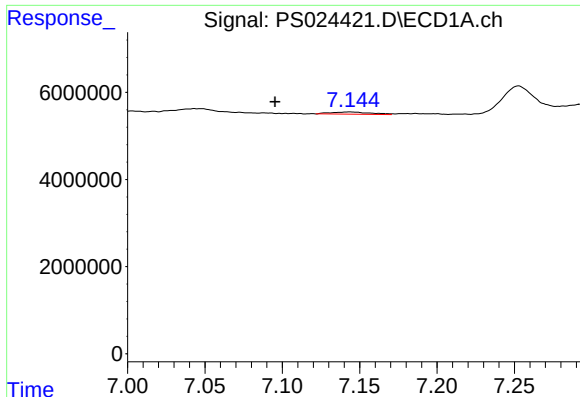

#8 DICHLORPROP


R.T.: 7.144 min
Delta R.T.: 0.049 min
Response: 905946
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

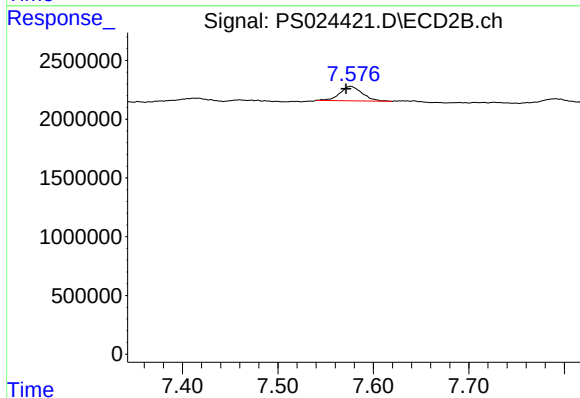


#8 DICHLORPROP

R.T.: 7.576 min
Delta R.T.: 0.005 min
Response: 2016624
Conc: 2.78 ng/ml

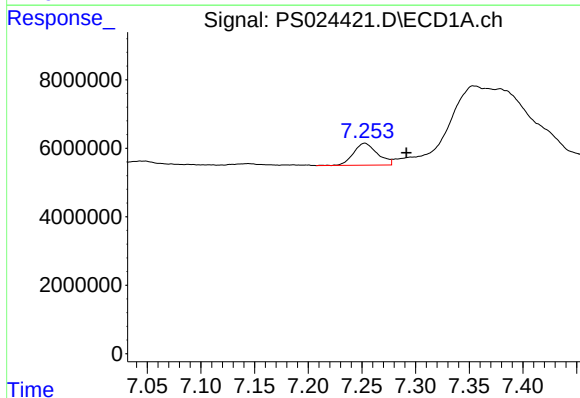


#9 2,4-D

R.T.: 7.253 min
Delta R.T.: -0.039 min
Response: 9932533
Conc: 3.73 ng/ml

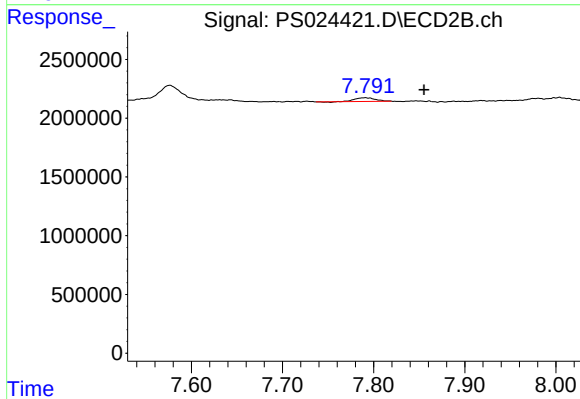

#9 2,4-D


R.T.: 7.791 min
Delta R.T.: -0.064 min
Response: 483732
Conc: N.D.

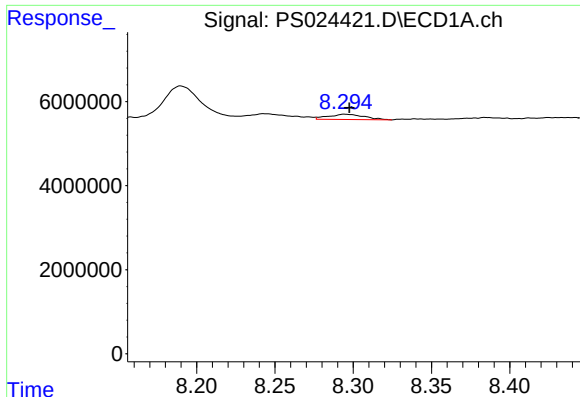

#12 2,4,5-T


R.T.: 8.295 min
Delta R.T.: -0.003 min
Response: 1952563
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

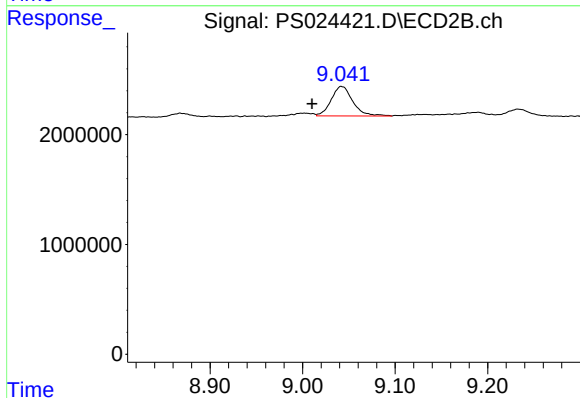


#12 2,4,5-T

R.T.: 9.042 min
Delta R.T.: 0.032 min
Response: 4364970
Conc: 1.09 ng/ml

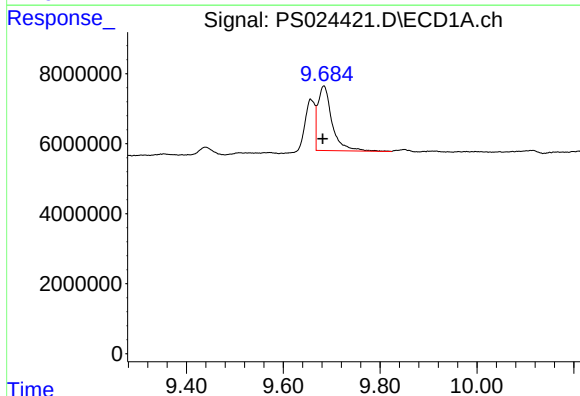


#15 Picloram

R.T.: 9.684 min
Delta R.T.: 0.002 min
Response: 37434670
Conc: 2.29 ng/ml

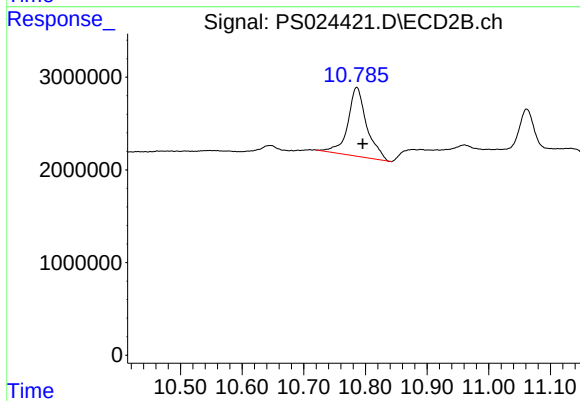

#15 Picloram


R.T.: 10.786 min
Delta R.T.: -0.010 min
Response: 15848539
Conc: 2.67 ng/ml

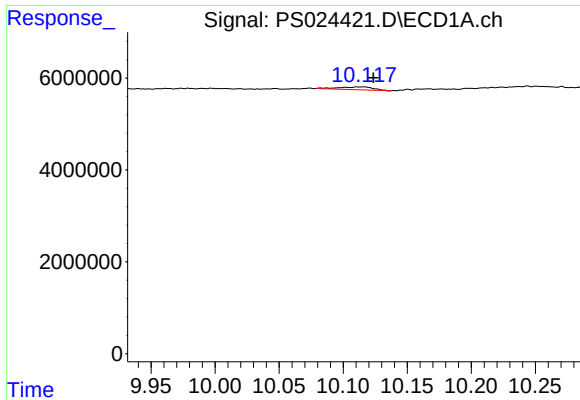

#16 DCPA

R.T.: 10.114 min
Delta R.T.: -0.010 min
Response: 1173706
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

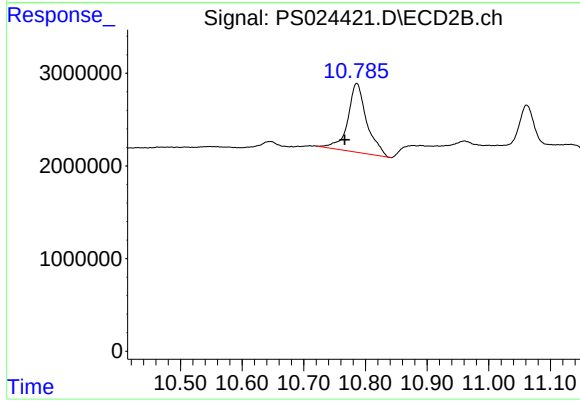

#16 DCPA

R.T.: 10.786 min
Delta R.T.: 0.020 min
Response: 15848539
Conc: 3.09 ng/ml