

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092920\
 Data File : PS012559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2020 20:29
 Operator : DD\AJ
 Sample : L4173-06MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-2-(0-6FT)MSD

Manual Integrations
 APPROVED

Ankita
 9/30/2020 2:21:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 01:42:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.213	6.912	5280315	2969307	5.391m	6.455m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092920\
Data File : PS012559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2020 20:29
Operator : DD\AJ
Sample : L4173-06MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-2-(0-6FT)MSD


Manual Integrations
APPROVED

Ankita
9/30/2020 2:21:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 01:42:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

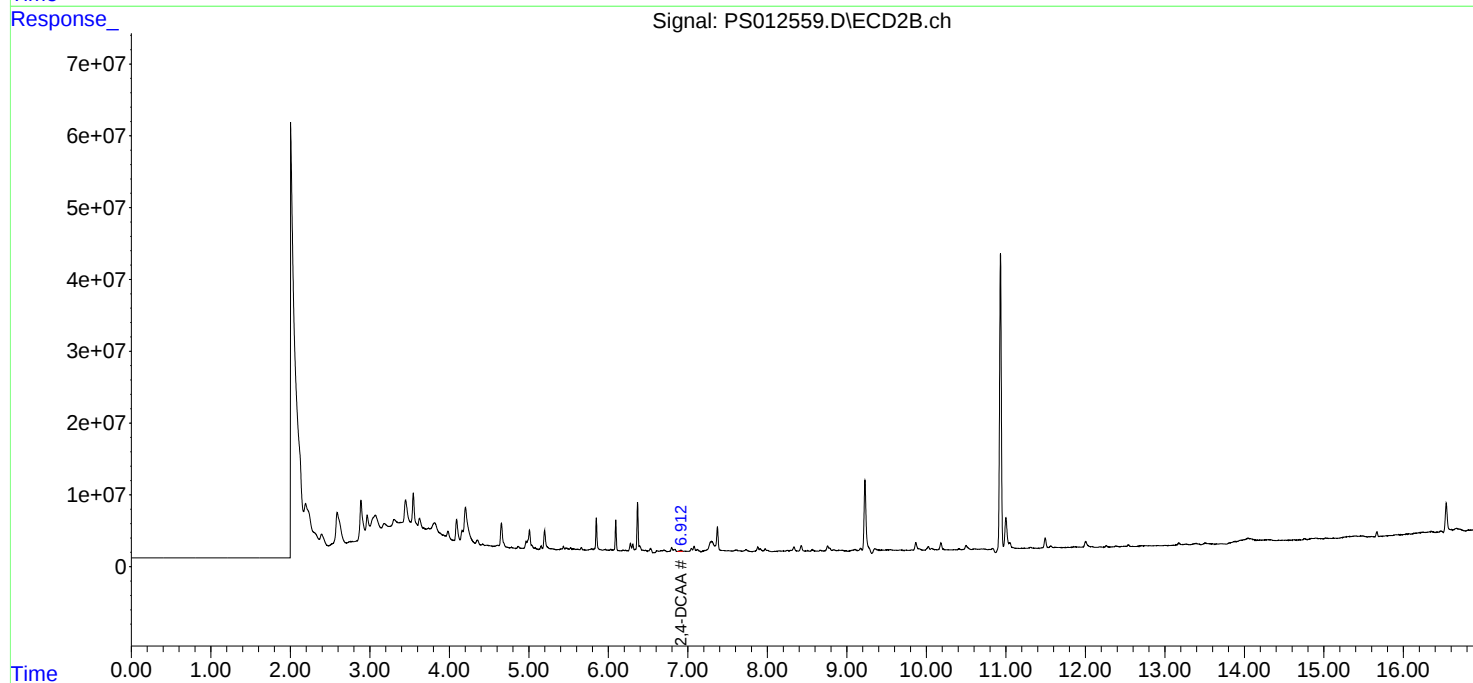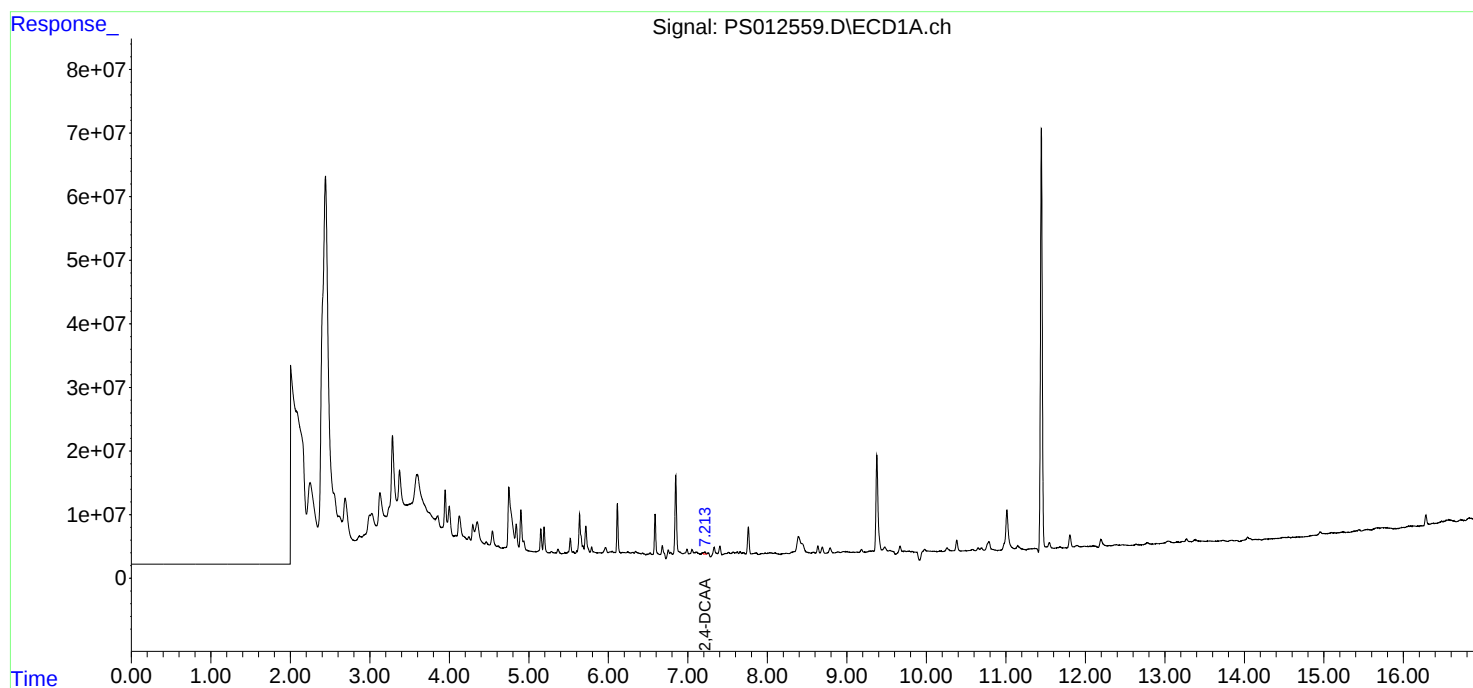

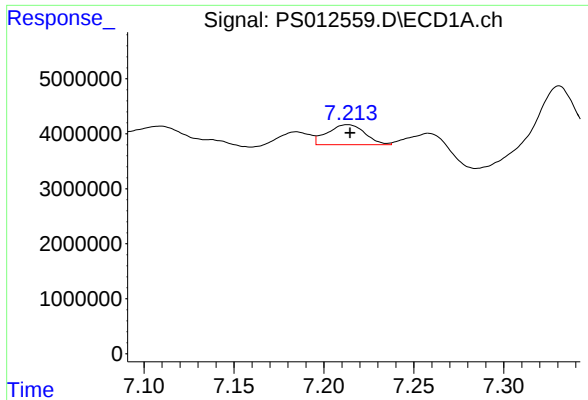


#4 2,4-DCAA

R.T.: 7.213 min
Delta R.T.: -0.001 min
Response: 5280315
Conc: 5.39 ng/ml m

Instrument :
ECD_S
ClientSampleId :
TP-2-(0-6FT)MSD

Manual Integrations
APPROVED

Ankita
9/30/2020 2:21:59 PM

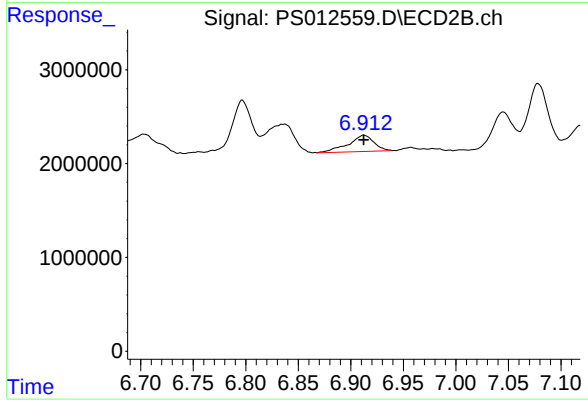

#4 2,4-DCAA

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 2969307
Conc: 6.45 ng/ml m