

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092922\
 Data File : PS020672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2022 10:13
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 00:14:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1)	T	Dalapon	3.046f	0.000	2249256	0	<MDL N.D. #
2)	T	3,5-DICHL...	6.331f	0.000	279531	0	<MDL N.D. #
6)	T	MCPP	7.471f	0.000	1155231	0	<MDL N.D. #
9)	T	2,4-D	8.354f	0.000	235.4E6	0	50.635 N.D. #
10)	T	Pentachlo...	8.610	0.000	248846	0	<MDL N.D. #
11)	T	2,4,5-TP ...	9.100f	0.000	1397319	0	<MDL N.D. #
13)	T	2,4-DB	10.030f	0.000	386254	0	<MDL N.D. #
14)	T	DINOSEB	11.134	0.000	56871691	0	3.097 N.D. #
15)	T	Picloram	10.990	10.746f	80851239	13909269	2.687 1.727 #
16)	T	DCPA	11.403	10.746	4592185	13909269	<MDL 1.886 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092922\
Data File : PS020672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2022 10:13
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 00:14:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

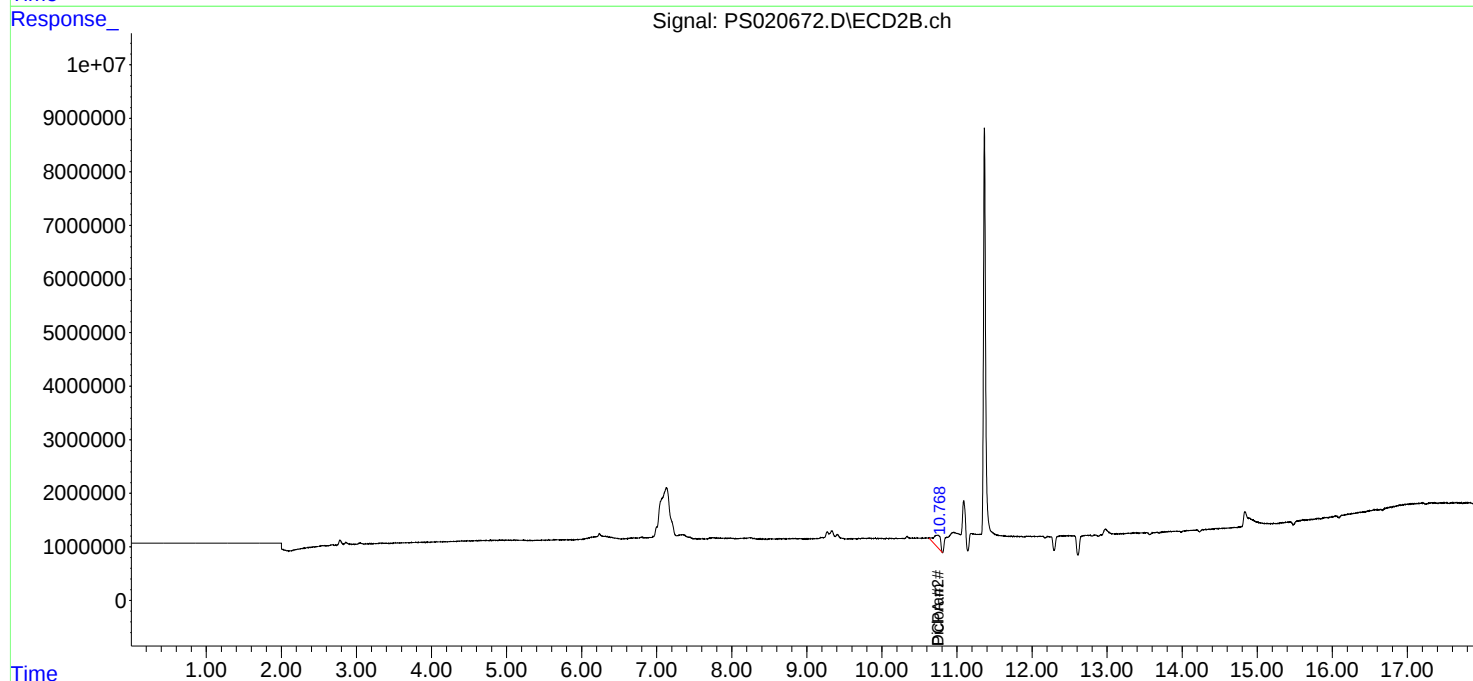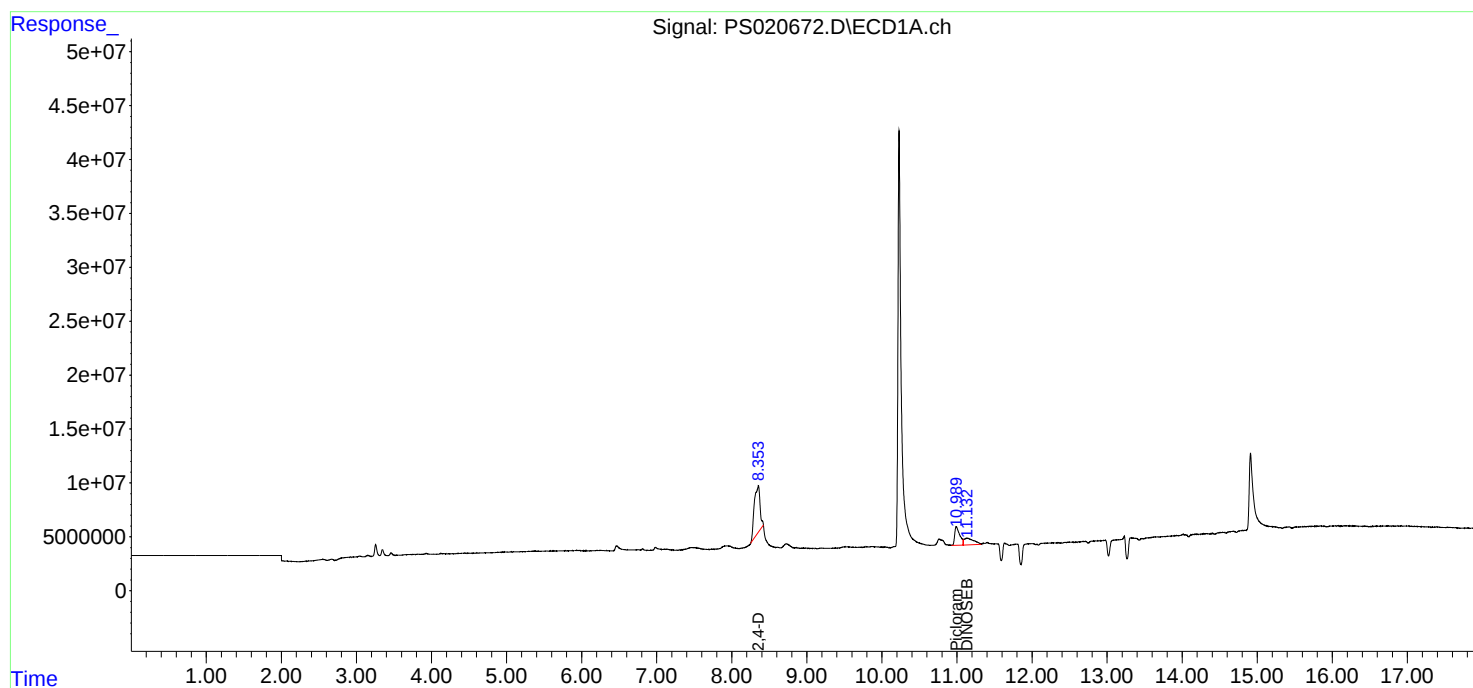


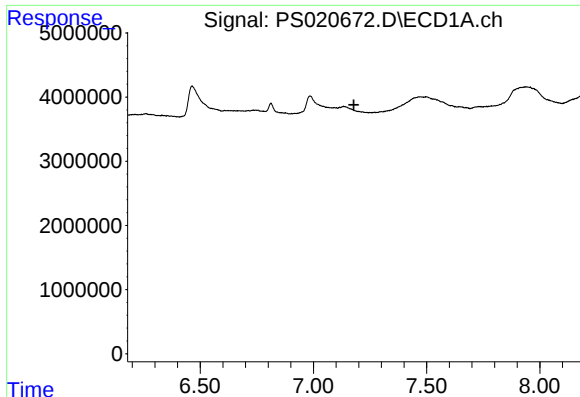

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.179 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

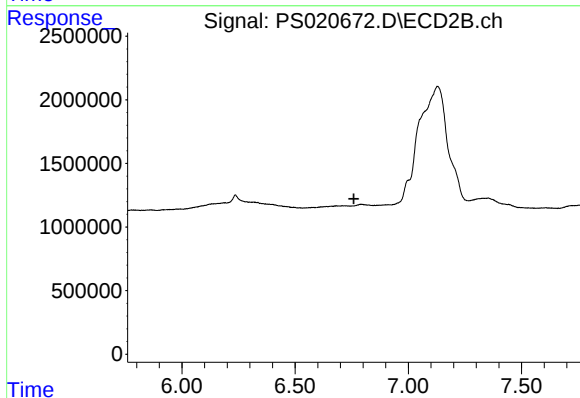


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.760 min
Response: 0
Conc: N.D.

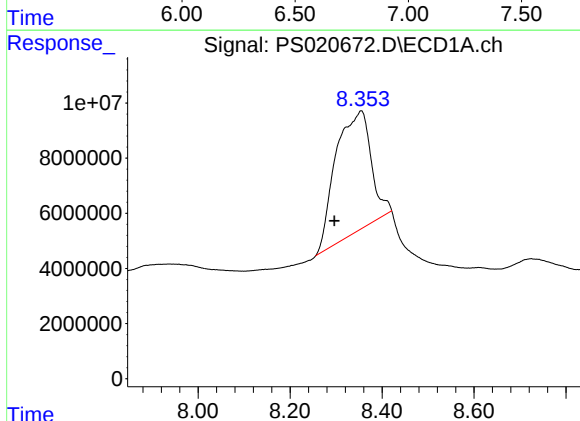


#9 2,4-D

R.T.: 8.354 min
Delta R.T.: 0.058 min
Response: 235355950
Conc: 50.64 ng/ml

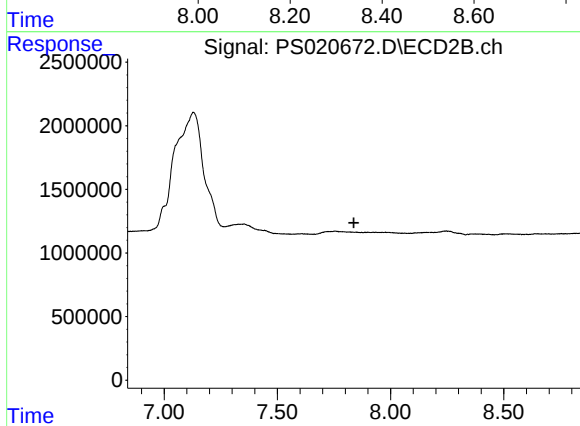

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.

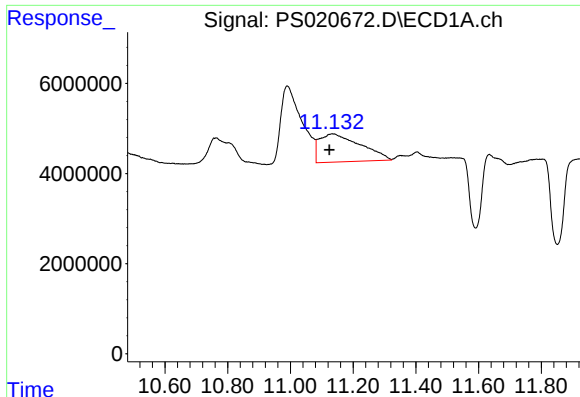

#14 DINOSEB


R.T.: 11.134 min
Delta R.T.: 0.009 min
Response: 56871691
Conc: 3.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

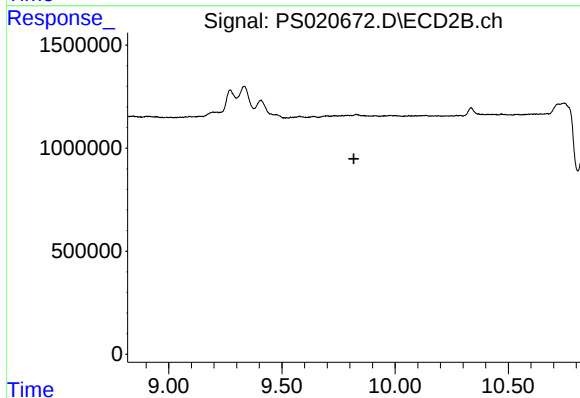


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.

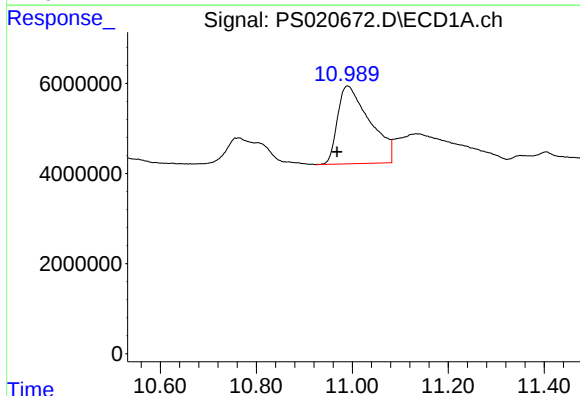


#15 Picloram

R.T.: 10.990 min
Delta R.T.: 0.022 min
Response: 80851239
Conc: 2.69 ng/ml

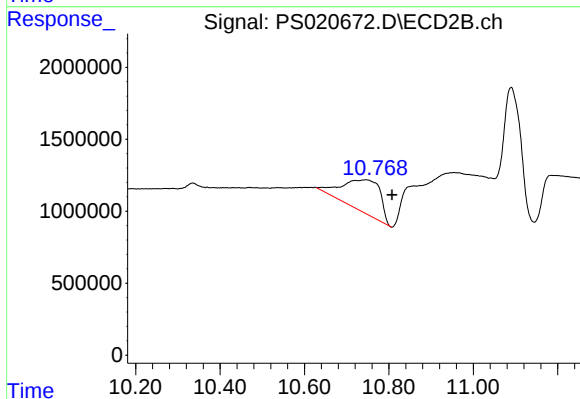

#15 Picloram


R.T.: 10.746 min
Delta R.T.: -0.062 min
Response: 13909269
Conc: 1.73 ng/ml

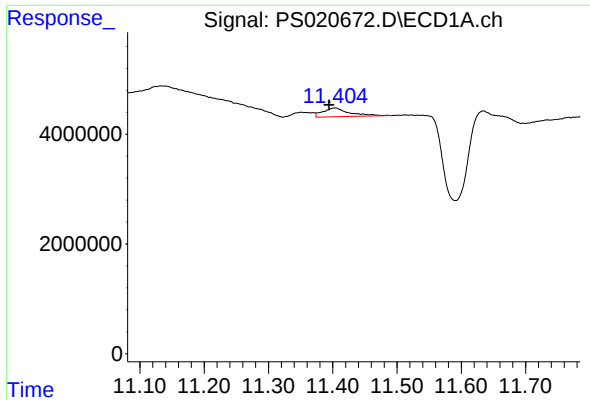

#16 DCPA

R.T.: 11.403 min
Delta R.T.: 0.009 min
Response: 4592185
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

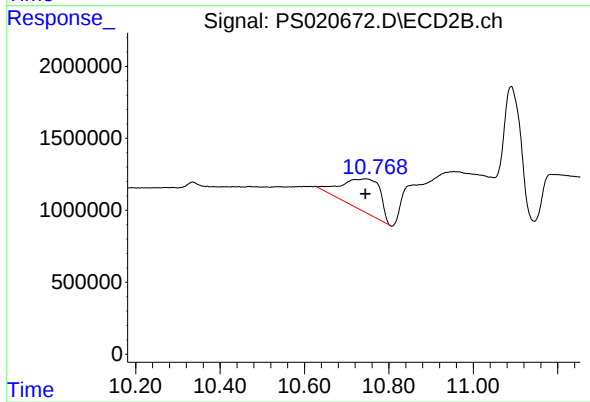

#16 DCPA

R.T.: 10.746 min
Delta R.T.: 0.002 min
Response: 13909269
Conc: 1.89 ng/ml