

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092922\
 Data File : PS020682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2022 14:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 00:23:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.179	6.761	1577.3E6	490.1E6	458.310	575.446 #
Target Compounds							
1) T	Dalapon	3.040	0.000	1425337	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.449f	0.000	103.1E6	0	20.667	N.D. #
5) T	DICAMBA	0.000	6.988f	0	19553425	N.D.	5.079
6) T	MCP	0.000	6.988	0	19553425	N.D.	6.771
7) T	MCPA	7.649	0.000	1167269	0	<MDL	N.D. #
10) T	Pentachlo...	8.594	0.000	191456	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.094f	0.000	2947395	0	<MDL	N.D. #
12) T	2,4,5-T	9.448	0.000	5376860	0	<MDL	N.D. #
13) T	2,4-DB	9.919f	0.000	2342339	0	<MDL	N.D. #
14) T	DINOSEB	11.132	0.000	12546780	0	<MDL	N.D. #
15) T	Picloram	10.960	10.747f	70207038	19030932	2.333	2.363
16) T	DCPA	11.428	10.747	7643312	19030932	<MDL	2.580 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092922\
Data File : PS020682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2022 14:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 00:23:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

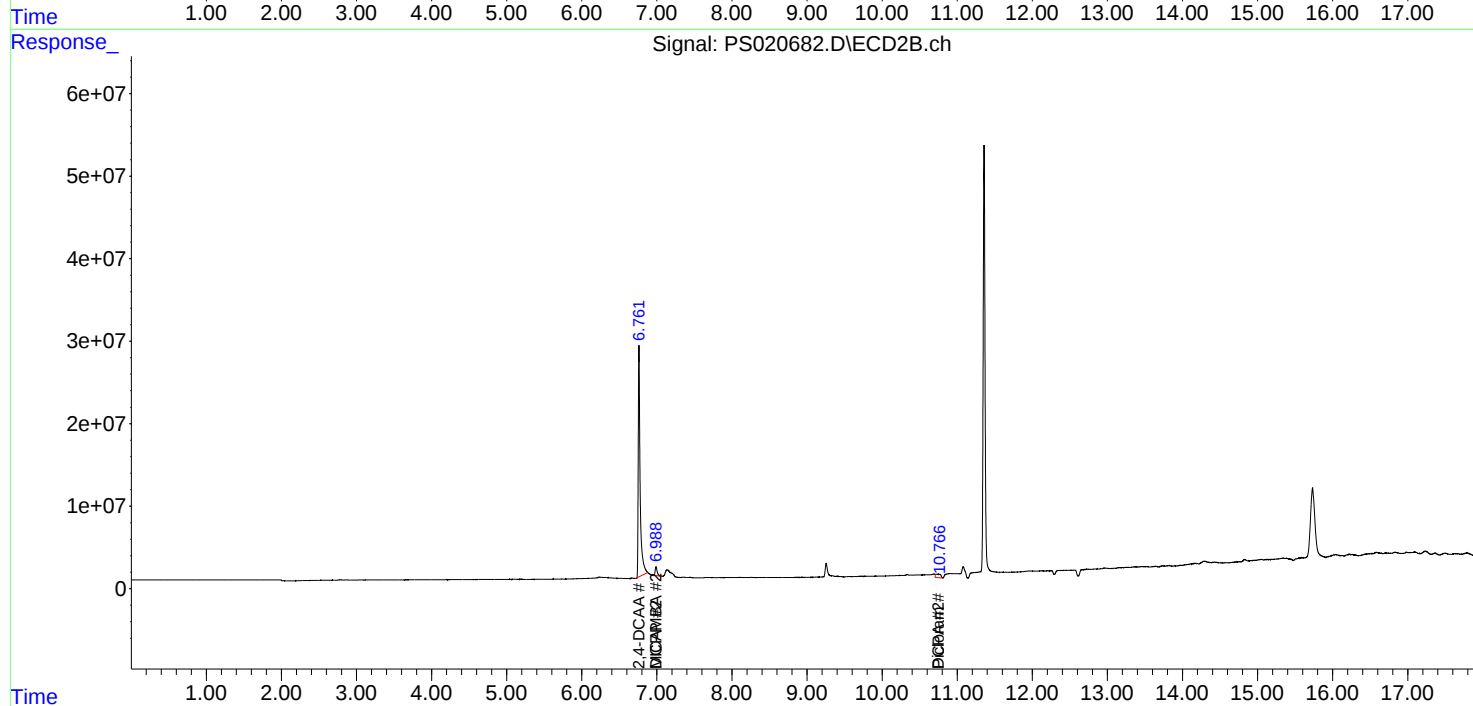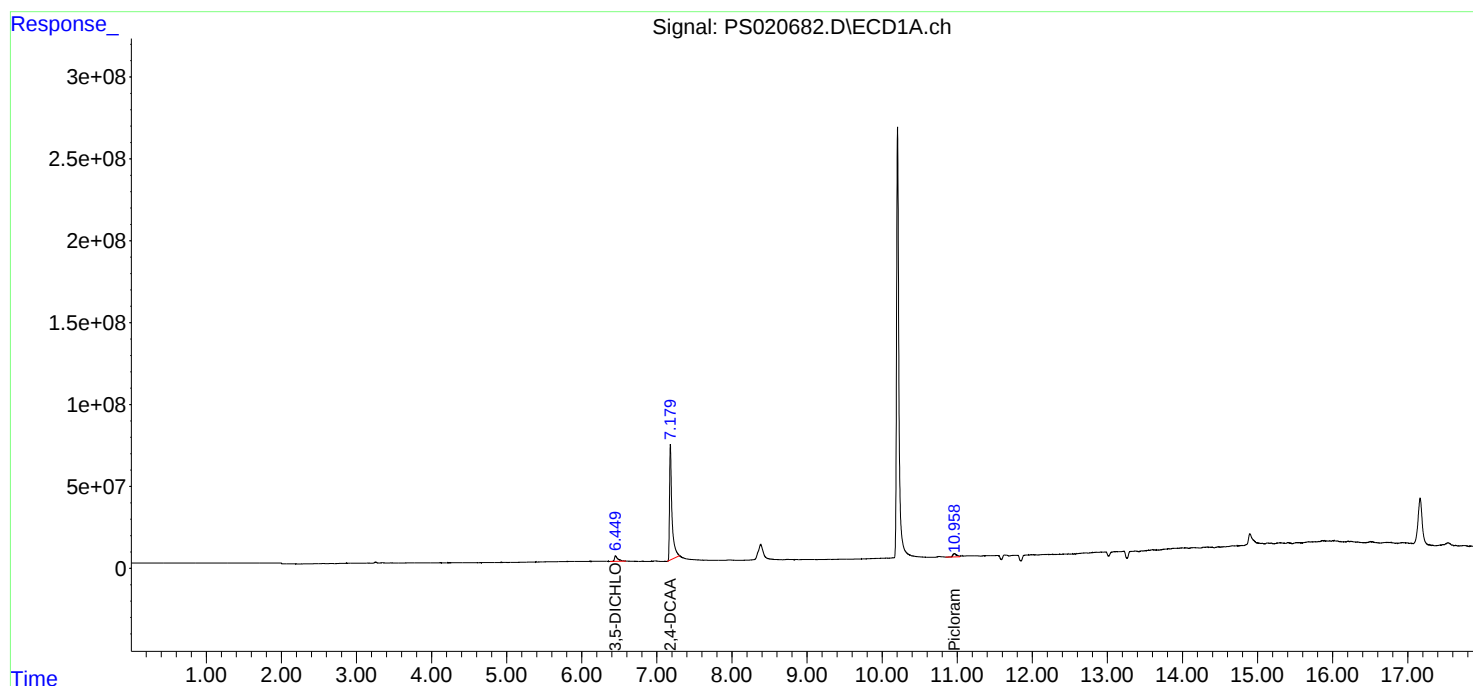


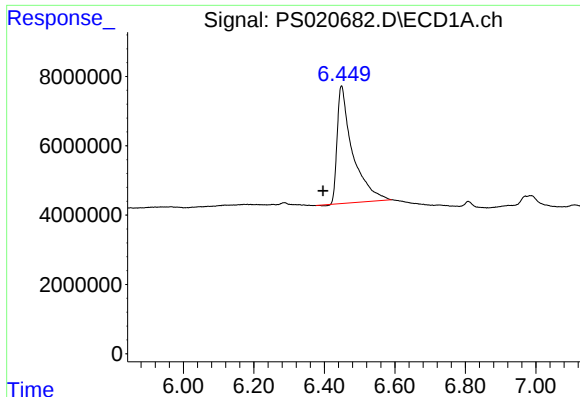

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.449 min
Delta R.T.: 0.053 min
Response: 103058171
Conc: 20.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

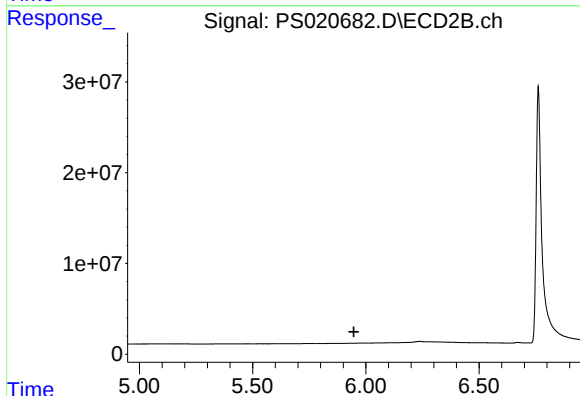


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

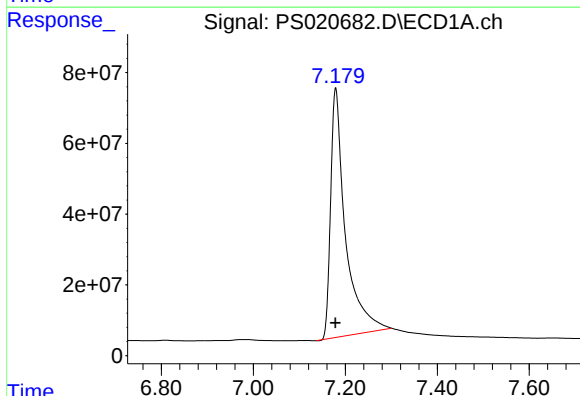


#4 2,4-DCAA

R.T.: 7.179 min
Delta R.T.: 0.000 min
Response: 1577267262
Conc: 458.31 ng/ml

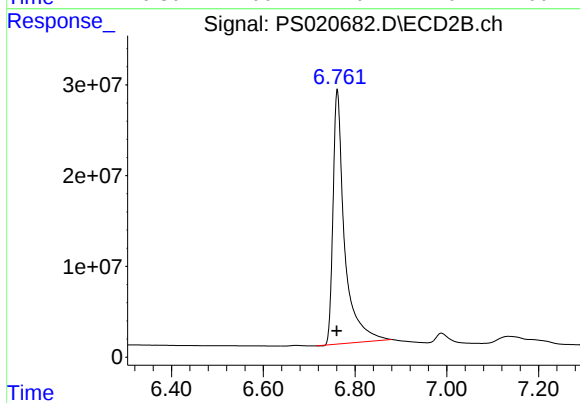

#4 2,4-DCAA


R.T.: 6.761 min
Delta R.T.: 0.002 min
Response: 490104337
Conc: 575.45 ng/ml

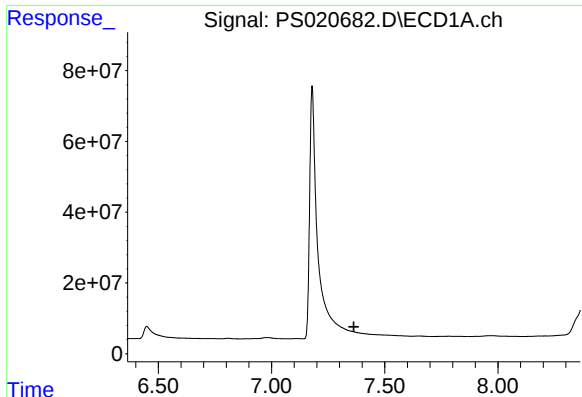

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

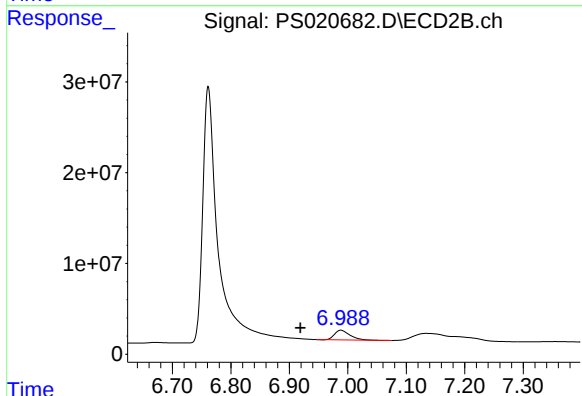


#5 DICAMBA

R.T.: 6.988 min
Delta R.T.: 0.069 min
Response: 19553425
Conc: 5.08 ng/ml

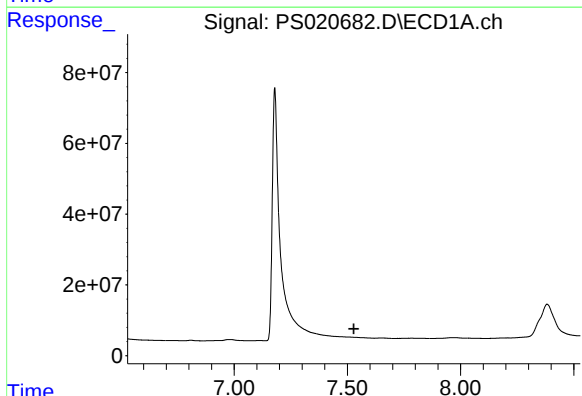


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.529 min
Response: 0
Conc: N.D.

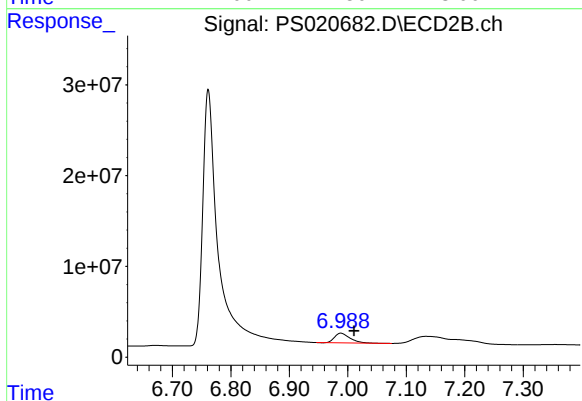

#6 MCP


R.T.: 6.988 min
Delta R.T.: -0.023 min
Response: 19553425
Conc: 6.77 ug/ml

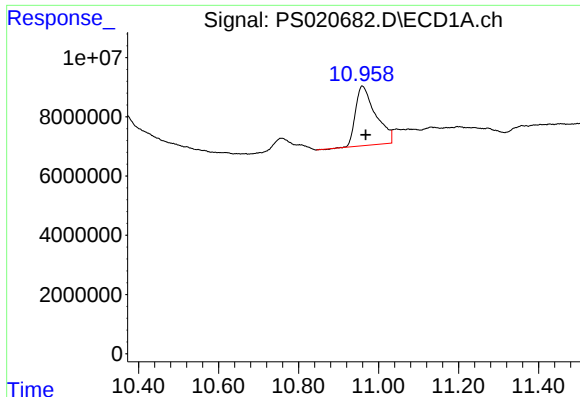

#15 Picloram


R.T.: 10.960 min
Delta R.T.: -0.009 min
Response: 70207038
Conc: 2.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

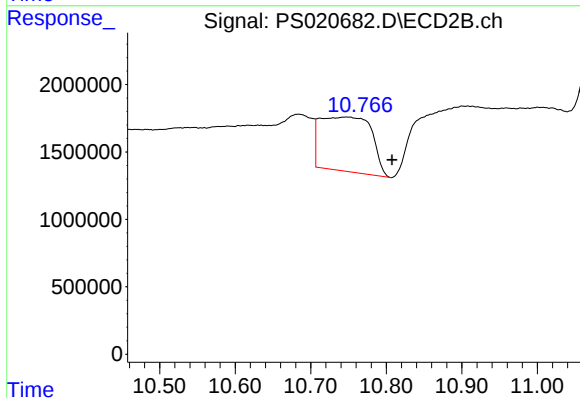


#15 Picloram

R.T.: 10.747 min
Delta R.T.: -0.061 min
Response: 19030932
Conc: 2.36 ng/ml

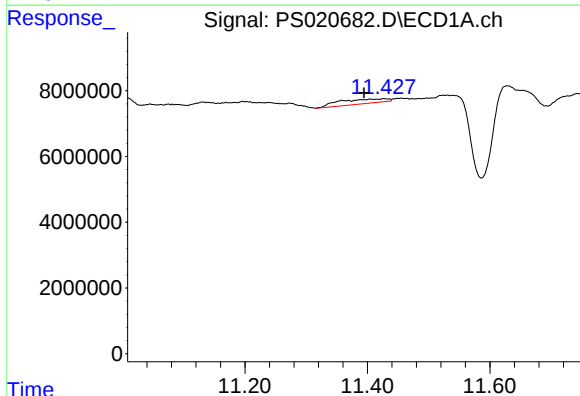

#16 DCPA

R.T.: 11.428 min
Delta R.T.: 0.033 min
Response: 7643312
Conc: N.D.

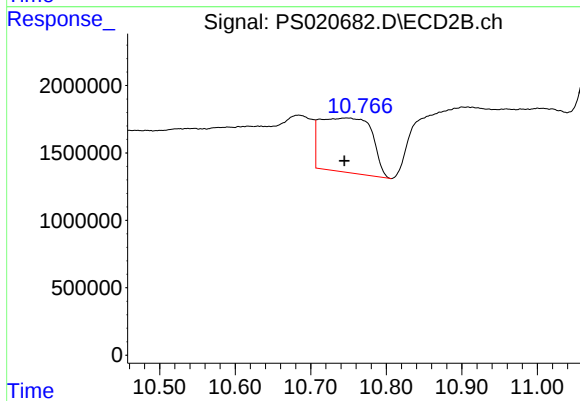

#16 DCPA

R.T.: 10.747 min
Delta R.T.: 0.003 min
Response: 19030932
Conc: 2.58 ng/ml