

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092925\  
 Data File : PS031868.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 29 Sep 2025 18:06  
 Operator : AR\AJ  
 Sample : PB169875BL  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 30 02:26:44 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS090925.M  
 Quant Title : 8080.M  
 QLast Update : Tue Sep 09 13:56:38 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1    | RT#2    | Resp#1   | Resp#2    | ng/ml   | ng/ml    |
|-----------------------------|--------------|---------|---------|----------|-----------|---------|----------|
| -----                       |              |         |         |          |           |         |          |
| System Monitoring Compounds |              |         |         |          |           |         |          |
| 4) S                        | 2,4-DCAA     | 7.282   | 7.739   | 1648.8E6 | 470.3E6   | 457.798 | 517.441  |
| Target Compounds            |              |         |         |          |           |         |          |
| 1) T                        | Dalapon      | 0.000   | 2.656f  | 0        | 1311.5E6  | N.D.    | 465.451  |
| 2) T                        | 3,5-DICHL... | 6.435   | 6.729f  | 9859172  | 11578661  | 1.849   | 7.593 #  |
| 6) T                        | MCPD         | 0.000   | 8.041   | 0        | 4888270   | N.D.    | 2.595    |
| 7) T                        | MCPA         | 7.788   | 0.000   | 3757467  | 0         | <MDL    | N.D. #   |
| 8) T                        | DICHLORPROP  | 8.150f  | 8.644   | 530735   | 6149370   | <MDL    | 4.226 #  |
| 9) T                        | 2,4-D        | 0.000   | 9.039f  | 0        | 2049799   | N.D.    | 1.246    |
| 10) T                       | Pentachlo... | 8.707   | 9.506   | 13633172 | 36839925  | <MDL    | <MDL #   |
| 11) T                       | 2,4,5-TP ... | 9.250f  | 9.876   | 1626879  | 327.2E6   | <MDL    | 21.734 # |
| 12) T                       | 2,4,5-T      | 9.580   | 10.338  | 111.5E6  | 111.6E6   | 6.094   | 8.290 #  |
| 13) T                       | 2,4-DB       | 10.183f | 10.919f | 357.8E6  | -12283463 | 153.399 | N.D. #   |
| 14) T                       | DINOSEB      | 11.315f | 11.285  | 136.1E6  | 13253631  | 9.437   | 1.363 #  |
| 15) T                       | Picloram     | 11.155  | 12.413f | 32415184 | 358.6E6   | 1.800   | 15.141 # |
| 16) T                       | DCPA         | 11.620f | 12.330  | 55892601 | 22895324  | 2.074   | <MDL #   |
| -----                       |              |         |         |          |           |         |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS092925\  
Data File : PS031868.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 29 Sep 2025 18:06  
Operator : AR\AJ  
Sample : PB169875BL  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 30 02:26:44 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS090925.M  
Quant Title : 8080.M  
QLast Update : Tue Sep 09 13:56:38 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

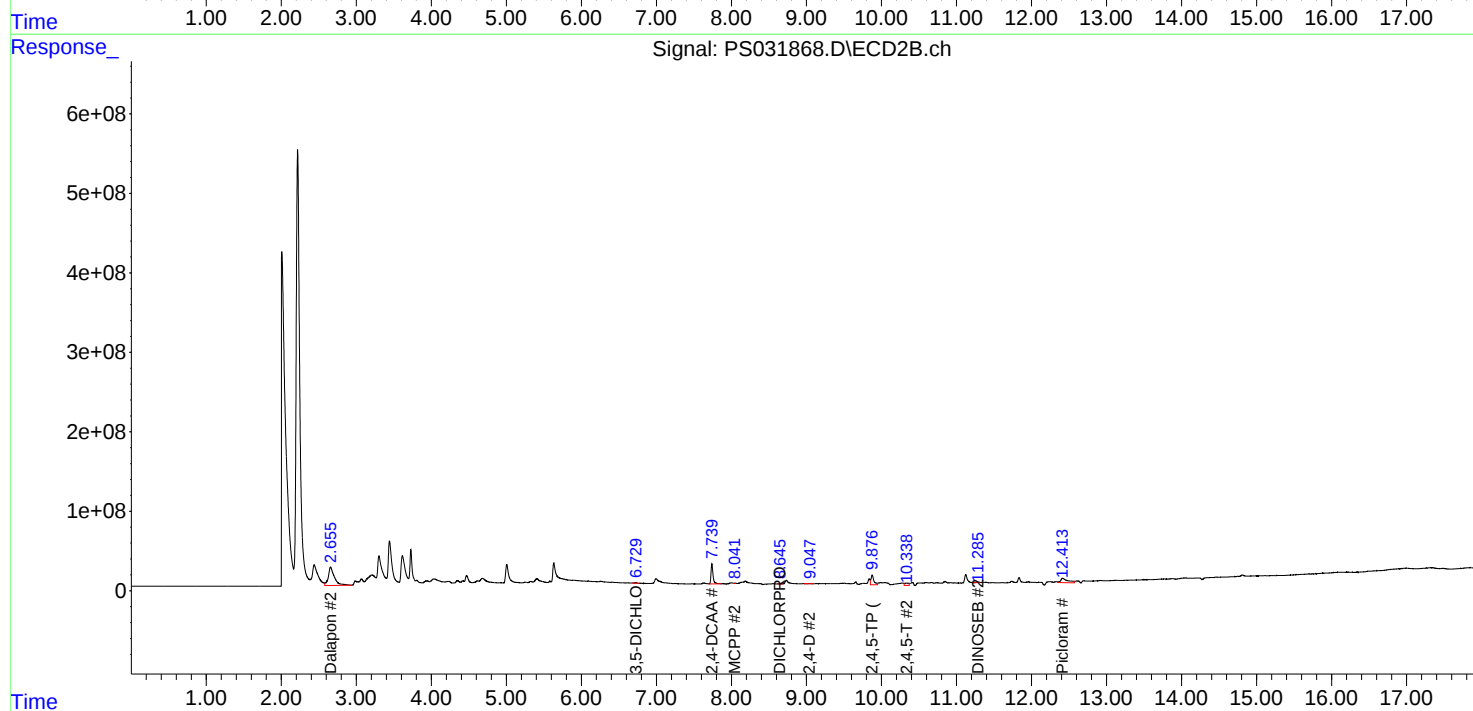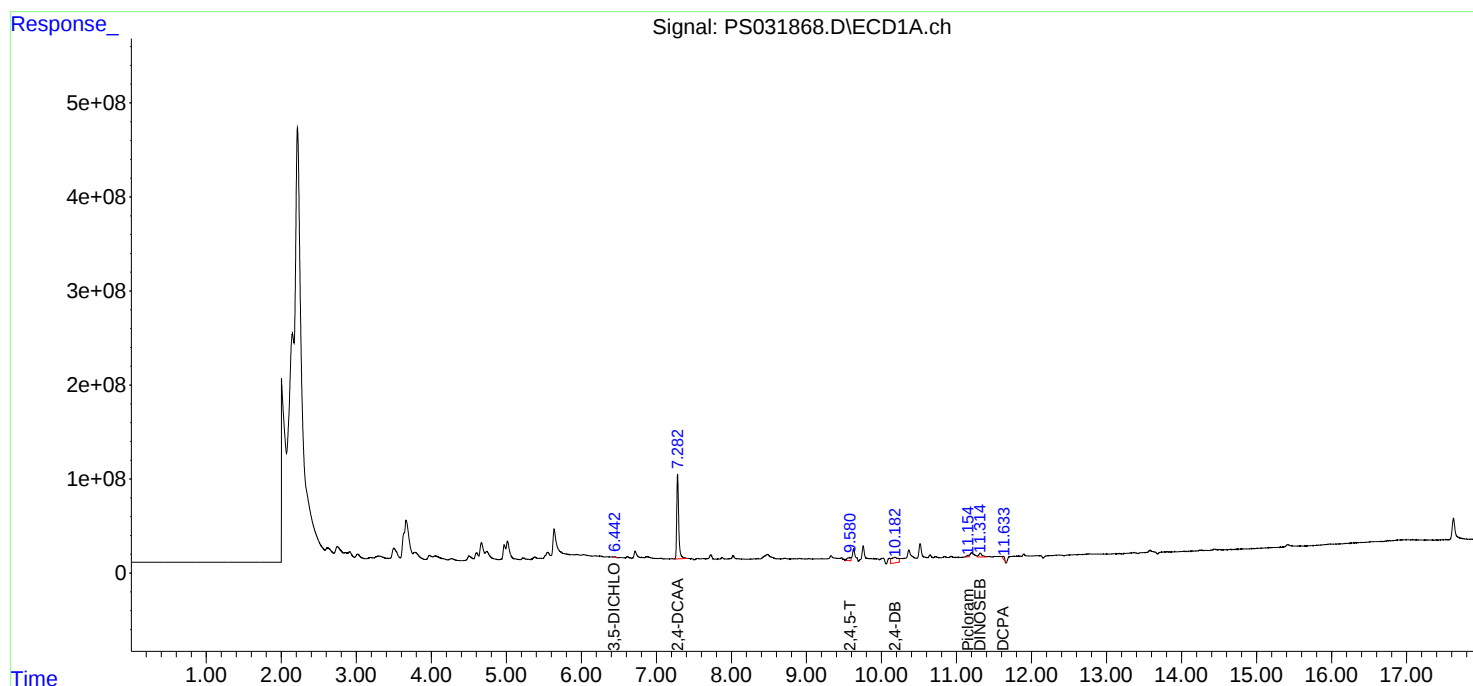


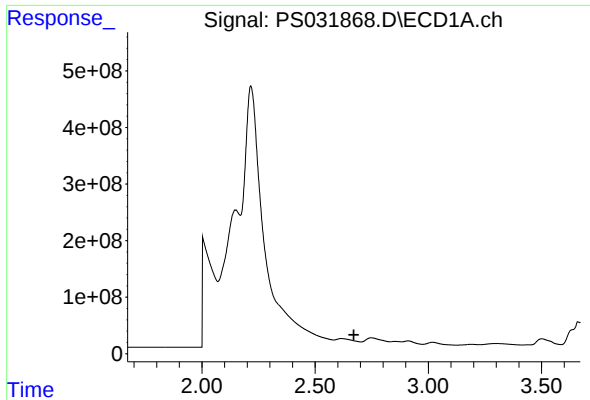

#1 Dalapon


R.T.: 0.000 min  
Exp R.T.: 2.671 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

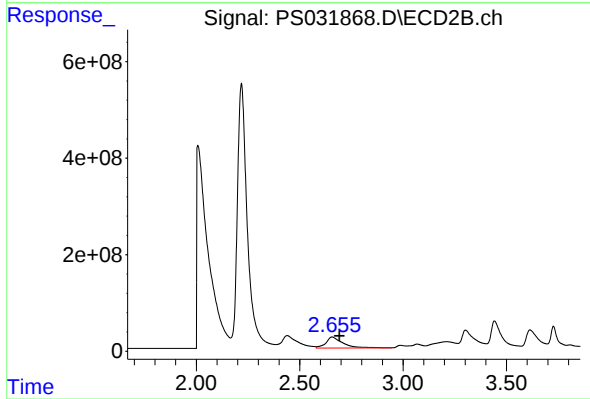


#1 Dalapon

R.T.: 2.656 min  
Delta R.T.: -0.036 min  
Response: 1311467297  
Conc: 465.45 ng/ml

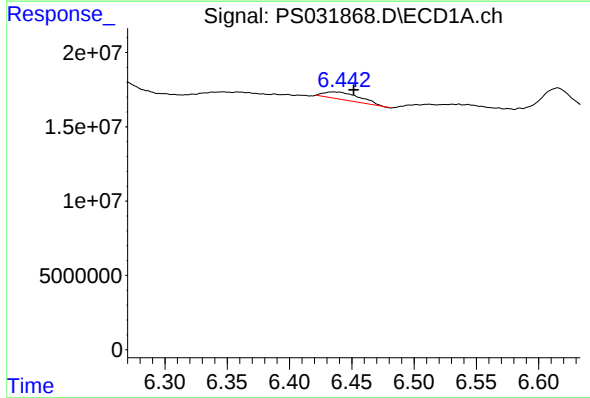


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.435 min  
Delta R.T.: -0.017 min  
Response: 9859172  
Conc: 1.85 ng/ml

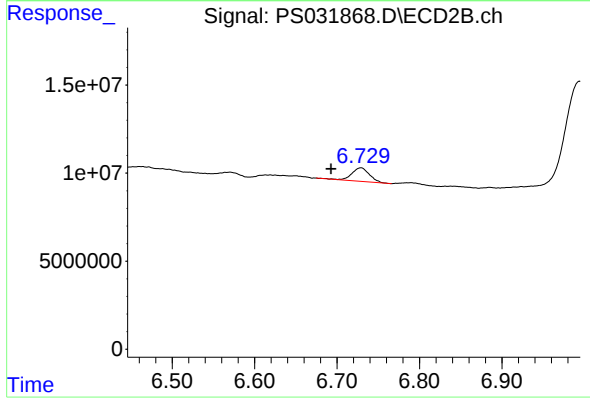

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.729 min  
Delta R.T.: 0.036 min  
Response: 11578661  
Conc: 7.59 ng/ml

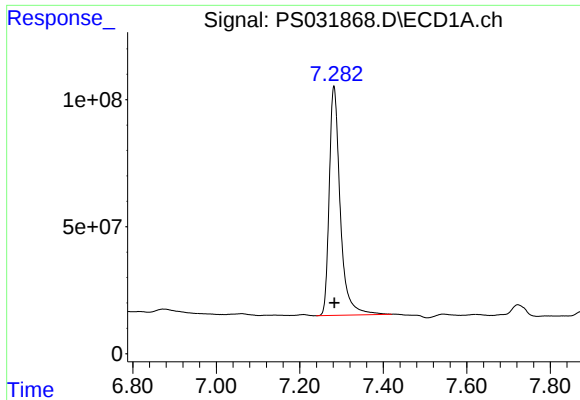

#4 2,4-DCAA


R.T.: 7.282 min  
Delta R.T.: -0.001 min  
Response: 1648770964  
Conc: 457.80 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

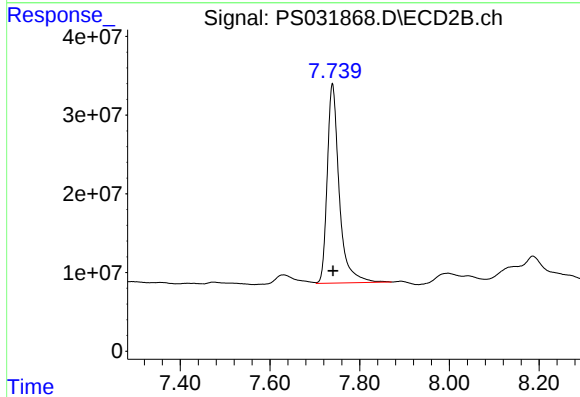


#4 2,4-DCAA

R.T.: 7.739 min  
Delta R.T.: -0.001 min  
Response: 470301760  
Conc: 517.44 ng/ml

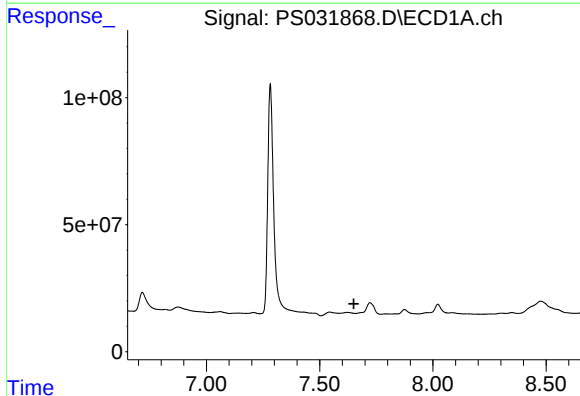


#6 MCP

R.T.: 0.000 min  
Exp R.T. : 7.651 min  
Response: 0  
Conc: N.D.

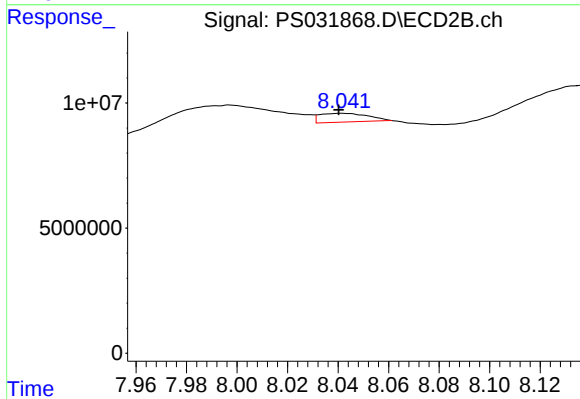

#6 MCP


R.T.: 8.041 min  
Delta R.T.: 0.001 min  
Response: 4888270  
Conc: 2.60 ug/ml

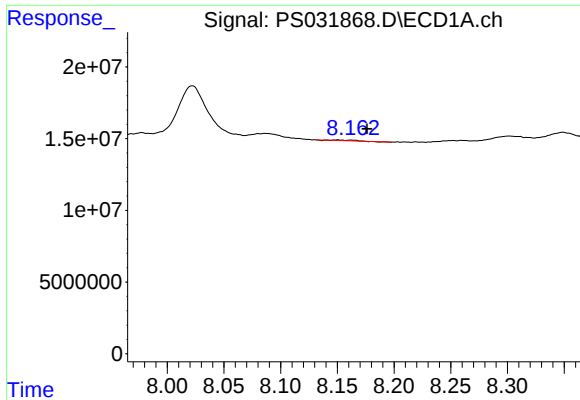

#8 DICHLORPROP


R.T.: 8.150 min  
Delta R.T.: -0.026 min  
Response: 530735  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

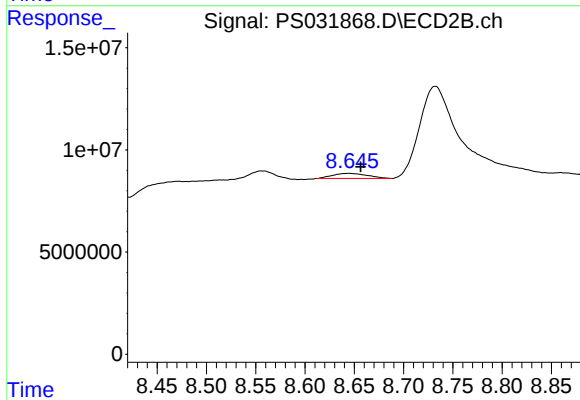


#8 DICHLORPROP

R.T.: 8.644 min  
Delta R.T.: -0.012 min  
Response: 6149370  
Conc: 4.23 ng/ml

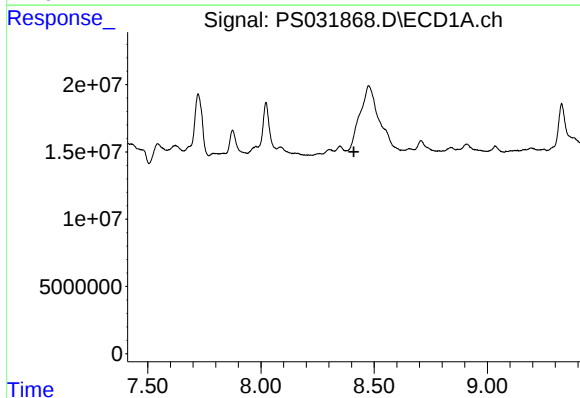


#9 2,4-D

R.T.: 0.000 min  
Exp R.T. : 8.411 min  
Response: 0  
Conc: N.D.

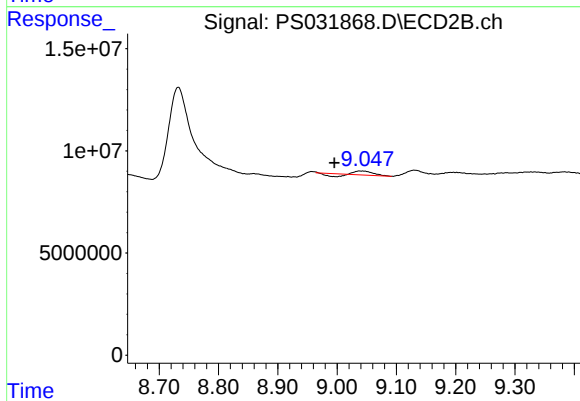

#9 2,4-D


R.T.: 9.039 min  
Delta R.T.: 0.043 min  
Response: 2049799  
Conc: 1.25 ng/ml

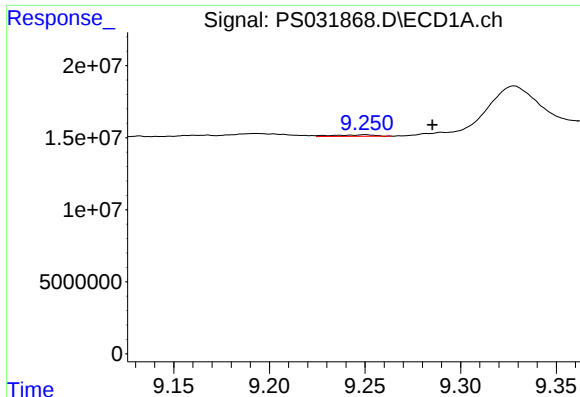

#11 2,4,5-TP (SILVEX)


R.T.: 9.250 min  
Delta R.T.: -0.035 min  
Response: 1626879  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

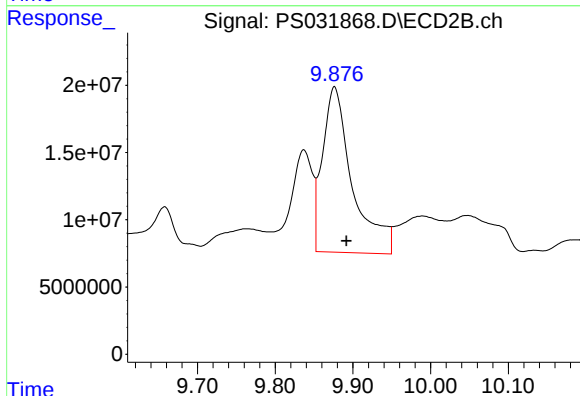


#11 2,4,5-TP (SILVEX)

R.T.: 9.876 min  
Delta R.T.: -0.015 min  
Response: 327192591  
Conc: 21.73 ng/ml

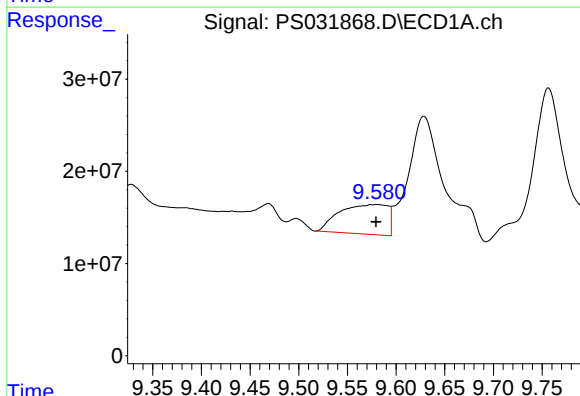


#12 2,4,5-T

R.T.: 9.580 min  
Delta R.T.: 0.000 min  
Response: 111510098  
Conc: 6.09 ng/ml

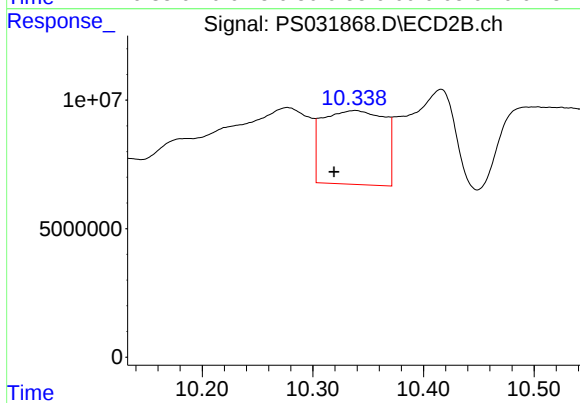

#12 2,4,5-T


R.T.: 10.338 min  
Delta R.T.: 0.019 min  
Response: 111556579  
Conc: 8.29 ng/ml

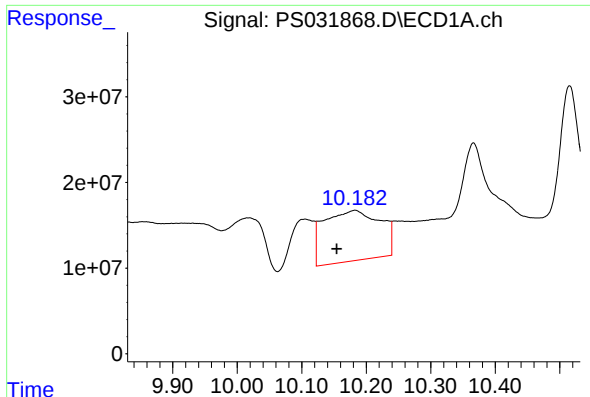

#13 2,4-DB


R.T.: 10.183 min  
Delta R.T.: 0.028 min  
Response: 357843736  
Conc: 153.40 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

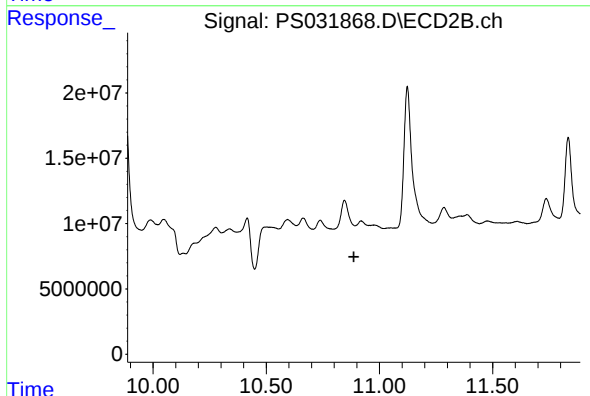


#13 2,4-DB

R.T.: 10.919 min  
Delta R.T.: 0.032 min  
Response: -12283463  
Conc: N.D.

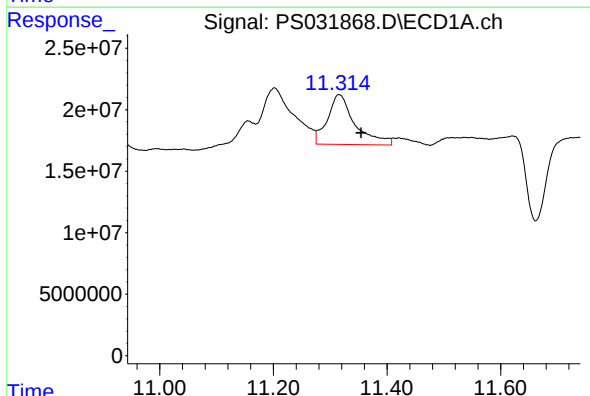


#14 DINOSEB

R.T.: 11.315 min  
Delta R.T.: -0.039 min  
Response: 136109319  
Conc: 9.44 ng/ml

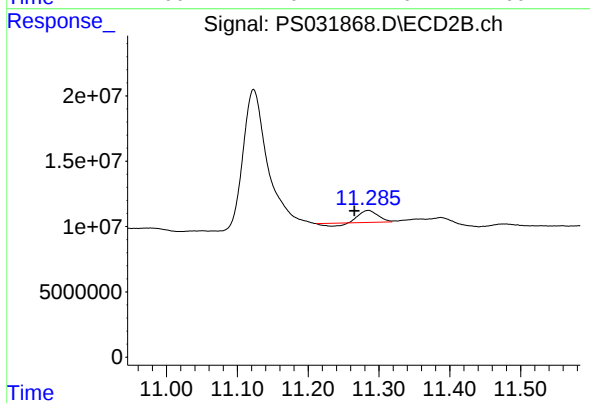

#14 DINOSEB


R.T.: 11.285 min  
Delta R.T.: 0.020 min  
Response: 13253631  
Conc: 1.36 ng/ml

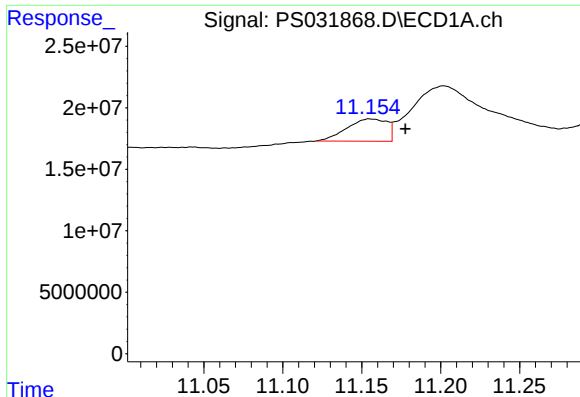

#15 Picloram


R.T.: 11.155 min  
Delta R.T.: -0.023 min  
Response: 32415184  
Conc: 1.80 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

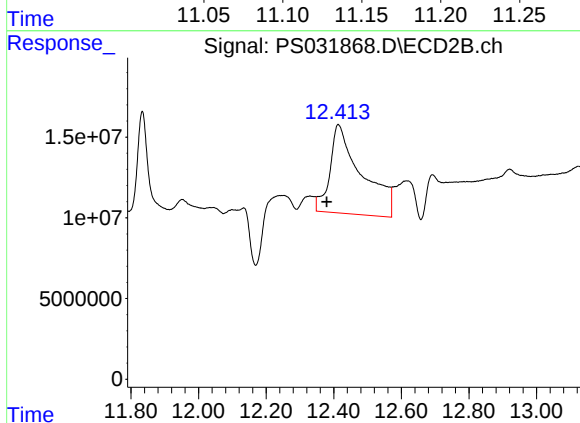


#15 Picloram

R.T.: 12.413 min  
Delta R.T.: 0.034 min  
Response: 358586339  
Conc: 15.14 ng/ml

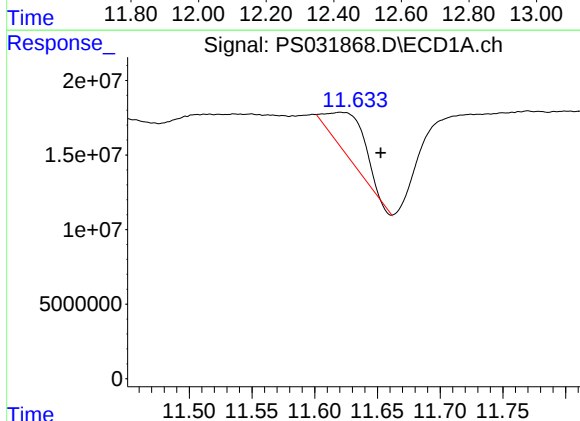

#16 DCPA

R.T.: 11.620 min  
Delta R.T.: -0.032 min  
Response: 55892601  
Conc: 2.07 ng/ml

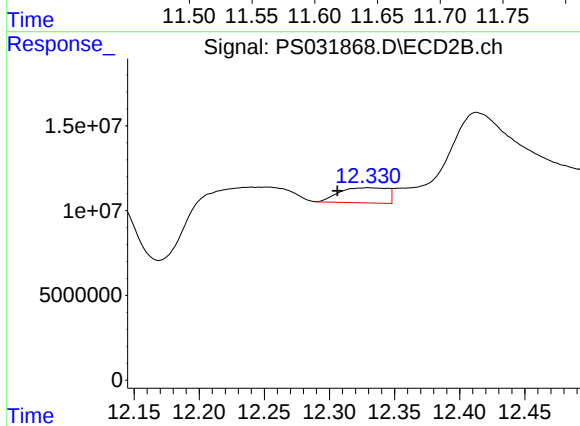

#16 DCPA

R.T.: 12.330 min  
Delta R.T.: 0.024 min  
Response: 22895324  
Conc: N.D.