

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092925\
 Data File : PS031878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2025 22:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 02:30:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.282	7.744	1872.9E6	529.4E6	520.031	582.499
Target Compounds							
1) T	Dalapon	0.000	2.652f	0	2292539	N.D.	<MDL
2) T	3,5-DICHL...	6.440	0.000	13665498	0	2.562	N.D. #
7) T	MCPA	7.847f	0.000	64011	0	<MDL	N.D. #
8) T	DICHLORPROP	8.179	8.692f	978131	397894	<MDL	<MDL #
9) T	2,4-D	0.000	8.983	0	3708050	N.D.	2.254
10) T	Pentachlo...	8.704	9.510	7965089	12026747	<MDL	<MDL #
11) T	2,4,5-TP ...	9.286	9.908	5922409	6828827	<MDL	<MDL #
12) T	2,4,5-T	9.574	0.000	262139	0	<MDL	N.D. #
13) T	2,4-DB	10.132	0.000	1732613	0	<MDL	N.D. #
14) T	DINOSEB	11.358	0.000	2669080	0	<MDL	N.D. #
15) T	Picloram	11.163	0.000	11607084	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092925\
Data File : PS031878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2025 22:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 02:30:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

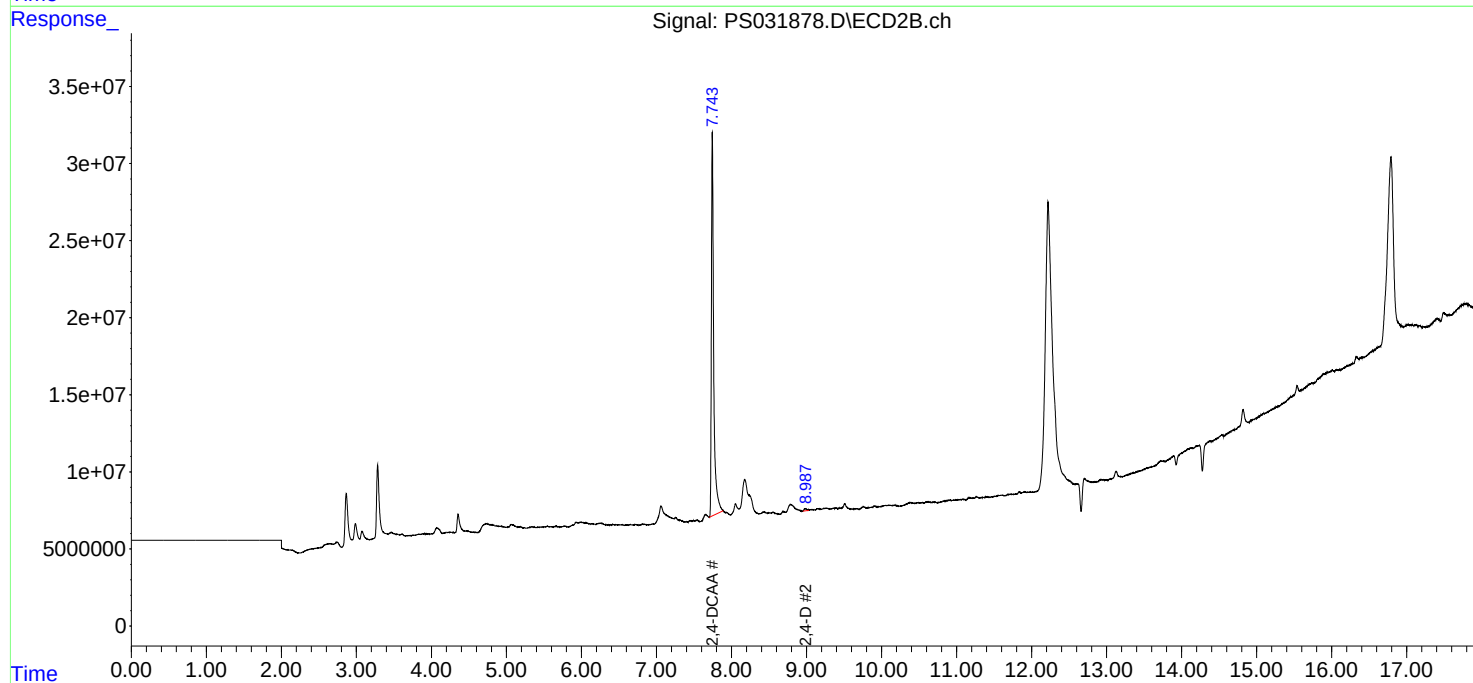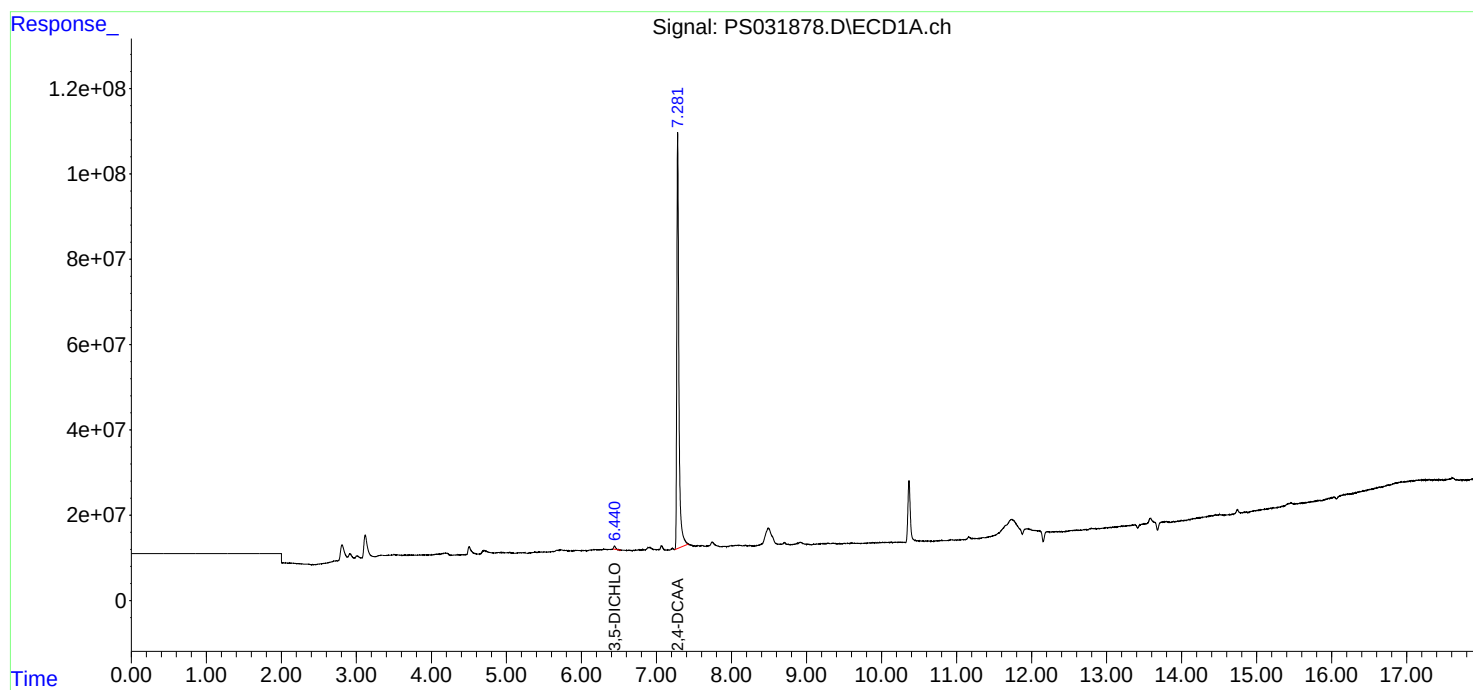


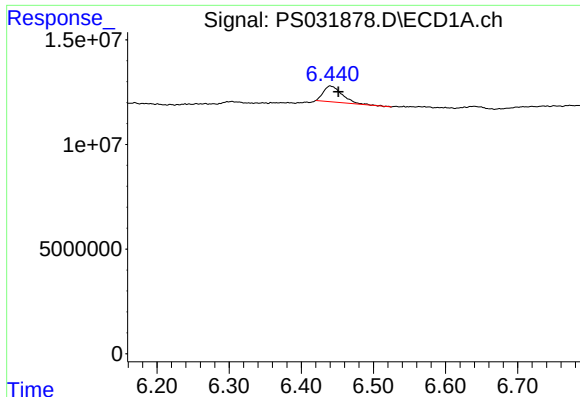

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.440 min
Delta R.T.: -0.011 min
Response: 13665498
Conc: 2.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

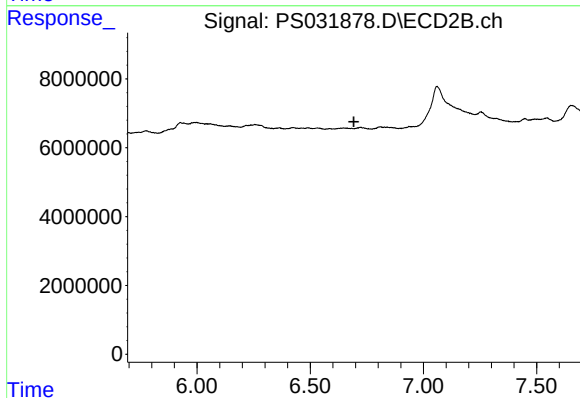


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

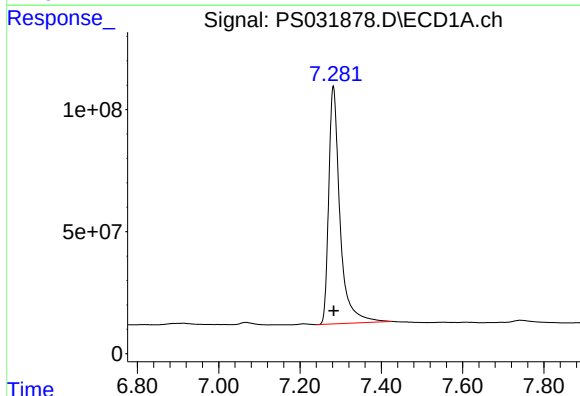


#4 2,4-DCAA

R.T.: 7.282 min
Delta R.T.: -0.001 min
Response: 1872904705
Conc: 520.03 ng/ml

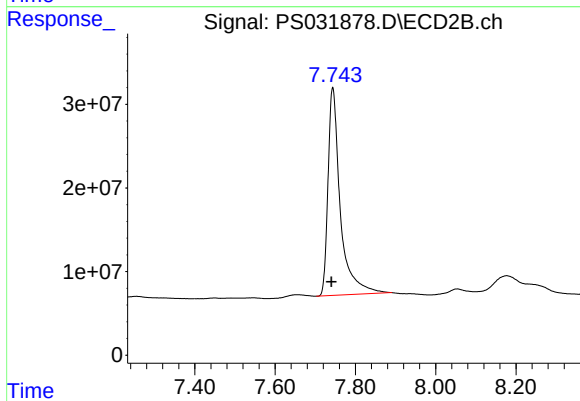

#4 2,4-DCAA


R.T.: 7.744 min
Delta R.T.: 0.003 min
Response: 529432787
Conc: 582.50 ng/ml

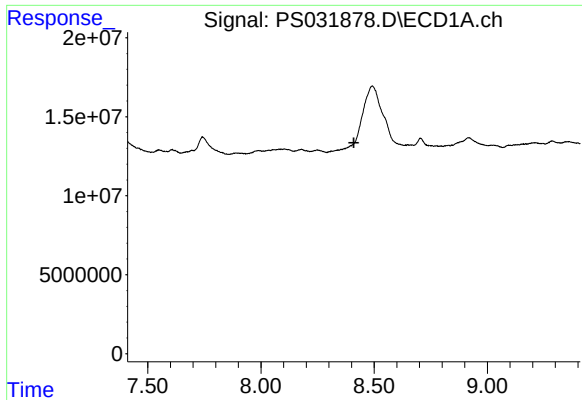

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

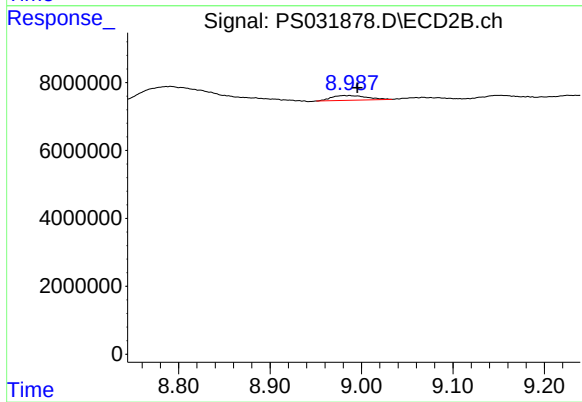

#9 2,4-D

R.T.: 8.983 min
Delta R.T.: -0.013 min
Response: 3708050
Conc: 2.25 ng/ml