

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
 Data File : PS006937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 08:35
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 03:13:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) T	4-Nitroph...	0.000	4.954	0	102.5E6	N.D. 424.048
12) T	2,4,5-T	0.000	7.279	0	13621801	N.D. 6.302
15) T	Picloram	9.012	8.977	100.7E6	56245107	15.012 15.453
16) T	DCPA	0.000	8.977	0	56245107	N.D. 17.701



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
Data File : PS006937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 08:35
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 03:13:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

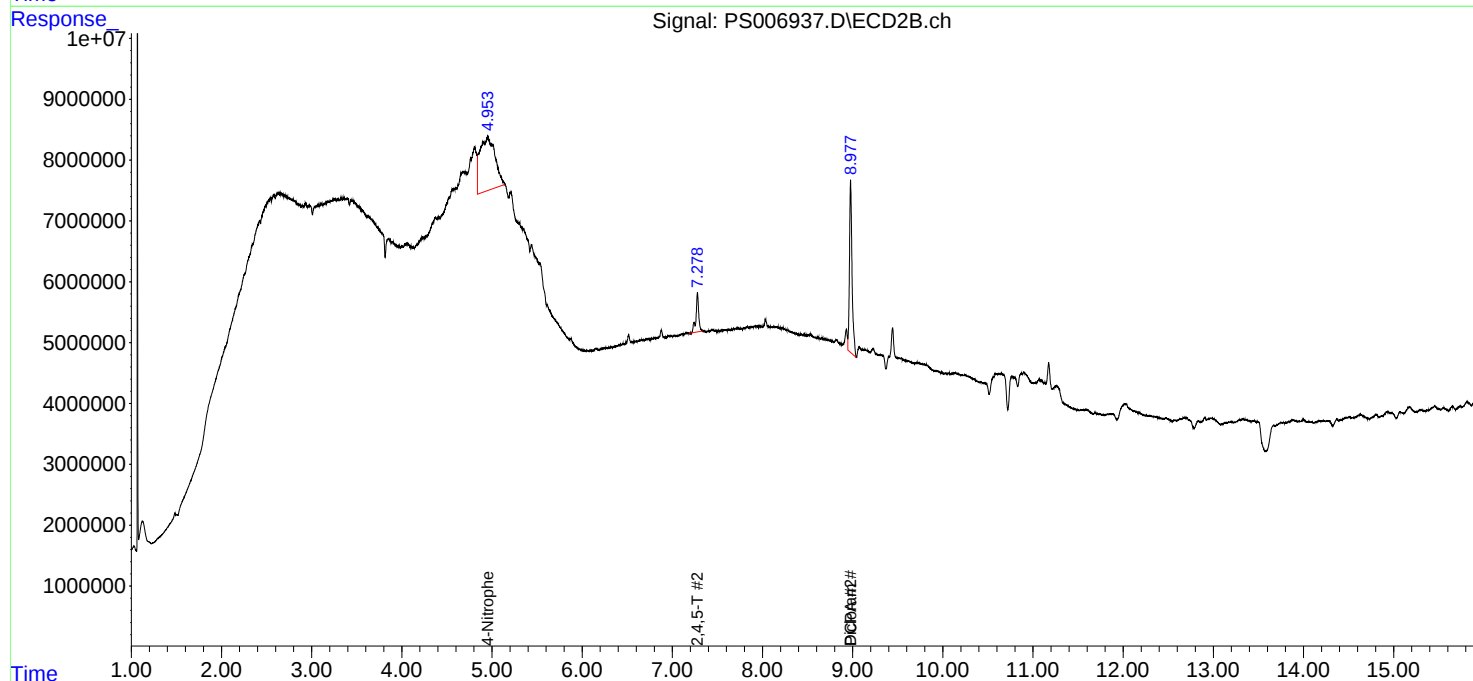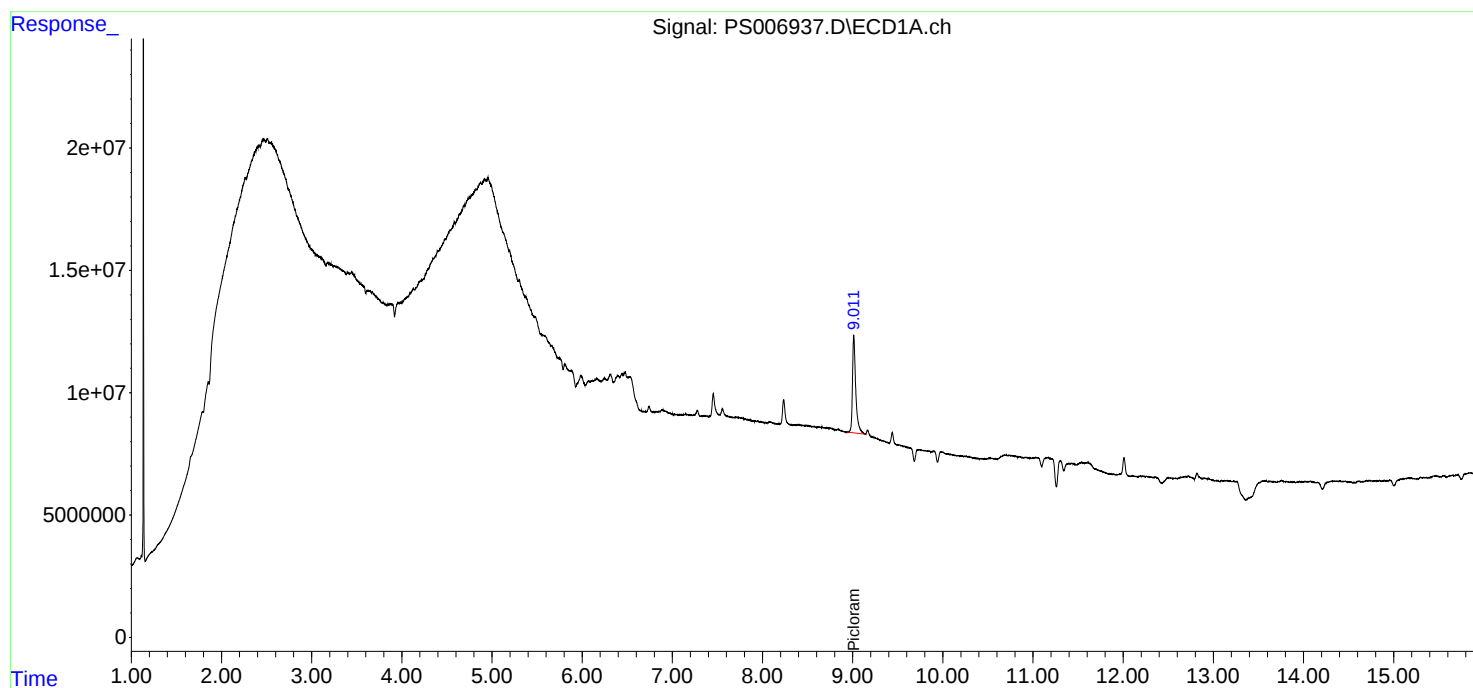


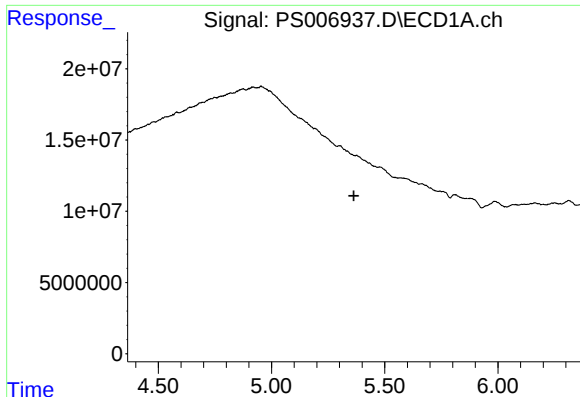

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.364 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

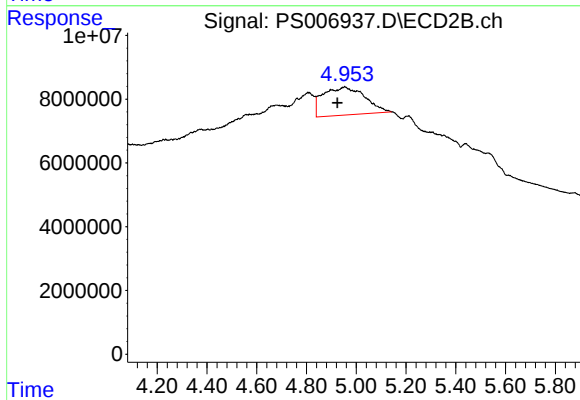


#3 4-Nitrophenol

R.T.: 4.954 min
Delta R.T.: 0.029 min
Response: 102505389
Conc: 424.05 ng/ml

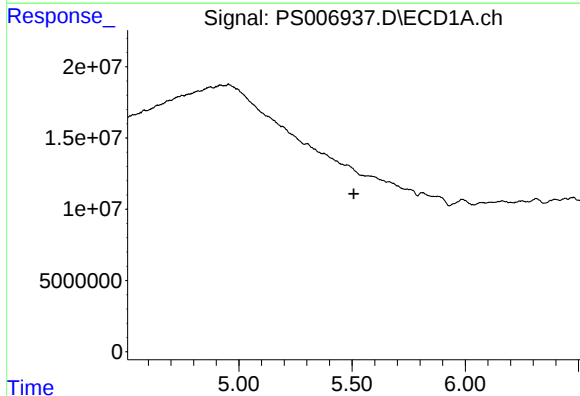


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

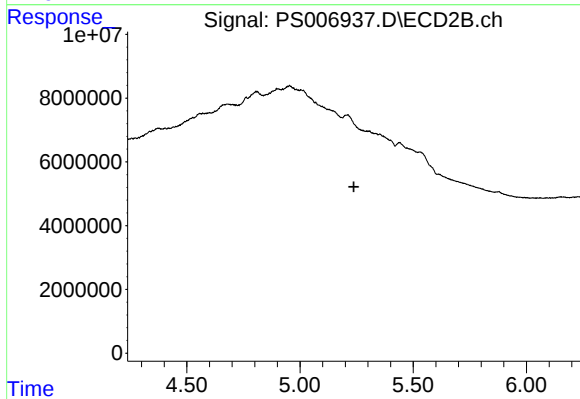

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.238 min
Response: 0
Conc: N.D.

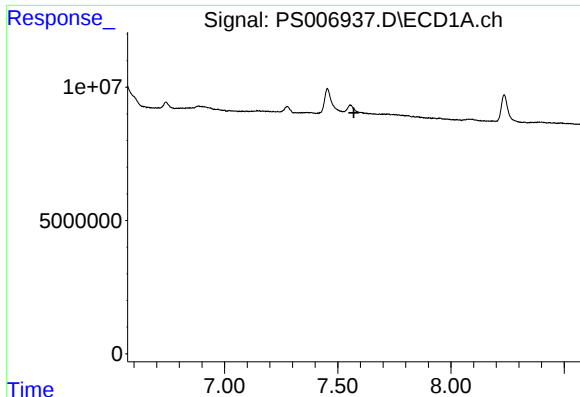

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

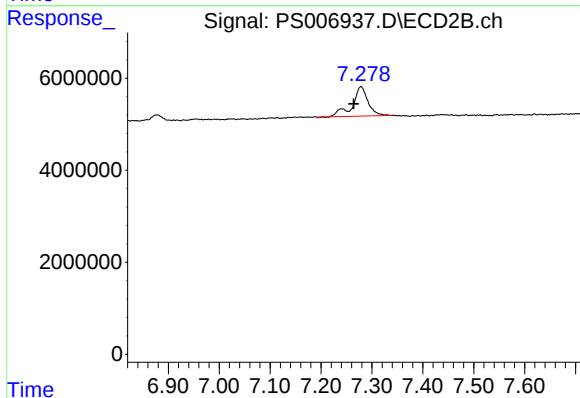


#12 2,4,5-T

R.T.: 7.279 min
Delta R.T.: 0.014 min
Response: 13621801
Conc: 6.30 ng/ml

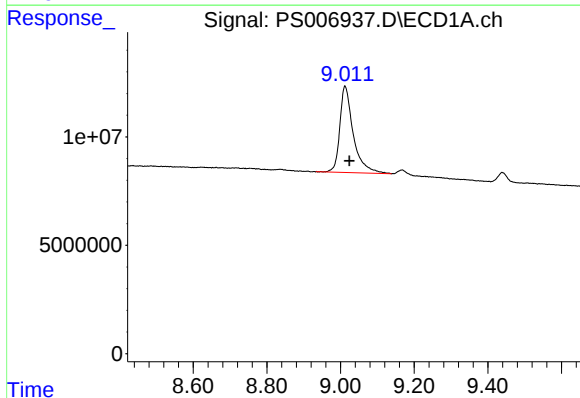


#15 Picloram

R.T.: 9.012 min
Delta R.T.: -0.012 min
Response: 100666429
Conc: 15.01 ng/ml

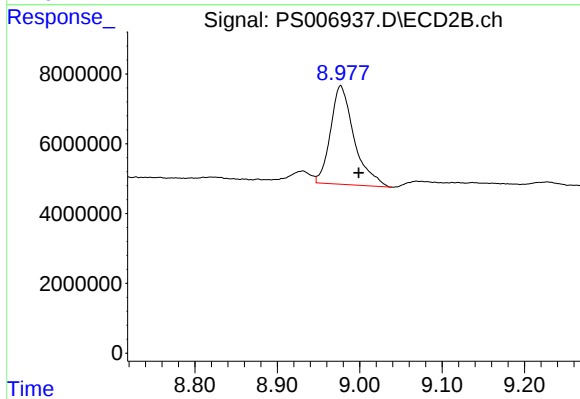

#15 Picloram


R.T.: 8.977 min
Delta R.T.: -0.022 min
Response: 56245107
Conc: 15.45 ng/ml

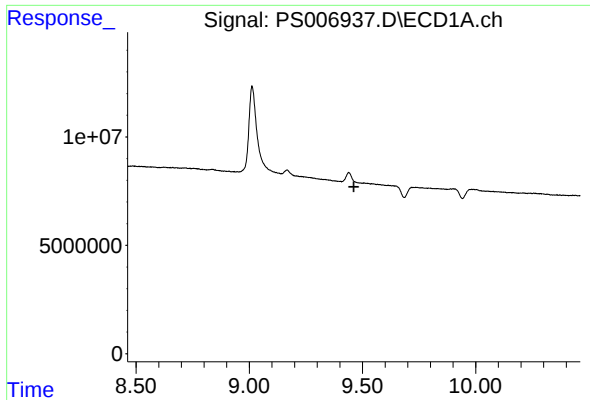

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.462 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

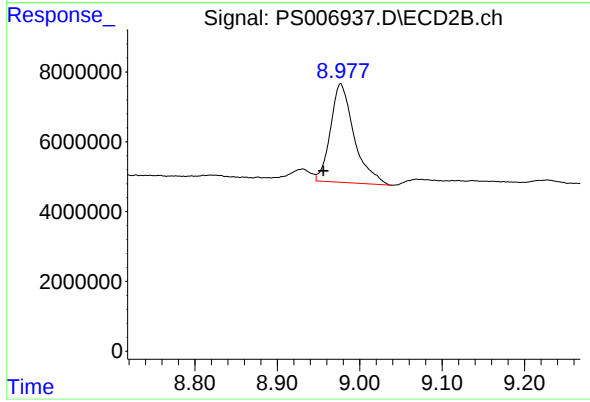

#16 DCPA

R.T.: 8.977 min
Delta R.T.: 0.021 min
Response: 56245107
Conc: 17.70 ng/ml