

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
 Data File : PS006941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 10:32
 Operator : SM\AJ
 Sample : PB123347TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 03:14:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.511	5.239	430.2E6	242.3E6	470.766	526.861
Target Compounds							
1) T	Dalapon	2.056	0.000	6833949	0	6.396	N.D. #
2) T	3,5-DICHL...	0.000	4.567	0	25363754	N.D.	44.122
3) T	4-Nitroph...	5.328	0.000	6967295	0	18.273	N.D. #
5) T	DICAMBA	5.603	0.000	32498773	0	10.058	N.D. #
7) T	MCPA	5.985	5.616	9774651	17968430	3.142	9.762 #
10) T	Pentachlo...	6.772	6.546	31729129	19440700	2.662	3.090
11) T	2,4,5-TP ...	0.000	6.859	0	26094875	N.D.	10.894
15) T	Picloram	0.000	9.035	0	4799898	N.D.	1.319



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
Data File : PS006941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 10:32
Operator : SM\AJ
Sample : PB123347TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 03:14:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

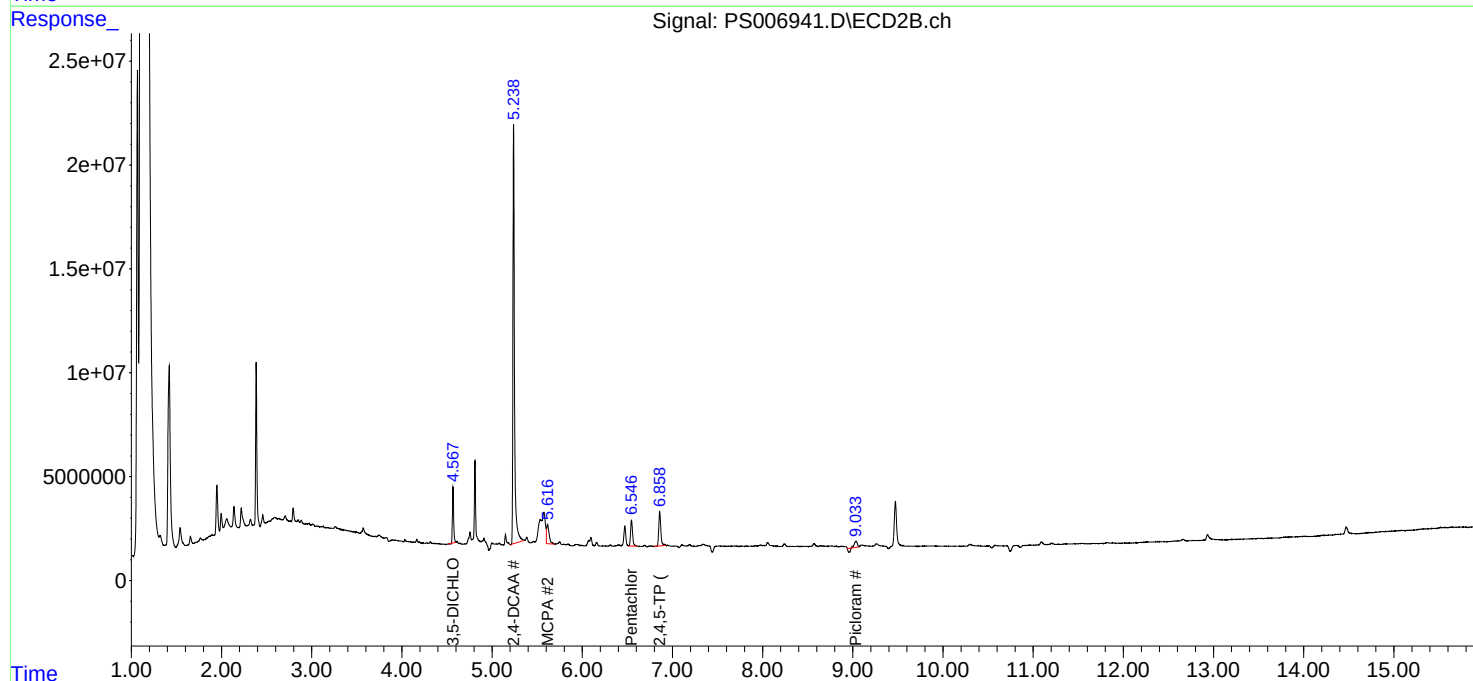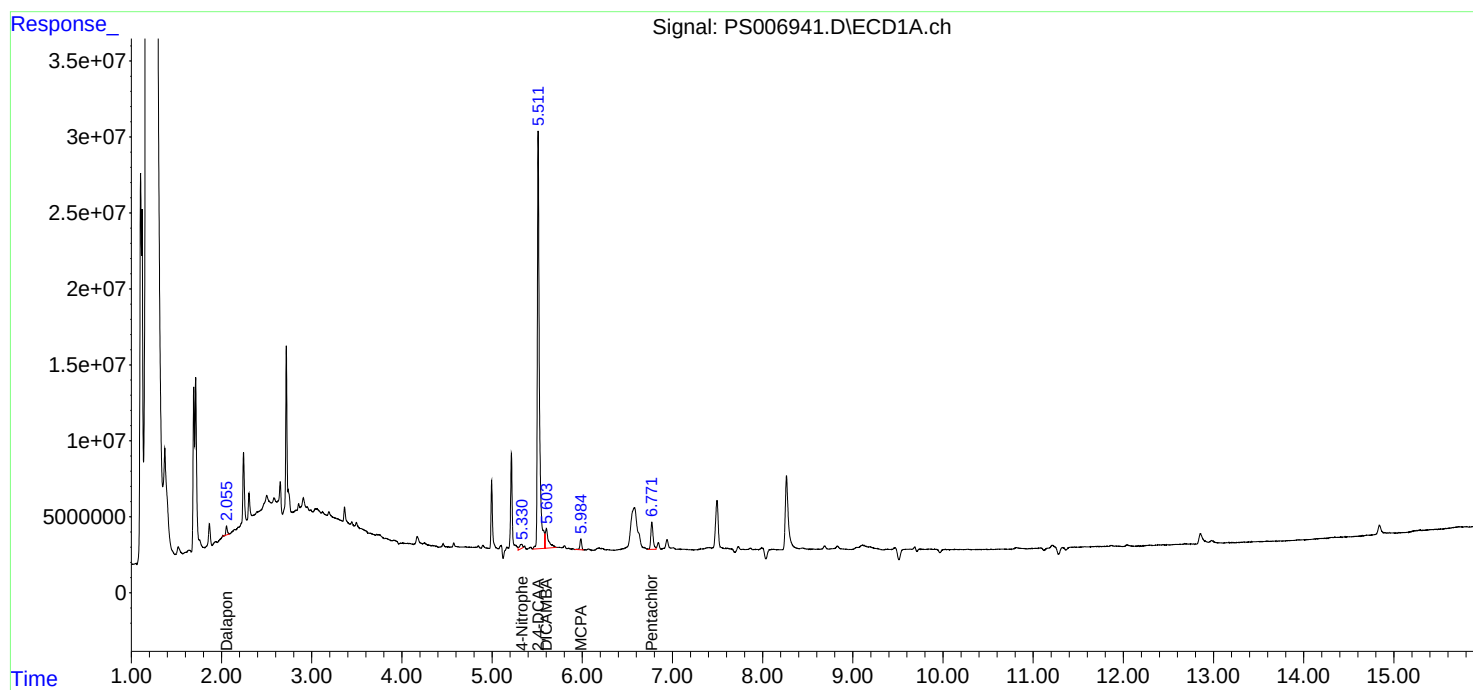


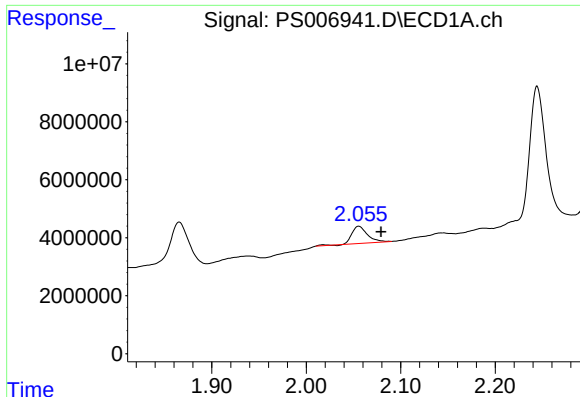

#1 Dalapon


R.T.: 2.056 min
Delta R.T.: -0.023 min
Response: 6833949
Conc: 6.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

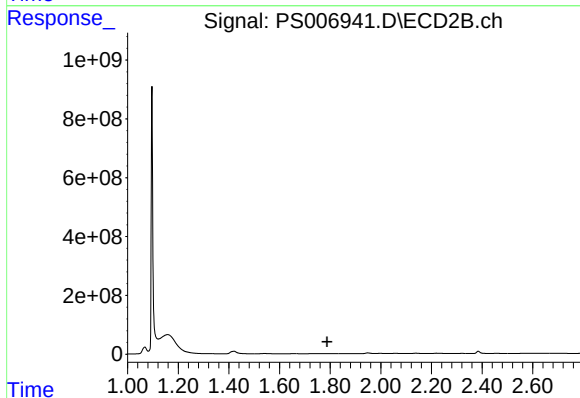


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

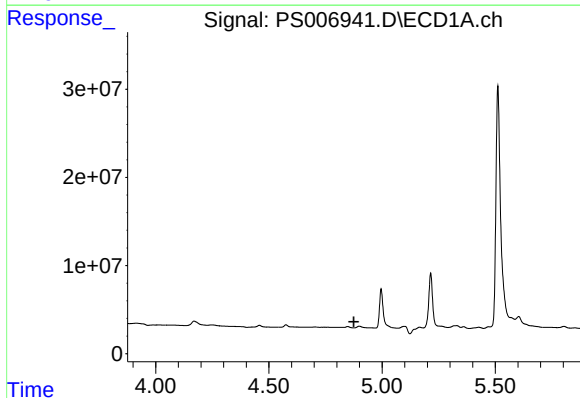


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.876 min
Response: 0
Conc: N.D.

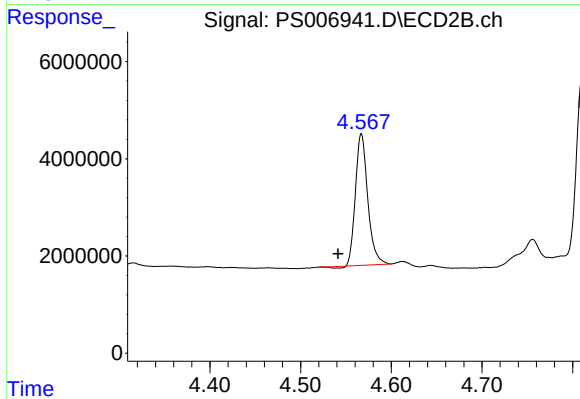

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.567 min
Delta R.T.: 0.026 min
Response: 25363754
Conc: 44.12 ng/ml

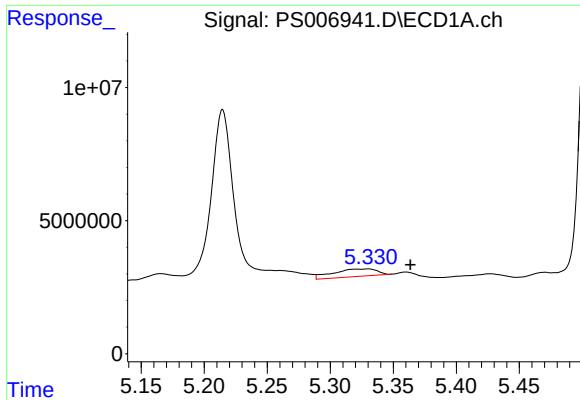

#3 4-Nitrophenol


R.T.: 5.328 min
Delta R.T.: -0.035 min
Response: 6967295
Conc: 18.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

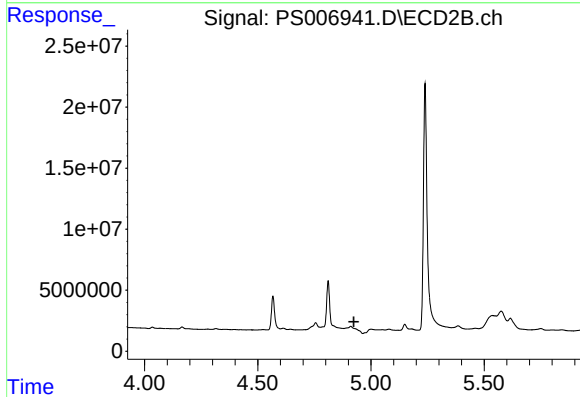


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

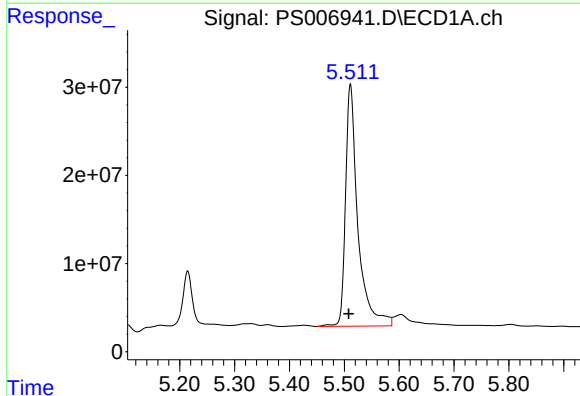


#4 2,4-DCAA

R.T.: 5.511 min
Delta R.T.: 0.003 min
Response: 430192338
Conc: 470.77 ng/ml

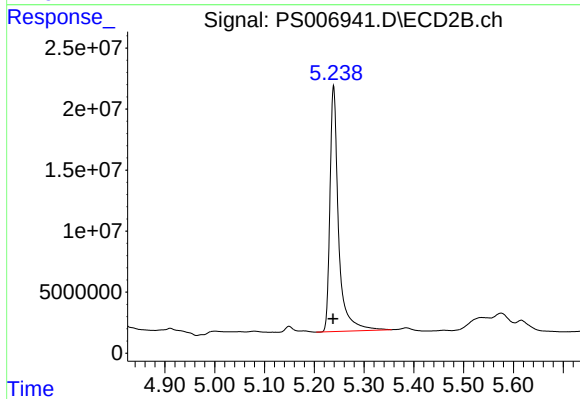

#4 2,4-DCAA


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 242272376
Conc: 526.86 ng/ml

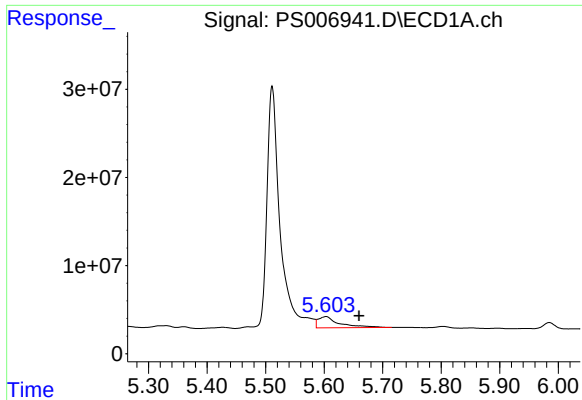

#5 DICAMBA


R.T.: 5.603 min
Delta R.T.: -0.057 min
Response: 32498773
Conc: 10.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

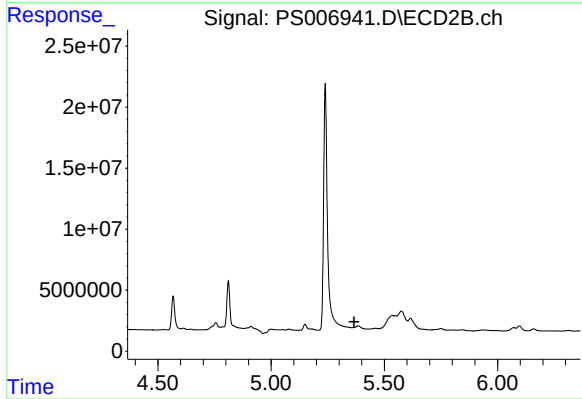


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

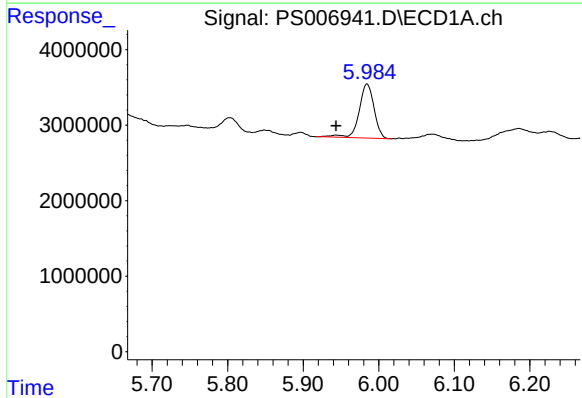


#7 MCPA

R.T.: 5.985 min
Delta R.T.: 0.041 min
Response: 9774651
Conc: 3.14 ug/ml

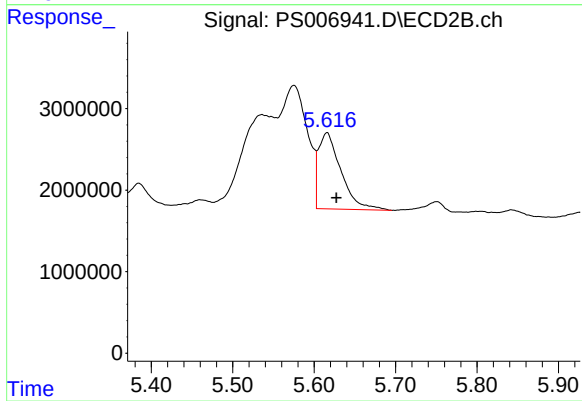

#7 MCPA


R.T.: 5.616 min
Delta R.T.: -0.012 min
Response: 17968430
Conc: 9.76 ug/ml

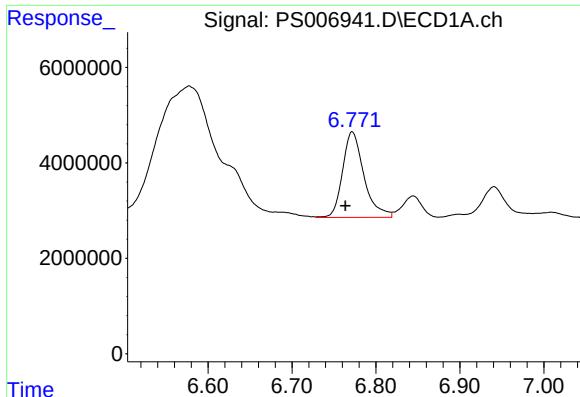

#10 Pentachlorophenol


R.T.: 6.772 min
Delta R.T.: 0.009 min
Response: 31729129
Conc: 2.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

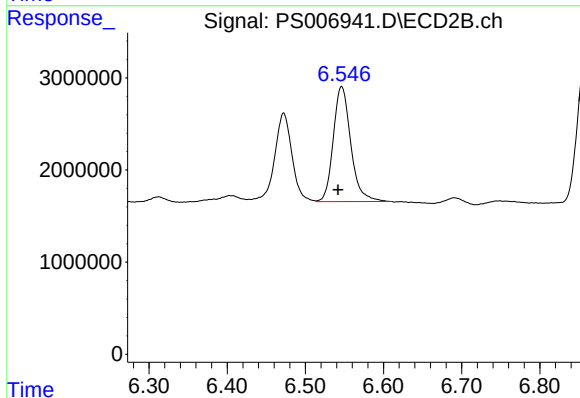


#10 Pentachlorophenol

R.T.: 6.546 min
Delta R.T.: 0.005 min
Response: 19440700
Conc: 3.09 ng/ml

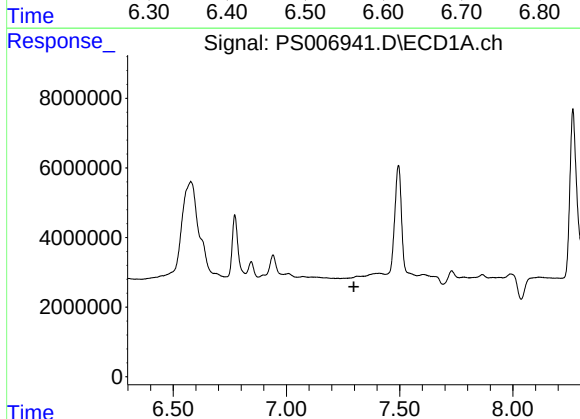


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.298 min
Response: 0
Conc: N.D.

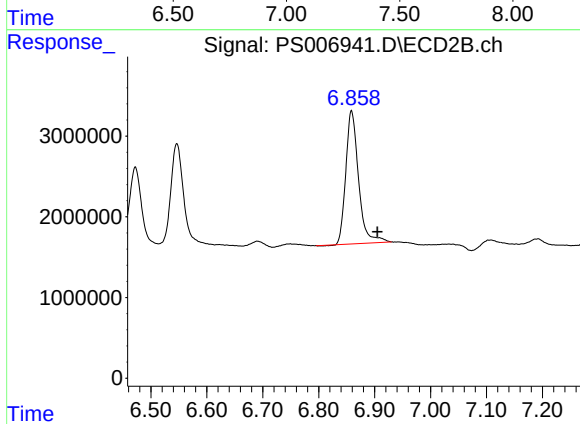

#11 2,4,5-TP (SILVEX)


R.T.: 6.859 min
Delta R.T.: -0.046 min
Response: 26094875
Conc: 10.89 ng/ml

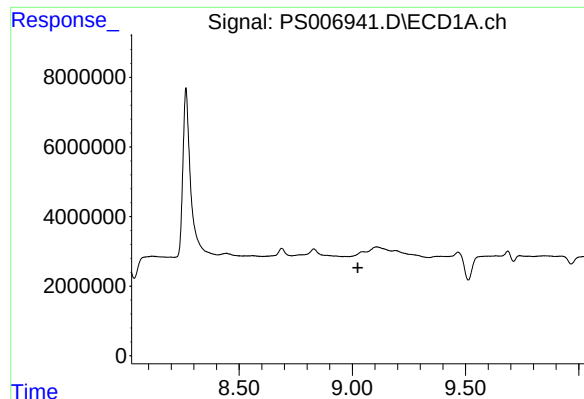

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.025 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

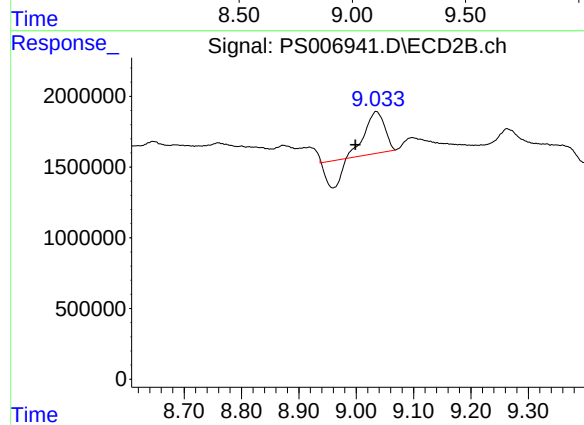

#15 Picloram

R.T.: 9.035 min
Delta R.T.: 0.036 min
Response: 4799898
Conc: 1.32 ng/ml