

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
 Data File : PS006953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 15:03
 Operator : SM\AJ
 Sample : PB123465BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 03:18:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.477	5.208	458.9E6	247.6E6	502.182	538.401
Target Compounds							
1) T	Dalapon	2.025	0.000	7295969	0	6.829	N.D. #
2) T	3,5-DICHL...	0.000	4.537	0	29140714	N.D.	50.692
3) T	4-Nitroph...	5.330	0.000	10893512	0	28.570	N.D. #
7) T	MCPA	5.953	5.585	8875425	19000085	2.853	10.323 #
9) T	2,4-D	6.542	0.000	129.3E6	0	157.836	N.D. #
10) T	Pentachlo...	6.735	6.514	39901016	20073659	3.348	3.191
15) T	Picloram	9.017	8.983	16608313	4707694	2.477	1.293 #
16) T	DCPA	0.000	8.983	0	4707694	N.D.	1.482



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
Data File : PS006953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 15:03
Operator : SM\AJ
Sample : PB123465BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 03:18:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

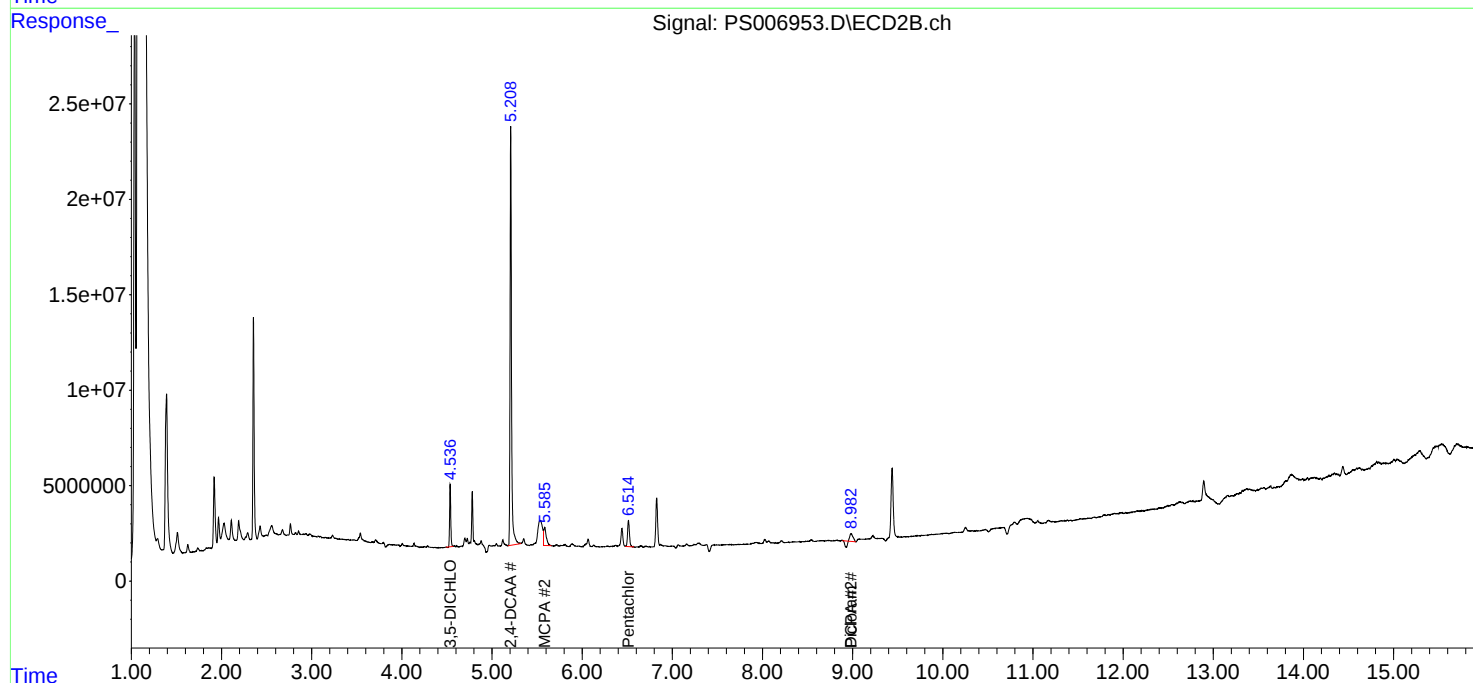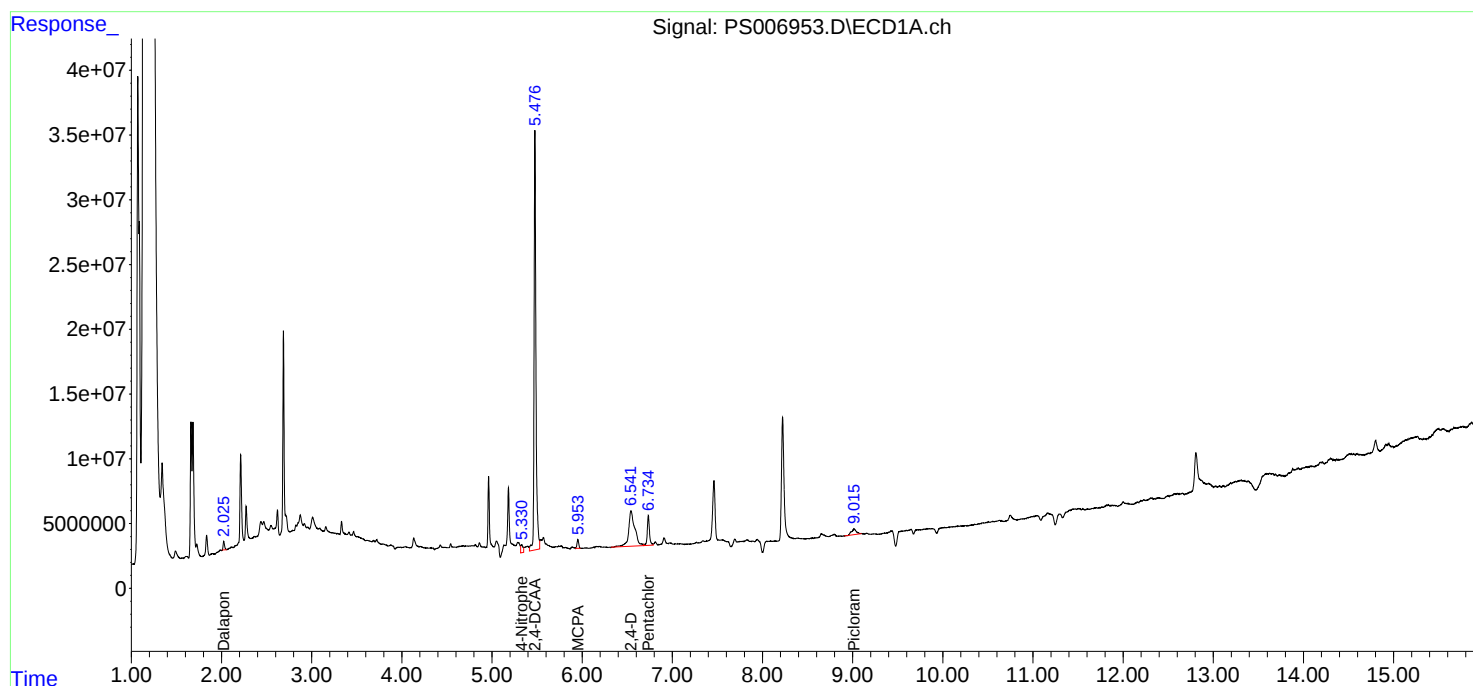


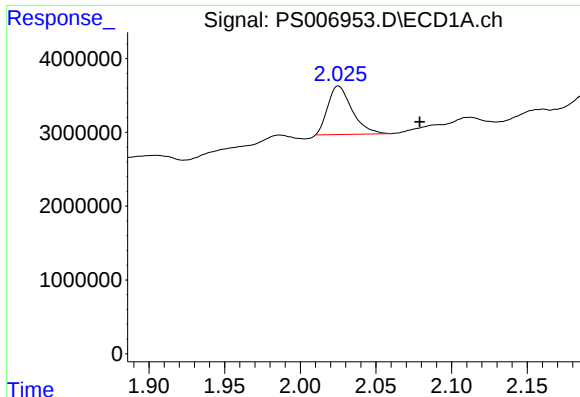

#1 Dalapon


R.T.: 2.025 min
Delta R.T.: -0.054 min
Response: 7295969
Conc: 6.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

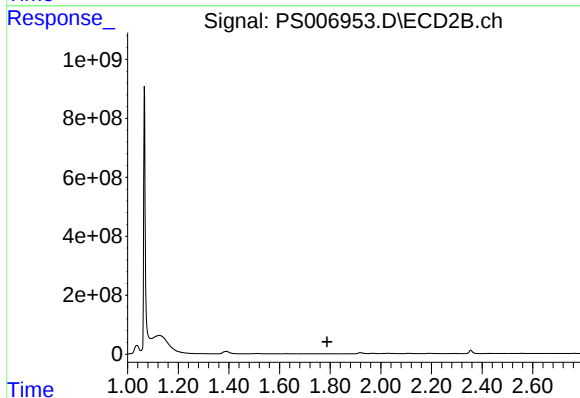


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

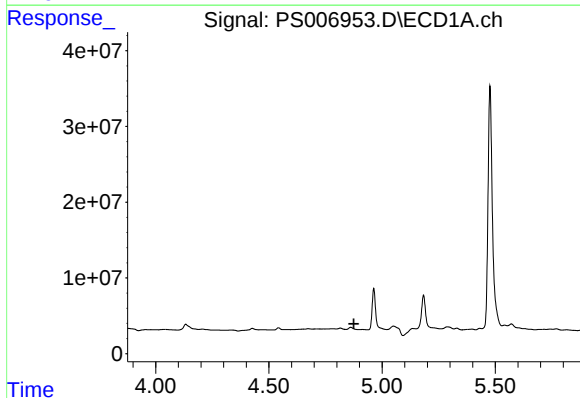


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.876 min
Response: 0
Conc: N.D.

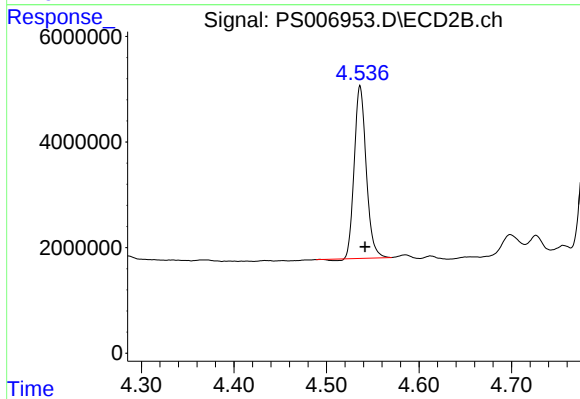

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.537 min
Delta R.T.: -0.005 min
Response: 29140714
Conc: 50.69 ng/ml

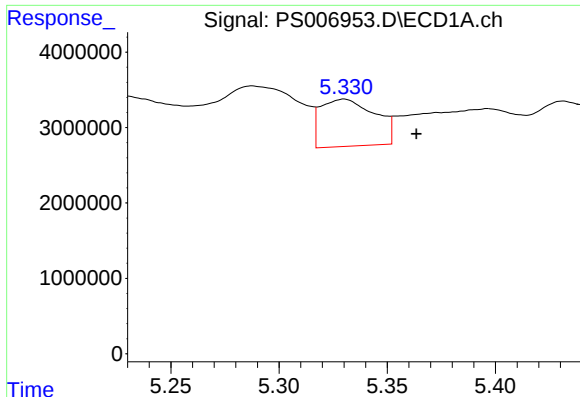

#3 4-Nitrophenol


R.T.: 5.330 min
Delta R.T.: -0.034 min
Response: 10893512
Conc: 28.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

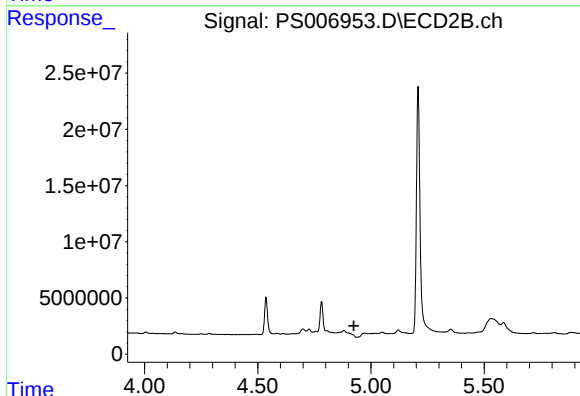


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

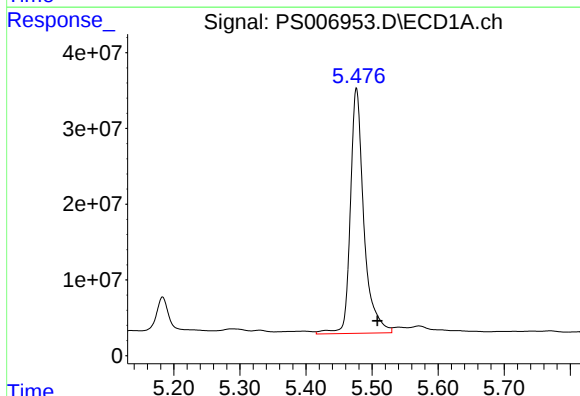


#4 2,4-DCAA

R.T.: 5.477 min
Delta R.T.: -0.031 min
Response: 458901173
Conc: 502.18 ng/ml

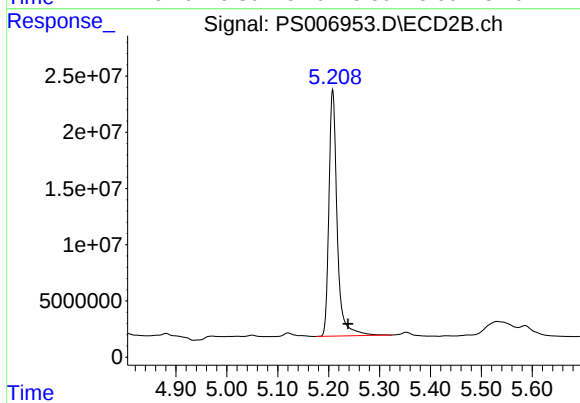

#4 2,4-DCAA


R.T.: 5.208 min
Delta R.T.: -0.030 min
Response: 247579150
Conc: 538.40 ng/ml

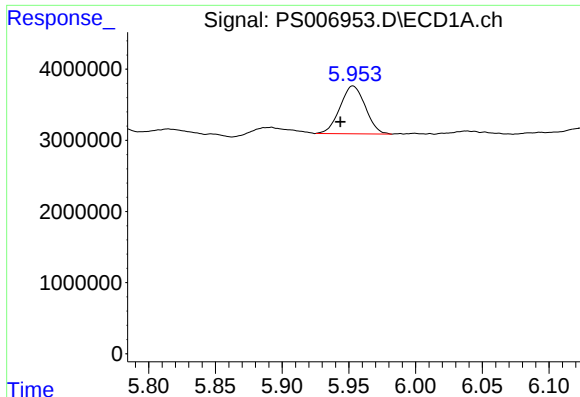

#7 MCPA


R.T.: 5.953 min
Delta R.T.: 0.010 min
Response: 8875425
Conc: 2.85 ug/ml

Instrument :
ECD_S
ClientSampleId :

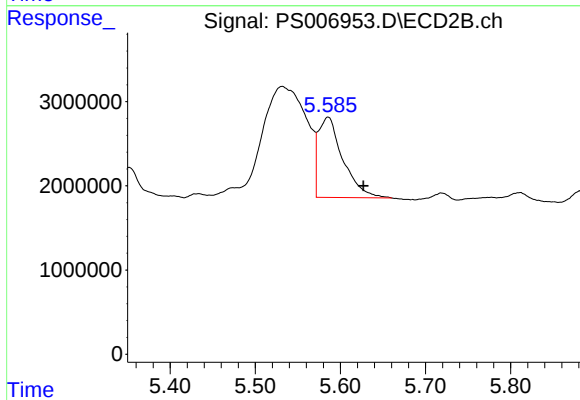


#7 MCPA

R.T.: 5.585 min
Delta R.T.: -0.042 min
Response: 19000085
Conc: 10.32 ug/ml

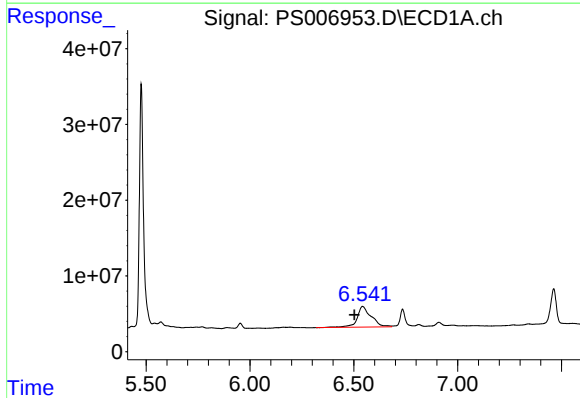


#9 2,4-D

R.T.: 6.542 min
Delta R.T.: 0.038 min
Response: 129348811
Conc: 157.84 ng/ml

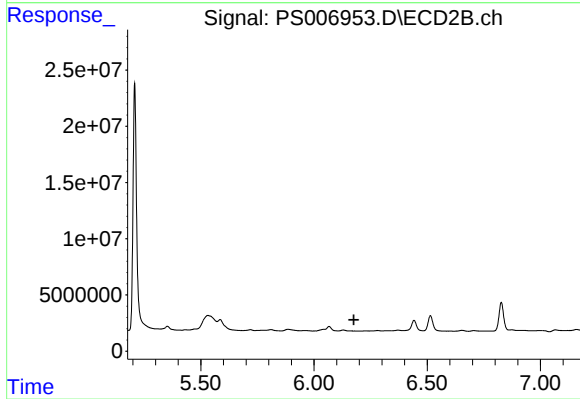

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

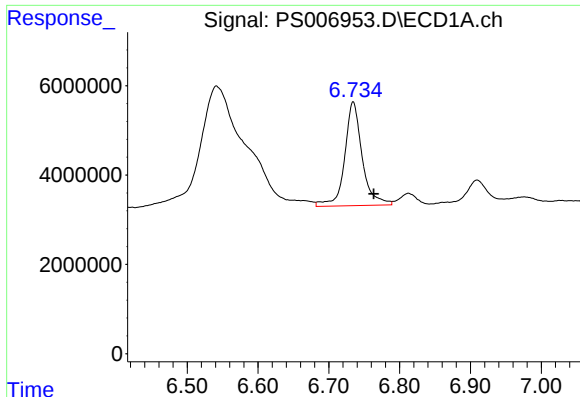

#10 Pentachlorophenol


R.T.: 6.735 min
Delta R.T.: -0.029 min
Response: 39901016
Conc: 3.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

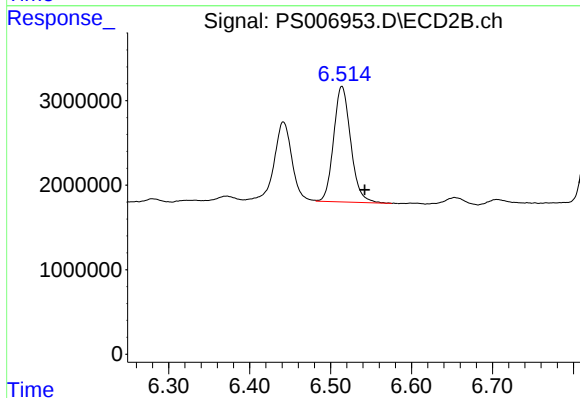


#10 Pentachlorophenol

R.T.: 6.514 min
Delta R.T.: -0.028 min
Response: 20073659
Conc: 3.19 ng/ml

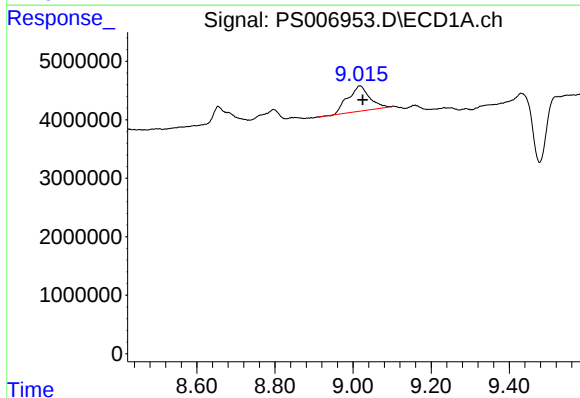


#15 Picloram

R.T.: 9.017 min
Delta R.T.: -0.007 min
Response: 16608313
Conc: 2.48 ng/ml

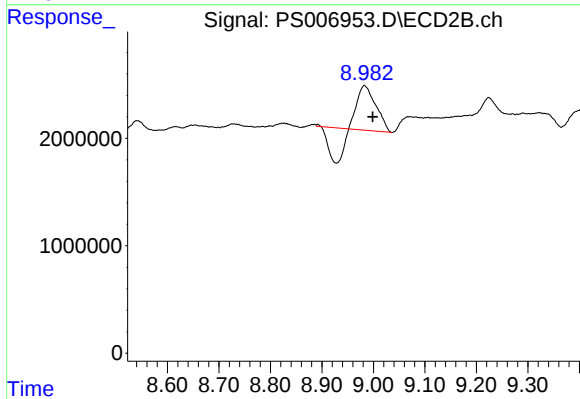

#15 Picloram


R.T.: 8.983 min
Delta R.T.: -0.016 min
Response: 4707694
Conc: 1.29 ng/ml

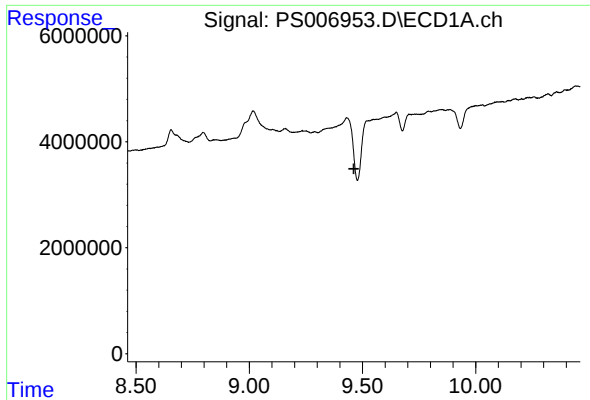

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.462 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

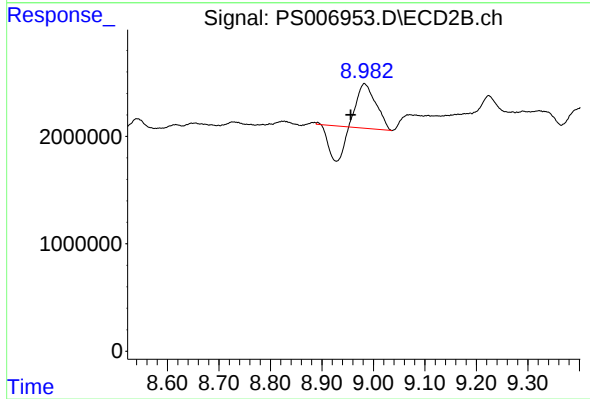

#16 DCPA

R.T.: 8.983 min
Delta R.T.: 0.027 min
Response: 4707694
Conc: 1.48 ng/ml