

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
 Data File : PS006955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 15:52
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 03:46:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.488	5.216	395.6E6	208.4E6	432.940	453.168
Target Compounds							
6) T	MCP	0.000	5.488	0 30177665		N.D.	25.981
9) T	2,4-D	6.553	0.000	204.0E6	0	248.938	N.D. #
10) T	Pentachlo...	6.747	0.000	9343057	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	7.298	0 19612380		N.D.	9.074
15) T	Picloram	9.034	8.990	174.3E6	82068325	25.992	22.548
16) T	DCPA	0.000	8.990	0 82068325		N.D.	25.828



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
Data File : PS006955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 15:52
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 03:46:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

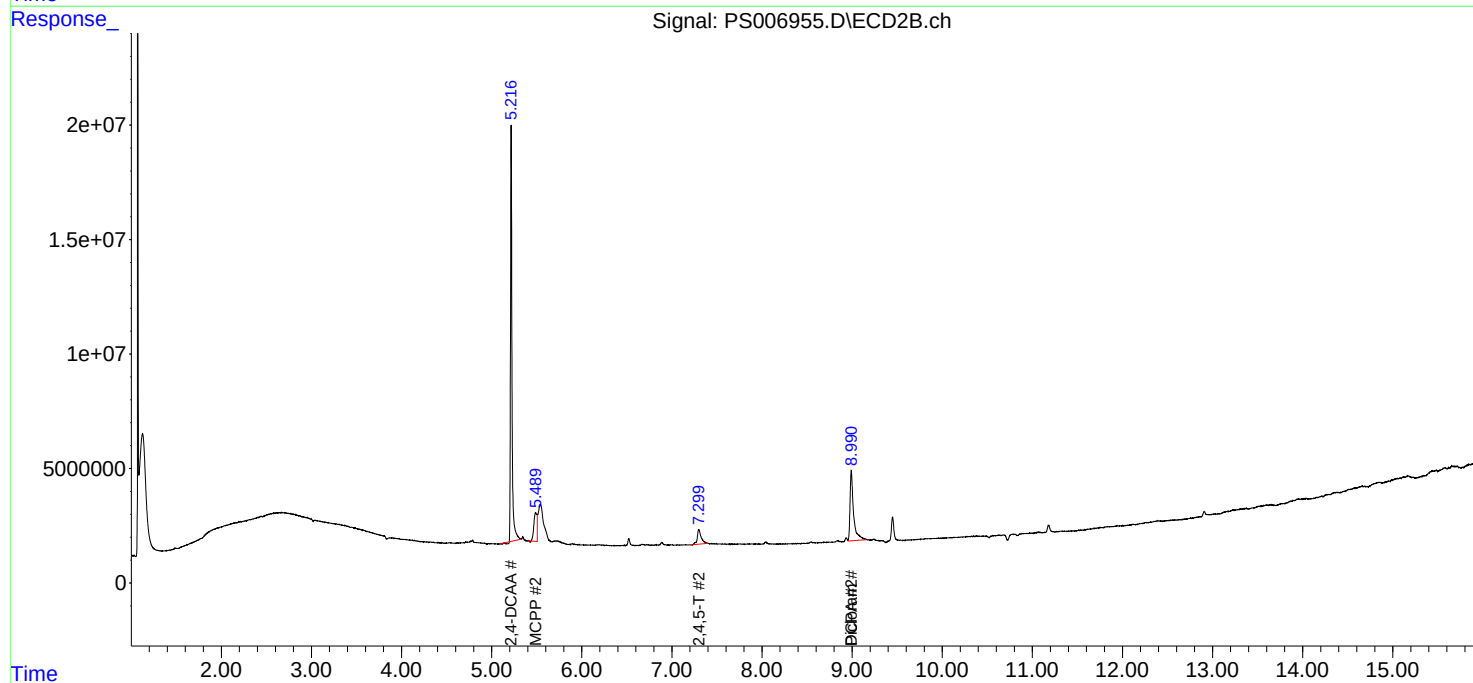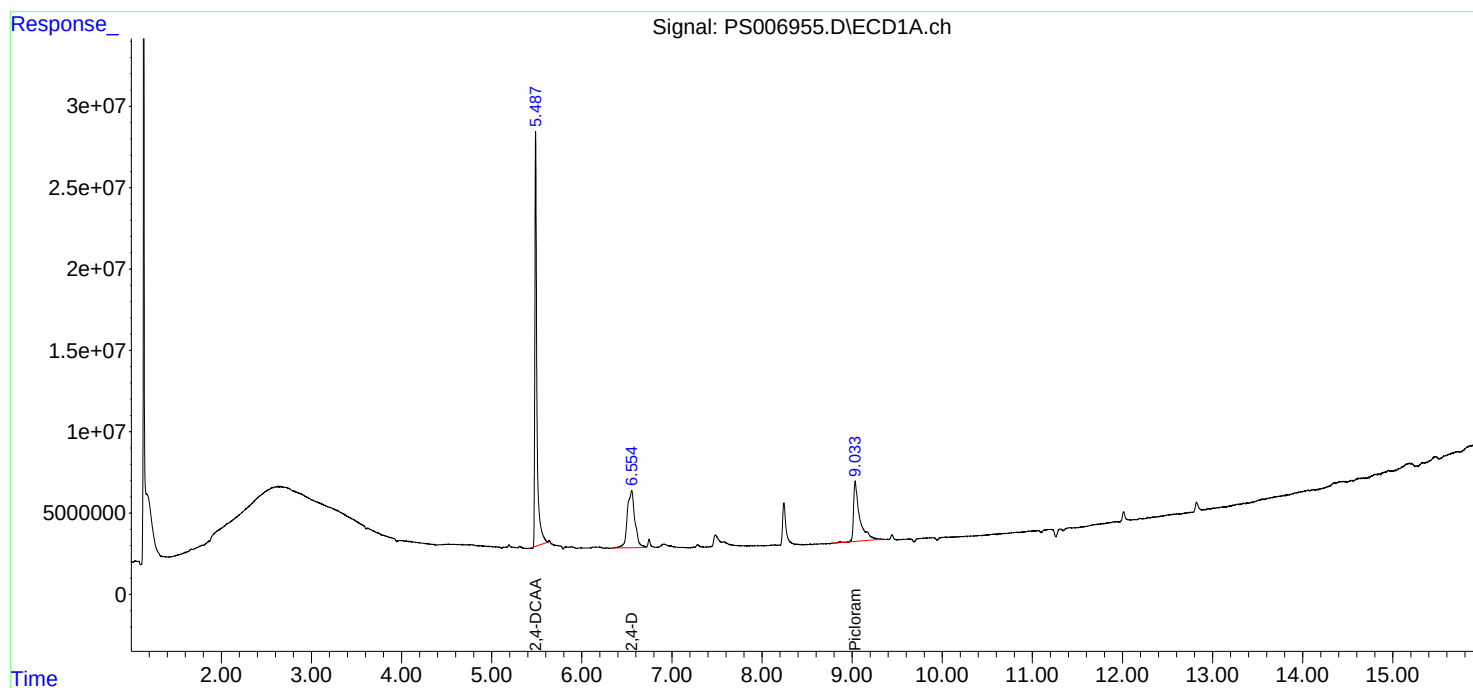


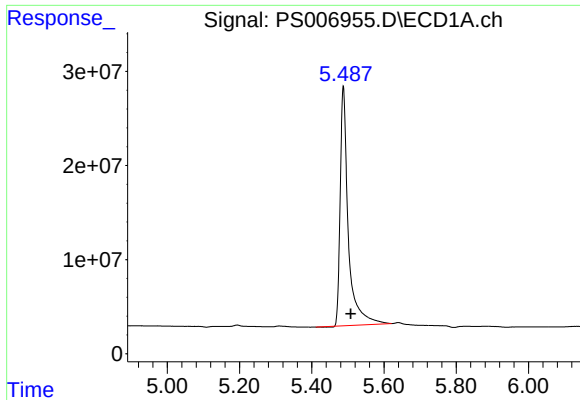

#4 2,4-DCAA


R.T.: 5.488 min
Delta R.T.: -0.020 min
Response: 395626993
Conc: 432.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

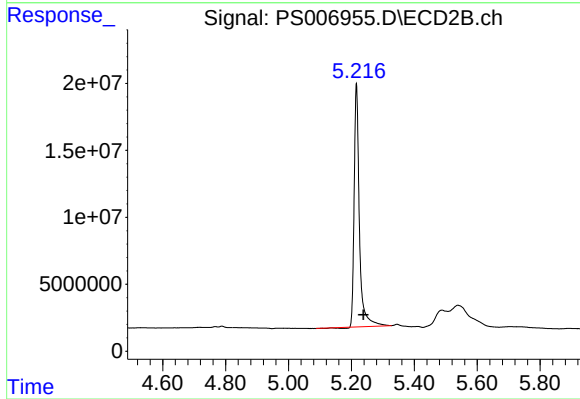


#4 2,4-DCAA

R.T.: 5.216 min
Delta R.T.: -0.022 min
Response: 208385598
Conc: 453.17 ng/ml

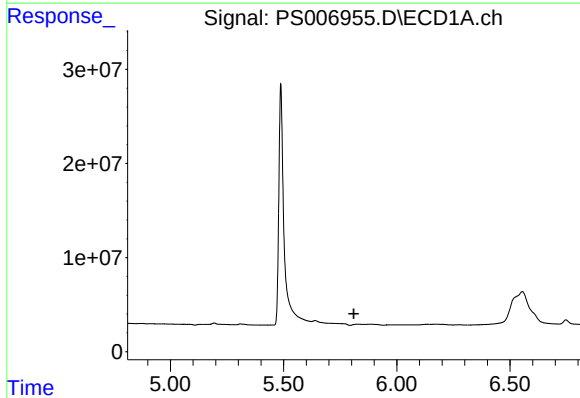


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.811 min
Response: 0
Conc: N.D.

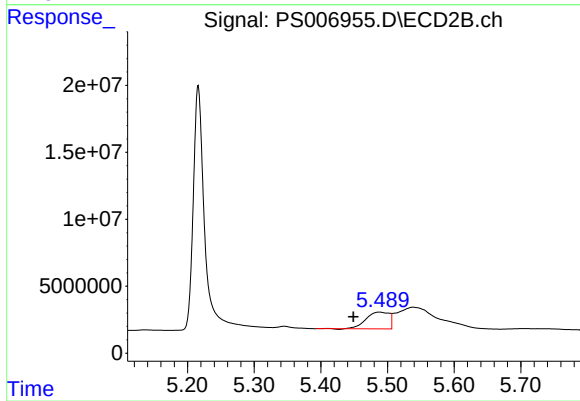

#6 MCP


R.T.: 5.488 min
Delta R.T.: 0.039 min
Response: 30177665
Conc: 25.98 ug/ml

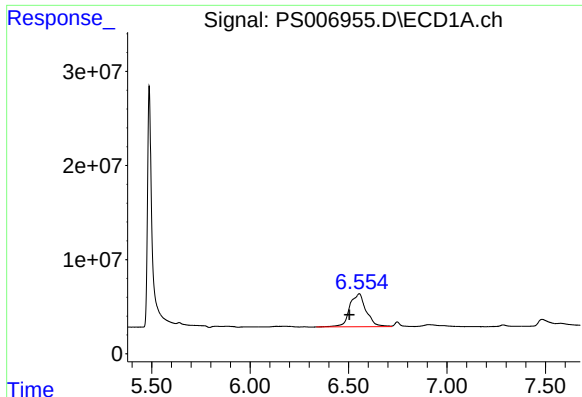

#9 2,4-D


R.T.: 6.553 min
Delta R.T.: 0.050 min
Response: 204008496
Conc: 248.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

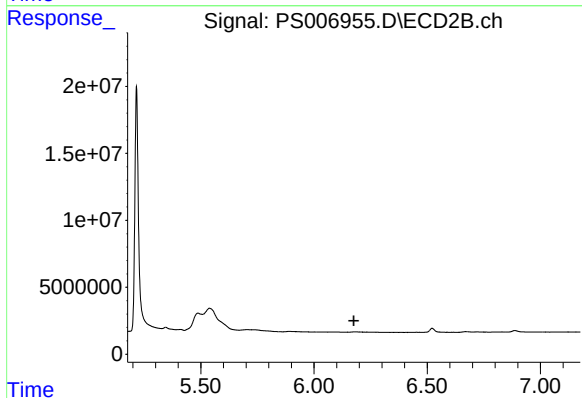


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

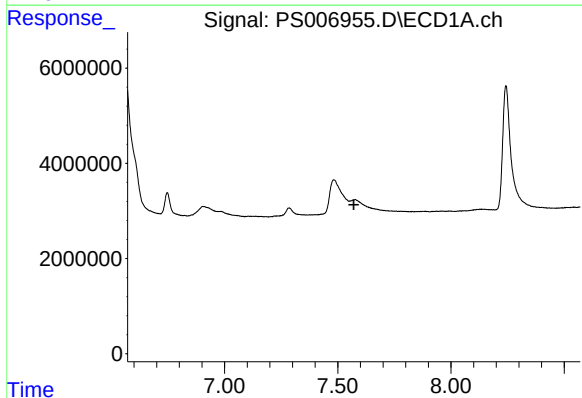


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.572 min
Response: 0
Conc: N.D.

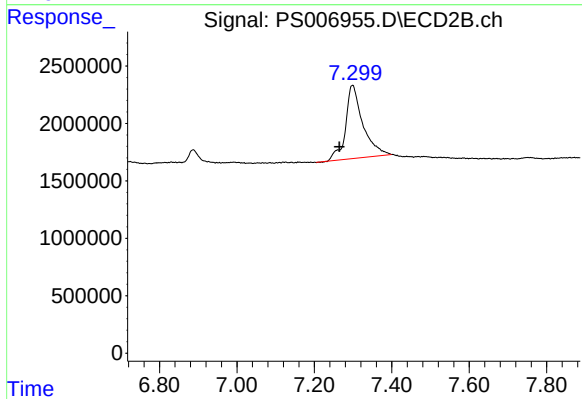

#12 2,4,5-T


R.T.: 7.298 min
Delta R.T.: 0.034 min
Response: 19612380
Conc: 9.07 ng/ml

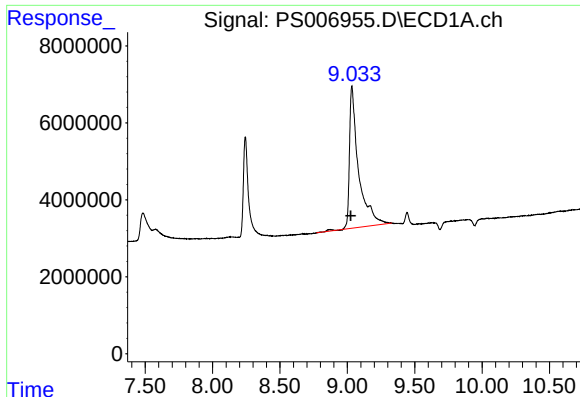

#15 Picloram


R.T.: 9.034 min
Delta R.T.: 0.009 min
Response: 174296598
Conc: 25.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

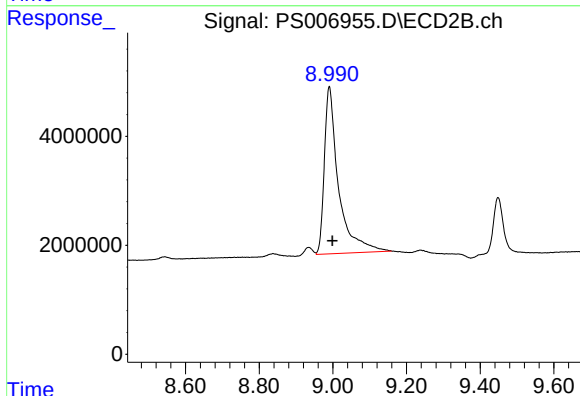


#15 Picloram

R.T.: 8.990 min
Delta R.T.: -0.008 min
Response: 82068325
Conc: 22.55 ng/ml

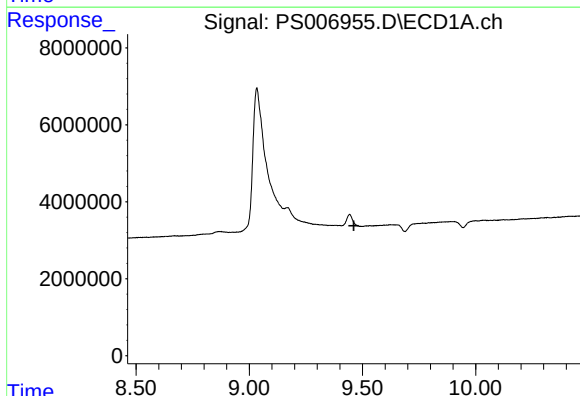

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.462 min
Response: 0
Conc: N.D.

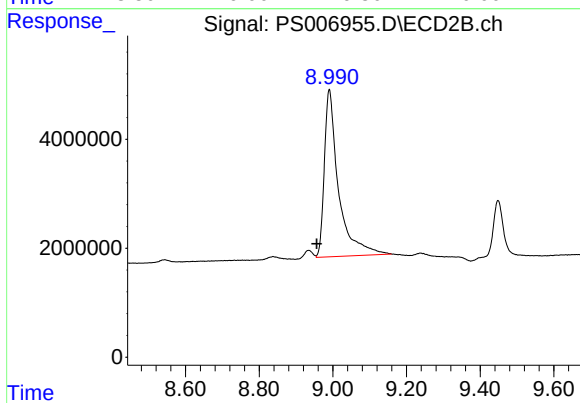

#16 DCPA

R.T.: 8.990 min
Delta R.T.: 0.035 min
Response: 82068325
Conc: 25.83 ng/ml