

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
 Data File : PS006957.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 16:40
 Operator : SM\AJ
 Sample : PB123482BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 03:47:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.512	5.241	474.1E6	250.1E6	518.783	543.903
Target Compounds							
1) T	Dalapon	2.059	0.000	7046881	0	6.596	N.D. #
2) T	3,5-DICHL...	0.000	4.569	0	29515743	N.D.	51.344
3) T	4-Nitroph...	5.364	0.000	11136623	0	29.207	N.D. #
5) T	DICAMBA	5.665	0.000	9089306	0	2.813	N.D. #
7) T	MCPA	5.988	5.617	9418150	16709632	3.027	9.078 #
10) T	Pentachlo...	6.770	6.547	52612152	28301920	4.414	4.498
11) T	2,4,5-TP ...	0.000	6.860	0	29920268	N.D.	12.491
12) T	2,4,5-T	0.000	7.318	0	45129100	N.D.	20.879
14) T	DINOSEB	9.193	0.000	14451726	0	3.805	N.D. #
15) T	Picloram	9.051	9.013	206.3E6	105.8E6	30.766	29.072
16) T	DCPA	9.466	9.013	49926341	105.8E6	8.556	33.300 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
Data File : PS006957.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 16:40
Operator : SM\AJ
Sample : PB123482BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 03:47:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

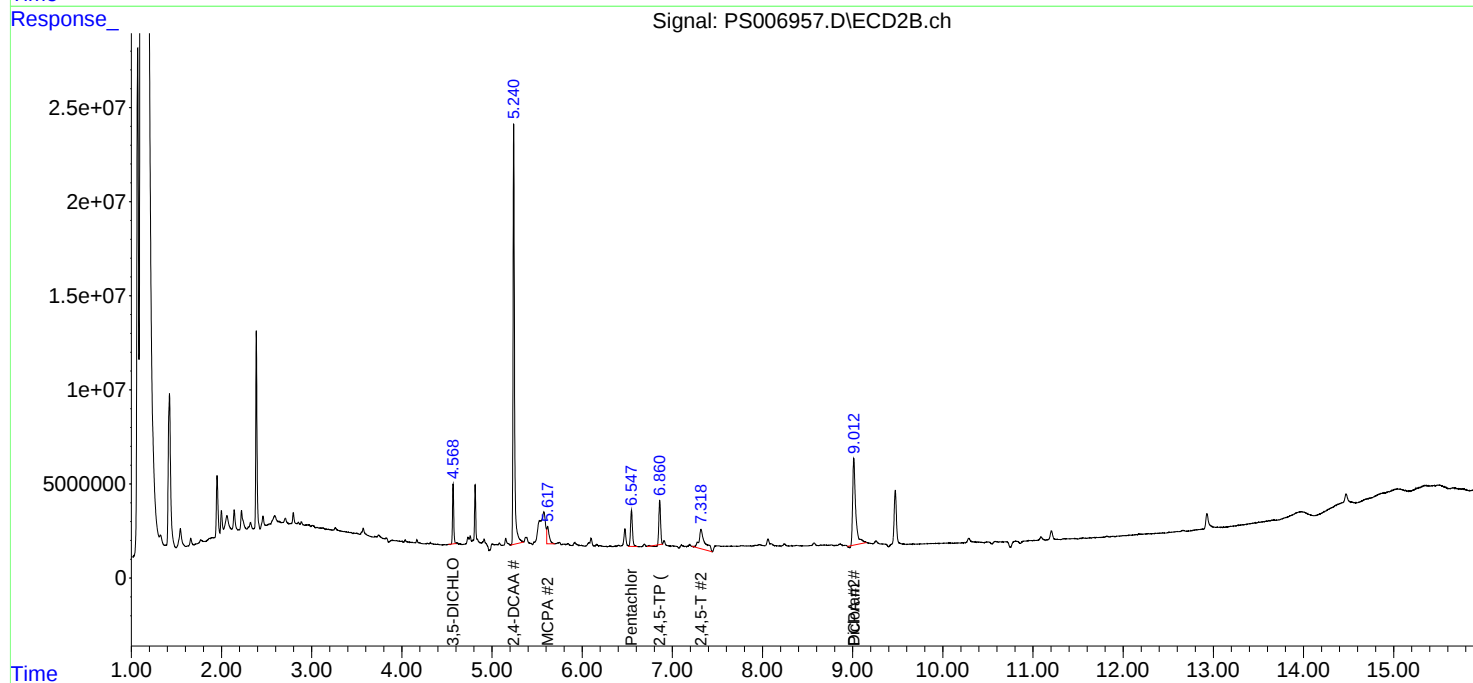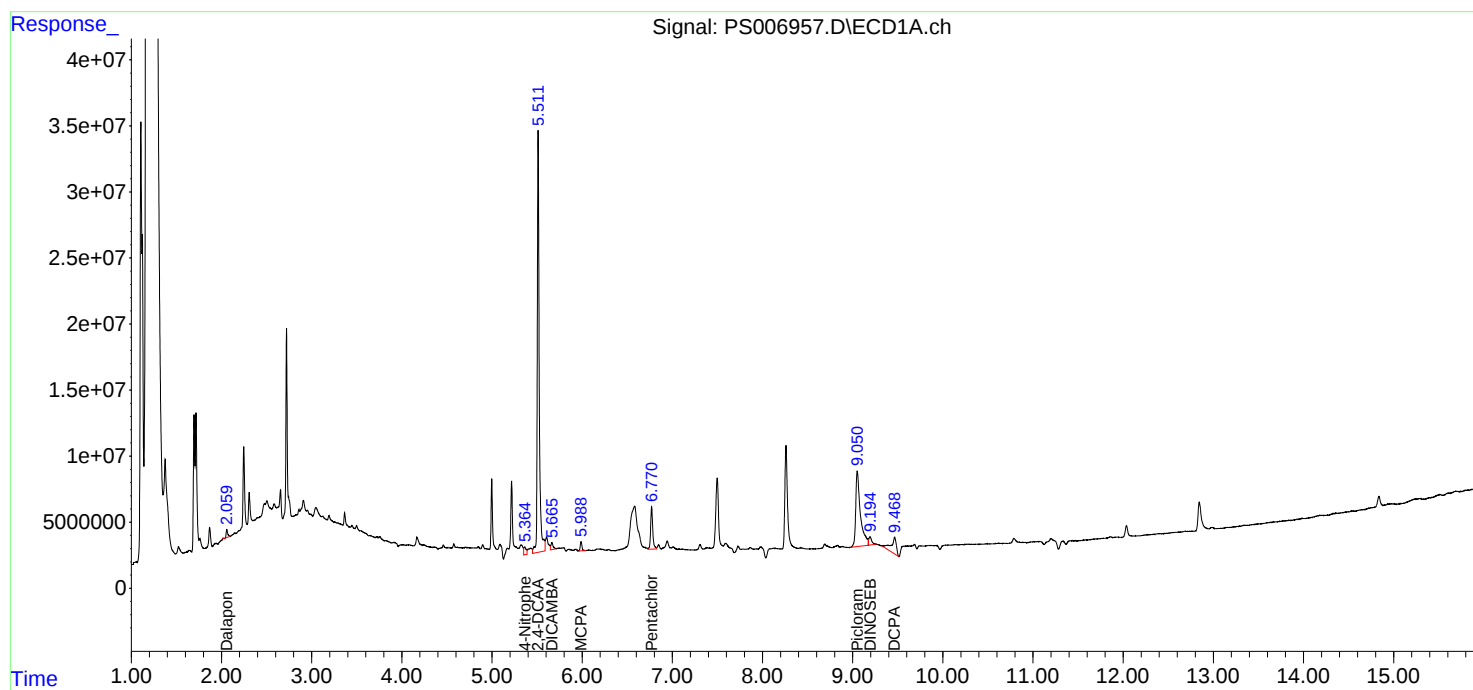


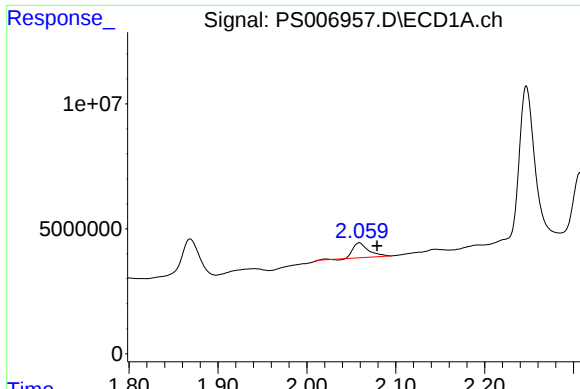

#1 Dalapon


R.T.: 2.059 min
Delta R.T.: -0.020 min
Response: 7046881
Conc: 6.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

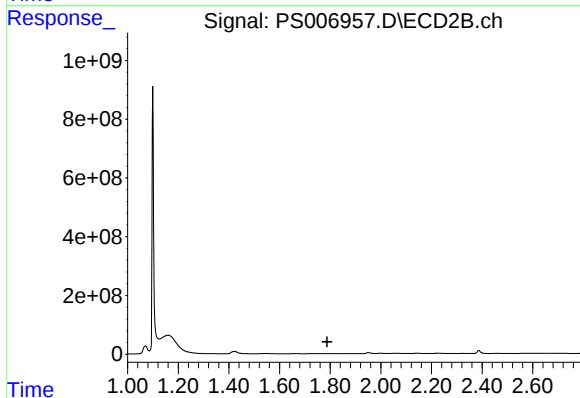


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

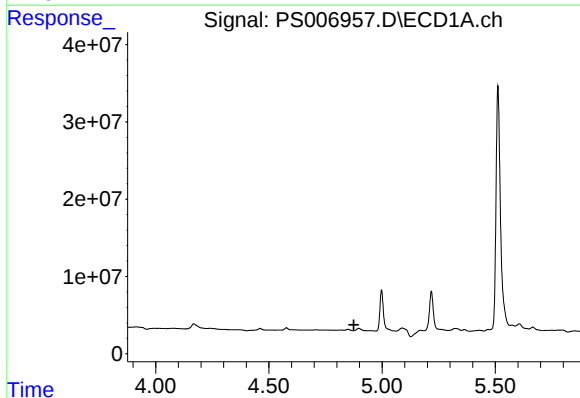


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.876 min
Response: 0
Conc: N.D.

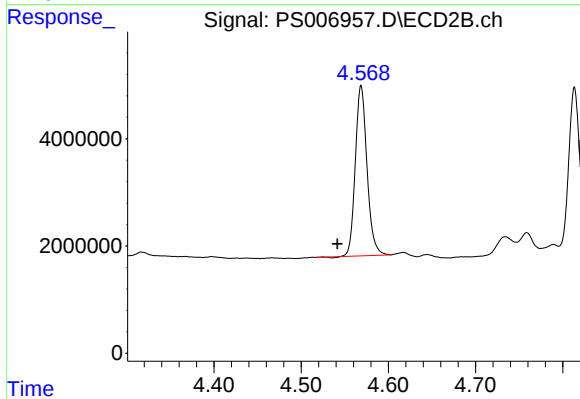

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.569 min
Delta R.T.: 0.027 min
Response: 29515743
Conc: 51.34 ng/ml

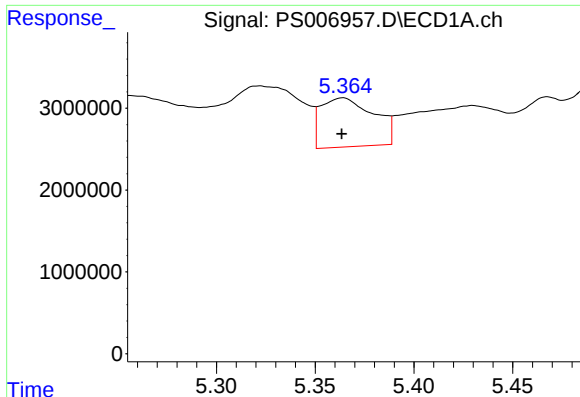

#3 4-Nitrophenol


R.T.: 5.364 min
Delta R.T.: 0.000 min
Response: 11136623
Conc: 29.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

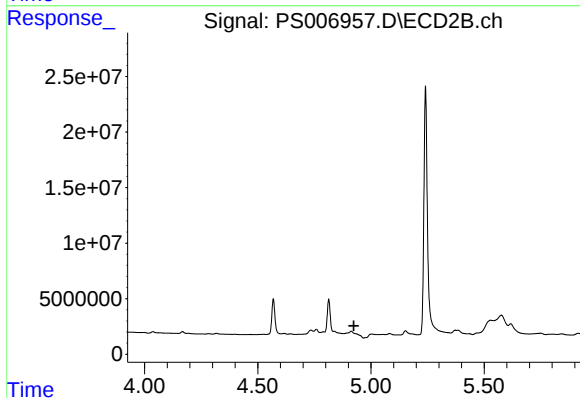


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

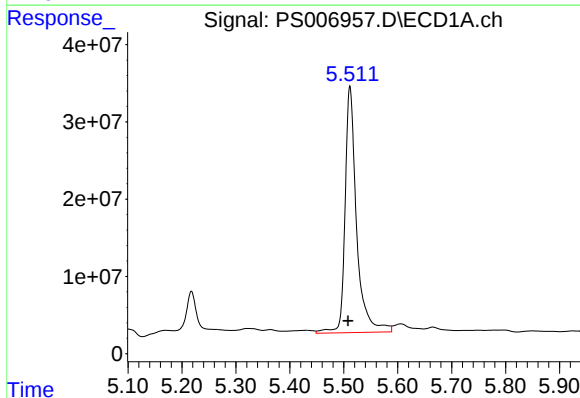


#4 2,4-DCAA

R.T.: 5.512 min
Delta R.T.: 0.004 min
Response: 474071358
Conc: 518.78 ng/ml

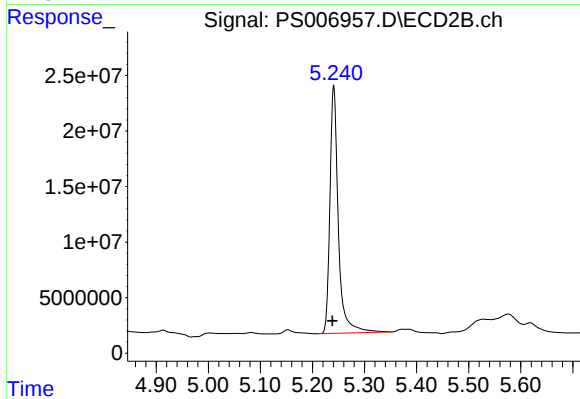

#4 2,4-DCAA


R.T.: 5.241 min
Delta R.T.: 0.003 min
Response: 250109257
Conc: 543.90 ng/ml

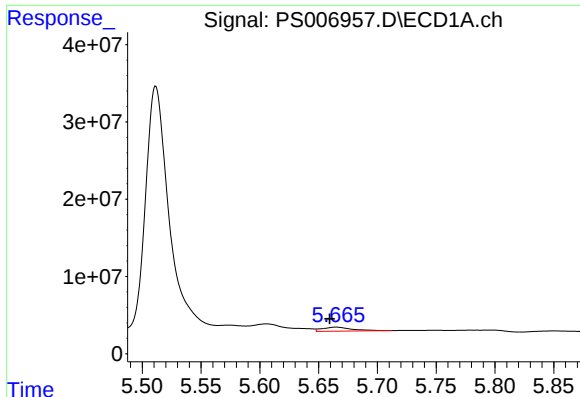

#5 DICAMBA


R.T.: 5.665 min
Delta R.T.: 0.005 min
Response: 9089306
Conc: 2.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

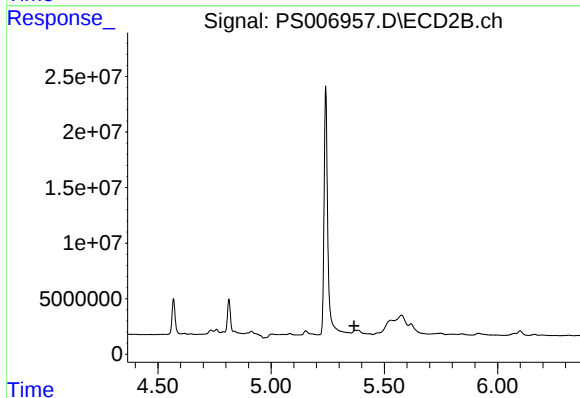


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

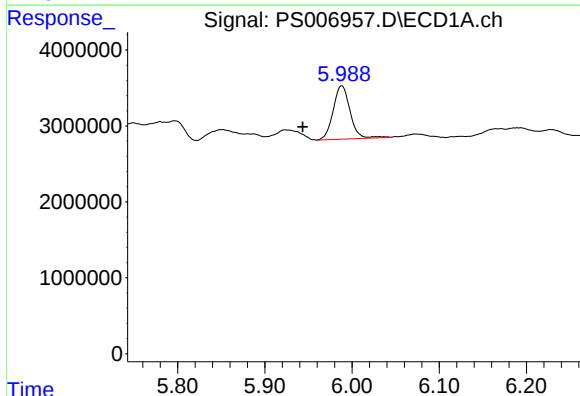


#7 MCPA

R.T.: 5.988 min
Delta R.T.: 0.045 min
Response: 9418150
Conc: 3.03 ug/ml

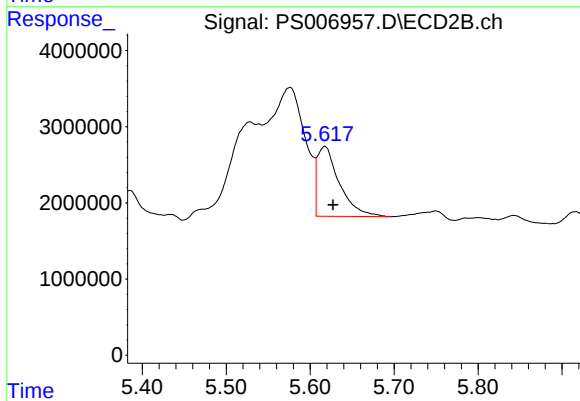

#7 MCPA


R.T.: 5.617 min
Delta R.T.: -0.010 min
Response: 16709632
Conc: 9.08 ug/ml

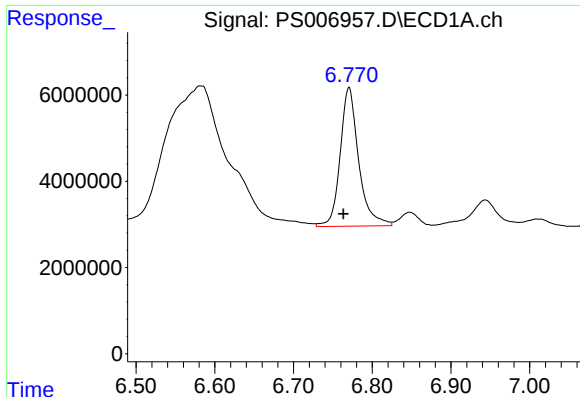

#10 Pentachlorophenol


R.T.: 6.770 min
Delta R.T.: 0.007 min
Response: 52612152
Conc: 4.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

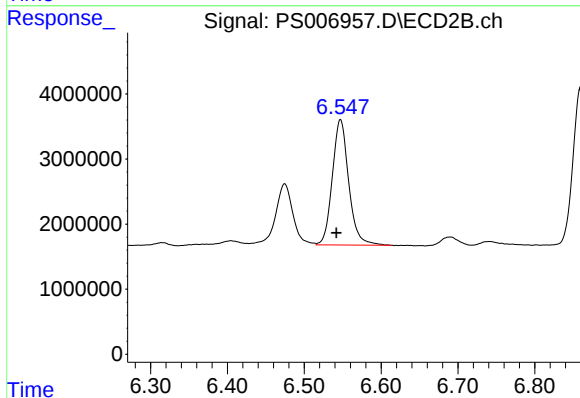


#10 Pentachlorophenol

R.T.: 6.547 min
Delta R.T.: 0.005 min
Response: 28301920
Conc: 4.50 ng/ml

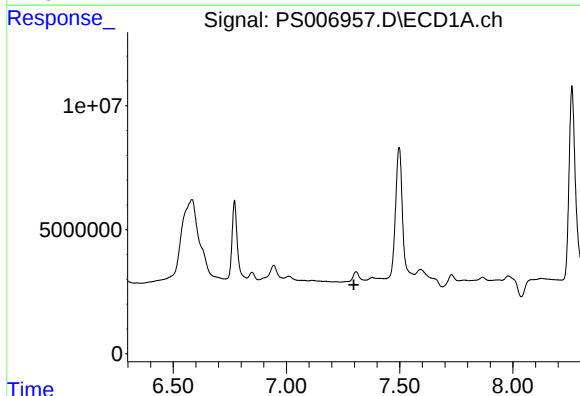


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.298 min
Response: 0
Conc: N.D.

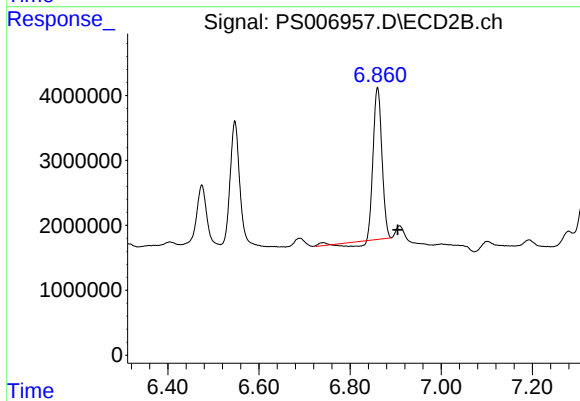

#11 2,4,5-TP (SILVEX)


R.T.: 6.860 min
Delta R.T.: -0.044 min
Response: 29920268
Conc: 12.49 ng/ml

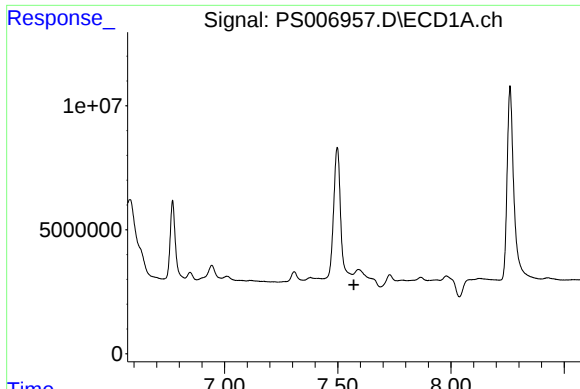

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

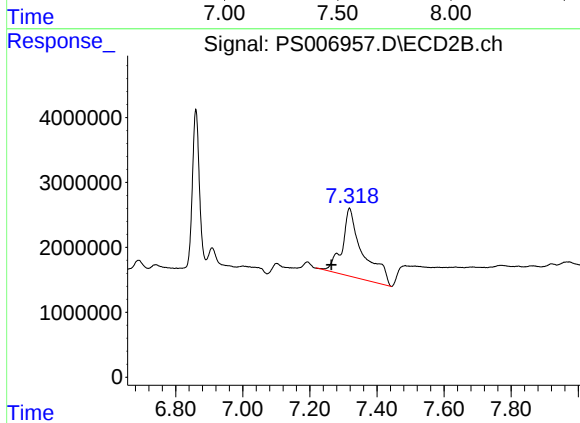


#12 2,4,5-T

R.T.: 7.318 min
Delta R.T.: 0.054 min
Response: 45129100
Conc: 20.88 ng/ml

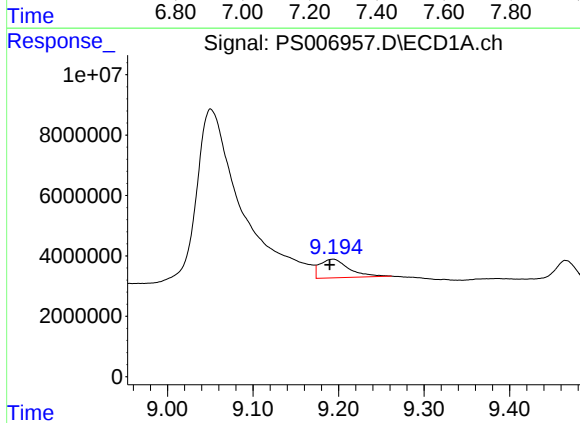


#14 DINOSEB

R.T.: 9.193 min
Delta R.T.: 0.003 min
Response: 14451726
Conc: 3.81 ng/ml

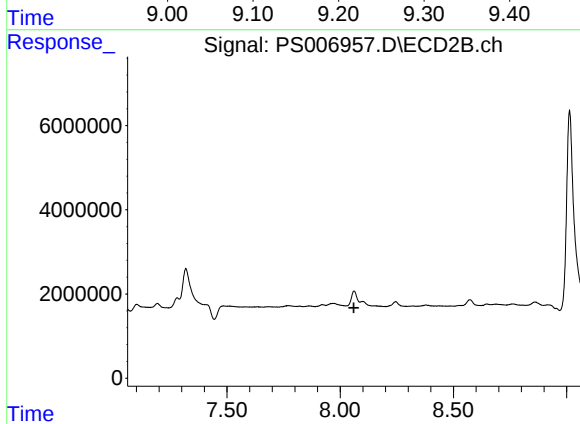

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 8.060 min
Response: 0
Conc: N.D.

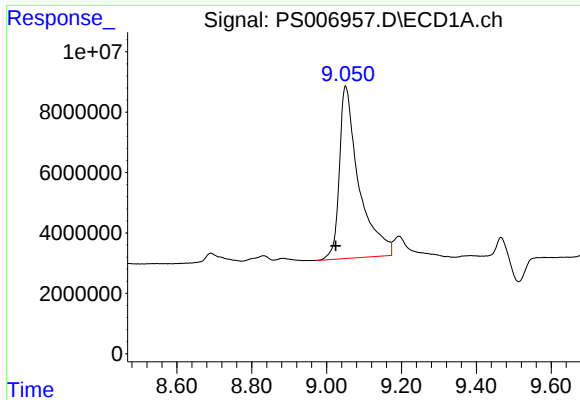

#15 Picloram


R.T.: 9.051 min
Delta R.T.: 0.026 min
Response: 206307346
Conc: 30.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

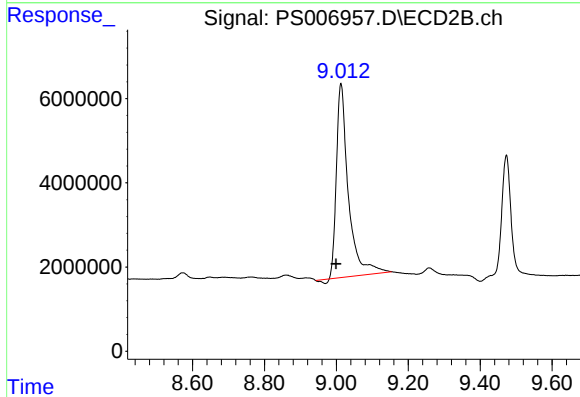


#15 Picloram

R.T.: 9.013 min
Delta R.T.: 0.014 min
Response: 105810959
Conc: 29.07 ng/ml

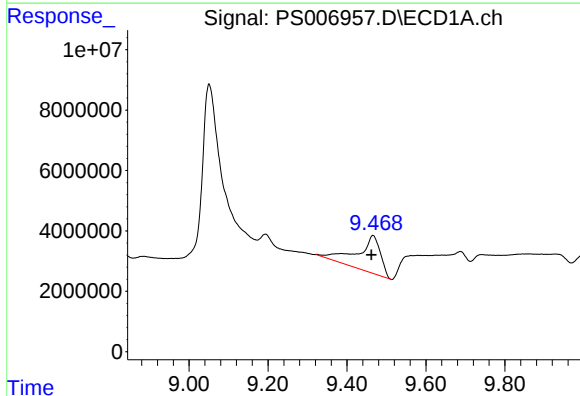

#16 DCPA

R.T.: 9.466 min
Delta R.T.: 0.004 min
Response: 49926341
Conc: 8.56 ng/ml

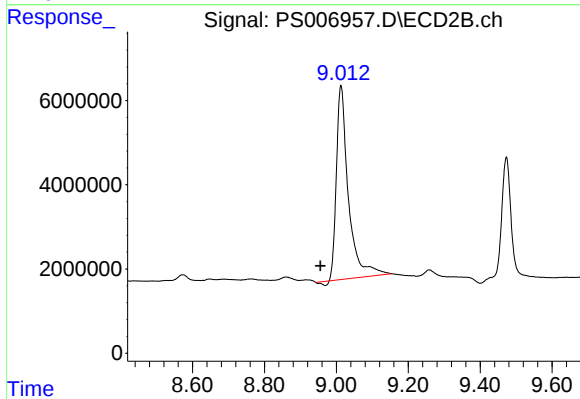

#16 DCPA

R.T.: 9.013 min
Delta R.T.: 0.057 min
Response: 105810959
Conc: 33.30 ng/ml