

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
 Data File : PS006960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 17:46
 Operator : SM\AJ
 Sample : K4668-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 03:48:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.499	5.230	332.7E6	169.4E6	364.061	368.451
Target Compounds							
1) T	Dalapon	2.046	1.761	114.4E6	109.0E6	107.046	204.529 #
2) T	3,5-DICHL...	0.000	4.558	0	65539372	N.D.	114.009
3) T	4-Nitroph...	5.351	0.000	6920190	0	18.149	N.D. #
5) T	DICAMBA	5.592	0.000	15708685	0	4.862	N.D. #
6) T	MCP	5.771	0.000	15406866	0	7.242	N.D. #
9) T	2,4-D	6.565	0.000	110.1E6	0	134.342	N.D. #
11) T	2,4,5-TP ...	0.000	6.849	0	78874114	N.D.	32.928
15) T	Picloram	9.037	9.006	18390014	5737234	2.742	1.576 #
16) T	DCPA	0.000	9.006	0	5737234	N.D.	1.806



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093019\
Data File : PS006960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 17:46
Operator : SM\AJ
Sample : K4668-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 03:48:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

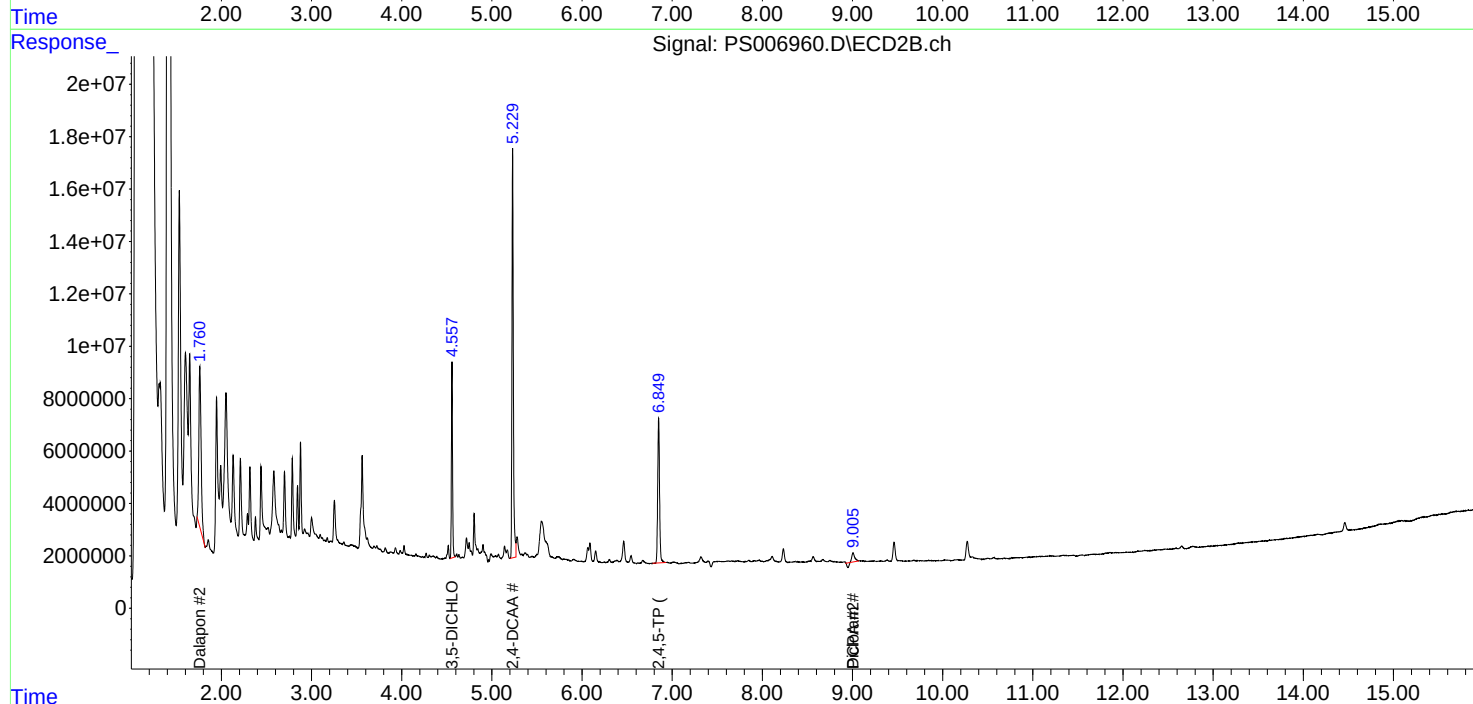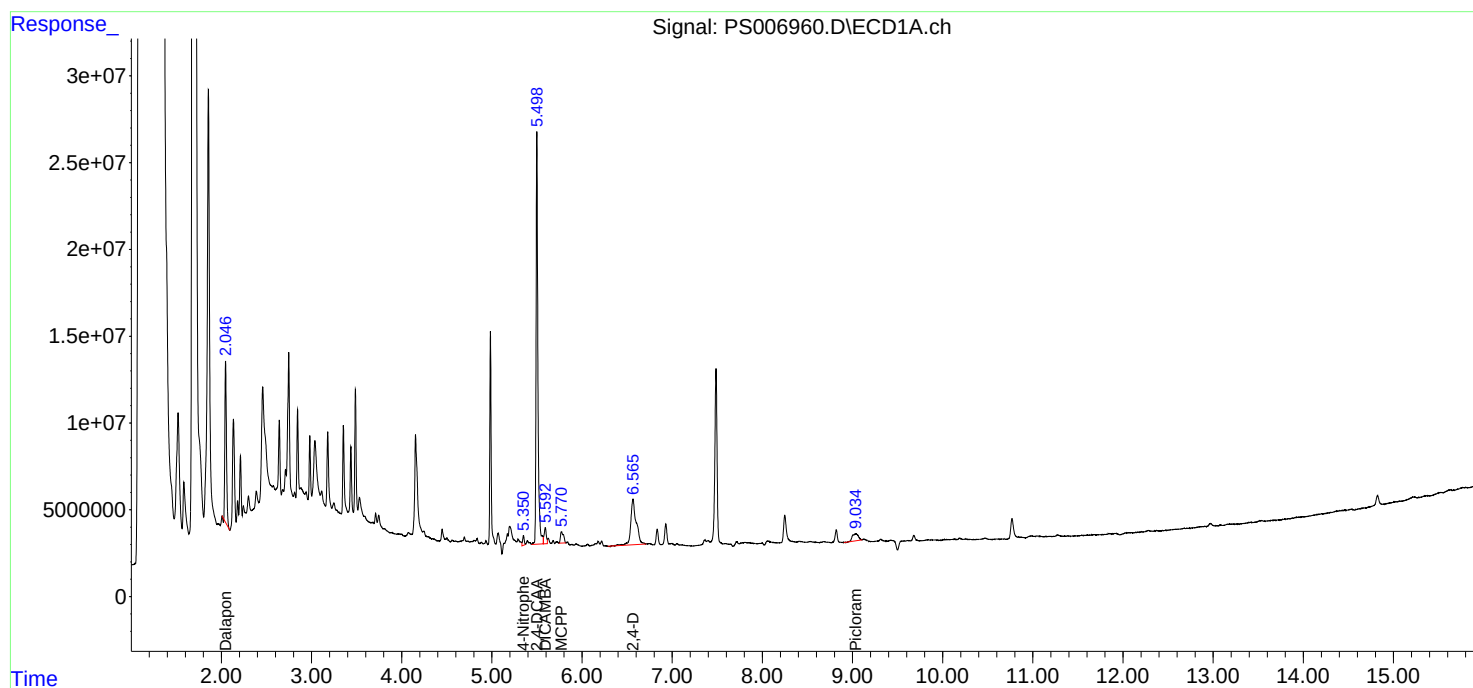


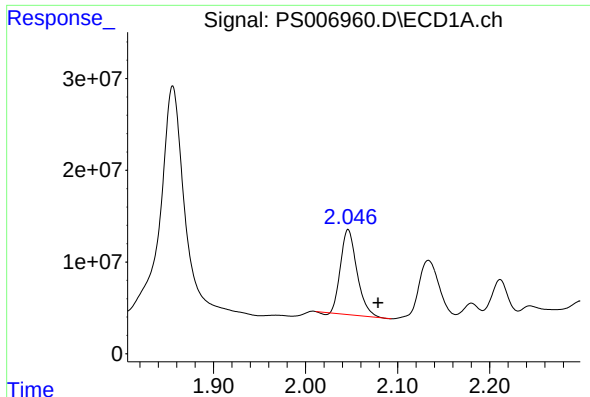

#1 Dalapon


R.T.: 2.046 min
Delta R.T.: -0.033 min
Response: 114368728
Conc: 107.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

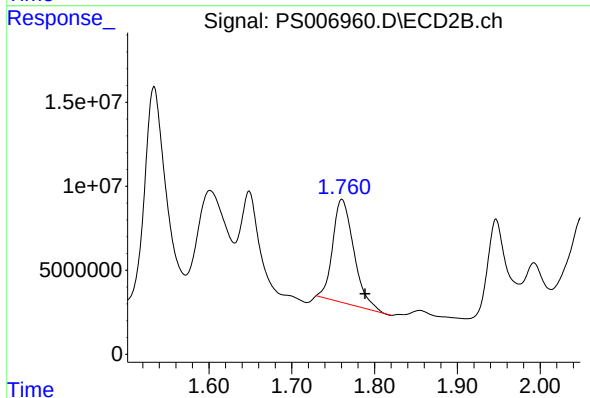


#1 Dalapon

R.T.: 1.761 min
Delta R.T.: -0.028 min
Response: 109027917
Conc: 204.53 ng/ml

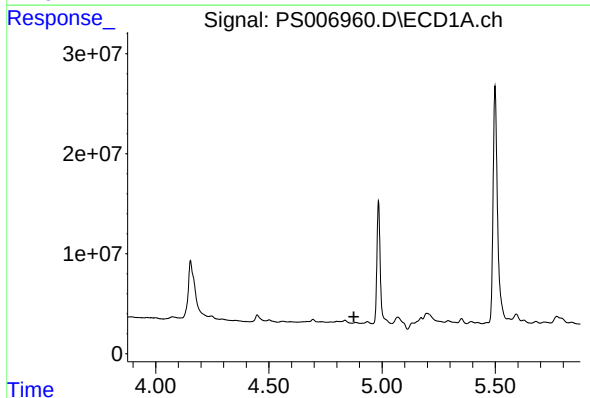


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.876 min
Response: 0
Conc: N.D.

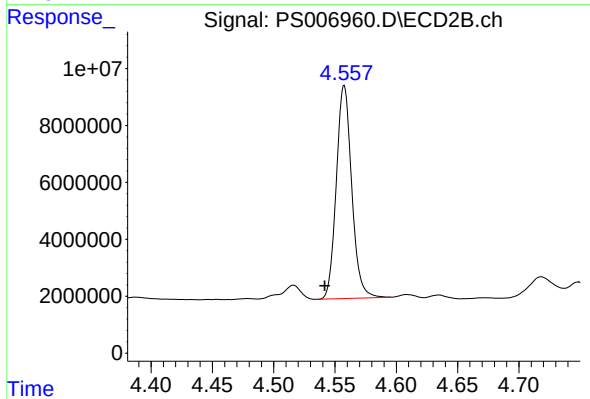

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.558 min
Delta R.T.: 0.016 min
Response: 65539372
Conc: 114.01 ng/ml

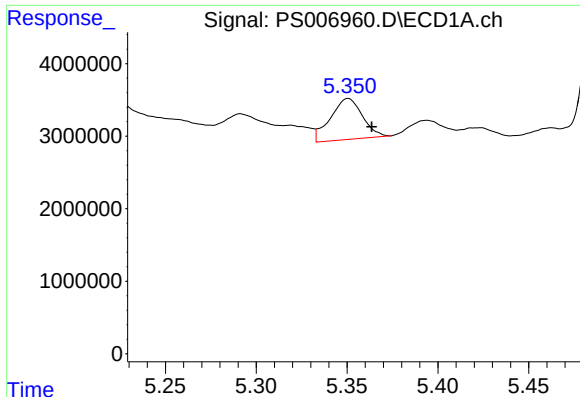

#3 4-Nitrophenol


R.T.: 5.351 min
Delta R.T.: -0.013 min
Response: 6920190
Conc: 18.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

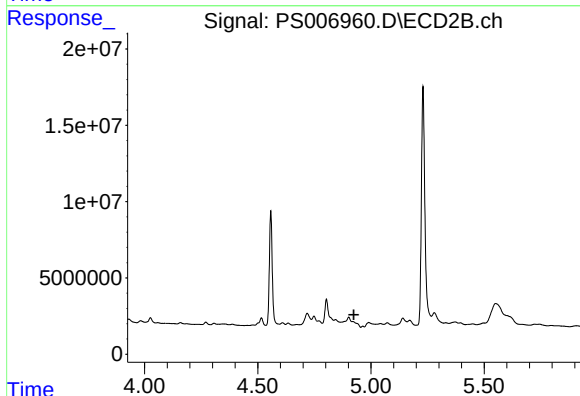


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

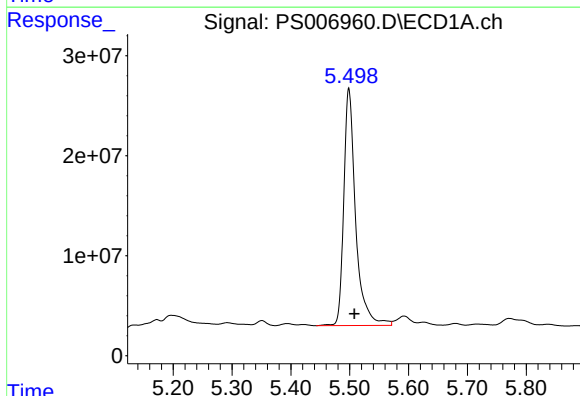


#4 2,4-DCAA

R.T.: 5.499 min
Delta R.T.: -0.009 min
Response: 332684114
Conc: 364.06 ng/ml

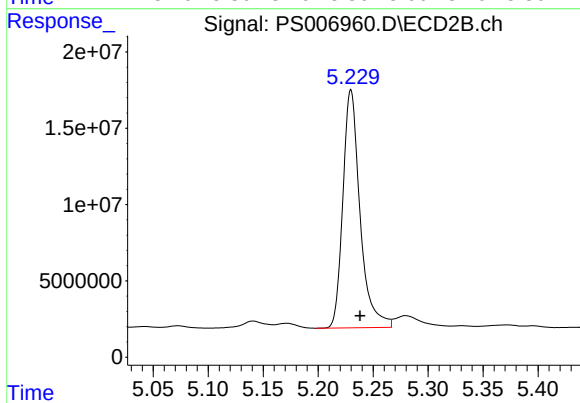

#4 2,4-DCAA


R.T.: 5.230 min
Delta R.T.: -0.008 min
Response: 169429110
Conc: 368.45 ng/ml

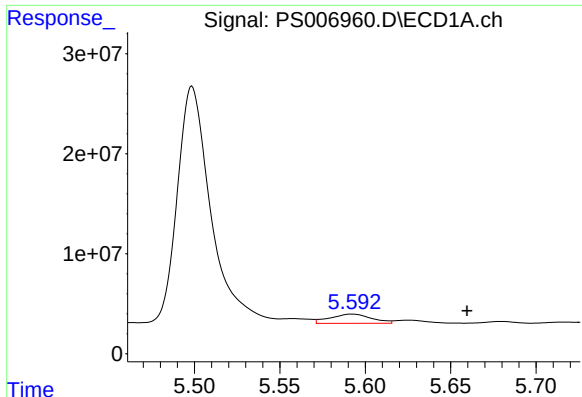

#5 DICAMBA


R.T.: 5.592 min
Delta R.T.: -0.067 min
Response: 15708685
Conc: 4.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

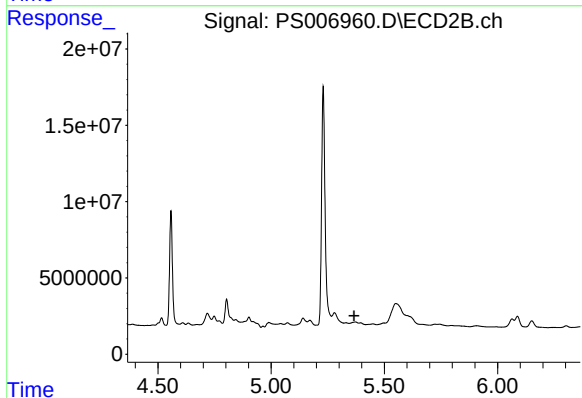


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

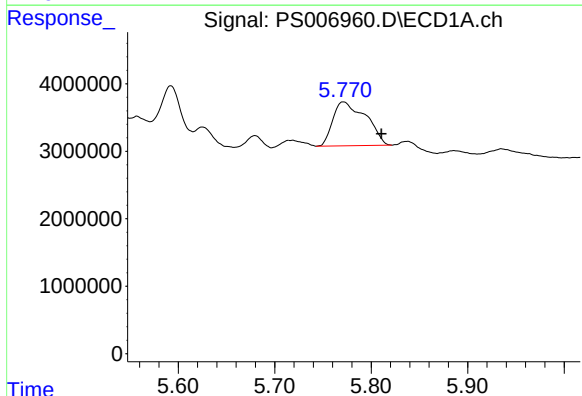


#6 MCP

R.T.: 5.771 min
Delta R.T.: -0.039 min
Response: 15406866
Conc: 7.24 ug/ml

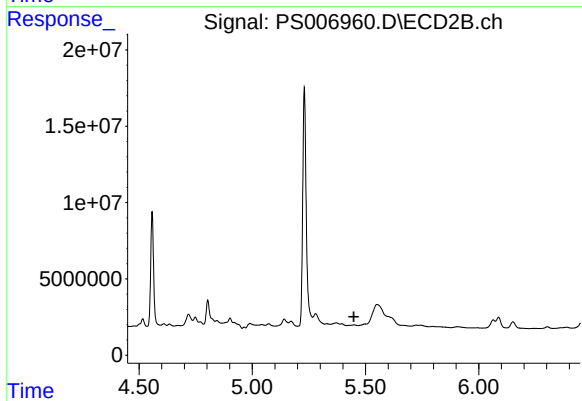

#6 MCP


R.T.: 0.000 min
Exp R.T. : 5.449 min
Response: 0
Conc: N.D.

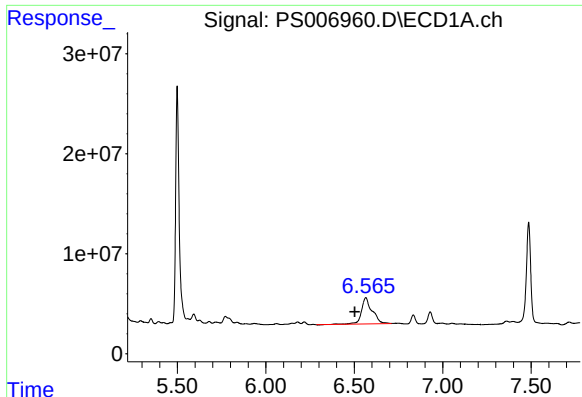

#9 2,4-D


R.T.: 6.565 min
Delta R.T.: 0.061 min
Response: 110095489
Conc: 134.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

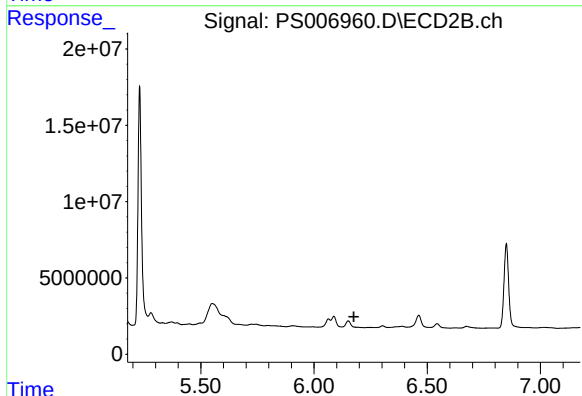


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

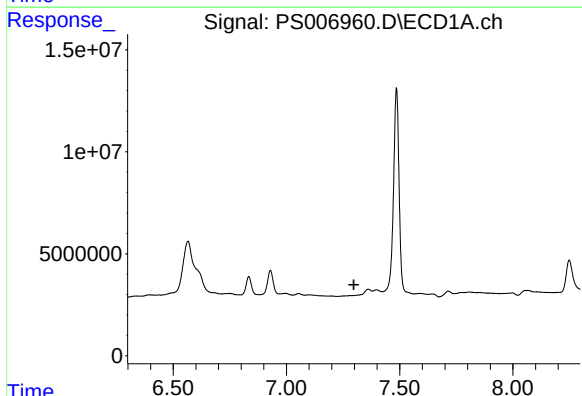


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.298 min
Response: 0
Conc: N.D.

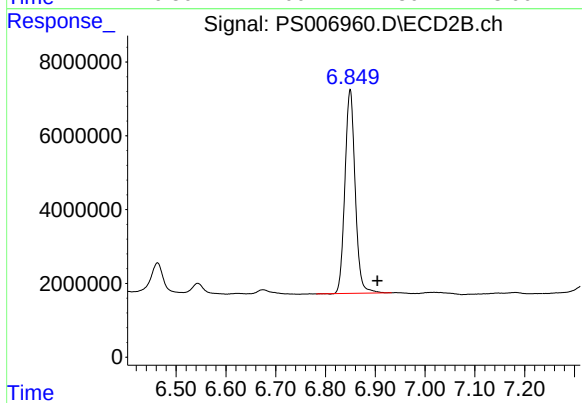

#11 2,4,5-TP (SILVEX)


R.T.: 6.849 min
Delta R.T.: -0.055 min
Response: 78874114
Conc: 32.93 ng/ml

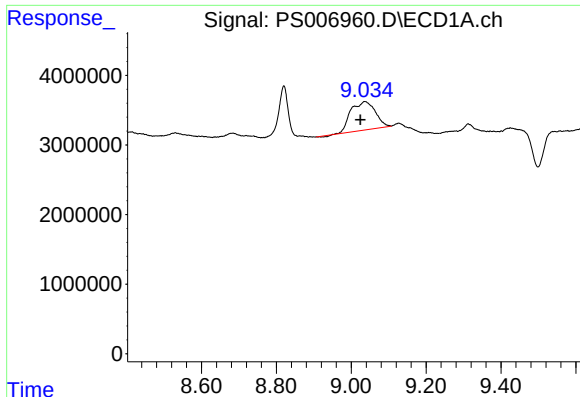

#15 Picloram


R.T.: 9.037 min
Delta R.T.: 0.012 min
Response: 18390014
Conc: 2.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

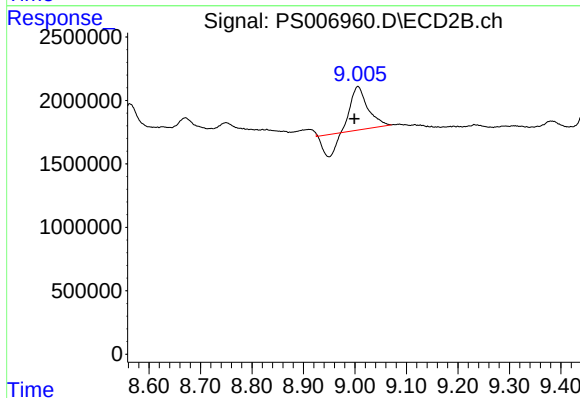


#15 Picloram

R.T.: 9.006 min
Delta R.T.: 0.007 min
Response: 5737234
Conc: 1.58 ng/ml

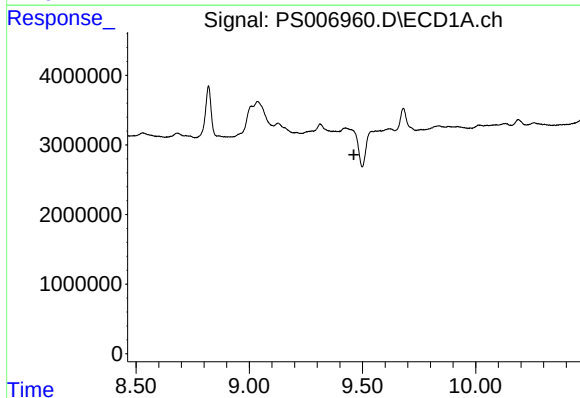

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.462 min
Response: 0
Conc: N.D.

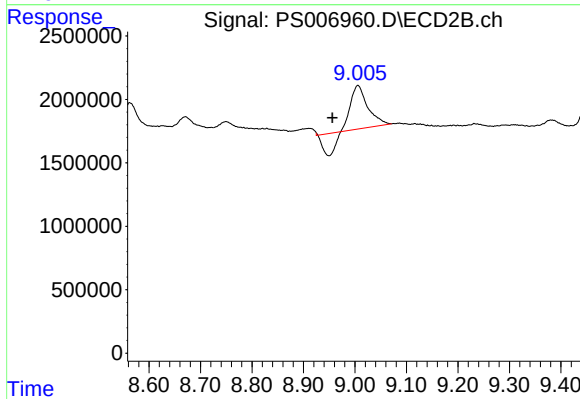

#16 DCPA

R.T.: 9.006 min
Delta R.T.: 0.050 min
Response: 5737234
Conc: 1.81 ng/ml