

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093022\
 Data File : PS020685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2022 09:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 11:46:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.182	6.762	1568.4E6	482.1E6	455.724	566.089
Target Compounds							
1) T	Dalapon	2.995	0.000	165237	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.452f	0.000	150.7E6	0	30.230	N.D. #
6) T	MCP	0.000	6.990	0	24621963	N.D.	8.526
7) T	MCPA	7.659	0.000	951863	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.176	0.000	5218928	0	<MDL	N.D. #
12) T	2,4,5-T	9.397	0.000	428173	0	<MDL	N.D. #
13) T	2,4-DB	9.923f	0.000	2140404	0	<MDL	N.D. #
14) T	DINOSEB	11.098	0.000	156.8E6	0	8.537	N.D. #
15) T	Picloram	10.972	10.746f	77426644	13760859	2.573	1.709 #
16) T	DCPA	11.399	10.746	6426333	13760859	<MDL	1.866 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093022\
Data File : PS020685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2022 09:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 11:46:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

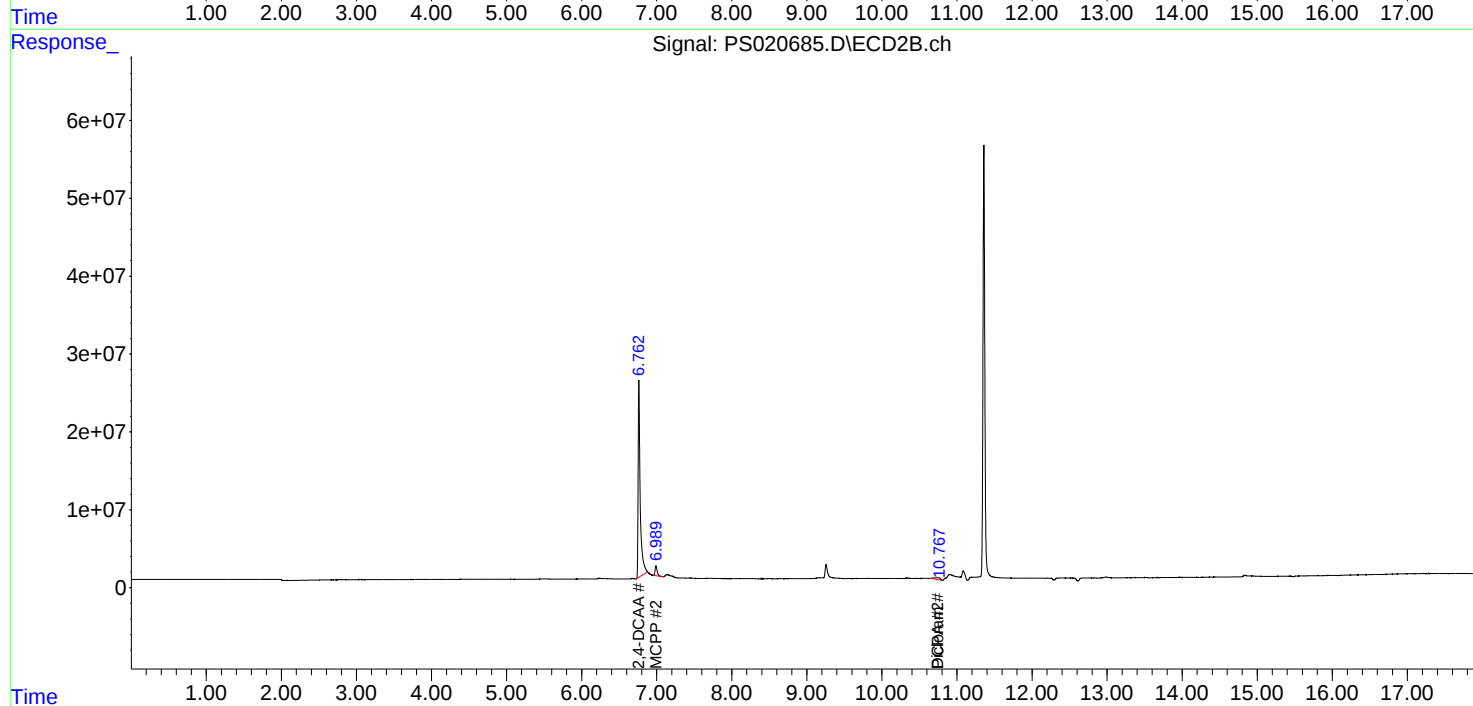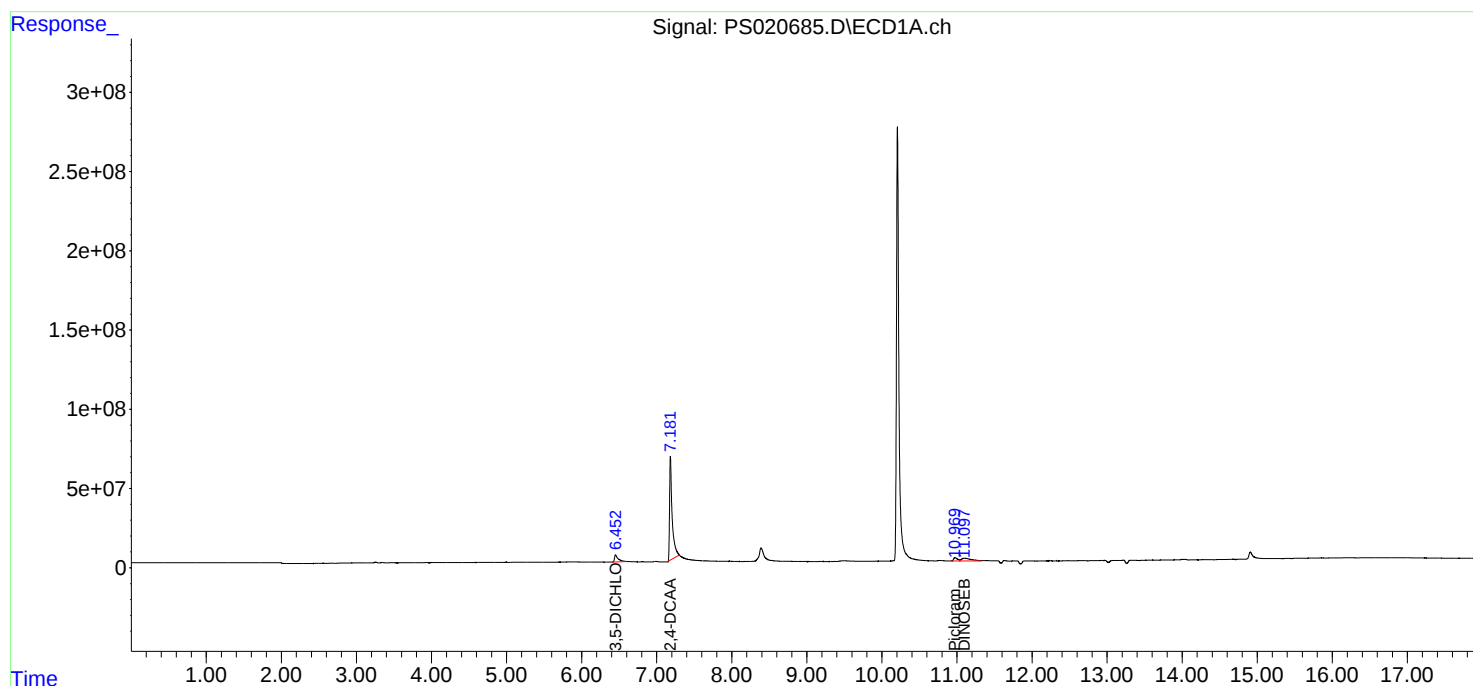


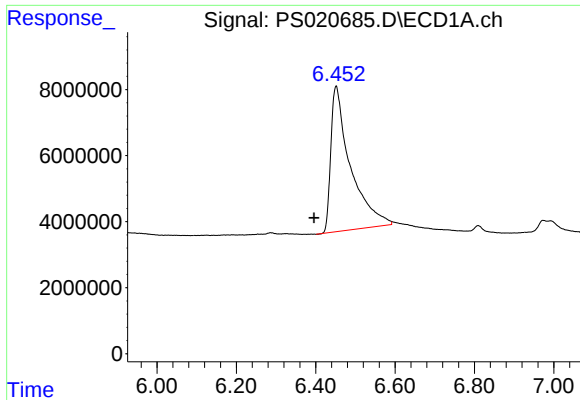

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.452 min
Delta R.T.: 0.055 min
Response: 150742358
Conc: 30.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

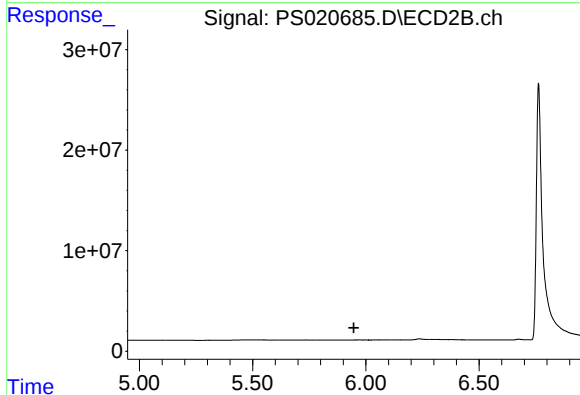


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

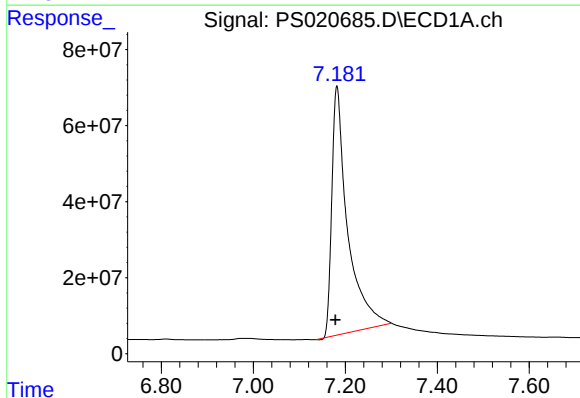


#4 2,4-DCAA

R.T.: 7.182 min
Delta R.T.: 0.003 min
Response: 1568369267
Conc: 455.72 ng/ml

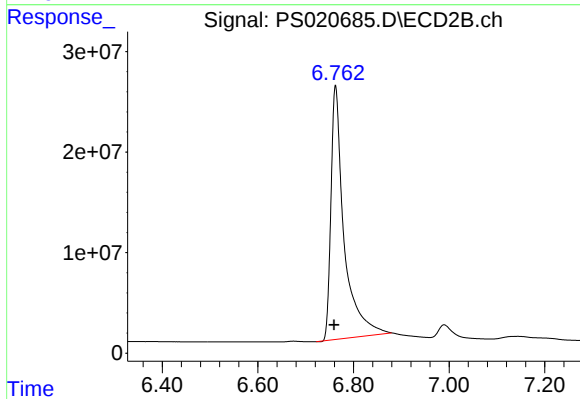

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: 0.003 min
Response: 482134981
Conc: 566.09 ng/ml

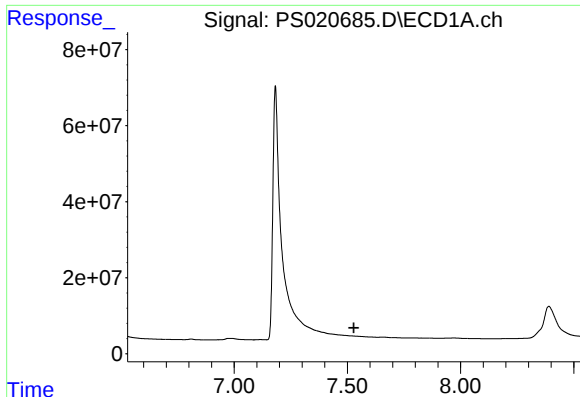

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

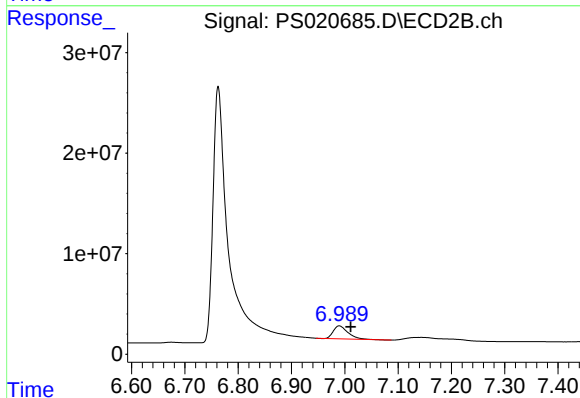


#6 MCP

R.T.: 6.990 min
Delta R.T.: -0.021 min
Response: 24621963
Conc: 8.53 ug/ml

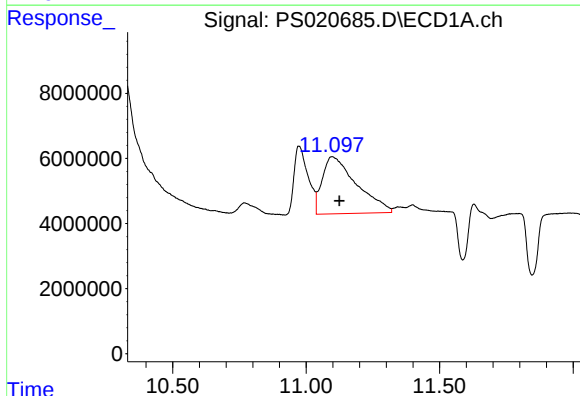


#14 DINOSEB

R.T.: 11.098 min
Delta R.T.: -0.027 min
Response: 156787176
Conc: 8.54 ng/ml

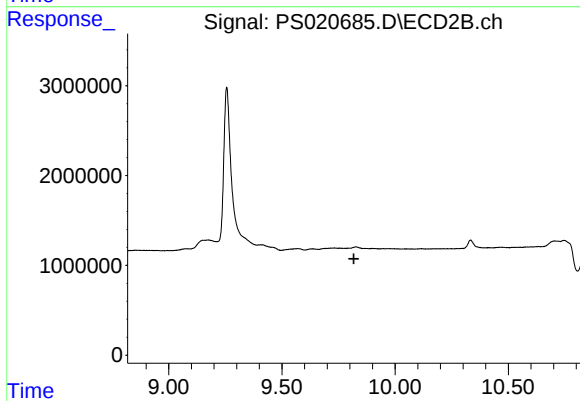

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.818 min
Response: 0
Conc: N.D.

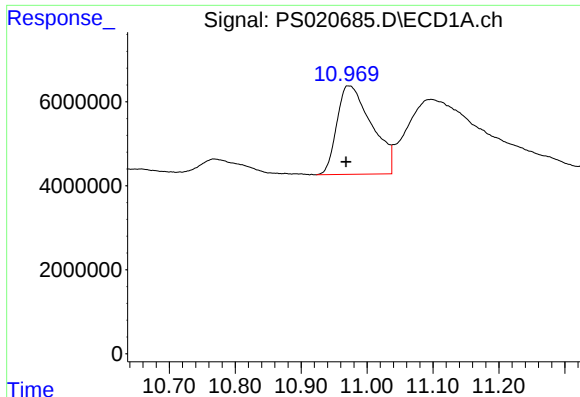

#15 Picloram


R.T.: 10.972 min
Delta R.T.: 0.003 min
Response: 77426644
Conc: 2.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

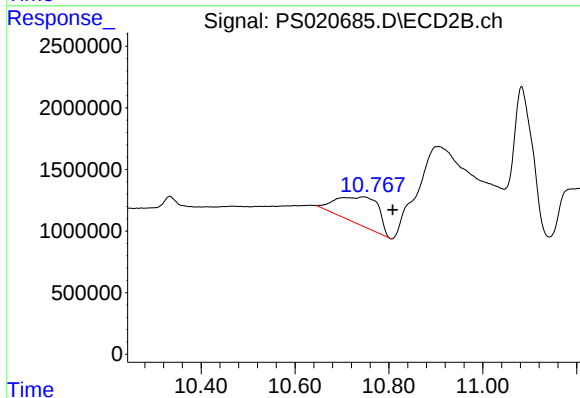


#15 Picloram

R.T.: 10.746 min
Delta R.T.: -0.061 min
Response: 13760859
Conc: 1.71 ng/ml

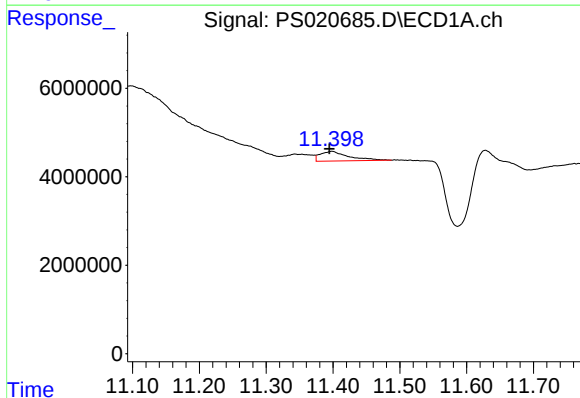

#16 DCPA

R.T.: 11.399 min
Delta R.T.: 0.004 min
Response: 6426333
Conc: N.D.

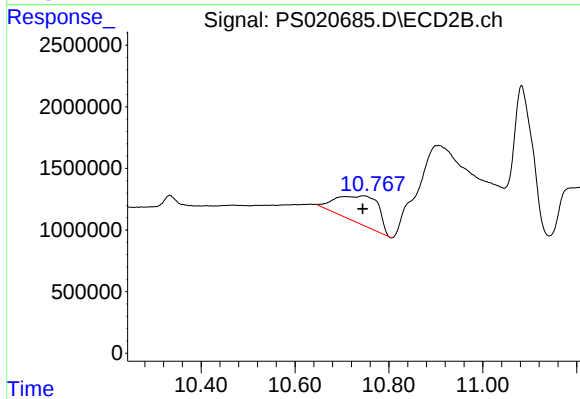

#16 DCPA

R.T.: 10.746 min
Delta R.T.: 0.002 min
Response: 13760859
Conc: 1.87 ng/ml