

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093022\
 Data File : PS020696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2022 14:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 17:45:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.181	6.762	1630.4E6	506.1E6	473.747	594.237 #
Target Compounds							
1) T	Dalapon	3.005	0.000	204348	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.448f	0.000	151.3E6	0	30.343	N.D. #
5) T	DICAMBA	0.000	6.988f	0	27573532	N.D.	7.163
6) T	MCP	0.000	6.988	0	27573532	N.D.	9.548
7) T	MCPA	7.656	0.000	692216	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.171	0.000	5379954	0	<MDL	N.D. #
13) T	2,4-DB	10.033f	0.000	6017400	0	1.657	N.D. #
14) T	DINOSEB	11.087	0.000	33471428	0	1.823	N.D. #
15) T	Picloram	10.963	0.000	93262658	0	3.099	N.D. #
16) T	DCPA	11.397	10.689f	7392385	6711901	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093022\
Data File : PS020696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2022 14:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 17:45:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

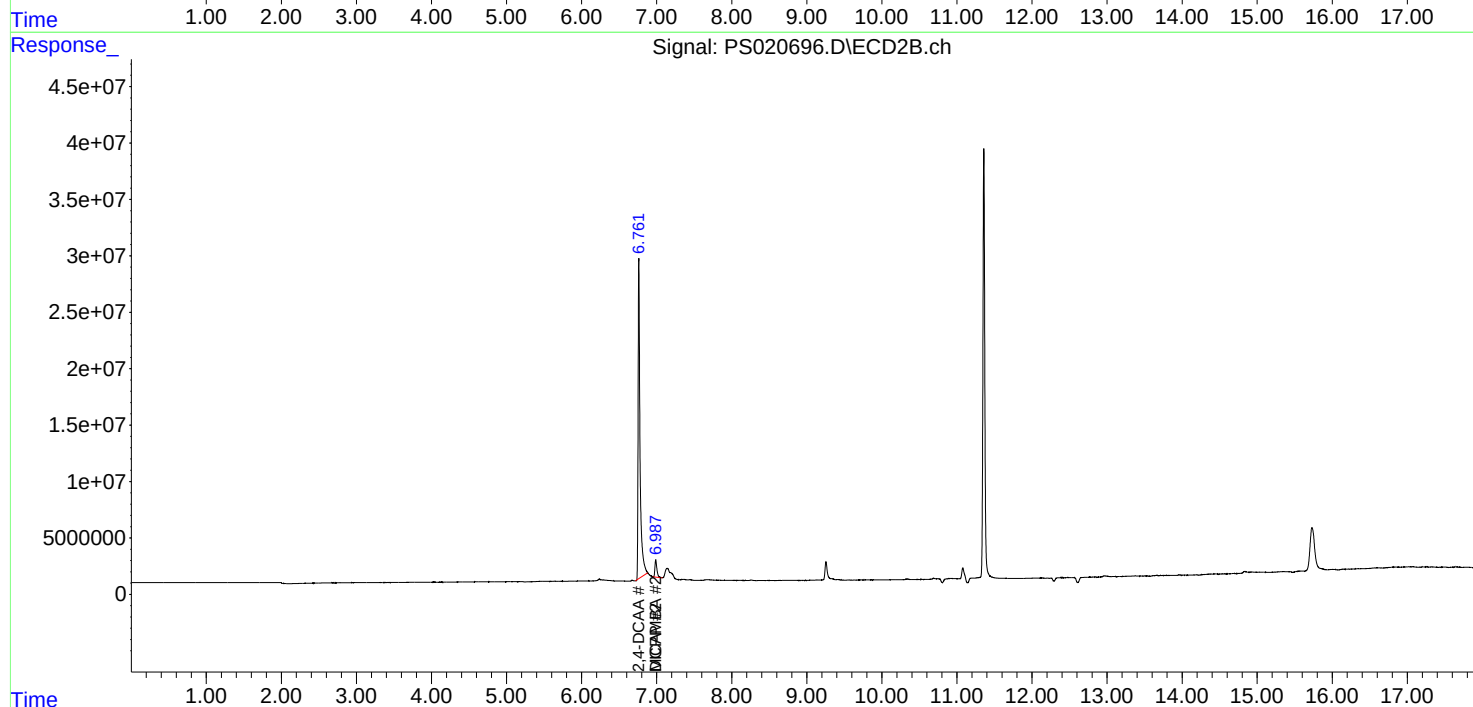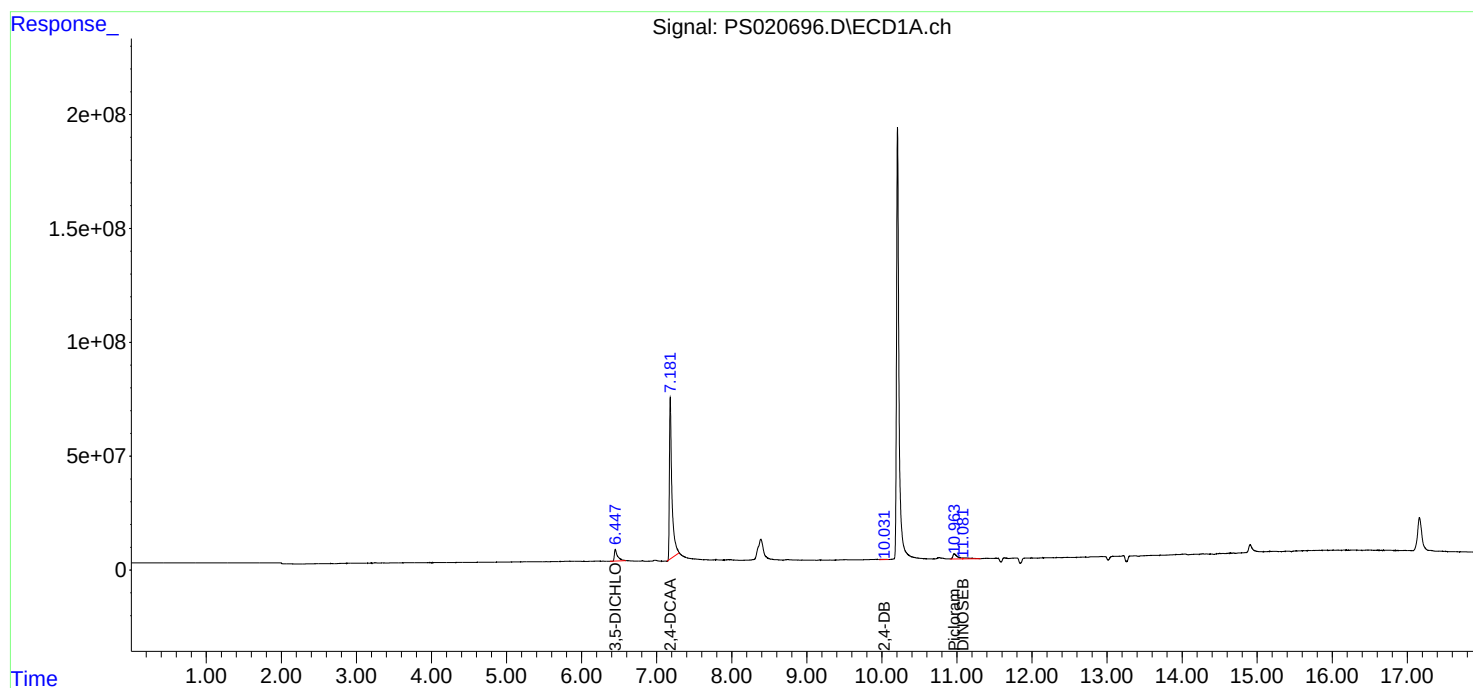


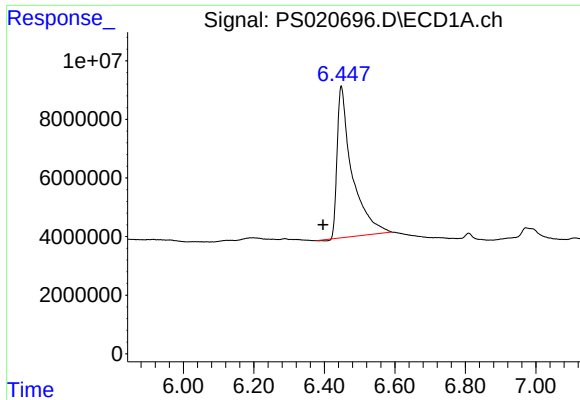

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.448 min
Delta R.T.: 0.052 min
Response: 151305718
Conc: 30.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

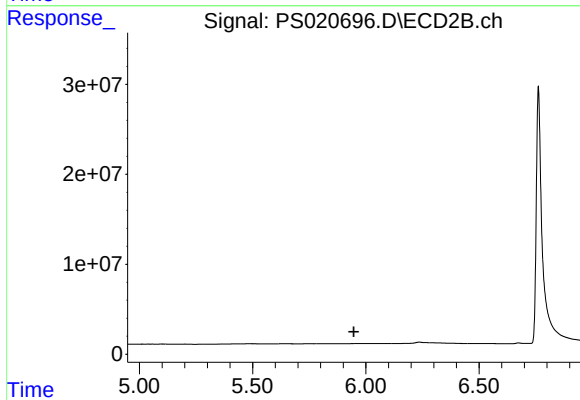


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

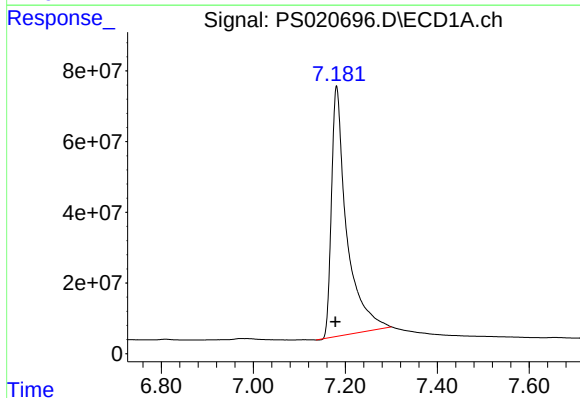


#4 2,4-DCAA

R.T.: 7.181 min
Delta R.T.: 0.002 min
Response: 1630392594
Conc: 473.75 ng/ml

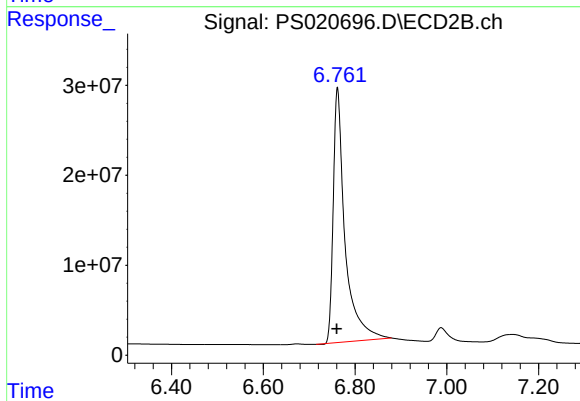

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: 0.002 min
Response: 506108601
Conc: 594.24 ng/ml

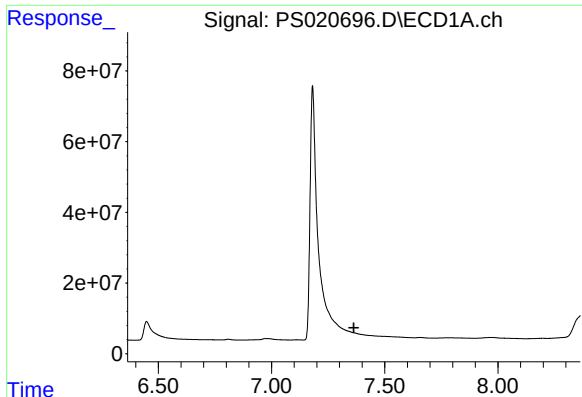

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

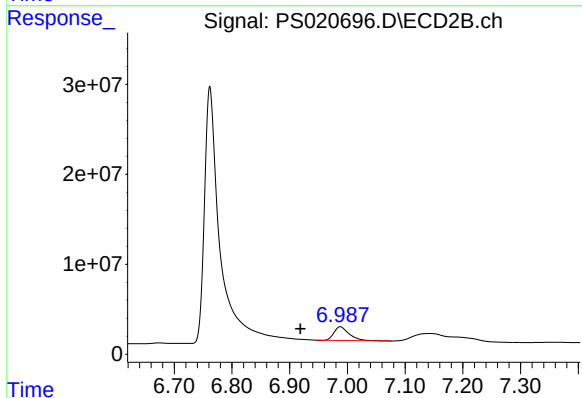


#5 DICAMBA

R.T.: 6.988 min
Delta R.T.: 0.069 min
Response: 27573532
Conc: 7.16 ng/ml

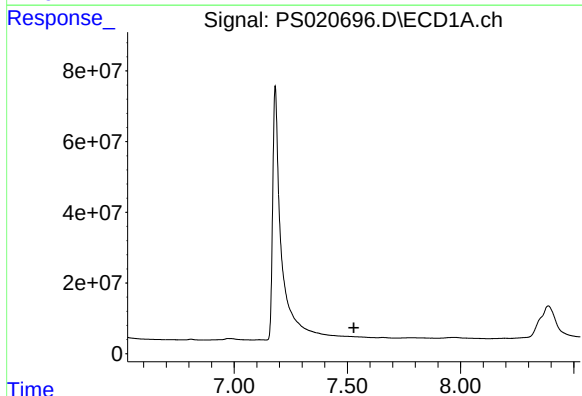


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.529 min
Response: 0
Conc: N.D.

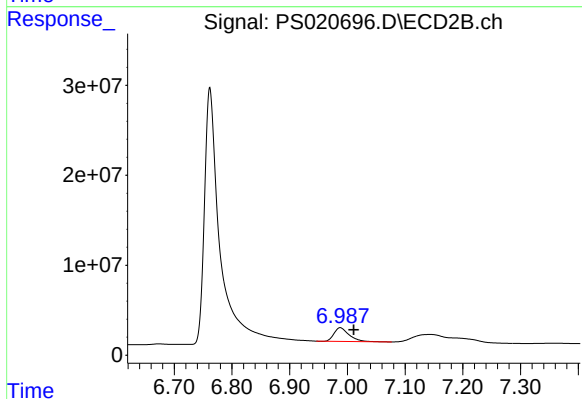

#6 MCP


R.T.: 6.988 min
Delta R.T.: -0.024 min
Response: 27573532
Conc: 9.55 ug/ml

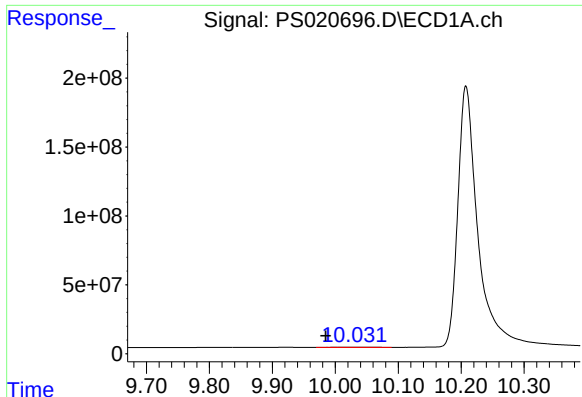

#13 2,4-DB


R.T.: 10.033 min
Delta R.T.: 0.048 min
Response: 6017400
Conc: 1.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

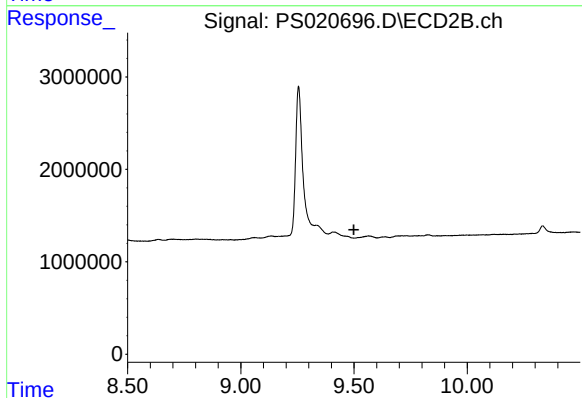


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.499 min
Response: 0
Conc: N.D.

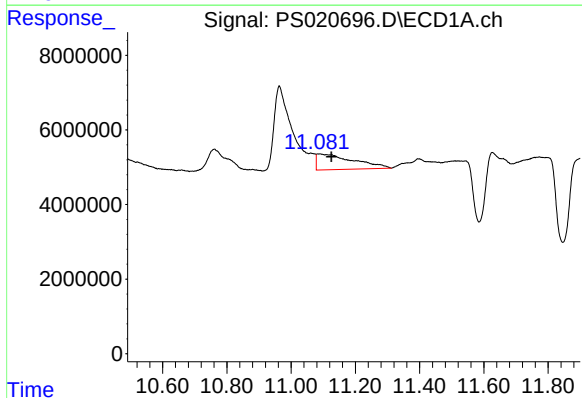


#14 DINOSEB

R.T.: 11.087 min
Delta R.T.: -0.038 min
Response: 33471428
Conc: 1.82 ng/ml

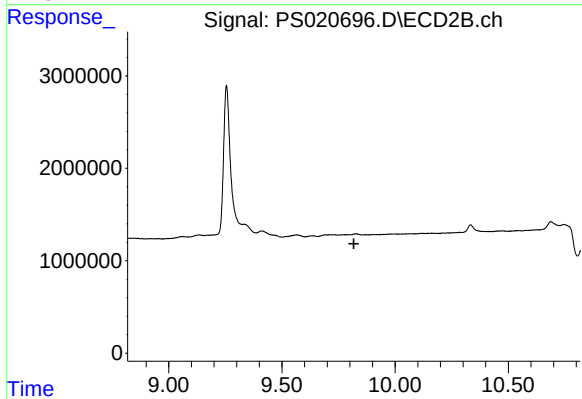

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.

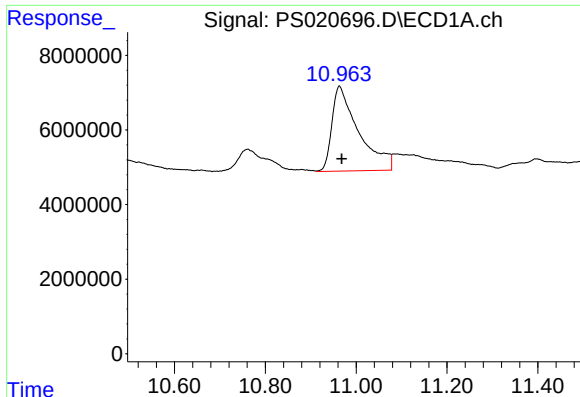

#15 Picloram

R.T.: 10.963 min
Delta R.T.: -0.005 min
Response: 93262658
Conc: 3.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

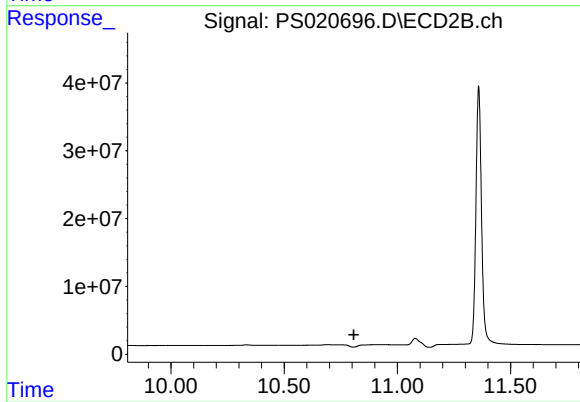

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.808 min
Response: 0
Conc: N.D.