

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093025\
 Data File : PS031893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2025 21:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 02:22:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.284	7.746	1891.1E6	530.2E6	525.070	583.301
Target Compounds							
1) T	Dalapon	2.716f	2.655f	14131006	46057302	2.444	16.346 #
2) T	3,5-DICHL...	6.444	0.000	21266214	0	3.987	N.D. #
7) T	MCPA	7.752f	0.000	17710604	0	1.594	N.D. #
8) T	DICHLORPROP	8.185	0.000	1465705	0	<MDL	N.D. #
10) T	Pentachlo...	8.707	9.513	10069610	6879983	<MDL	<MDL #
11) T	2,4,5-TP ...	9.295	9.917	6481660	1873860	<MDL	<MDL #
12) T	2,4,5-T	9.582	0.000	1033953	0	<MDL	N.D. #
13) T	2,4-DB	10.185f	0.000	2798150	0	1.199	N.D. #
14) T	DINOSEB	11.356	0.000	3120488	0	<MDL	N.D. #
15) T	Picloram	11.178	0.000	11661042	0	<MDL	N.D. #
16) T	DCPA	11.659	0.000	3621812	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093025\
Data File : PS031893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2025 21:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 02:22:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

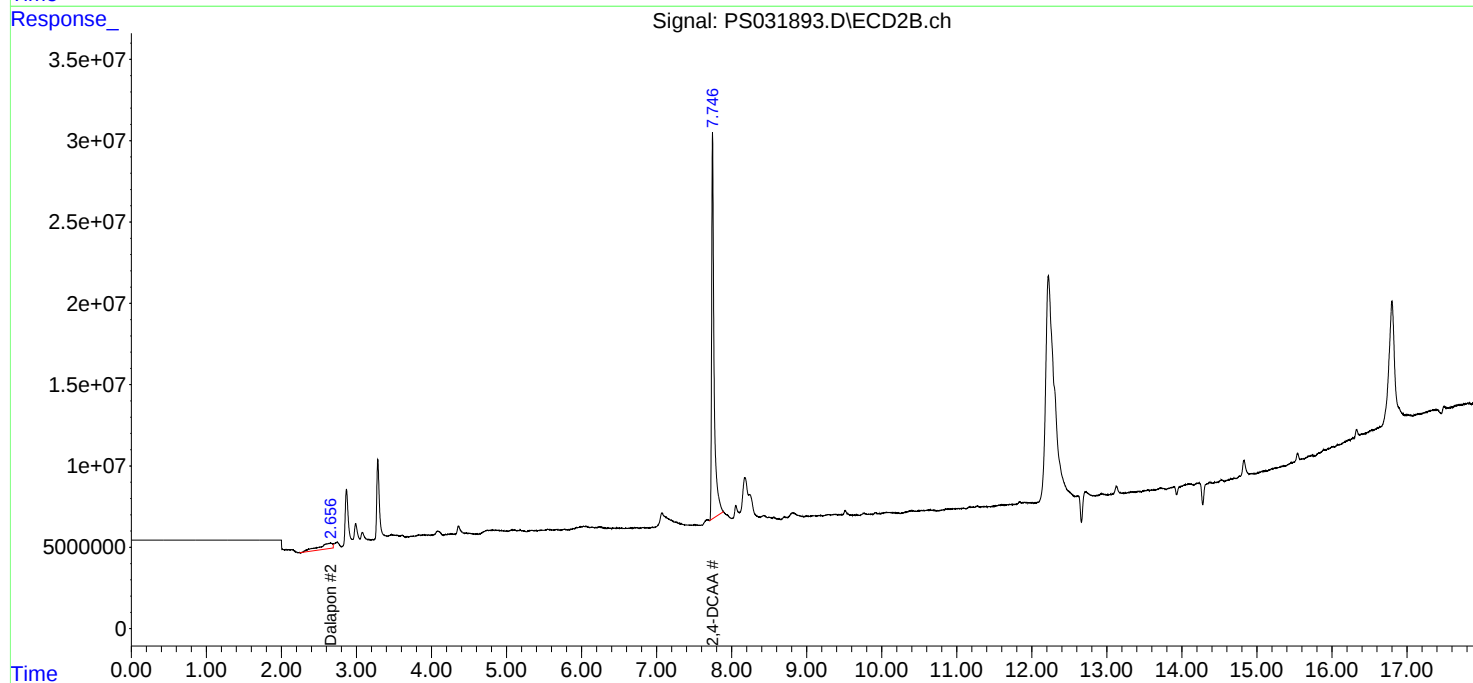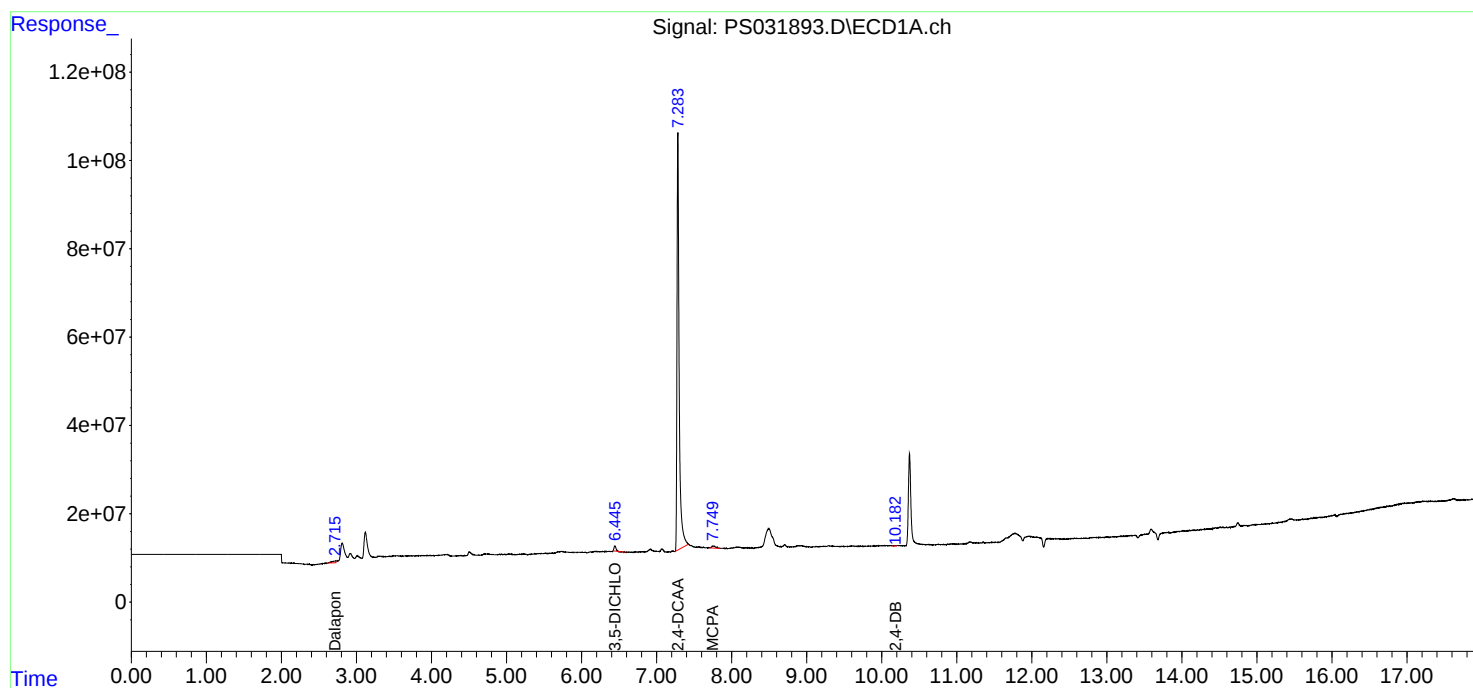


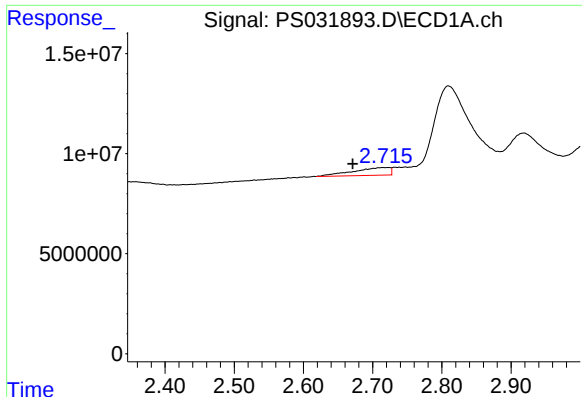

#1 Dalapon


R.T.: 2.716 min
Delta R.T.: 0.045 min
Response: 14131006
Conc: 2.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

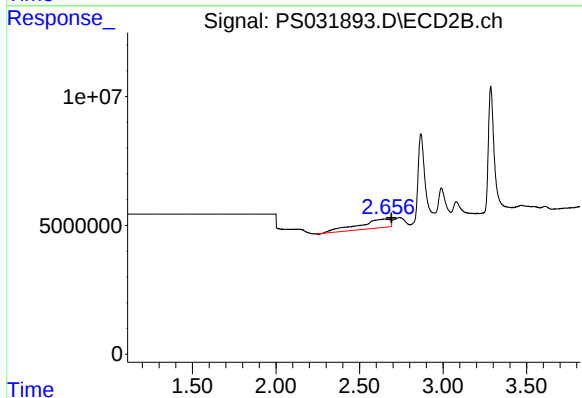


#1 Dalapon

R.T.: 2.655 min
Delta R.T.: -0.036 min
Response: 46057302
Conc: 16.35 ng/ml

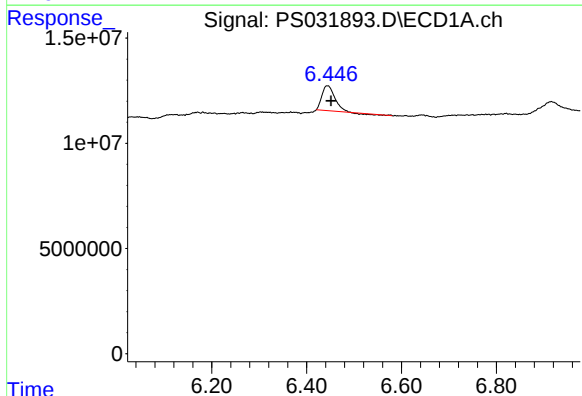


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.444 min
Delta R.T.: -0.008 min
Response: 21266214
Conc: 3.99 ng/ml

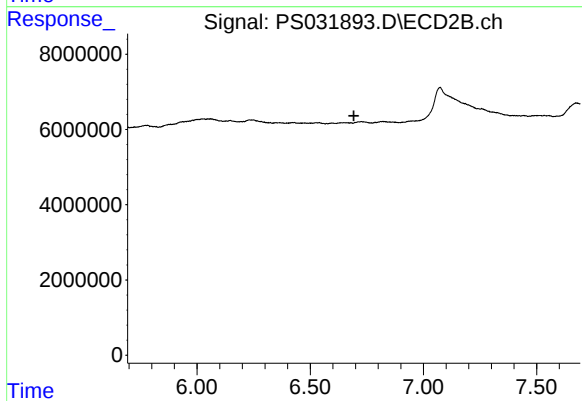

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.693 min
Response: 0
Conc: N.D.

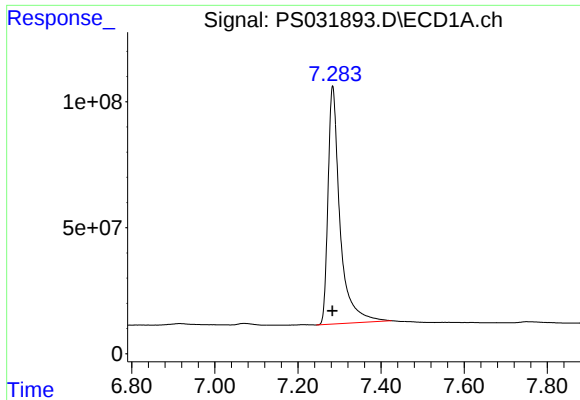

#4 2,4-DCAA


R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 1891052775
Conc: 525.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

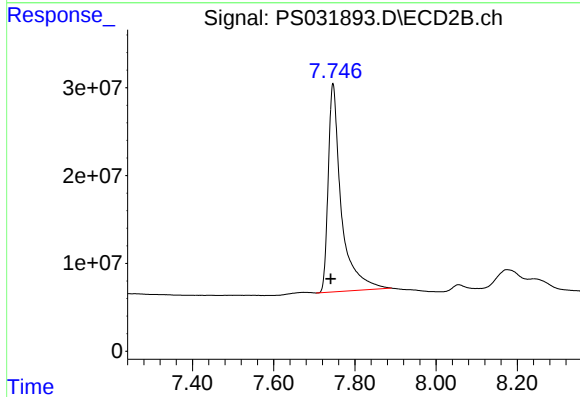


#4 2,4-DCAA

R.T.: 7.746 min
Delta R.T.: 0.006 min
Response: 530162337
Conc: 583.30 ng/ml

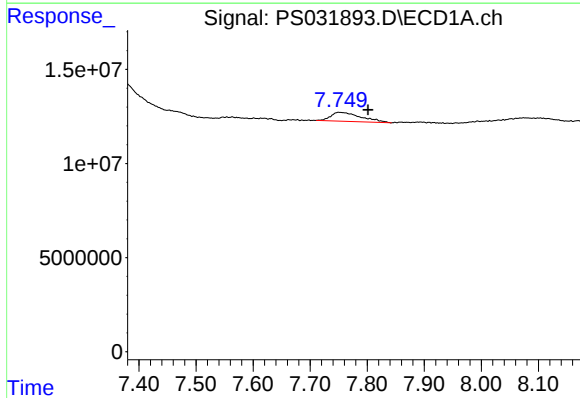


#7 MCPA

R.T.: 7.752 min
Delta R.T.: -0.050 min
Response: 17710604
Conc: 1.59 ug/ml

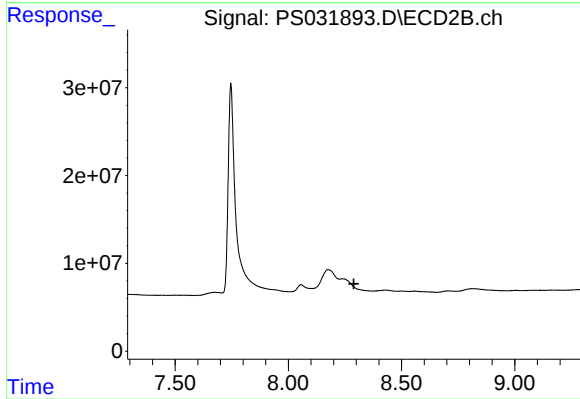

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 8.290 min
Response: 0
Conc: N.D.

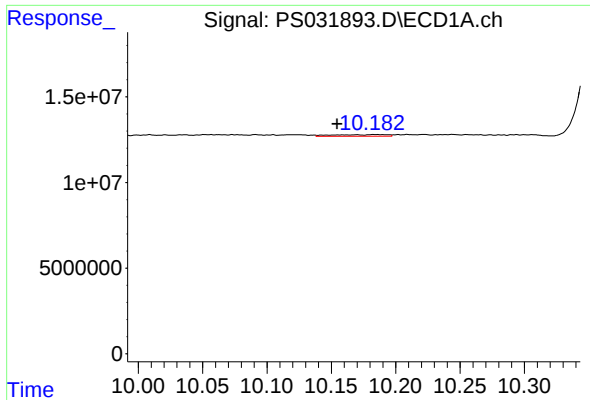

#13 2,4-DB

R.T.: 10.185 min
Delta R.T.: 0.030 min
Response: 2798150
Conc: 1.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

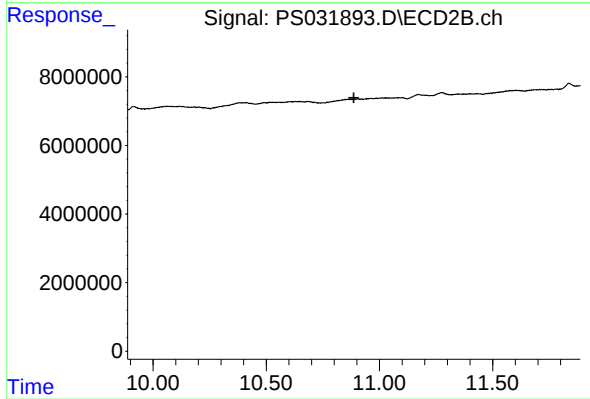

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.887 min
Response: 0
Conc: N.D.