

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093025\
 Data File : PS031906.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2025 02:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 07:58:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.282	7.743	1944.5E6	556.7E6	539.920	612.528
Target Compounds							
1) T	Dalapon	2.700f	2.662f	26144368	6655688	4.523	2.362 #
2) T	3,5-DICHL...	6.442	0.000	23592480	0	4.424	N.D. #
7) T	MCPA	0.000	8.242f	0	32487319	N.D.	11.598
8) T	DICHLORPROP	8.175	8.682f	8841594	1971979	2.482	1.355 #
9) T	2,4-D	0.000	8.981	0	2068963	N.D.	1.258
10) T	Pentachlo...	8.705	9.508	7519481	18892964	<MDL	<MDL #
11) T	2,4,5-TP ...	9.286	9.903	7018133	2720206	<MDL	<MDL #
12) T	2,4,5-T	9.600	0.000	2547761	0	<MDL	N.D. #
13) T	2,4-DB	10.133	0.000	909918	0	<MDL	N.D. #
14) T	DINOSEB	11.353	11.264	2243312	2152728	<MDL	<MDL #
15) T	Picloram	11.162	0.000	17093019	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS093025\
Data File : PS031906.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2025 02:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 07:58:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

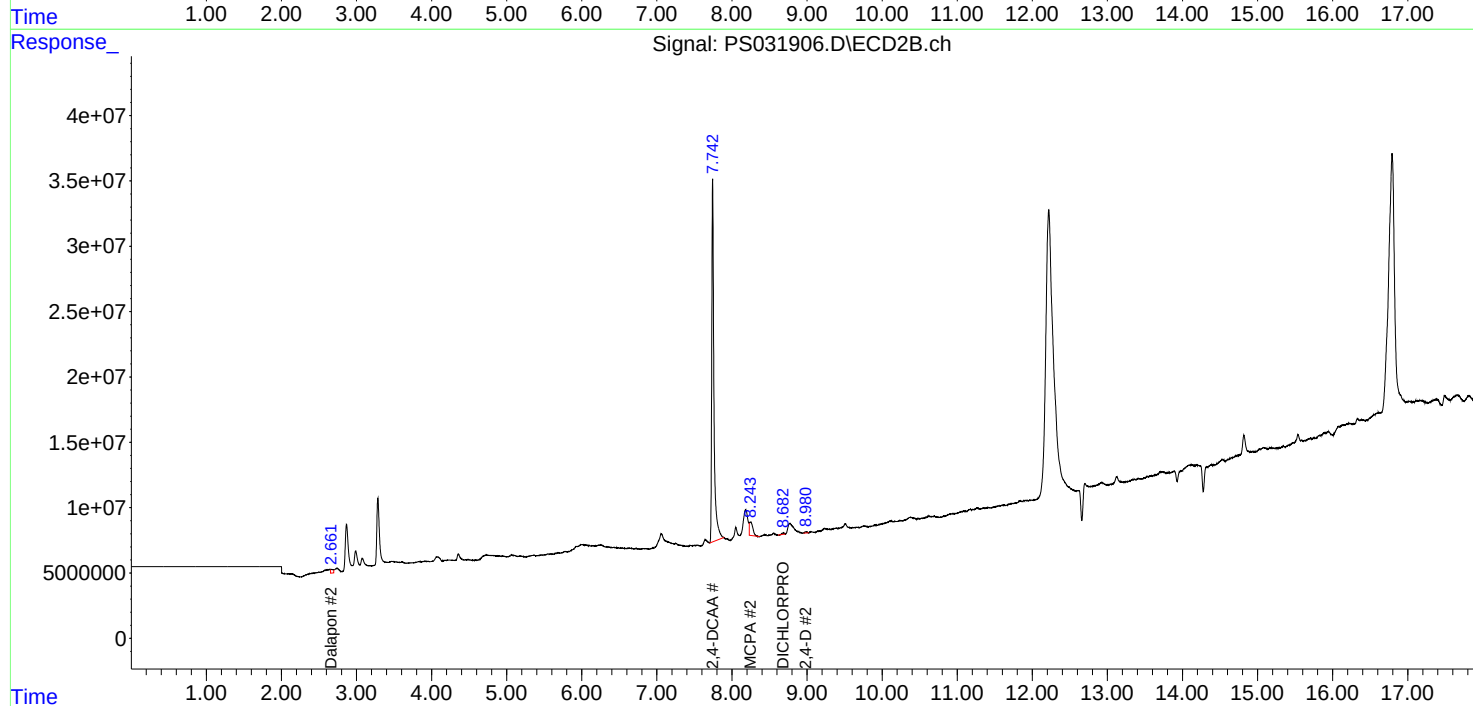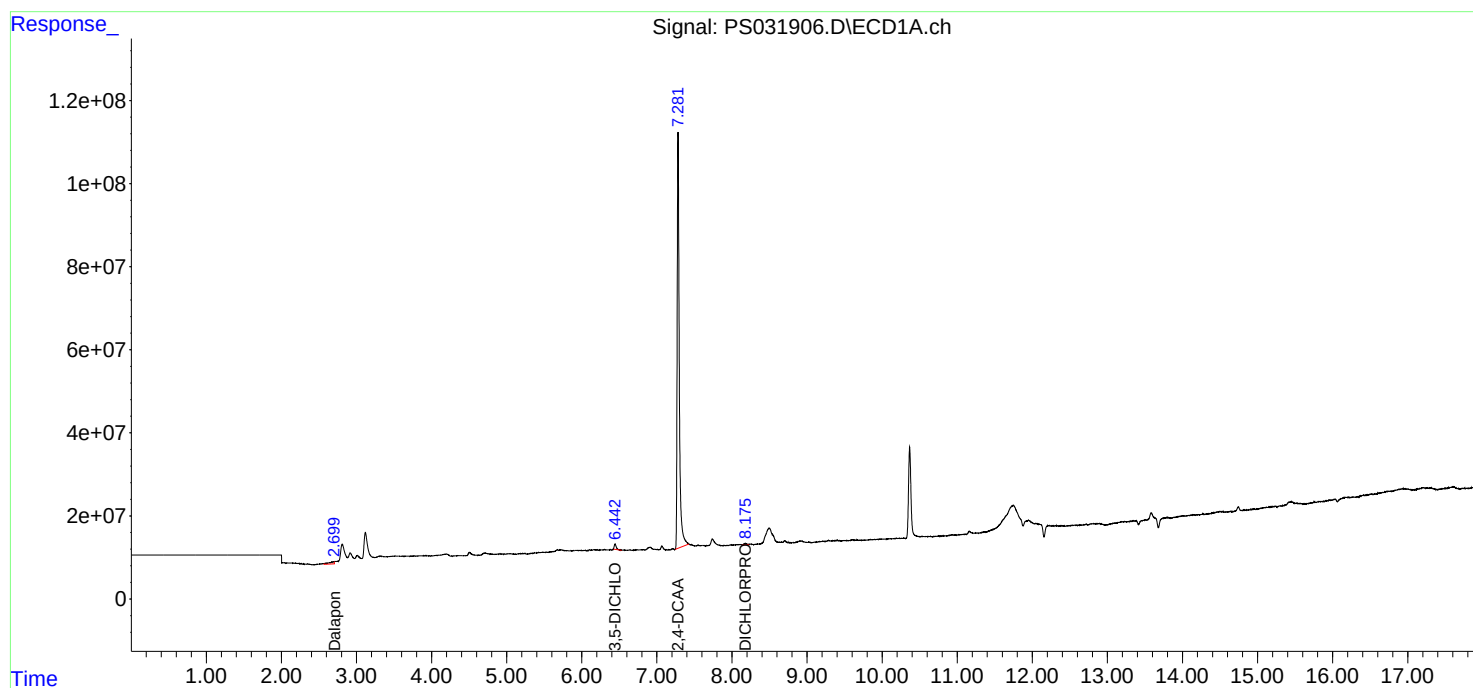


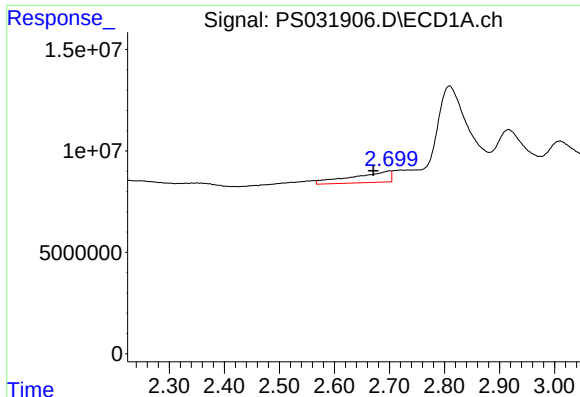

#1 Dalapon


R.T.: 2.700 min
Delta R.T.: 0.029 min
Response: 26144368
Conc: 4.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

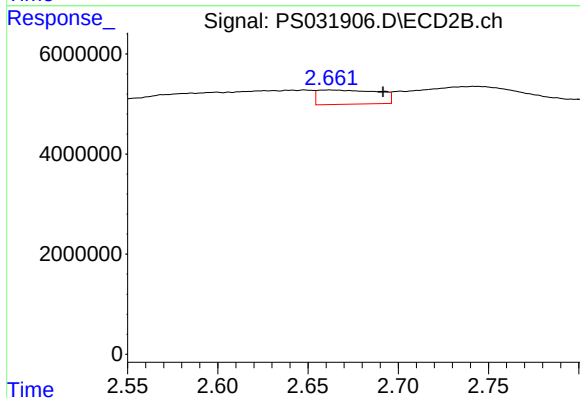


#1 Dalapon

R.T.: 2.662 min
Delta R.T.: -0.030 min
Response: 6655688
Conc: 2.36 ng/ml

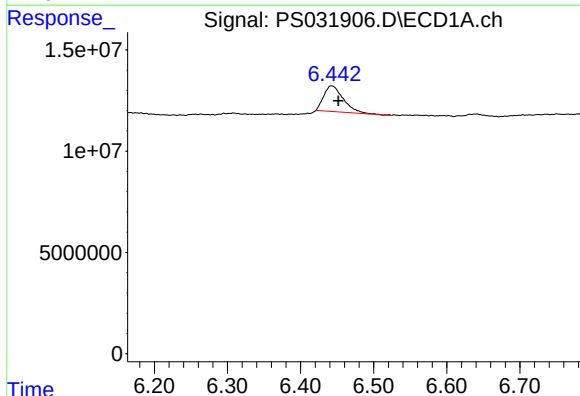


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.442 min
Delta R.T.: -0.009 min
Response: 23592480
Conc: 4.42 ng/ml

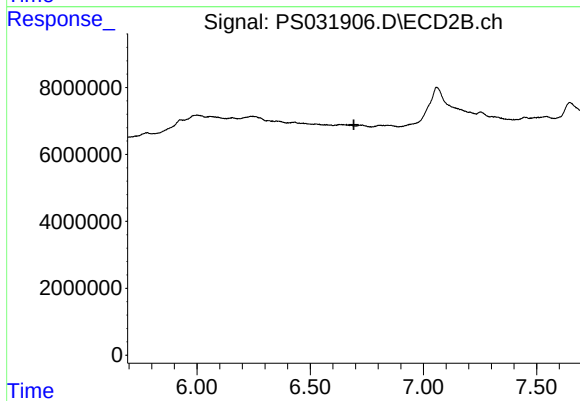

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

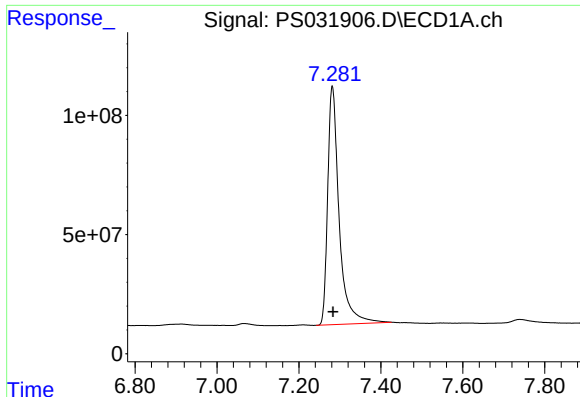

#4 2,4-DCAA


R.T.: 7.282 min
Delta R.T.: -0.002 min
Response: 1944537230
Conc: 539.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

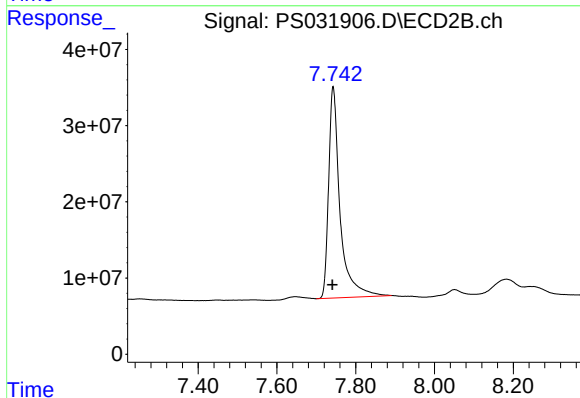


#4 2,4-DCAA

R.T.: 7.743 min
Delta R.T.: 0.002 min
Response: 556726099
Conc: 612.53 ng/ml

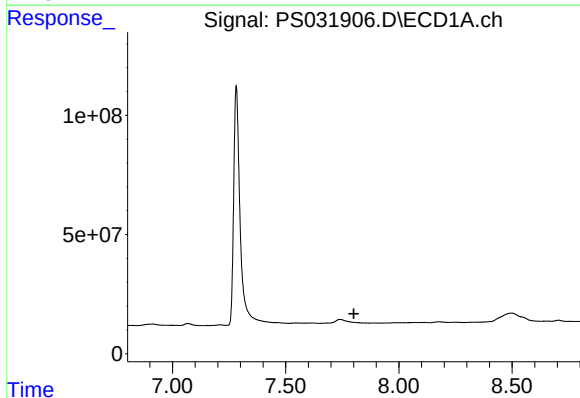


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.802 min
Response: 0
Conc: N.D.

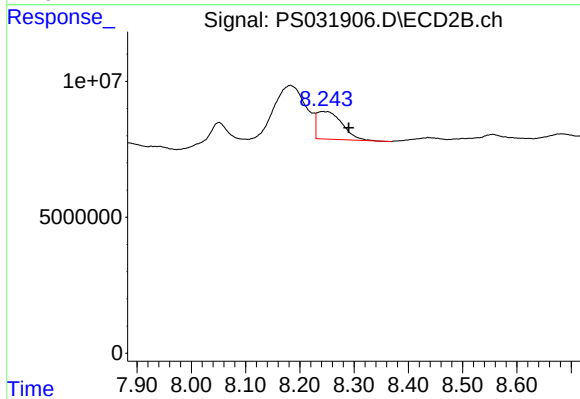

#7 MCPA


R.T.: 8.242 min
Delta R.T.: -0.048 min
Response: 32487319
Conc: 11.60 ug/ml

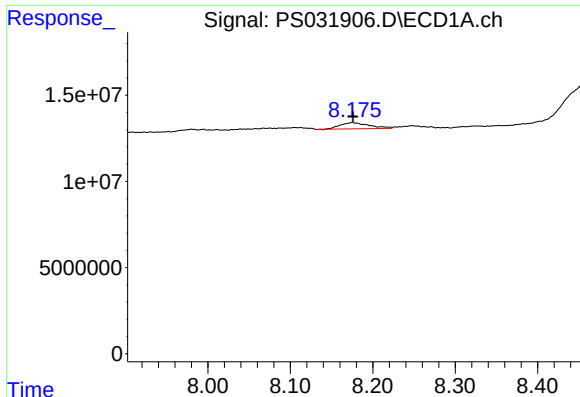

#8 DICHLORPROP


R.T.: 8.175 min
Delta R.T.: -0.001 min
Response: 8841594
Conc: 2.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

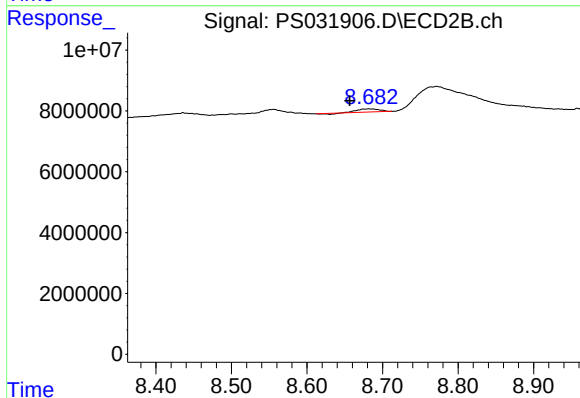


#8 DICHLORPROP

R.T.: 8.682 min
Delta R.T.: 0.026 min
Response: 1971979
Conc: 1.36 ng/ml

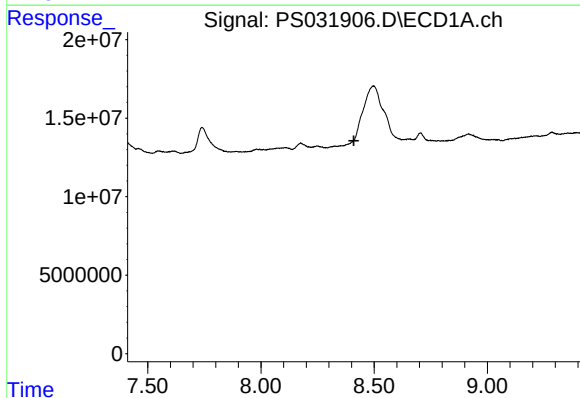

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.411 min
Response: 0
Conc: N.D.

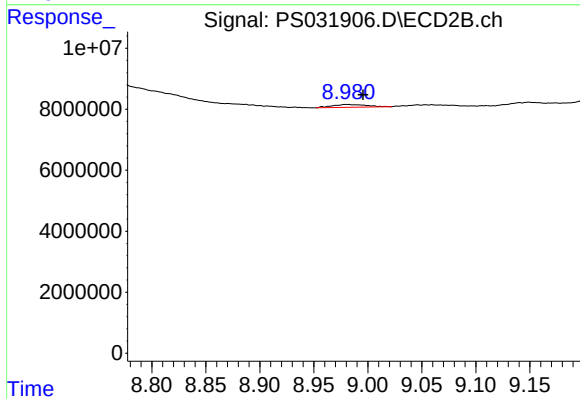

#9 2,4-D

R.T.: 8.981 min
Delta R.T.: -0.014 min
Response: 2068963
Conc: 1.26 ng/ml