

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
 Data File : PS001846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2018 16:51
 Operator : EI\SJ
 Sample : J4777-34
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:50:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.456	10.944	93241120	94773785	415.669	373.101
Target Compounds							
1) T	Dalapon	0.000	2.356	0	8319404	N.D.	28.162 #
2) T	3,5-DICHL...	0.000	9.095	0	2378229	N.D.	7.535 #
6) T	MCP	12.145	11.550	30613064	5732274	48.040	9.728 #
9) T	2,4-D	13.344	0.000	4719372	0	17.123	N.D. #
15) T	Picloram	16.977	16.883	7830989	24511756	4.497	14.412 #
16) T	DCPA	0.000	16.883	0	24511756	N.D.	13.290 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
Data File : PS001846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2018 16:51
Operator : EI\SJ
Sample : J4777-34
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:50:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

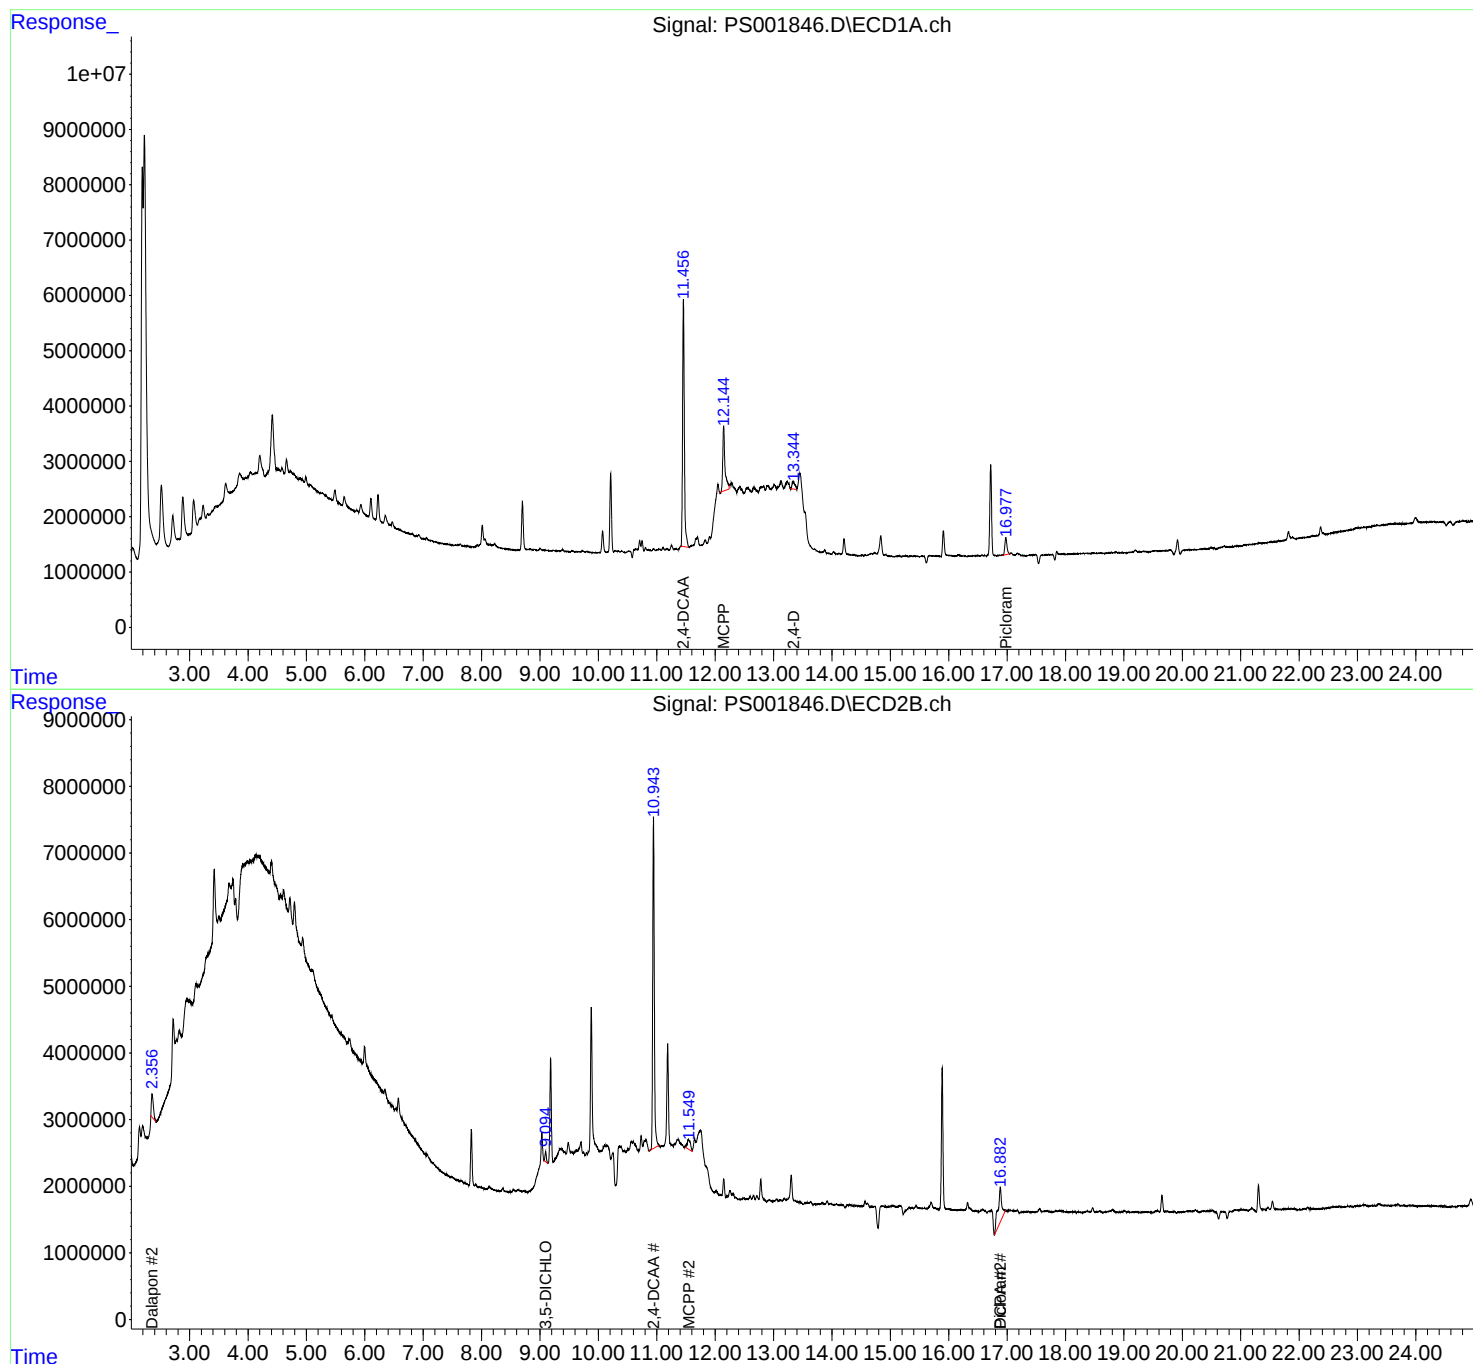


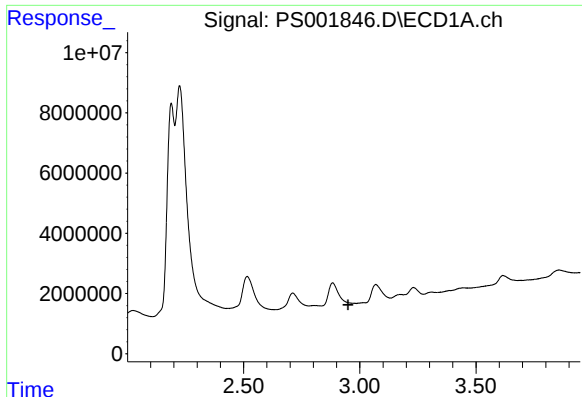

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

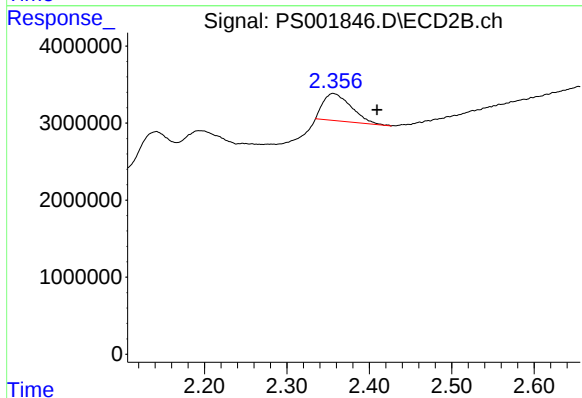


#1 Dalapon

R.T.: 2.356 min
Delta R.T.: -0.054 min
Response: 8319404
Conc: 28.16 ng/ml

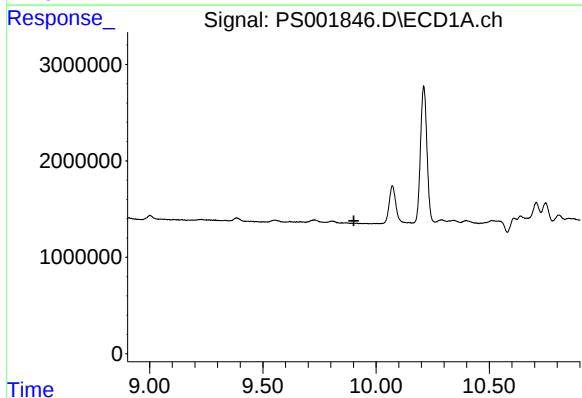


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.902 min
Response: 0
Conc: N.D.

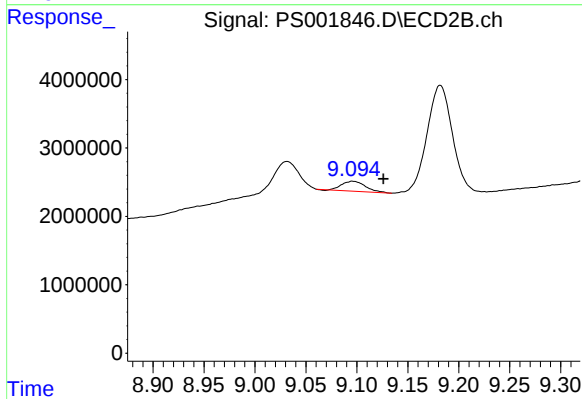

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.095 min
Delta R.T.: -0.031 min
Response: 2378229
Conc: 7.53 ng/ml

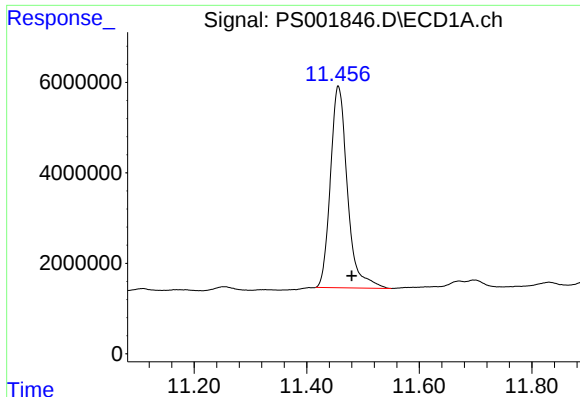

#4 2,4-DCAA


R.T.: 11.456 min
Delta R.T.: -0.023 min
Response: 93241120
Conc: 415.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

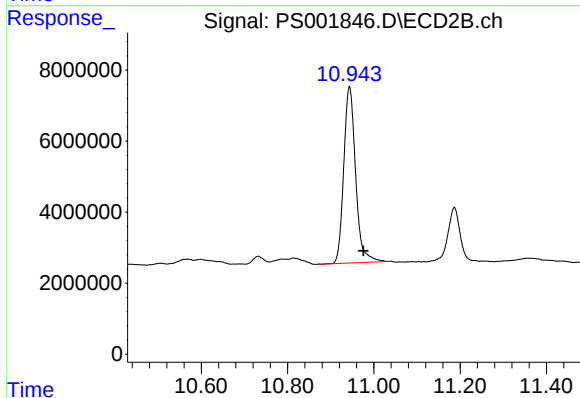


#4 2,4-DCAA

R.T.: 10.944 min
Delta R.T.: -0.032 min
Response: 94773785
Conc: 373.10 ng/ml

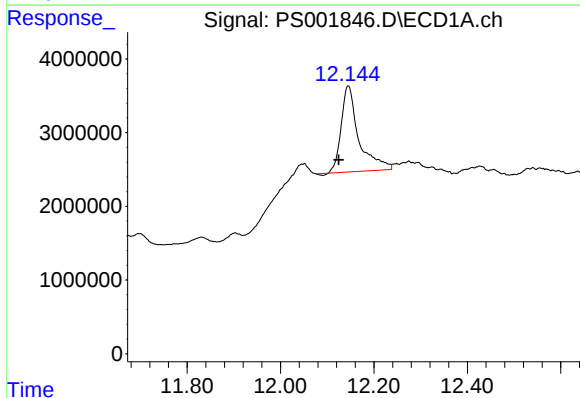


#6 MCPP

R.T.: 12.145 min
Delta R.T.: 0.020 min
Response: 30613064
Conc: 48.04 ug/ml

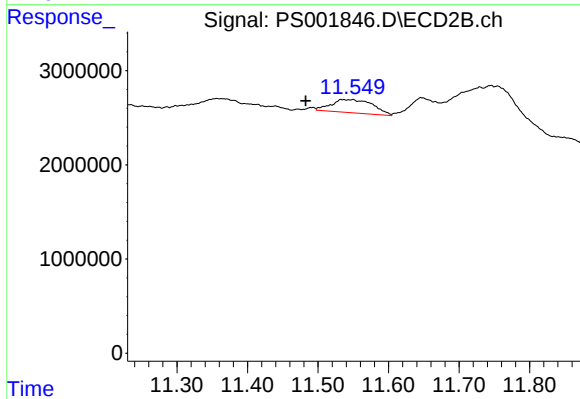

#6 MCPP


R.T.: 11.550 min
Delta R.T.: 0.067 min
Response: 5732274
Conc: 9.73 ug/ml

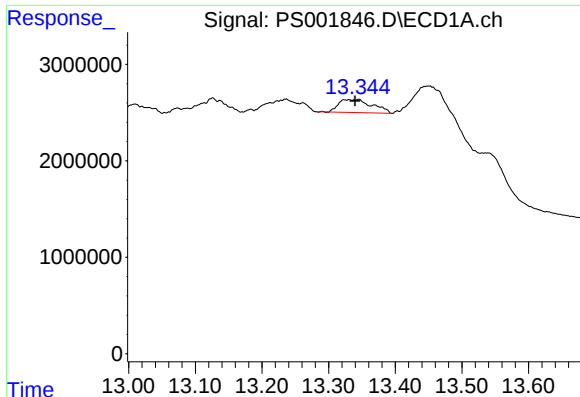

#9 2,4-D


R.T.: 13.344 min
Delta R.T.: 0.004 min
Response: 4719372
Conc: 17.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

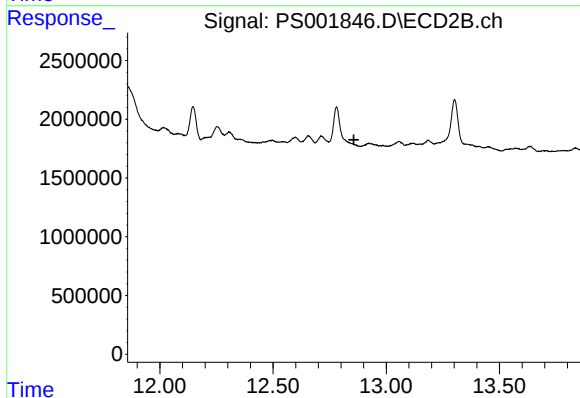


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.857 min
Response: 0
Conc: N.D.

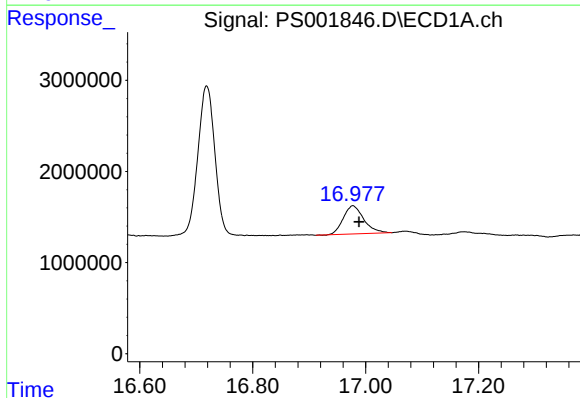


#15 Picloram

R.T.: 16.977 min
Delta R.T.: -0.011 min
Response: 7830989
Conc: 4.50 ng/ml

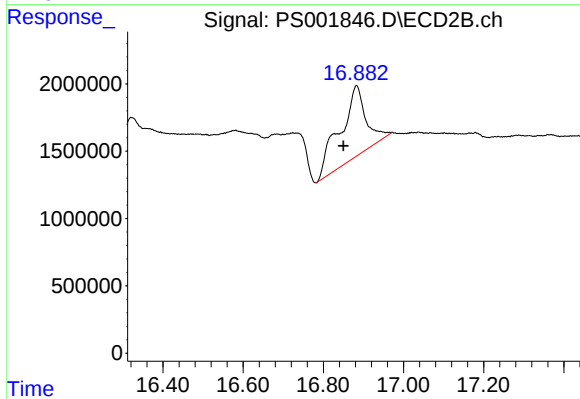

#15 Picloram


R.T.: 16.883 min
Delta R.T.: 0.033 min
Response: 24511756
Conc: 14.41 ng/ml

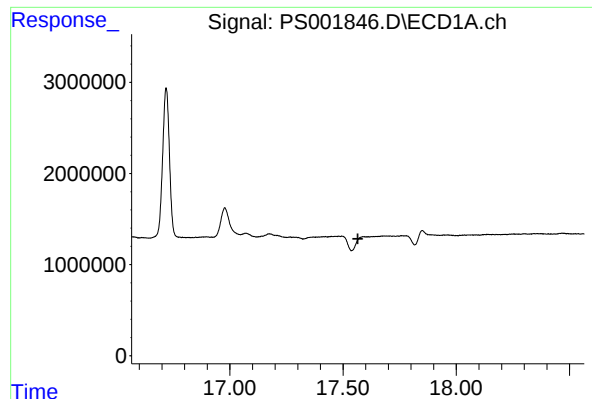

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

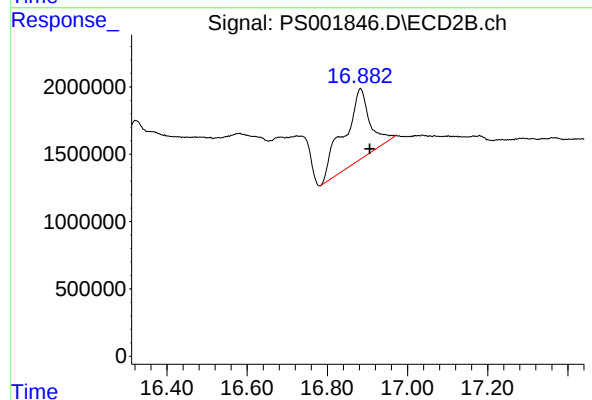

#16 DCPA

R.T.: 16.883 min
Delta R.T.: -0.023 min
Response: 24511756
Conc: 13.29 ng/ml