

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
 Data File : PS001847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2018 17:23
 Operator : EI\SJ
 Sample : J4777-36
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:51:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.441	10.934	84231824	127.1E6	375.506	500.412 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.091	0	2872793	N.D.	9.102 #
6) T	MCP	12.128	0.000	31559984	0	49.526	N.D. #
14) T	DINOSEB	0.000	15.687	0	2042279	N.D.	2.155 #
15) T	Picloram	16.951	16.868	3067547	12329962	1.762	7.250 #
16) T	DCPA	0.000	16.868	0	12329962	N.D.	6.685 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
Data File : PS001847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2018 17:23
Operator : EI\SJ
Sample : J4777-36
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:51:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

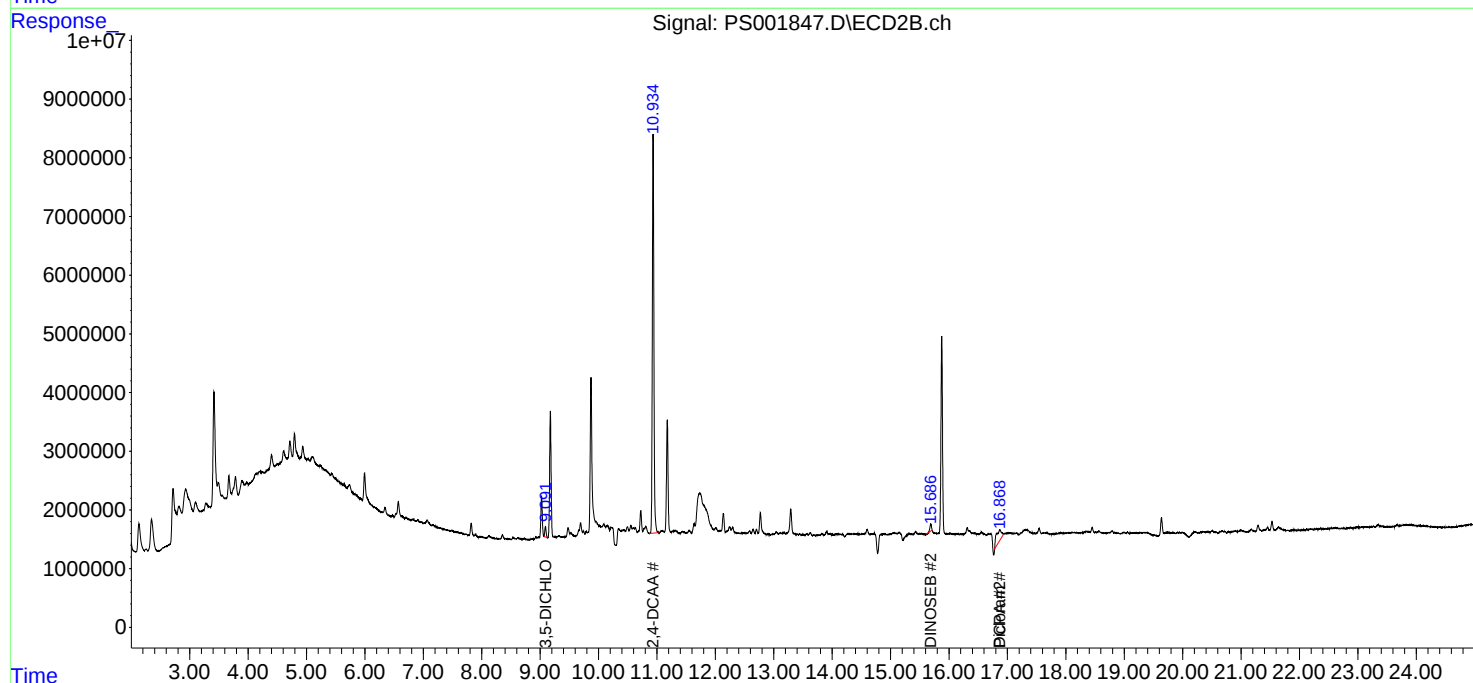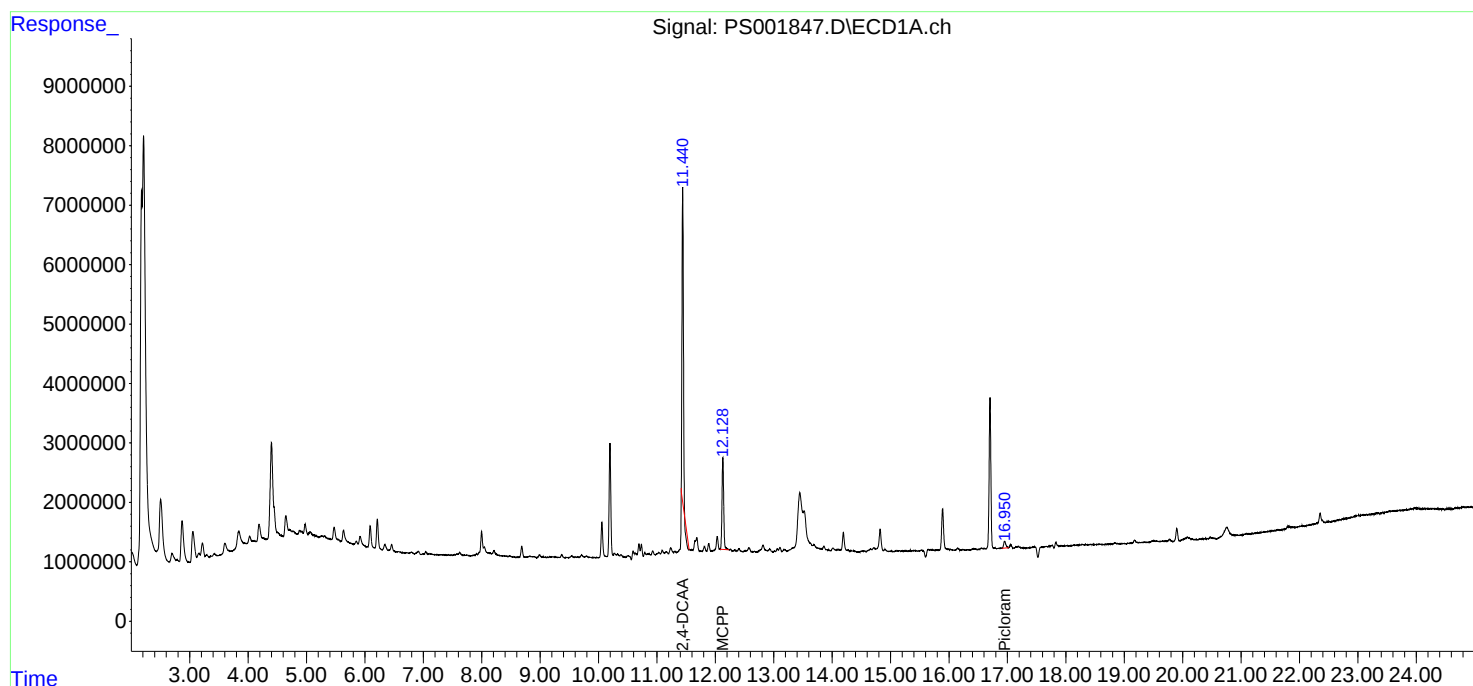


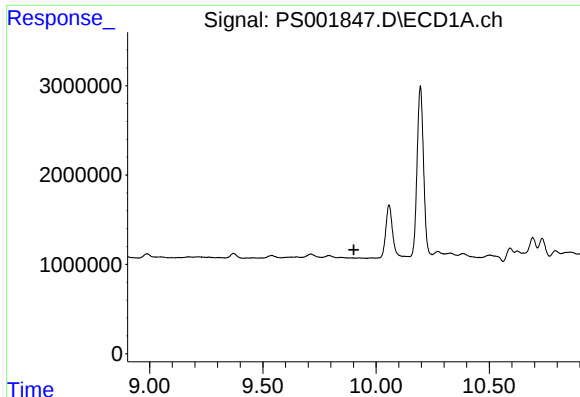

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.902 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

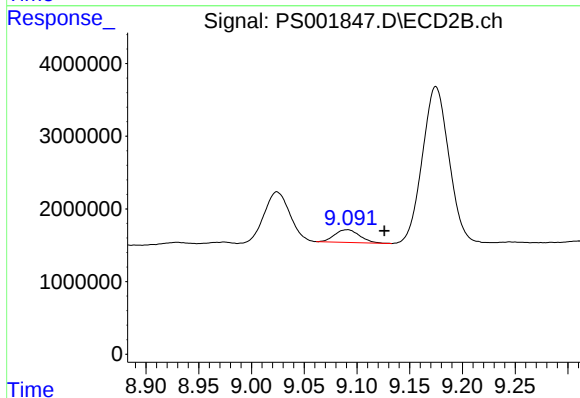


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.091 min
Delta R.T.: -0.035 min
Response: 2872793
Conc: 9.10 ng/ml

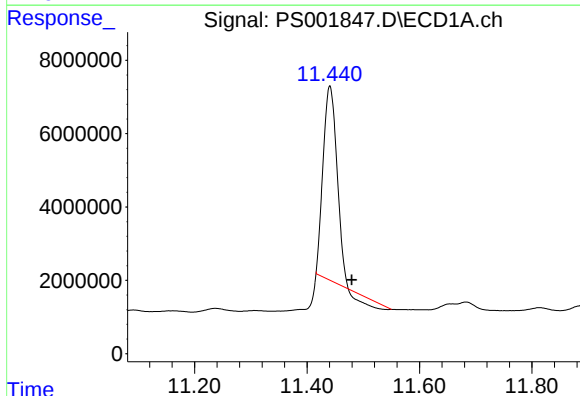


#4 2,4-DCAA

R.T.: 11.441 min
Delta R.T.: -0.039 min
Response: 84231824
Conc: 375.51 ng/ml

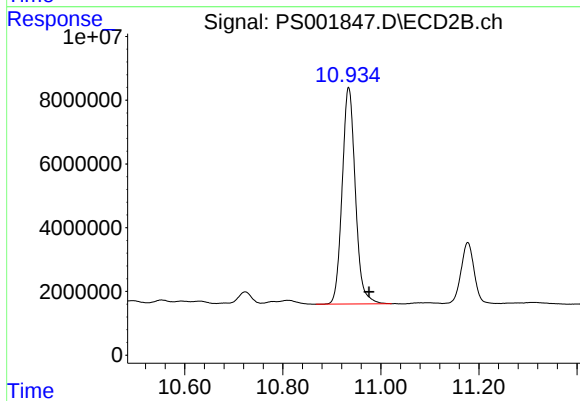

#4 2,4-DCAA


R.T.: 10.934 min
Delta R.T.: -0.042 min
Response: 127112982
Conc: 500.41 ng/ml

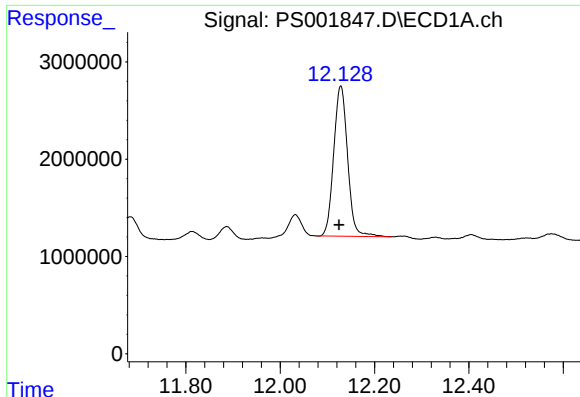

#6 MCP


R.T.: 12.128 min
Delta R.T.: 0.003 min
Response: 31559984
Conc: 49.53 ug/ml

Instrument :
ECD_S
ClientSampleId :

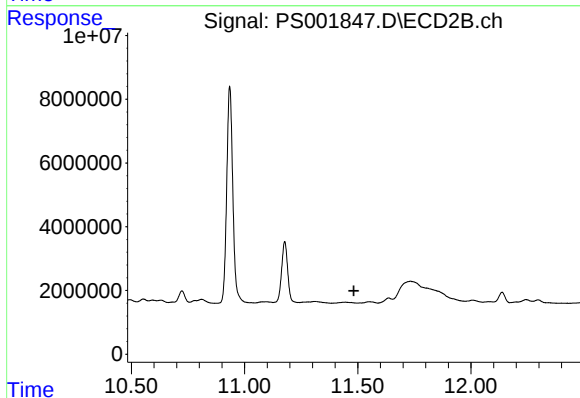


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

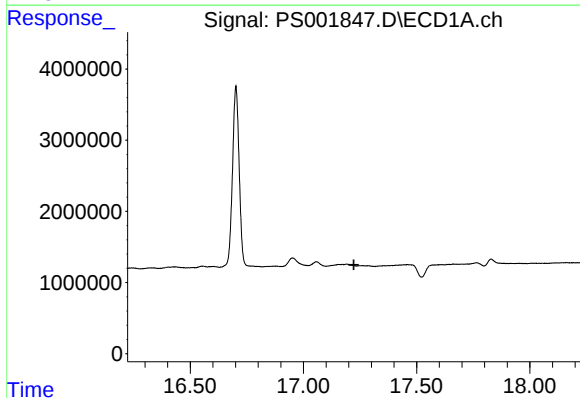


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.223 min
Response: 0
Conc: N.D.

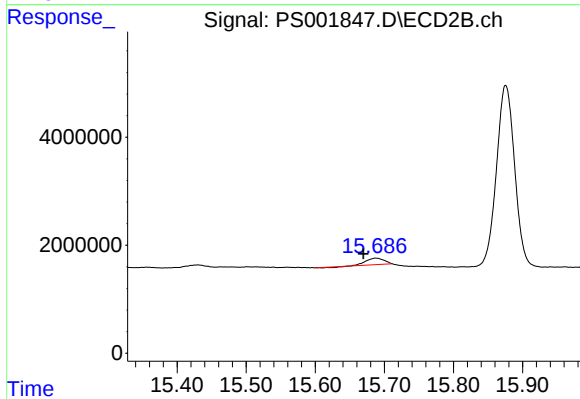

#14 DINOSEB


R.T.: 15.687 min
Delta R.T.: 0.017 min
Response: 2042279
Conc: 2.15 ng/ml

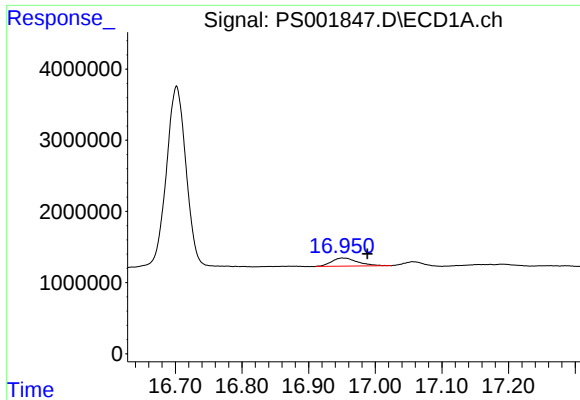

#15 Picloram


R.T.: 16.951 min
Delta R.T.: -0.037 min
Response: 3067547
Conc: 1.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

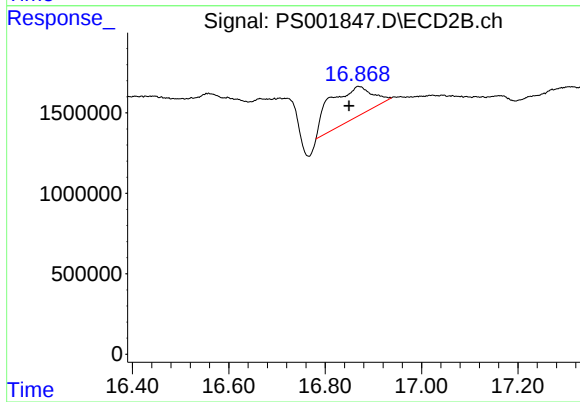


#15 Picloram

R.T.: 16.868 min
Delta R.T.: 0.018 min
Response: 12329962
Conc: 7.25 ng/ml

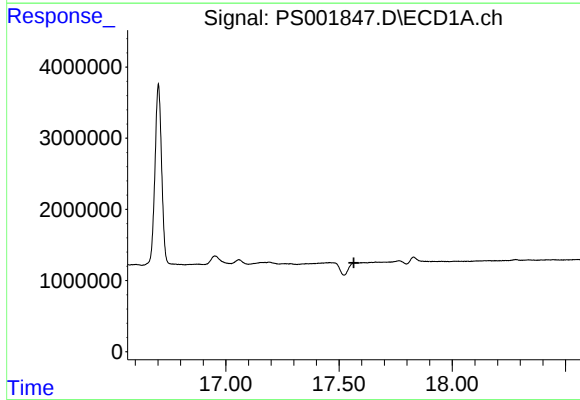

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.565 min
Response: 0
Conc: N.D.

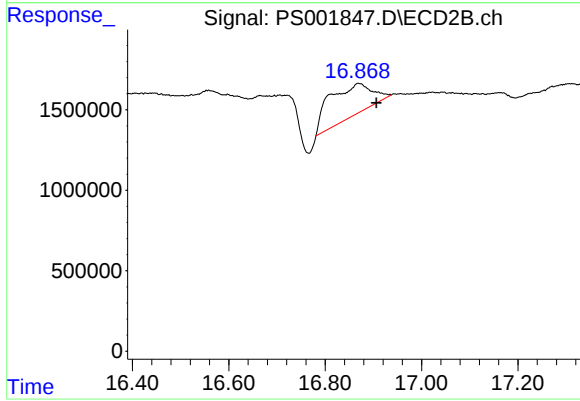

#16 DCPA

R.T.: 16.868 min
Delta R.T.: -0.038 min
Response: 12329962
Conc: 6.68 ng/ml