

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
 Data File : PS001848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2018 17:55
 Operator : EI\SJ
 Sample : J4777-38
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:51:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.474	10.970	113.6E6	116.2E6	506.610	457.603
Target Compounds							
1) T	Dalapon	2.904	2.382	22021917	21053880	67.725	71.268
2) T	3,5-DICHL...	0.000	9.125	0	750157	N.D.	2.377 #
5) T	DICAMBA	0.000	11.212	0	18469269	N.D.	20.708 #
6) T	MCP	12.161	0.000	24625463	0	38.644	N.D. #
9) T	2,4-D	0.000	12.805	0	555283	N.D.	1.785 #
15) T	Picloram	0.000	16.906	0	4017386	N.D.	2.362 #
16) T	DCPA	0.000	16.906	0	4017386	N.D.	2.178 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
Data File : PS001848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2018 17:55
Operator : EI\SJ
Sample : J4777-38
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:51:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

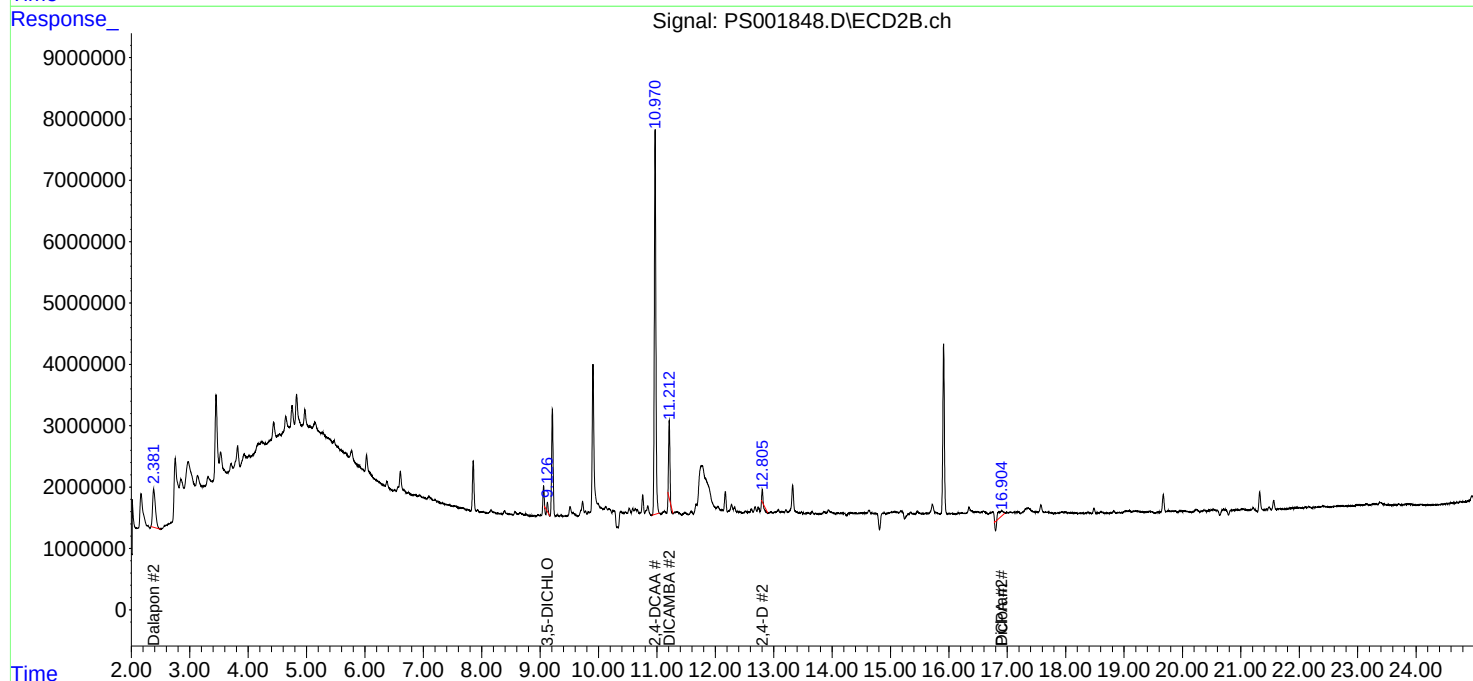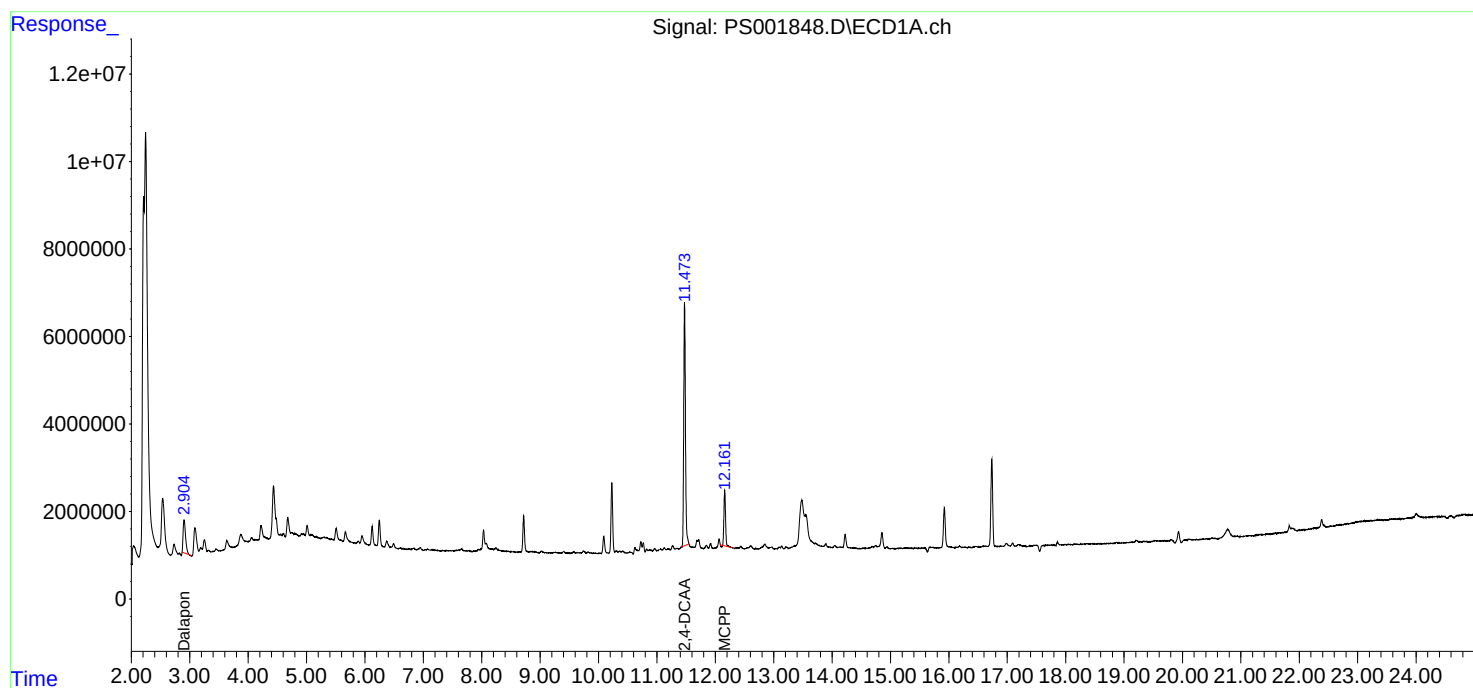


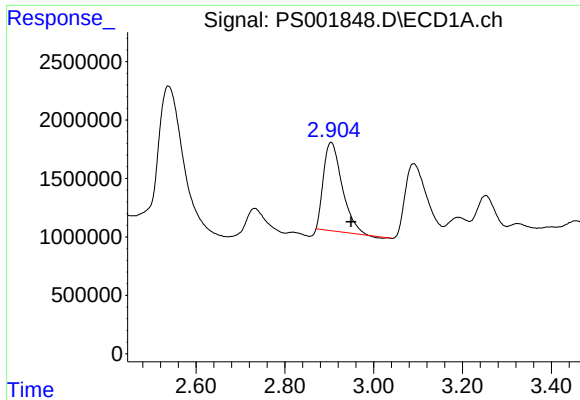

#1 Dalapon


R.T.: 2.904 min
Delta R.T.: -0.045 min
Response: 22021917
Conc: 67.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

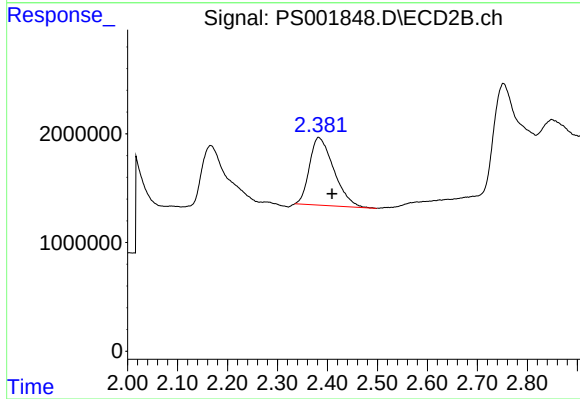


#1 Dalapon

R.T.: 2.382 min
Delta R.T.: -0.028 min
Response: 21053880
Conc: 71.27 ng/ml

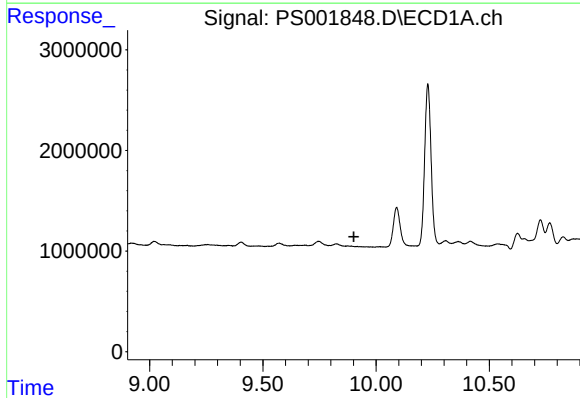


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.902 min
Response: 0
Conc: N.D.

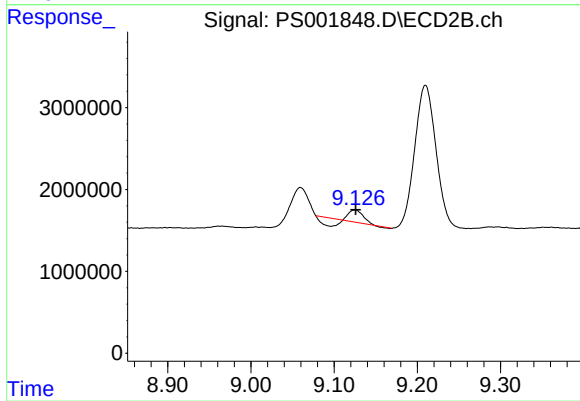

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 750157
Conc: 2.38 ng/ml

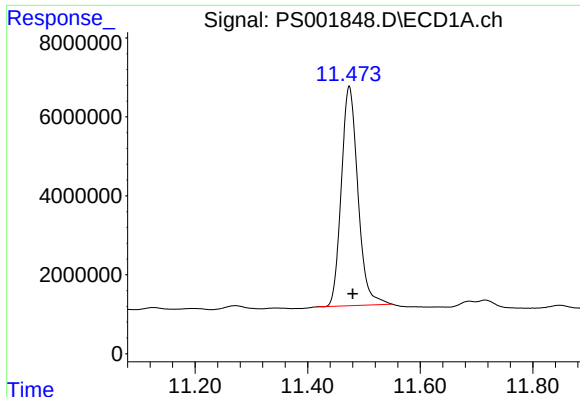

#4 2,4-DCAA


R.T.: 11.474 min
Delta R.T.: -0.006 min
Response: 113640578
Conc: 506.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

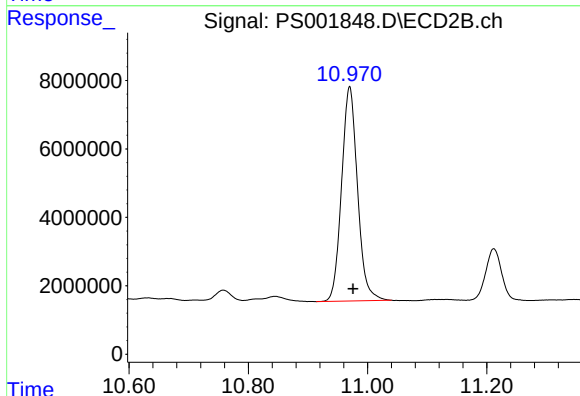


#4 2,4-DCAA

R.T.: 10.970 min
Delta R.T.: -0.006 min
Response: 116238795
Conc: 457.60 ng/ml

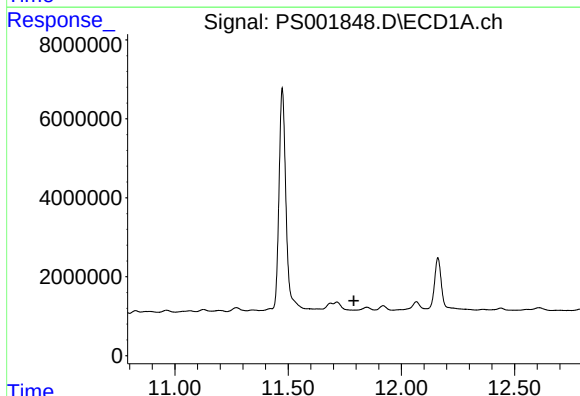


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.790 min
Response: 0
Conc: N.D.

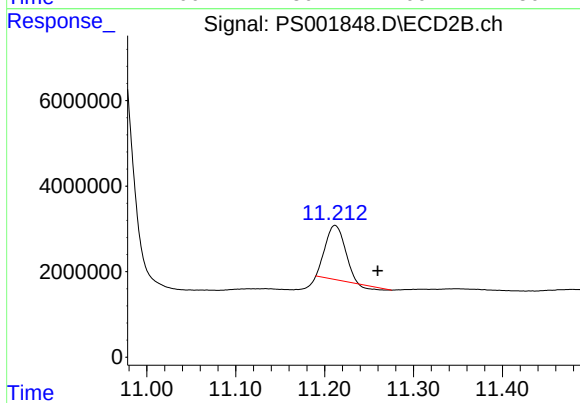

#5 DICAMBA


R.T.: 11.212 min
Delta R.T.: -0.048 min
Response: 18469269
Conc: 20.71 ng/ml

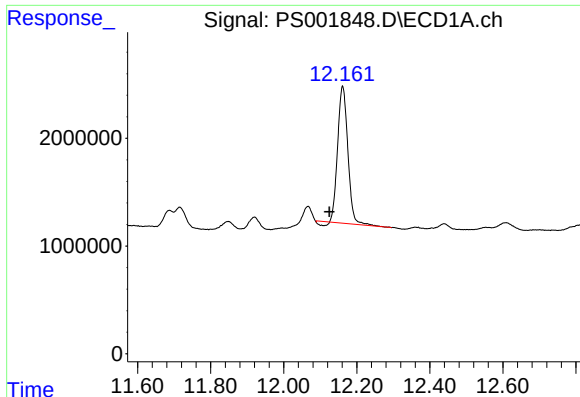

#6 MCP


R.T.: 12.161 min
Delta R.T.: 0.036 min
Response: 24625463
Conc: 38.64 ug/ml

Instrument :
ECD_S
ClientSampleId :

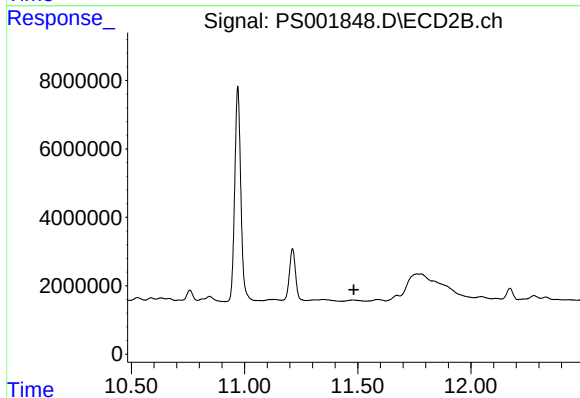


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

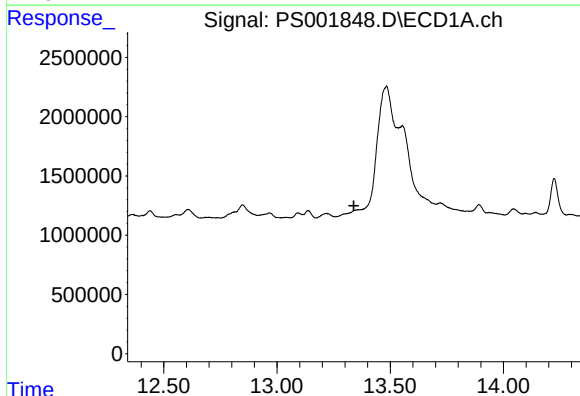


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.340 min
Response: 0
Conc: N.D.

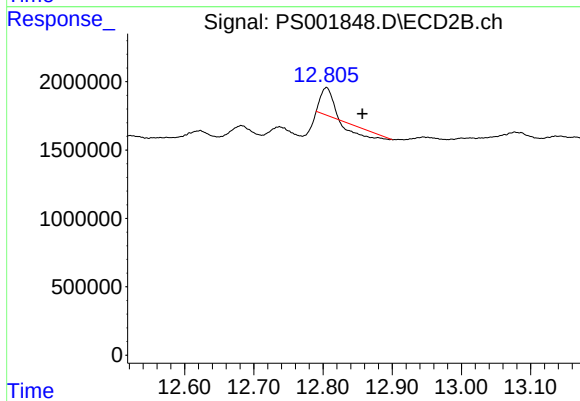

#9 2,4-D


R.T.: 12.805 min
Delta R.T.: -0.052 min
Response: 555283
Conc: 1.78 ng/ml

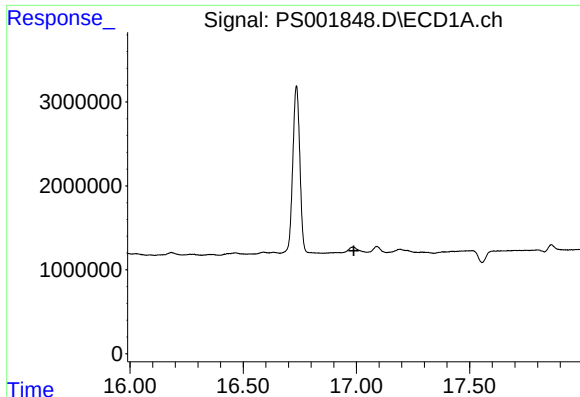

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

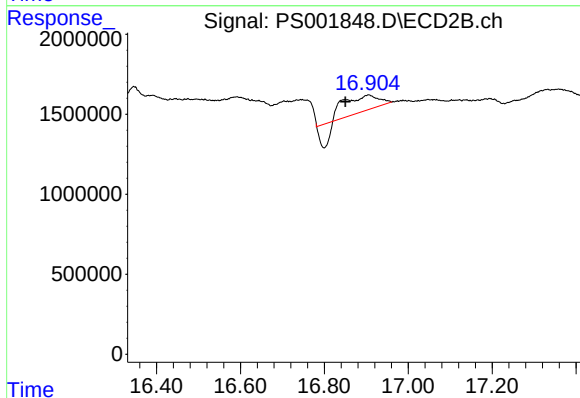


#15 Picloram

R.T.: 16.906 min
Delta R.T.: 0.056 min
Response: 4017386
Conc: 2.36 ng/ml

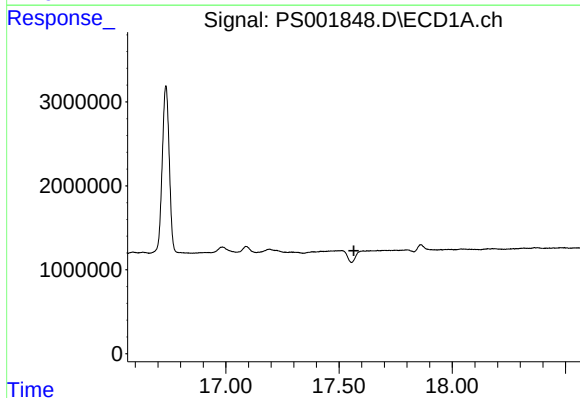

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.565 min
Response: 0
Conc: N.D.

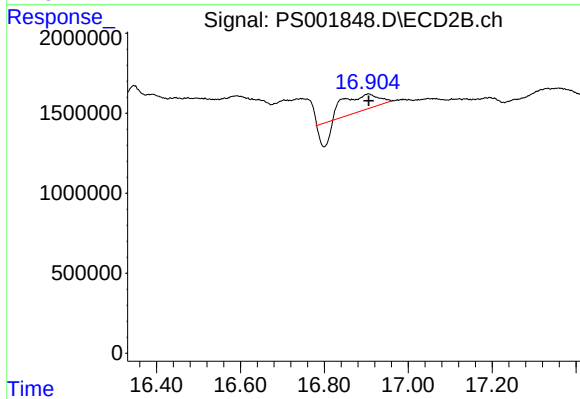

#16 DCPA

R.T.: 16.906 min
Delta R.T.: 0.000 min
Response: 4017386
Conc: 2.18 ng/ml