

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
 Data File : PS001849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2018 18:26
 Operator : EI\SJ
 Sample : J4777-40
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:51:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.474	10.971	106.4E6	108.3E6	474.207	426.506
Target Compounds							
1) T	Dalapon	2.905	2.384	24103785	21061236	74.127	71.293
5) T	DICAMBA	0.000	11.213	0	18888664	N.D.	21.178 #
6) T	MCPD	12.161	0.000	17281258	0	27.119	N.D. #
9) T	2,4-D	0.000	12.806	0	744722	N.D.	2.394 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
Data File : PS001849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2018 18:26
Operator : EI\SJ
Sample : J4777-40
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :




Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:51:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

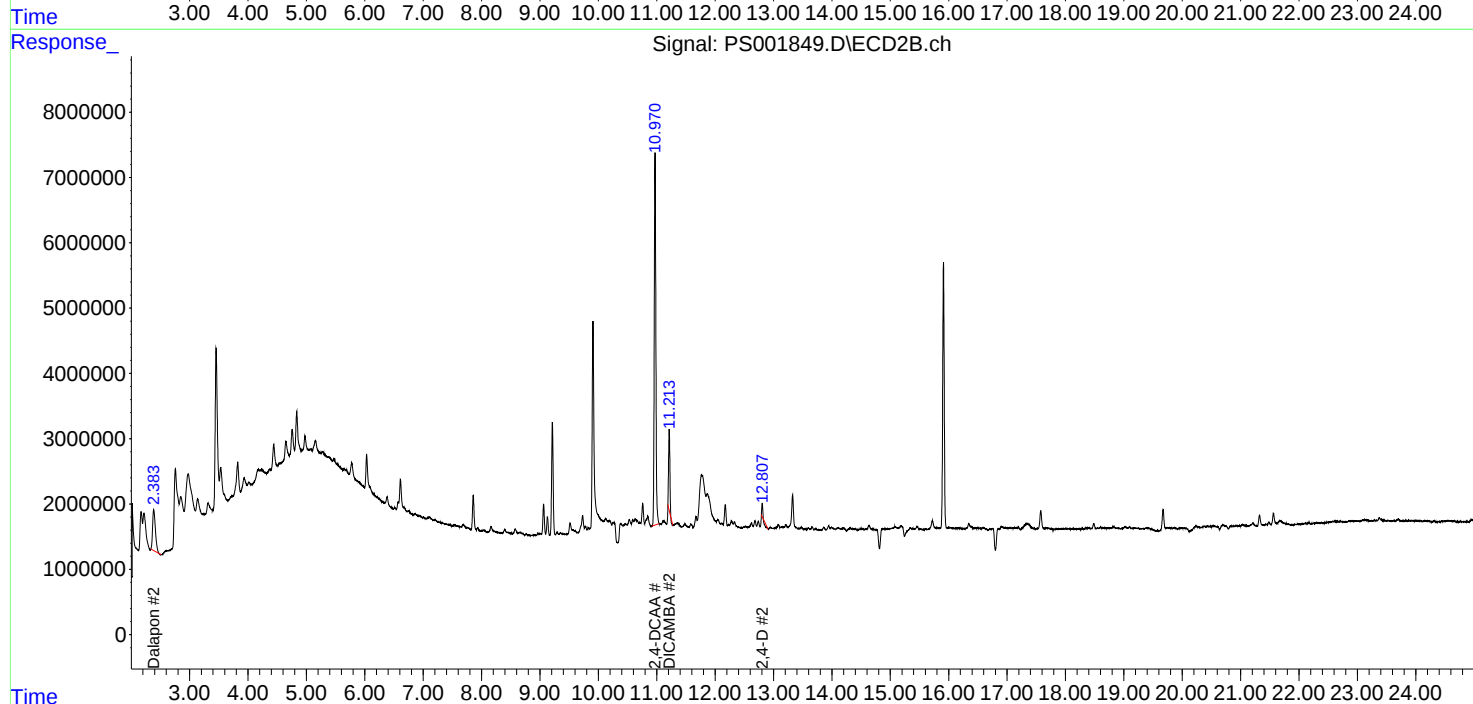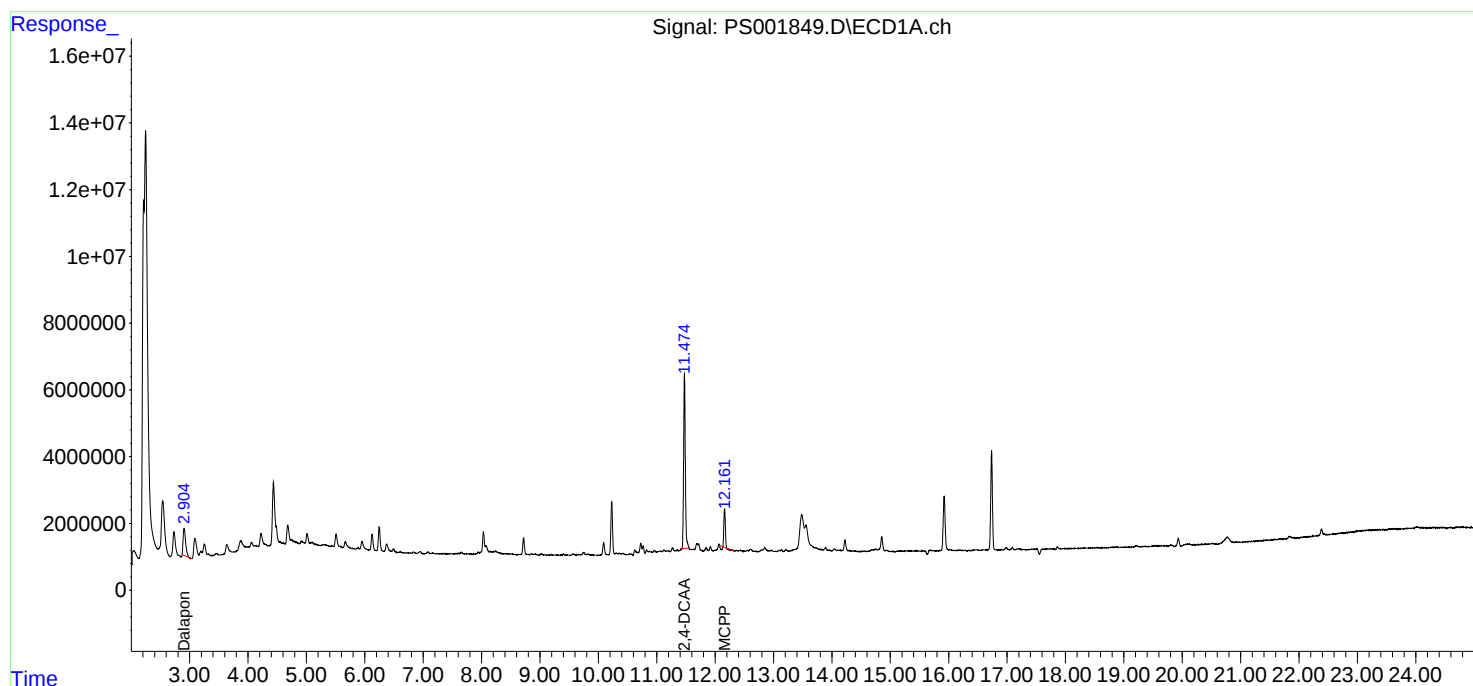

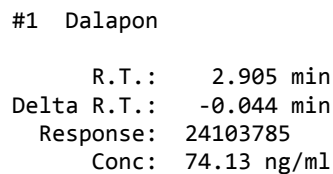

Instrument :
ECD_S
ClientSampleId :

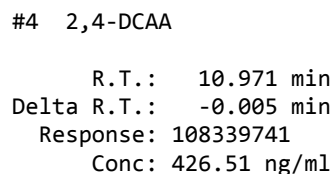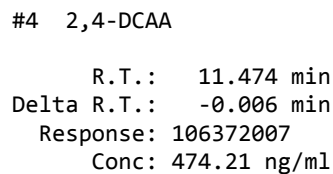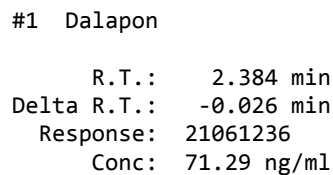


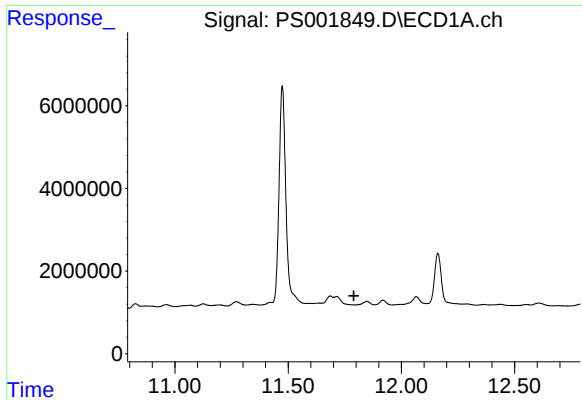

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

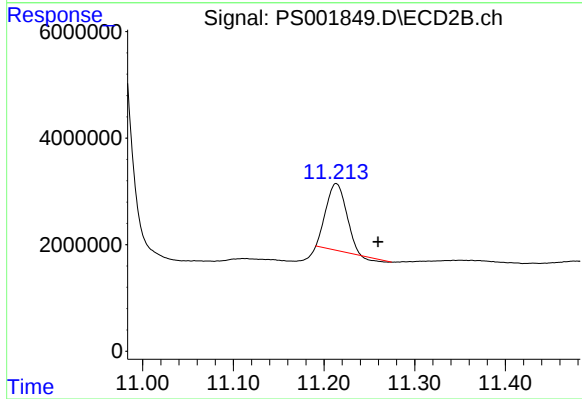


#5 DICAMBA

R.T.: 11.213 min
Delta R.T.: -0.046 min
Response: 18888664
Conc: 21.18 ng/ml

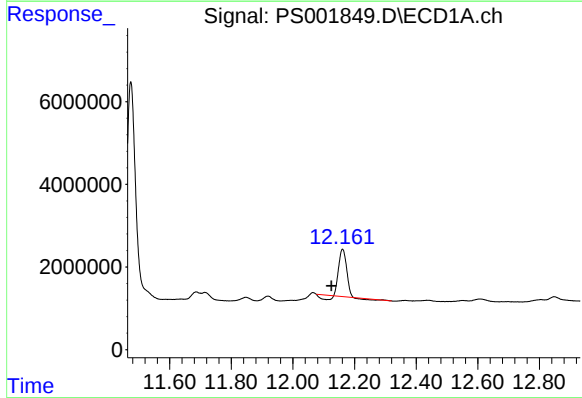


#6 MCP

R.T.: 12.161 min
Delta R.T.: 0.036 min
Response: 17281258
Conc: 27.12 ug/ml

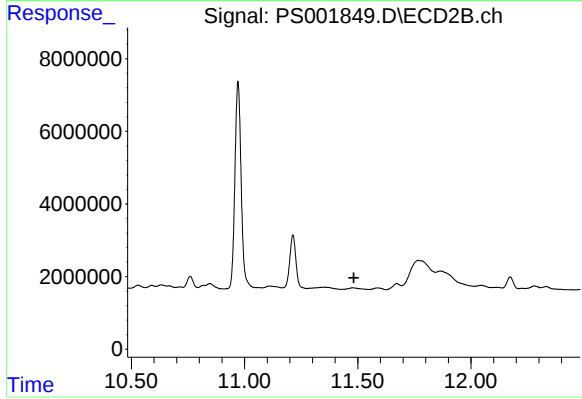

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.483 min
Response: 0
Conc: N.D.

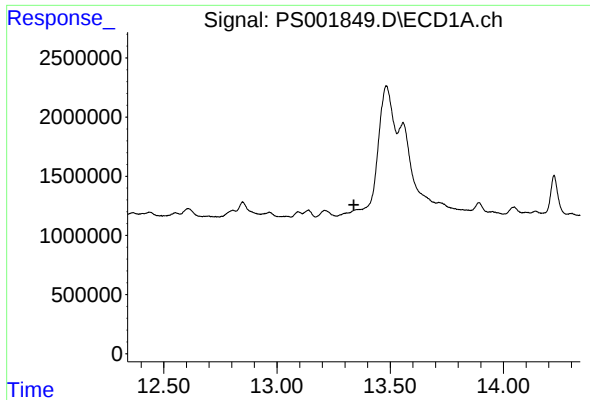

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

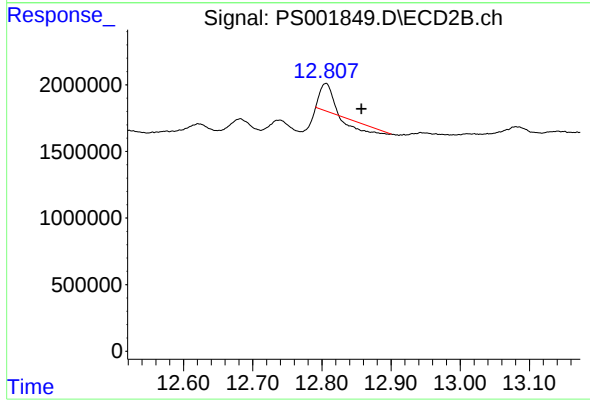

#9 2,4-D

R.T.: 12.806 min
Delta R.T.: -0.051 min
Response: 744722
Conc: 2.39 ng/ml