

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
 Data File : PS001855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2018 21:33
 Operator : EI\SJ
 Sample : J5170-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:53:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.435	10.932	29058541	106.4E6	129.543	419.016 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.088	0	1800520	N.D.	5.704 #
6) T	MCP	12.122	0.000	25443790	0	39.928	N.D. #
15) T	Picloram	0.000	16.864	0	4691728	N.D.	2.759 #
16) T	DCPA	0.000	16.864	0	4691728	N.D.	2.544 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
Data File : PS001855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2018 21:33
Operator : EI\SJ
Sample : J5170-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:53:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

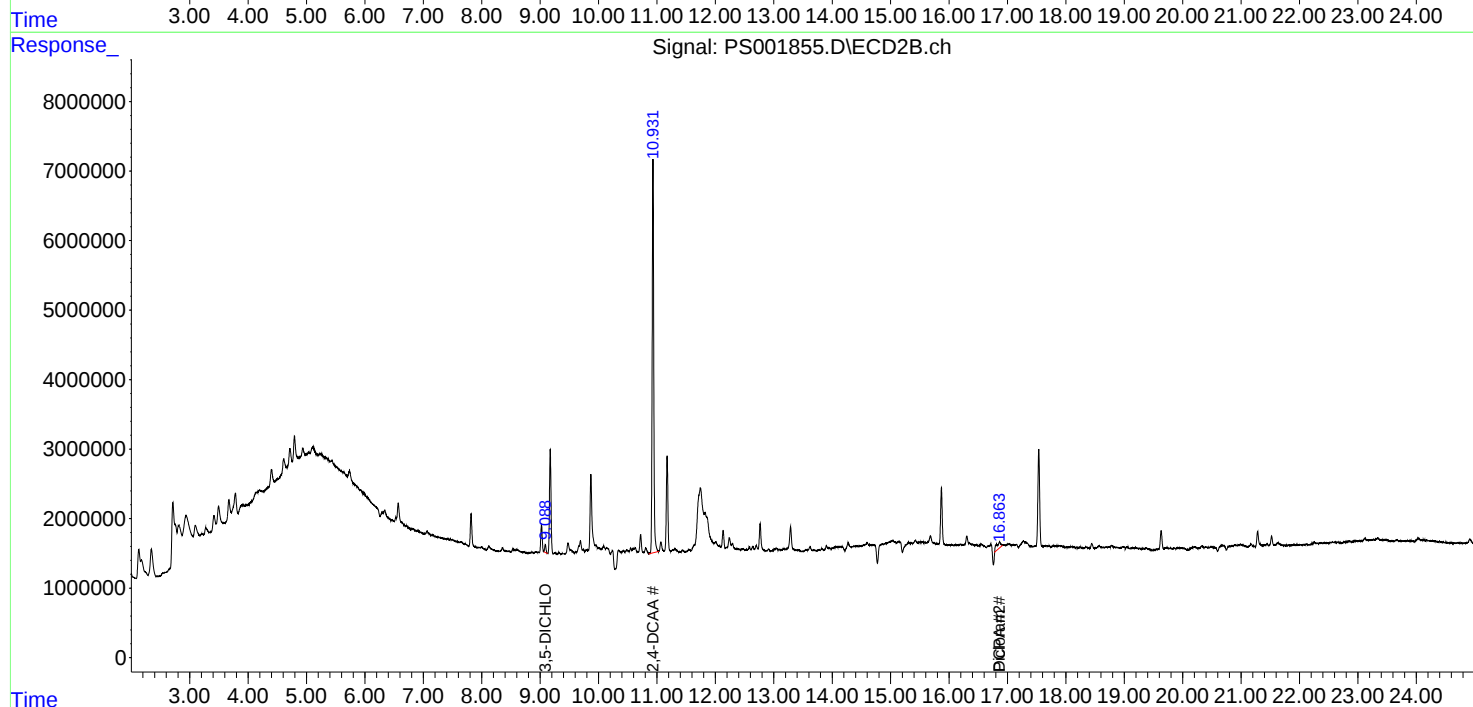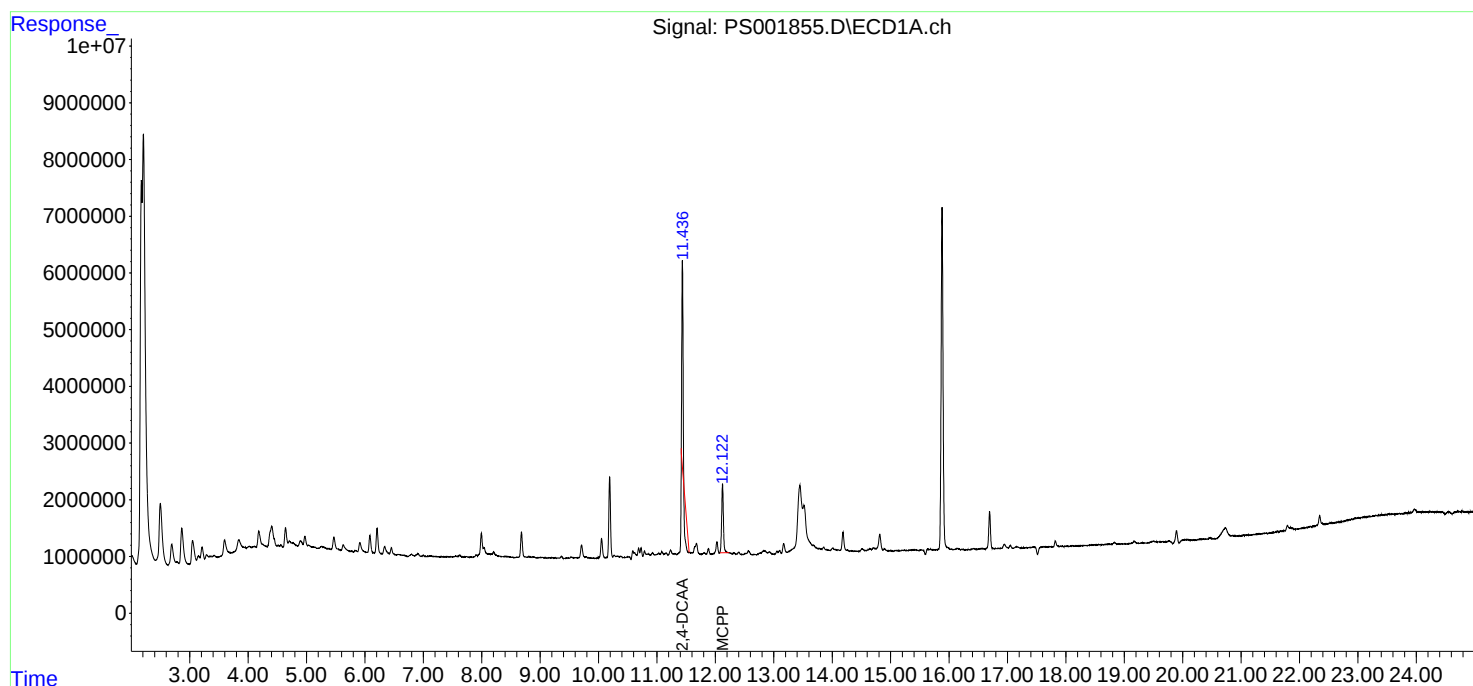


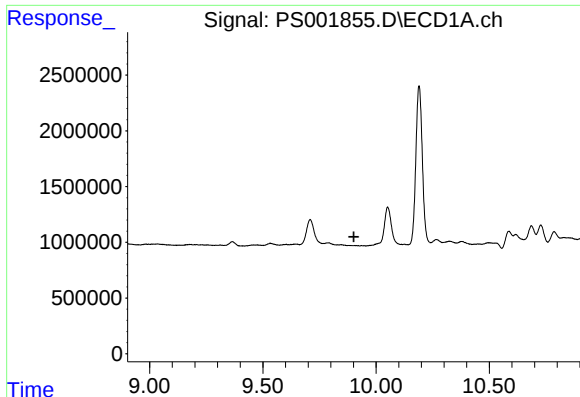

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.902 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

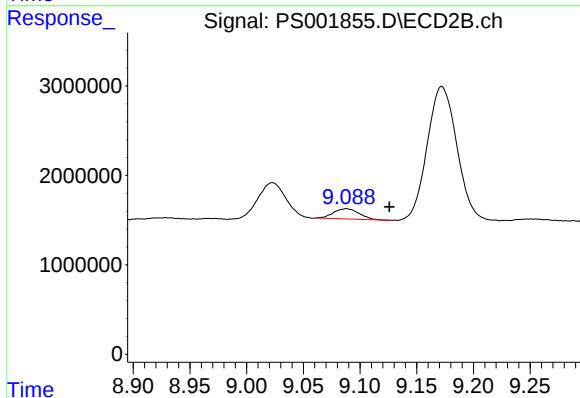


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.088 min
Delta R.T.: -0.038 min
Response: 1800520
Conc: 5.70 ng/ml

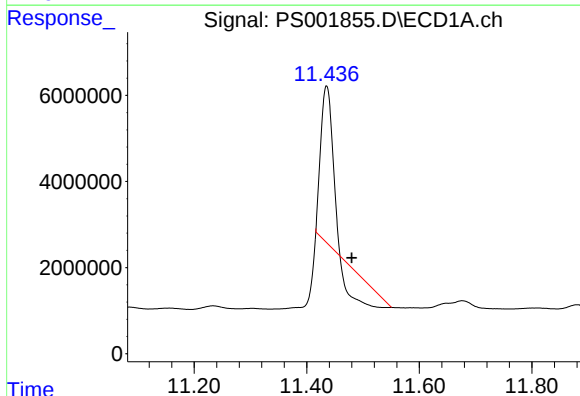


#4 2,4-DCAA

R.T.: 11.435 min
Delta R.T.: -0.044 min
Response: 29058541
Conc: 129.54 ng/ml

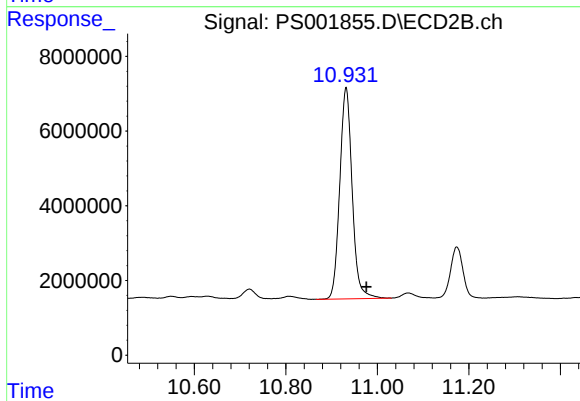

#4 2,4-DCAA


R.T.: 10.932 min
Delta R.T.: -0.044 min
Response: 106437135
Conc: 419.02 ng/ml

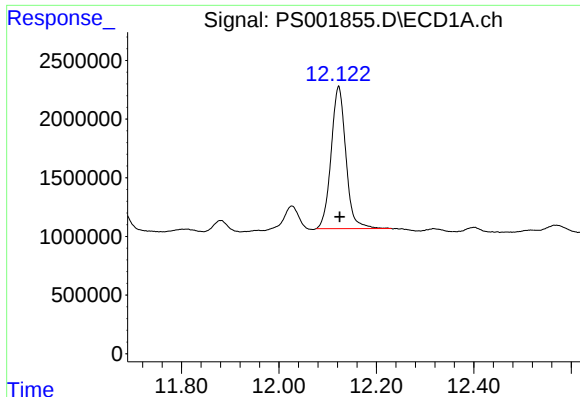

#6 MCP


R.T.: 12.122 min
Delta R.T.: -0.003 min
Response: 25443790
Conc: 39.93 ug/ml

Instrument :
ECD_S
ClientSampleId :

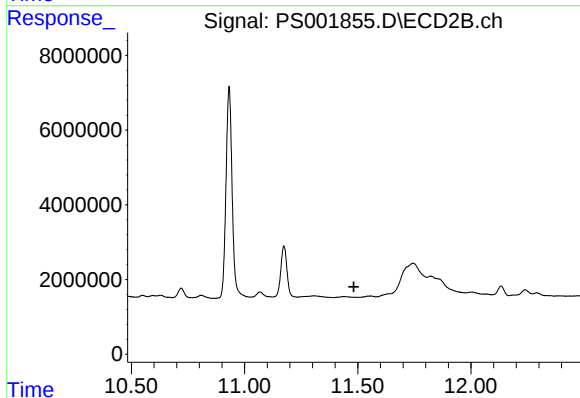


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

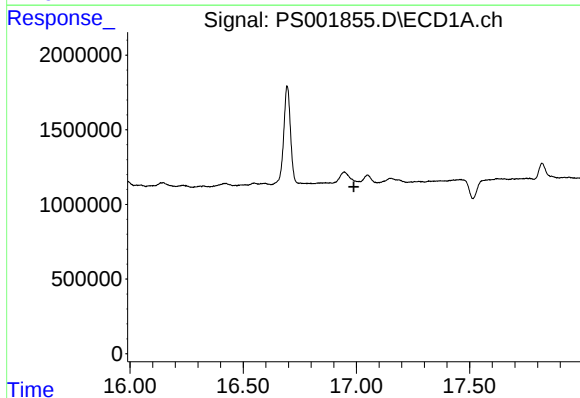


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.988 min
Response: 0
Conc: N.D.

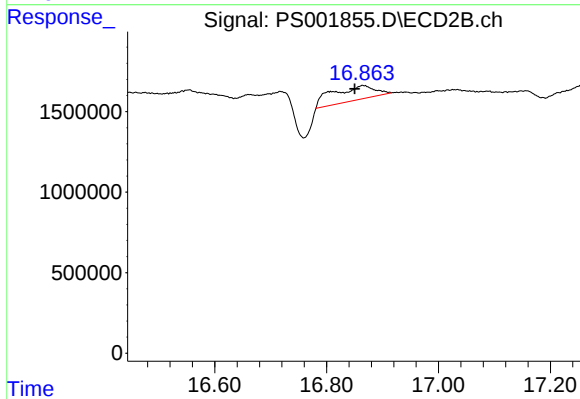

#15 Picloram


R.T.: 16.864 min
Delta R.T.: 0.014 min
Response: 4691728
Conc: 2.76 ng/ml

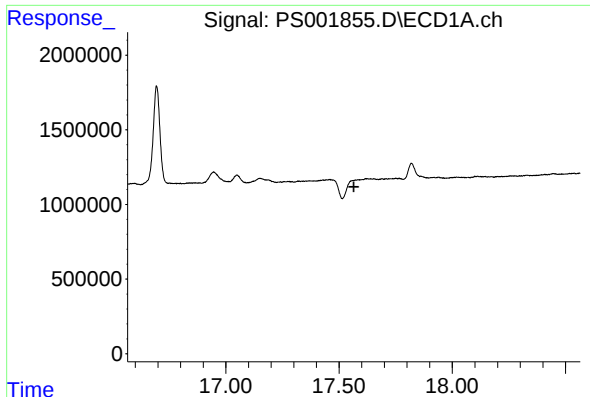

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

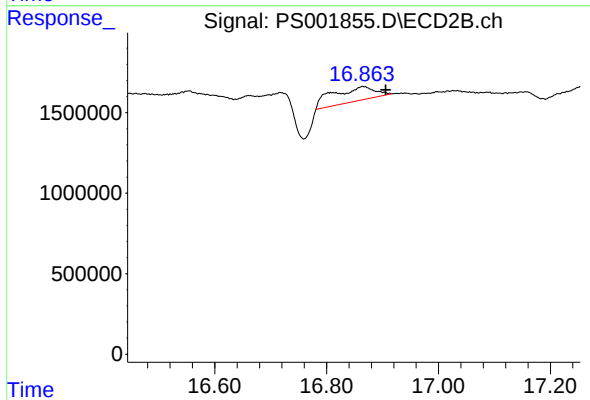

#16 DCPA

R.T.: 16.864 min
Delta R.T.: -0.042 min
Response: 4691728
Conc: 2.54 ng/ml