

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
 Data File : PS001861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 00:39
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:55:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.474	10.971	157.9E6	170.0E6	703.819	669.073
Target Compounds							
1) T	Dalapon	2.948	2.410	204.7E6	186.2E6	629.637	630.301
2) T	3,5-DICHL...	9.897	9.121	216.6E6	212.0E6	658.145	671.567
3) T	4-Nitroph...	11.064	10.116	97282613	87994927	691.170	701.723
5) T	DICAMBA	11.785	11.256	554.1E6	585.4E6	639.288	656.397
6) T	MCPD	12.126	11.483	44599643	43160659	69.989	73.246
7) T	MCPA	12.376	11.860	73587318	59764064	70.118	68.947
8) T	DICHLORPROP	12.975	12.380	143.7E6	148.0E6	619.399	637.059
9) T	2,4-D	13.333	12.851	185.2E6	201.0E6	672.071	646.140
10) T	Pentachlo...	13.714	13.401	2104.0E6	2387.4E6	684.608	696.555
11) T	2,4,5-TP ...	14.585	14.018	816.4E6	967.3E6	690.032	705.445
12) T	2,4,5-T	14.983	14.585	820.5E6	767.0E6	687.308	694.537
13) T	2,4-DB	15.731	15.235	109.4E6	114.6E6	671.579	692.356
14) T	DINOSEB	17.219	15.664	570.3E6	660.1E6	684.135	696.422
15) T	Picloram	16.981	16.844	1190.1E6	1176.8E6	683.515	691.963
16) T	DCPA	17.560	16.899	1020.0E6	1276.7E6	693.166	692.193



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100118\
Data File : PS001861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 00:39
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:55:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

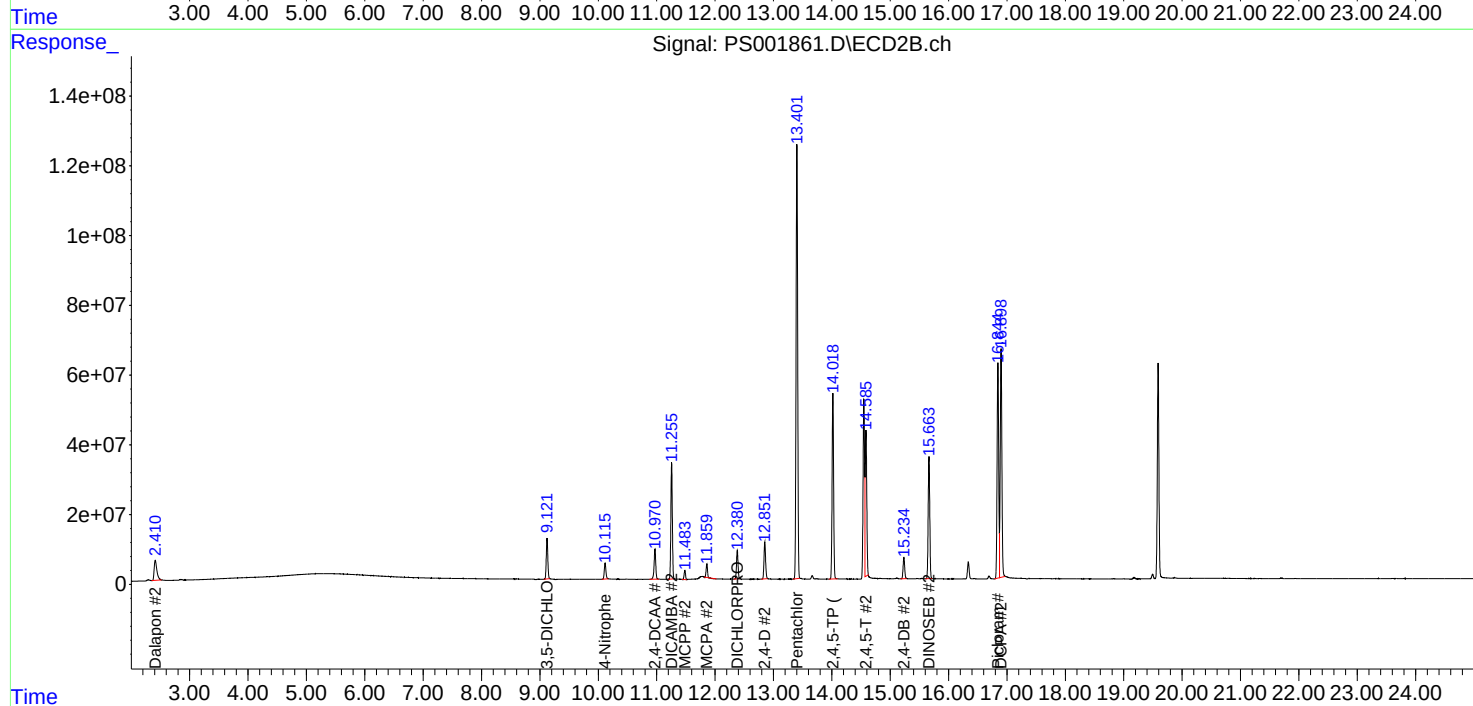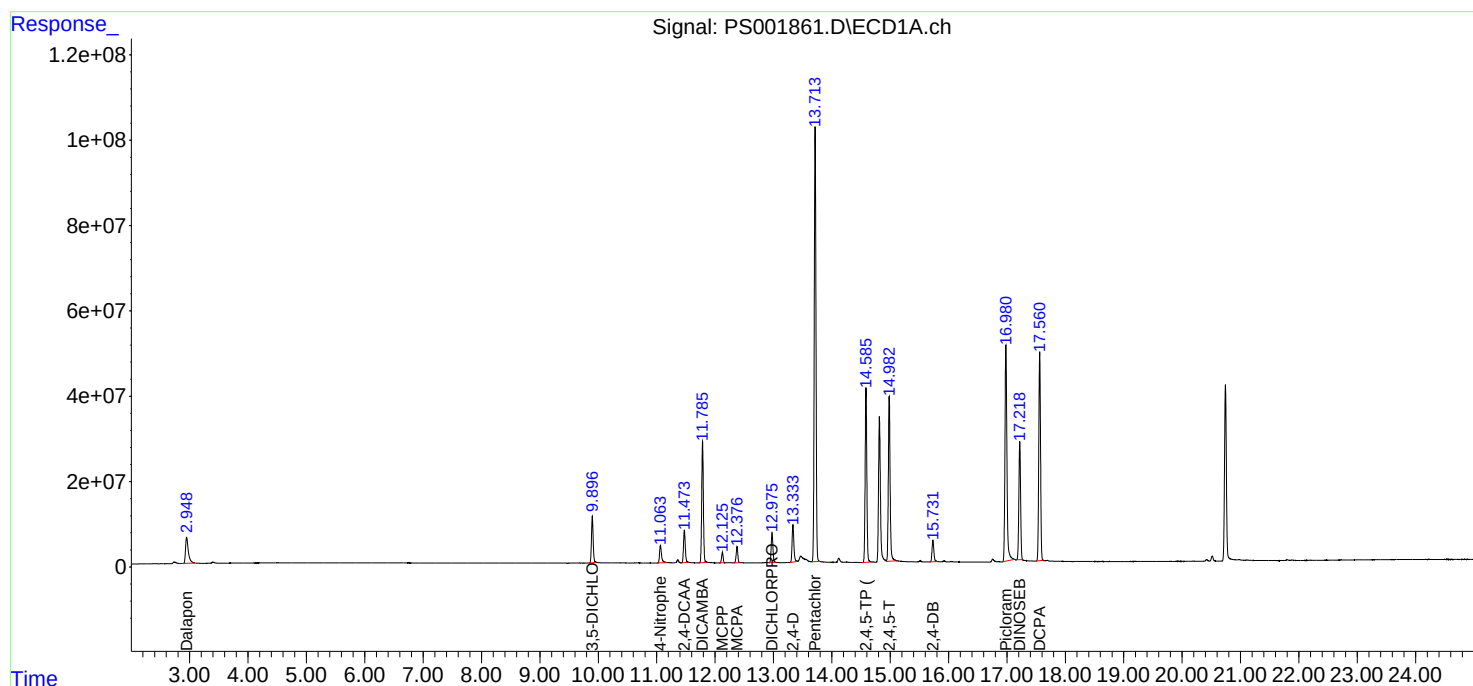


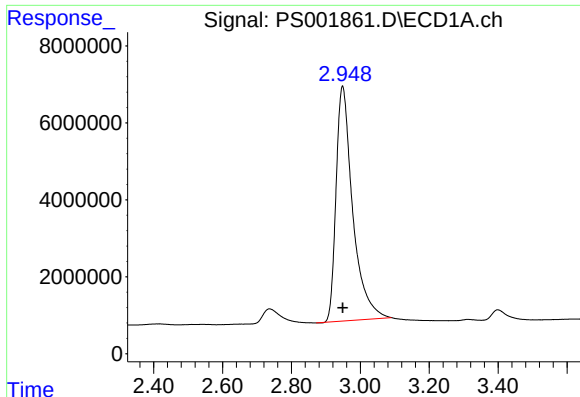

#1 Dalapon


R.T.: 2.948 min
Delta R.T.: 0.000 min
Response: 204737523
Conc: 629.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

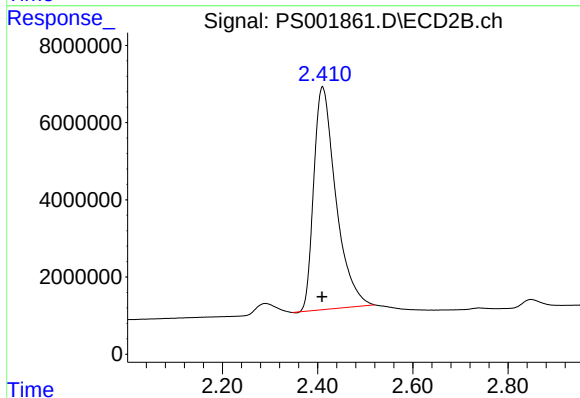


#1 Dalapon

R.T.: 2.410 min
Delta R.T.: 0.000 min
Response: 186201616
Conc: 630.30 ng/ml

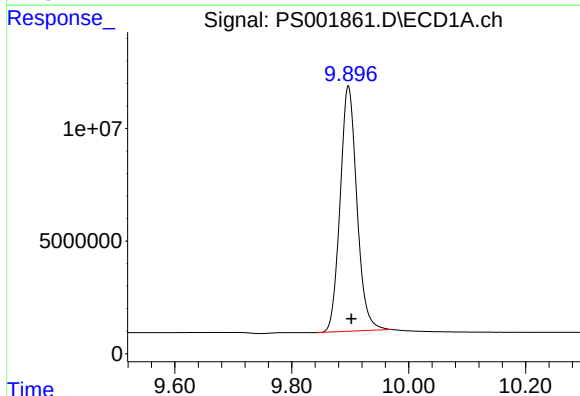


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.897 min
Delta R.T.: -0.005 min
Response: 216617231
Conc: 658.15 ng/ml

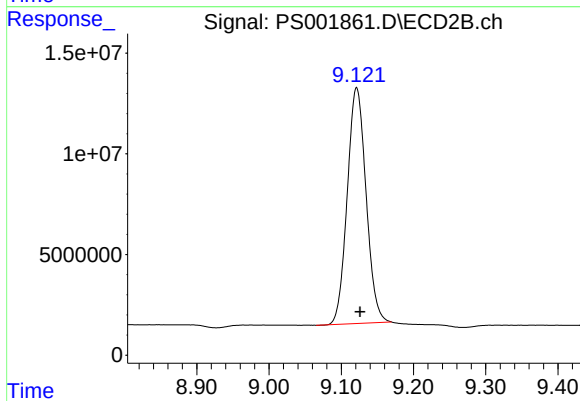

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 211968726
Conc: 671.57 ng/ml

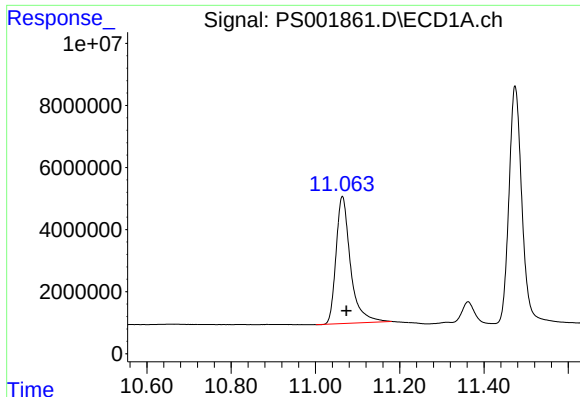

#3 4-Nitrophenol


R.T.: 11.064 min
Delta R.T.: -0.010 min
Response: 97282613
Conc: 691.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

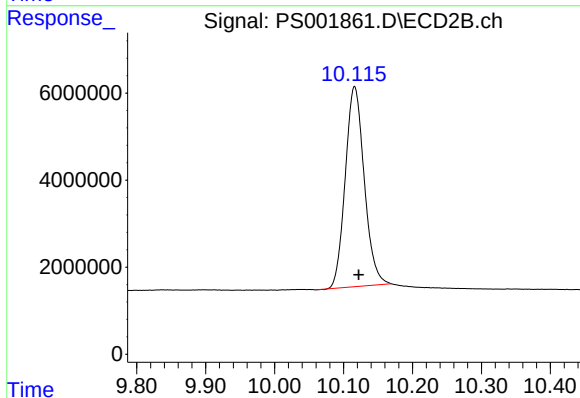


#3 4-Nitrophenol

R.T.: 10.116 min
Delta R.T.: -0.006 min
Response: 87994927
Conc: 701.72 ng/ml

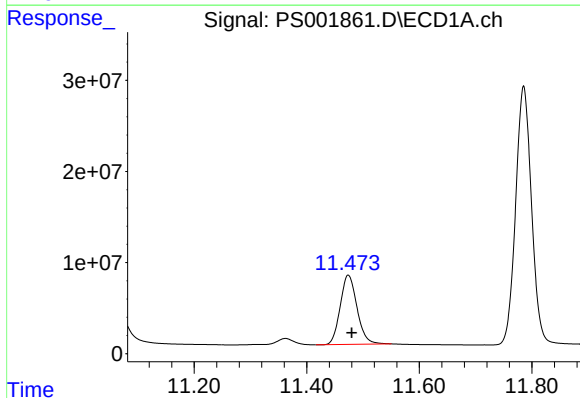


#4 2,4-DCAA

R.T.: 11.474 min
Delta R.T.: -0.006 min
Response: 157877596
Conc: 703.82 ng/ml

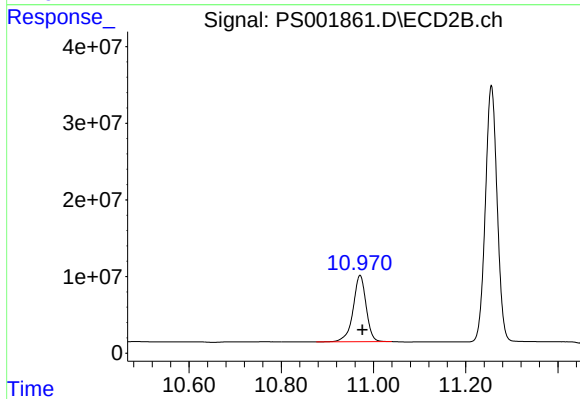

#4 2,4-DCAA


R.T.: 10.971 min
Delta R.T.: -0.005 min
Response: 169955821
Conc: 669.07 ng/ml

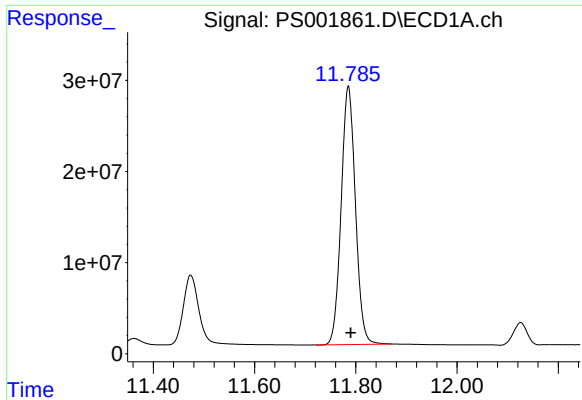

#5 DICAMBA


R.T.: 11.785 min
Delta R.T.: -0.005 min
Response: 554079315
Conc: 639.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

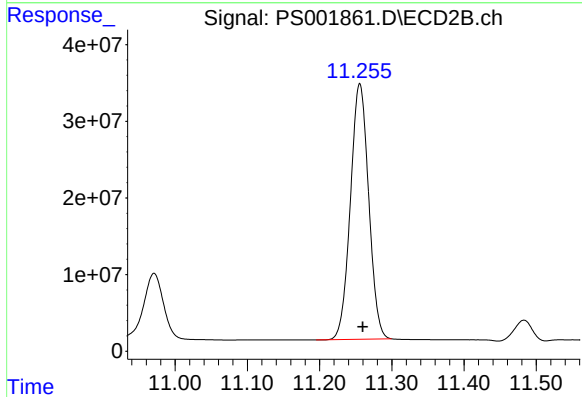


#5 DICAMBA

R.T.: 11.256 min
Delta R.T.: -0.004 min
Response: 585428205
Conc: 656.40 ng/ml

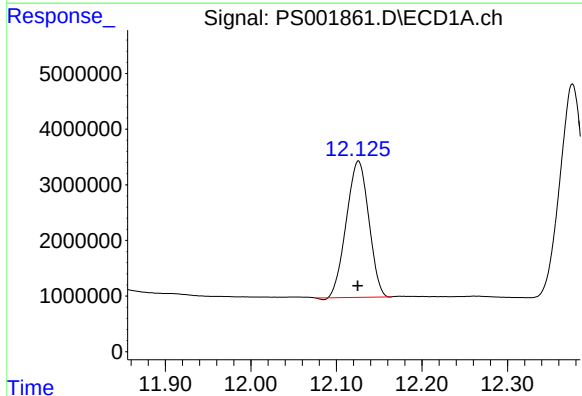


#6 MCP

R.T.: 12.126 min
Delta R.T.: 0.000 min
Response: 44599643
Conc: 69.99 ug/ml

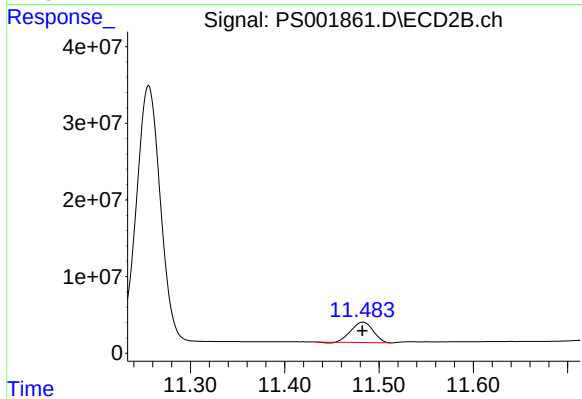

#6 MCP


R.T.: 11.483 min
Delta R.T.: 0.000 min
Response: 43160659
Conc: 73.25 ug/ml

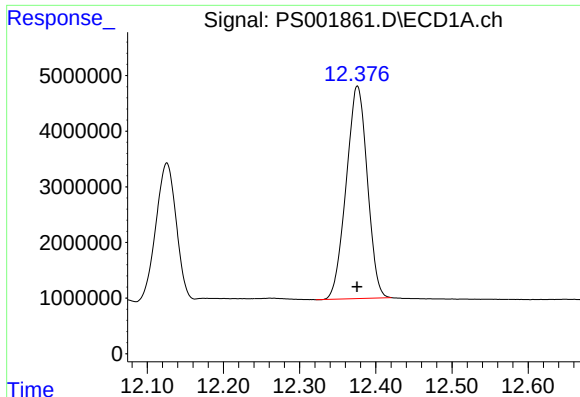

#7 MCPA


R.T.: 12.376 min
Delta R.T.: 0.000 min
Response: 73587318
Conc: 70.12 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

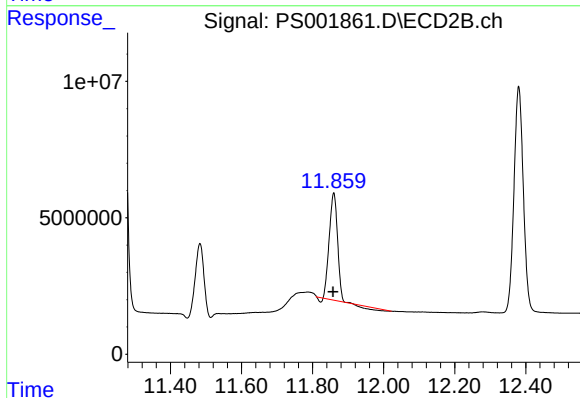


#7 MCPA

R.T.: 11.860 min
Delta R.T.: 0.002 min
Response: 59764064
Conc: 68.95 ug/ml

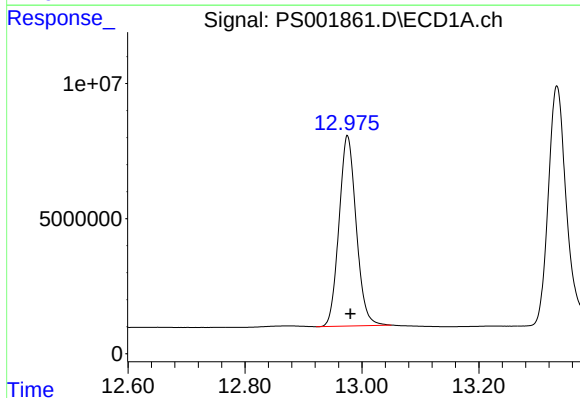


#8 DICHLORPROP

R.T.: 12.975 min
Delta R.T.: -0.005 min
Response: 143741070
Conc: 619.40 ng/ml

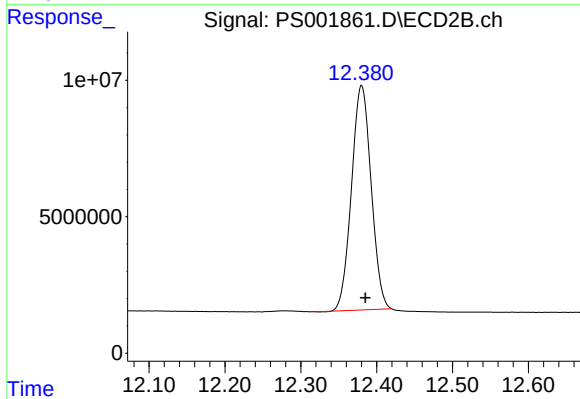

#8 DICHLORPROP


R.T.: 12.380 min
Delta R.T.: -0.005 min
Response: 147972245
Conc: 637.06 ng/ml

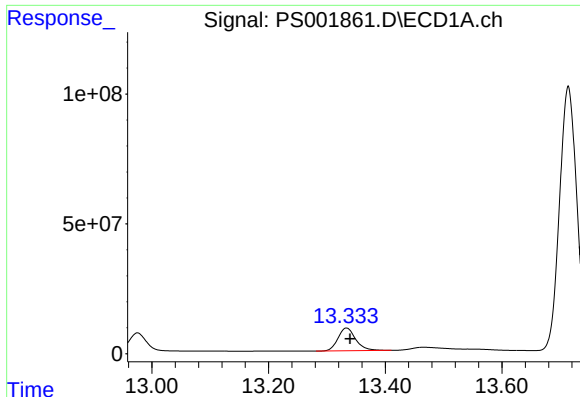

#9 2,4-D


R.T.: 13.333 min
Delta R.T.: -0.006 min
Response: 185238125
Conc: 672.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

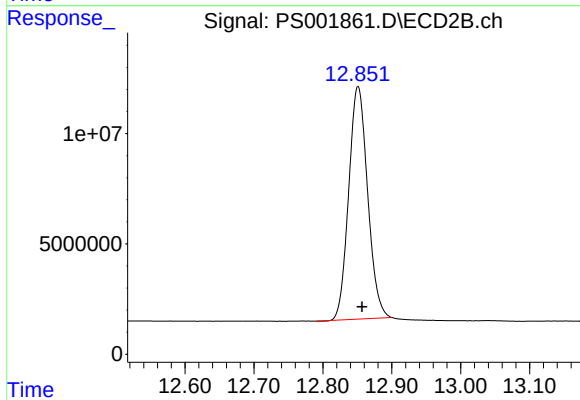


#9 2,4-D

R.T.: 12.851 min
Delta R.T.: -0.006 min
Response: 201018135
Conc: 646.14 ng/ml

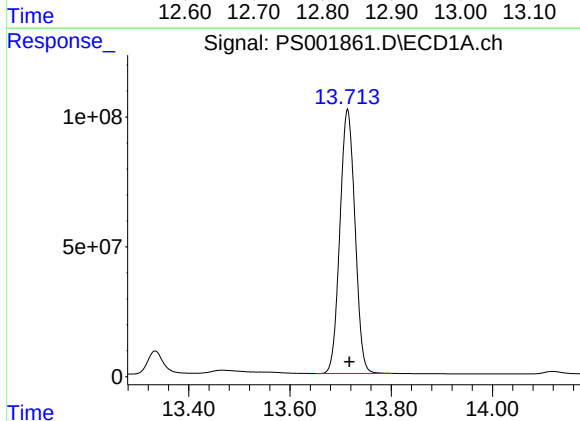


#10 Pentachlorophenol

R.T.: 13.714 min
Delta R.T.: -0.004 min
Response: 2103968480
Conc: 684.61 ng/ml

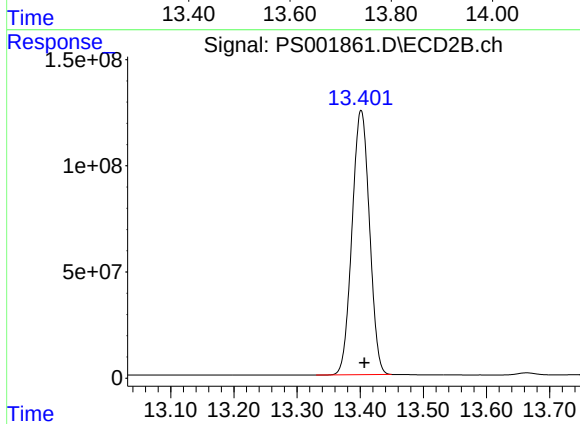

#10 Pentachlorophenol


R.T.: 13.401 min
Delta R.T.: -0.005 min
Response: 2387352489
Conc: 696.56 ng/ml

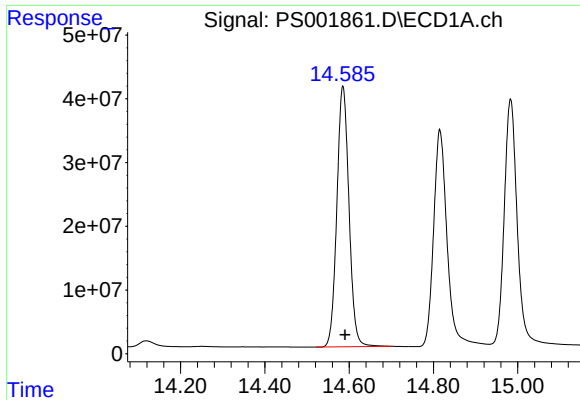

#11 2,4,5-TP (SILVEX)


R.T.: 14.585 min
Delta R.T.: -0.005 min
Response: 816350312
Conc: 690.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

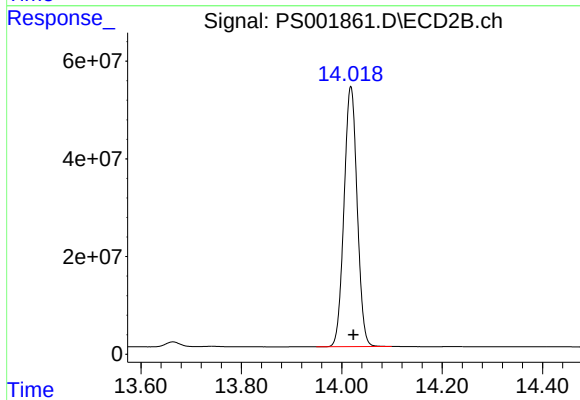


#11 2,4,5-TP (SILVEX)

R.T.: 14.018 min
Delta R.T.: -0.005 min
Response: 967254485
Conc: 705.44 ng/ml

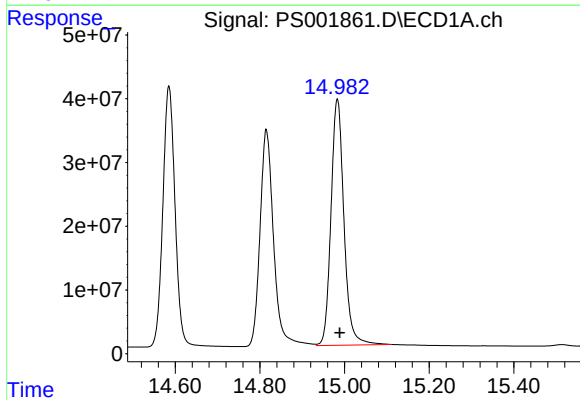


#12 2,4,5-T

R.T.: 14.983 min
Delta R.T.: -0.005 min
Response: 820486936
Conc: 687.31 ng/ml

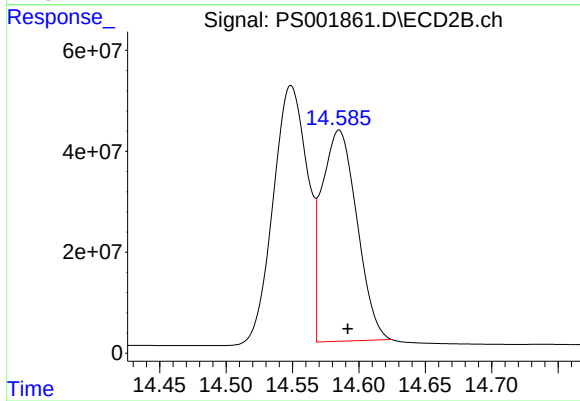

#12 2,4,5-T


R.T.: 14.585 min
Delta R.T.: -0.006 min
Response: 766972311
Conc: 694.54 ng/ml

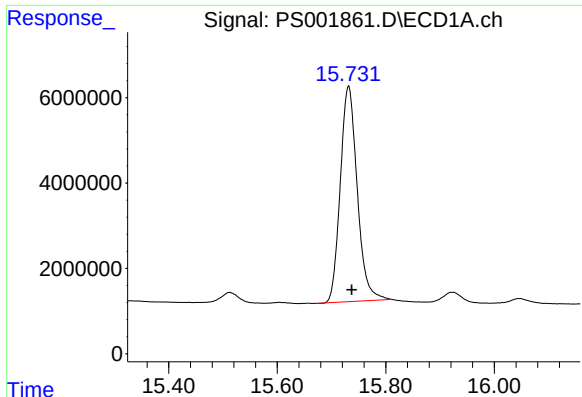

#13 2,4-DB


R.T.: 15.731 min
Delta R.T.: -0.006 min
Response: 109368496
Conc: 671.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

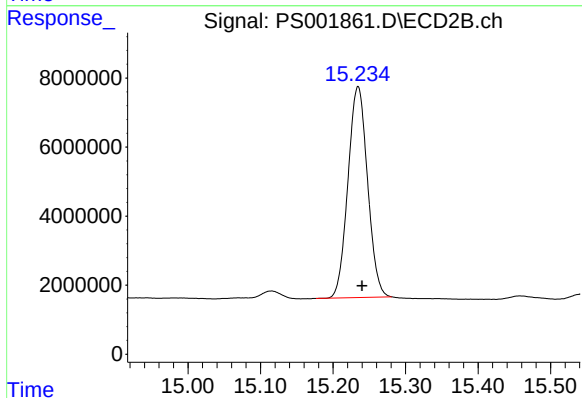


#13 2,4-DB

R.T.: 15.235 min
Delta R.T.: -0.006 min
Response: 114599473
Conc: 692.36 ng/ml

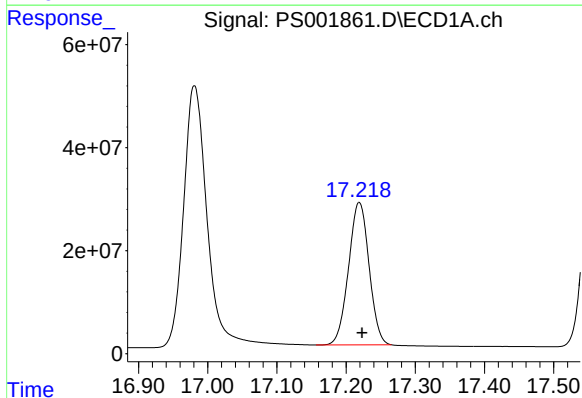


#14 DINOSEB

R.T.: 17.219 min
Delta R.T.: -0.004 min
Response: 570294466
Conc: 684.14 ng/ml

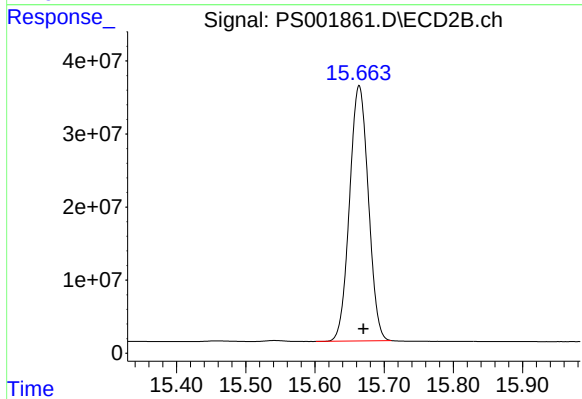

#14 DINOSEB


R.T.: 15.664 min
Delta R.T.: -0.006 min
Response: 660078299
Conc: 696.42 ng/ml

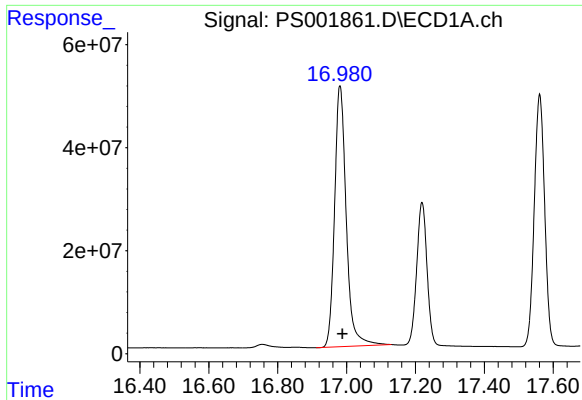

#15 Picloram


R.T.: 16.981 min
Delta R.T.: -0.008 min
Response: 1190137925
Conc: 683.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

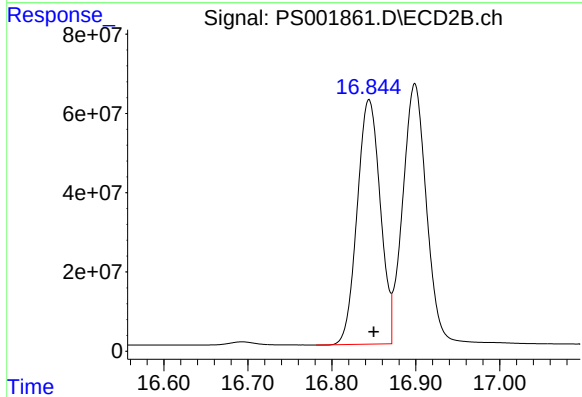


#15 Picloram

R.T.: 16.844 min
Delta R.T.: -0.006 min
Response: 1176849014
Conc: 691.96 ng/ml

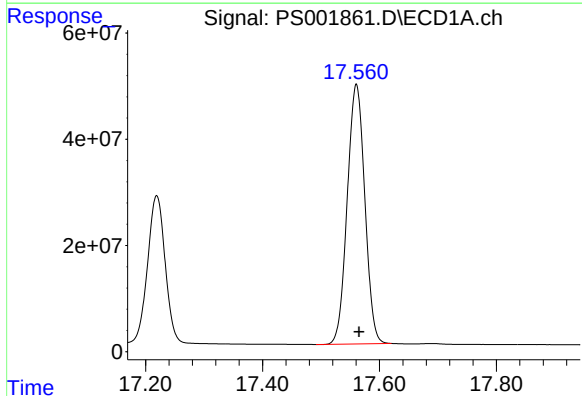

#16 DCPA

R.T.: 17.560 min
Delta R.T.: -0.005 min
Response: 1019997624
Conc: 693.17 ng/ml

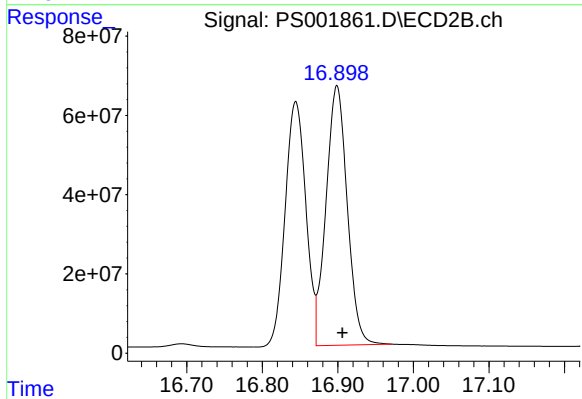

#16 DCPA

R.T.: 16.899 min
Delta R.T.: -0.007 min
Response: 1276698916
Conc: 692.19 ng/ml